

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
 Data File : PD052565.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 3:02
 Operator : AJ\SJ
 Sample : K2168-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 07:06:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	22537595	502.7E6	15.889	15.731
27)	SA Decachlor...	7.817	9.159	37300244	484.1E6	24.829	24.899
Target Compounds							
2)	A alpha-BHC	0.000	4.406f	0 26009976	N.D.	0.540	
3)	MA gamma-BHC...	3.921	0.000	7819982	0	3.535	N.D. #
6)	B beta-BHC	0.000	4.937f	0 25357826	N.D.	1.223	
8)	B Heptachlo...	0.000	5.916	0 38672280	N.D.	1.015	
10)	B trans-Chl...	0.000	6.114f	0 4693119	N.D.	0.124	
15)	B Endosulfa...	0.000	6.981	0 17299401	N.D.	0.607	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
Data File : PD052565.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 3:02
Operator : AJ\SJ
Sample : K2168-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:06:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

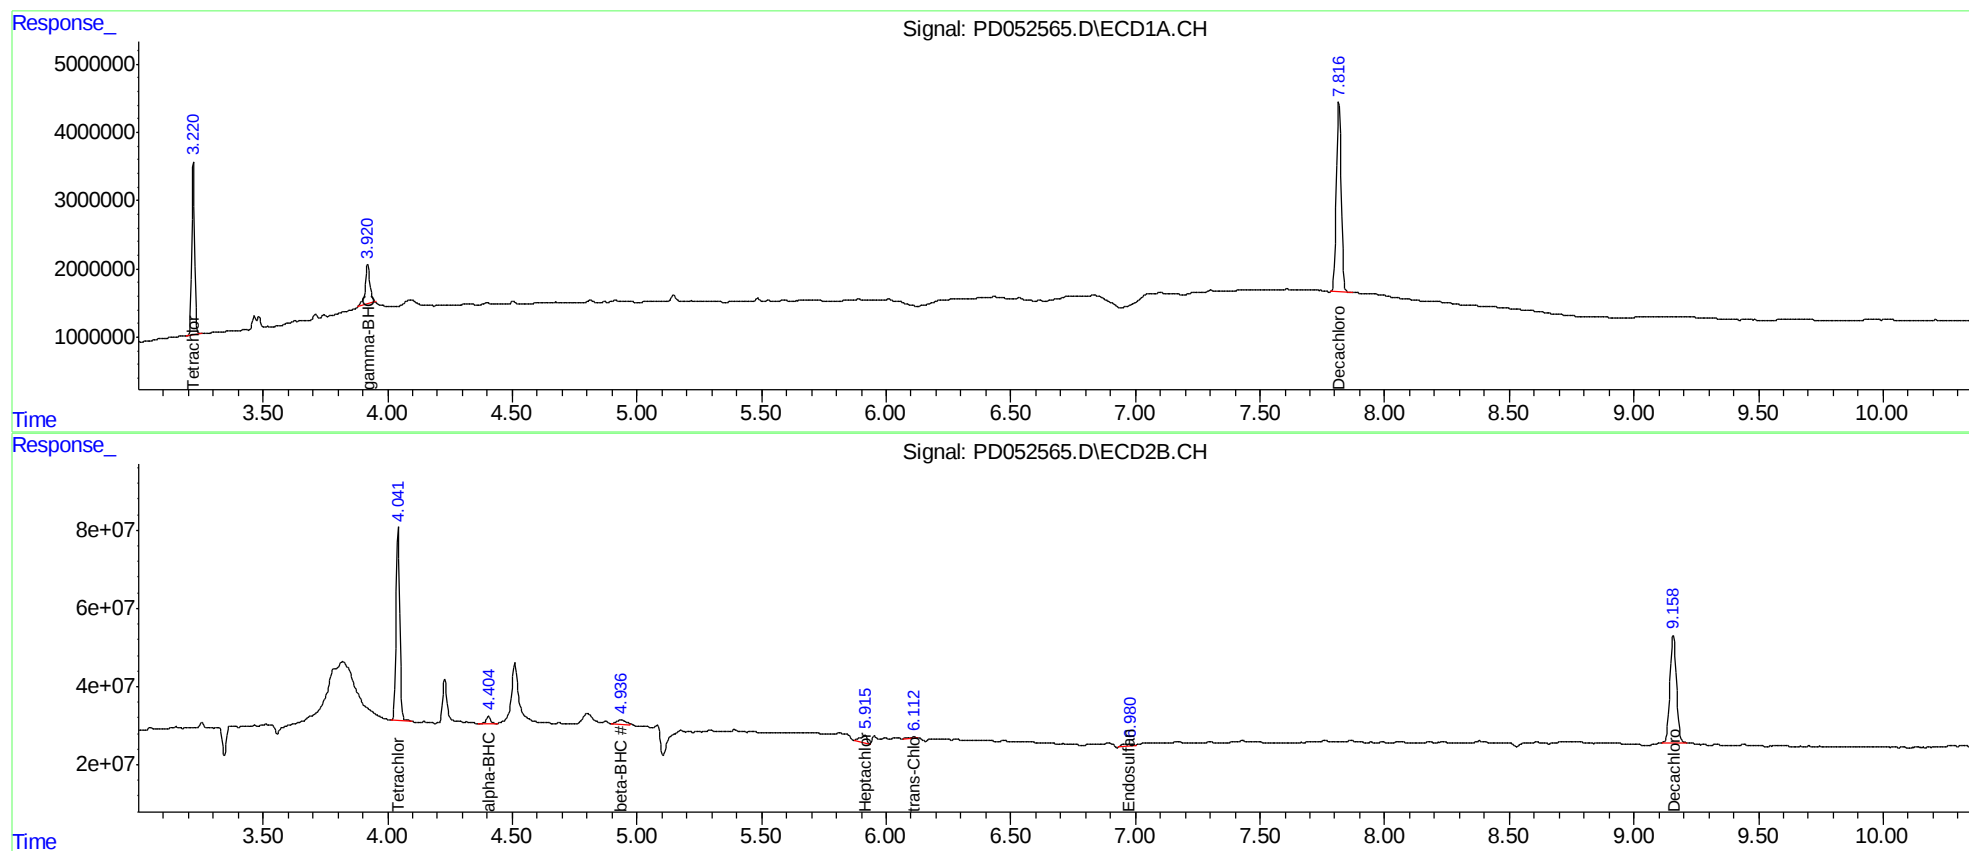


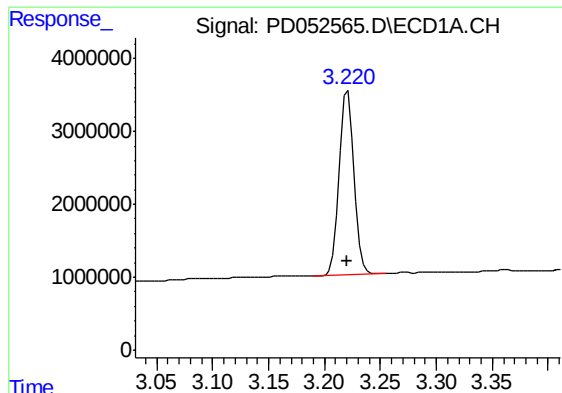

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 22537595
Conc: 15.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

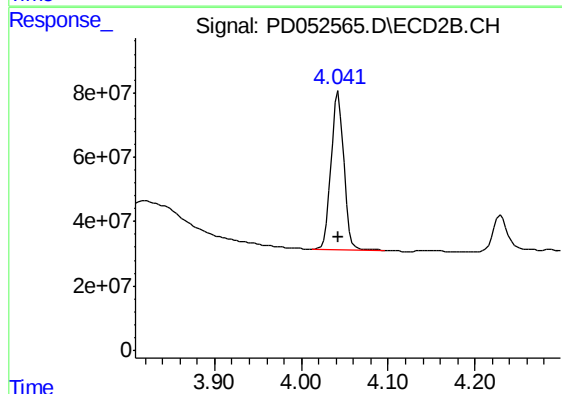


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 502716626
Conc: 15.73 ng/ml

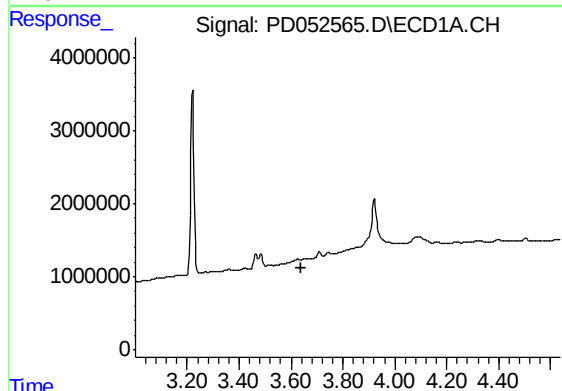


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

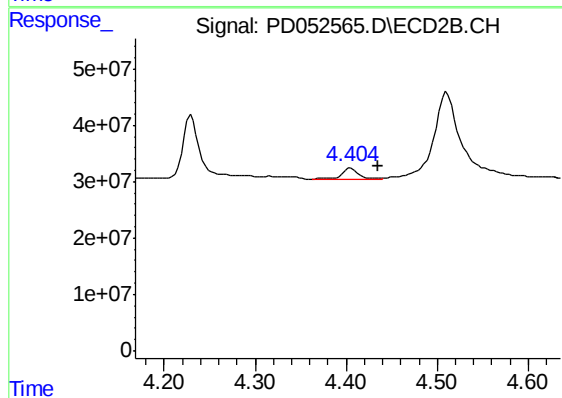

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: -0.029 min
Response: 26009976
Conc: 0.54 ng/ml

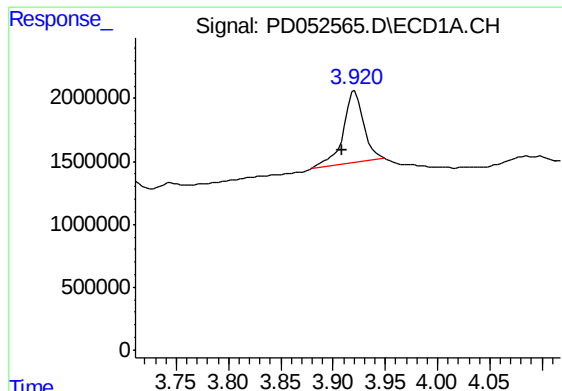

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.013 min
Response: 7819982
Conc: 3.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

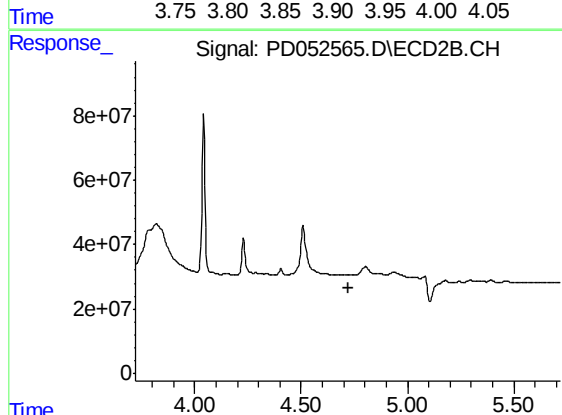


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

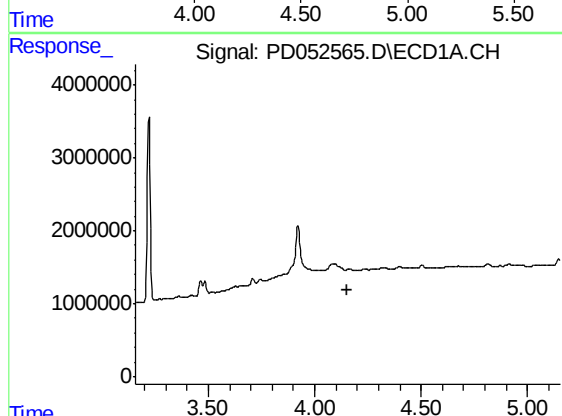


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

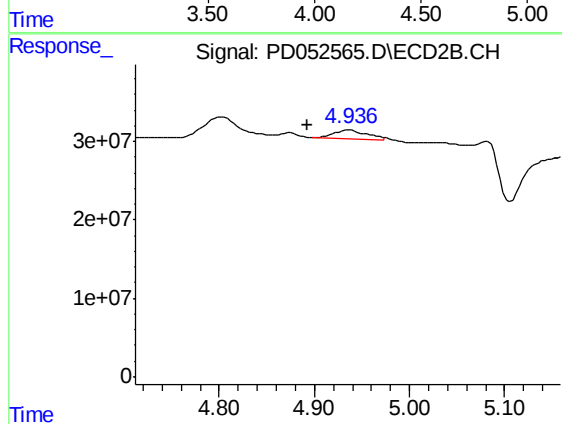

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.045 min
Response: 25357826
Conc: 1.22 ng/ml

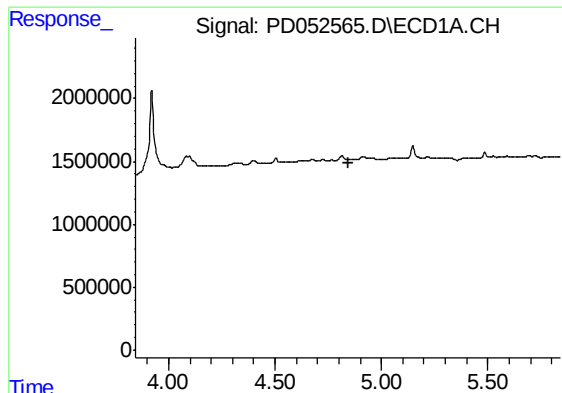

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

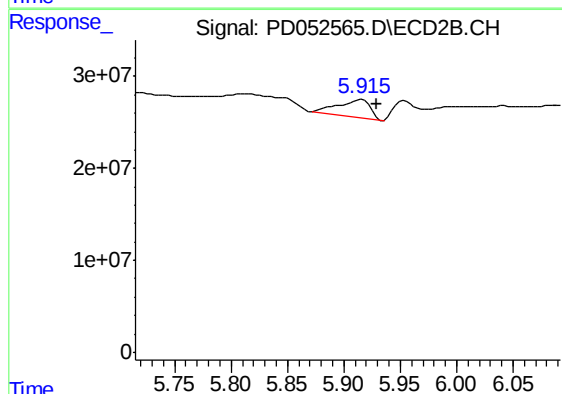


#8 Heptachlor epoxide

R.T.: 5.916 min
Delta R.T.: -0.014 min
Response: 38672280
Conc: 1.01 ng/ml

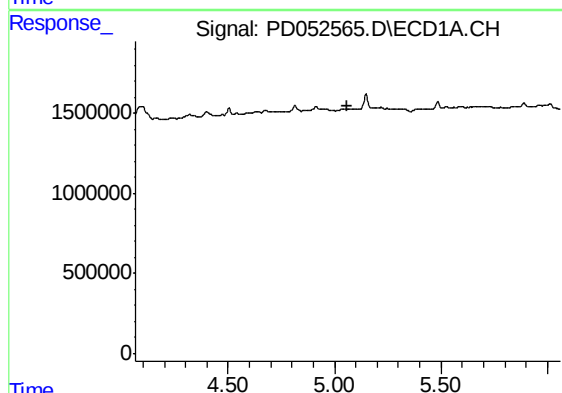


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

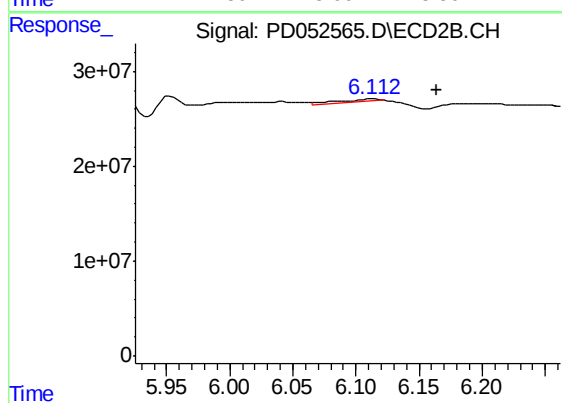

#10 trans-Chlordane


R.T.: 6.114 min
Delta R.T.: -0.051 min
Response: 4693119
Conc: 0.12 ng/ml

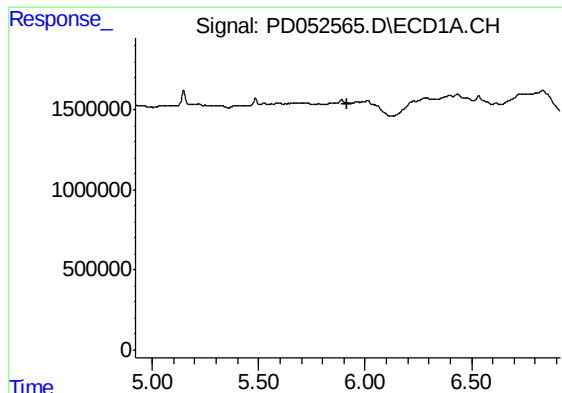

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

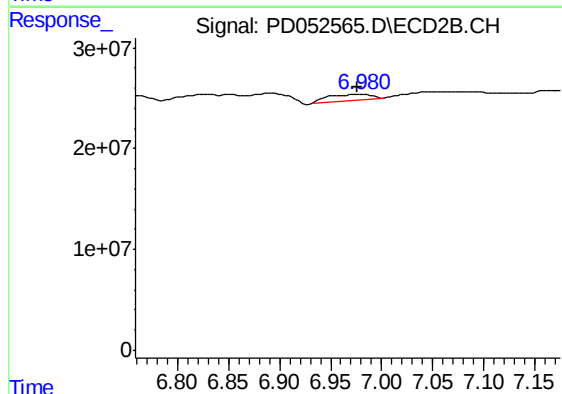


#15 Endosulfan II

R.T.: 6.981 min
Delta R.T.: 0.005 min
Response: 17299401
Conc: 0.61 ng/ml

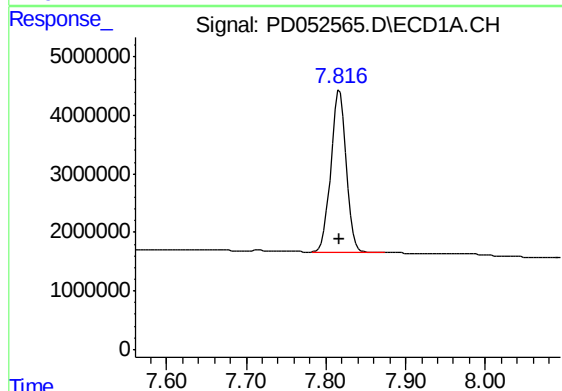

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: 0.000 min
Response: 37300244
Conc: 24.83 ng/ml

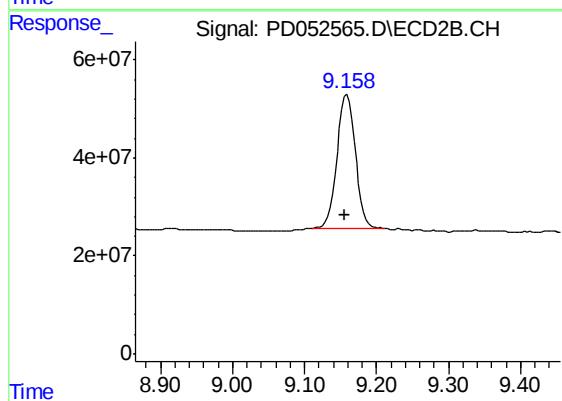

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 484058429
Conc: 24.90 ng/ml