

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
 Data File : PD052546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 22:32
 Operator : AJ\SJ
 Sample : K2122-04DL2 20X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5B9DL2

Manual Integrations
 APPROVED

Sohil
 4/4/2019 5:17:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:28:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.042	442054	12886087	0.312m	0.403 #
2)	SA Decachlor...	7.801	9.156	2854457	17048504	1.900m	0.877m#
Target Compounds							
10)	B trans-Chl...	5.062	6.164	77140691	1727.8E6	37.490	45.699m
11)	B cis-Chlor...	5.117	6.240	104.2E6	2406.1E6	51.905	66.605 #
15)	B Endosulfa...	5.920	6.981	4003070	17035897	2.137m	0.598 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
Data File : PD052546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 22:32
Operator : AJ\SJ
Sample : K2122-04DL2 20X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:28:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

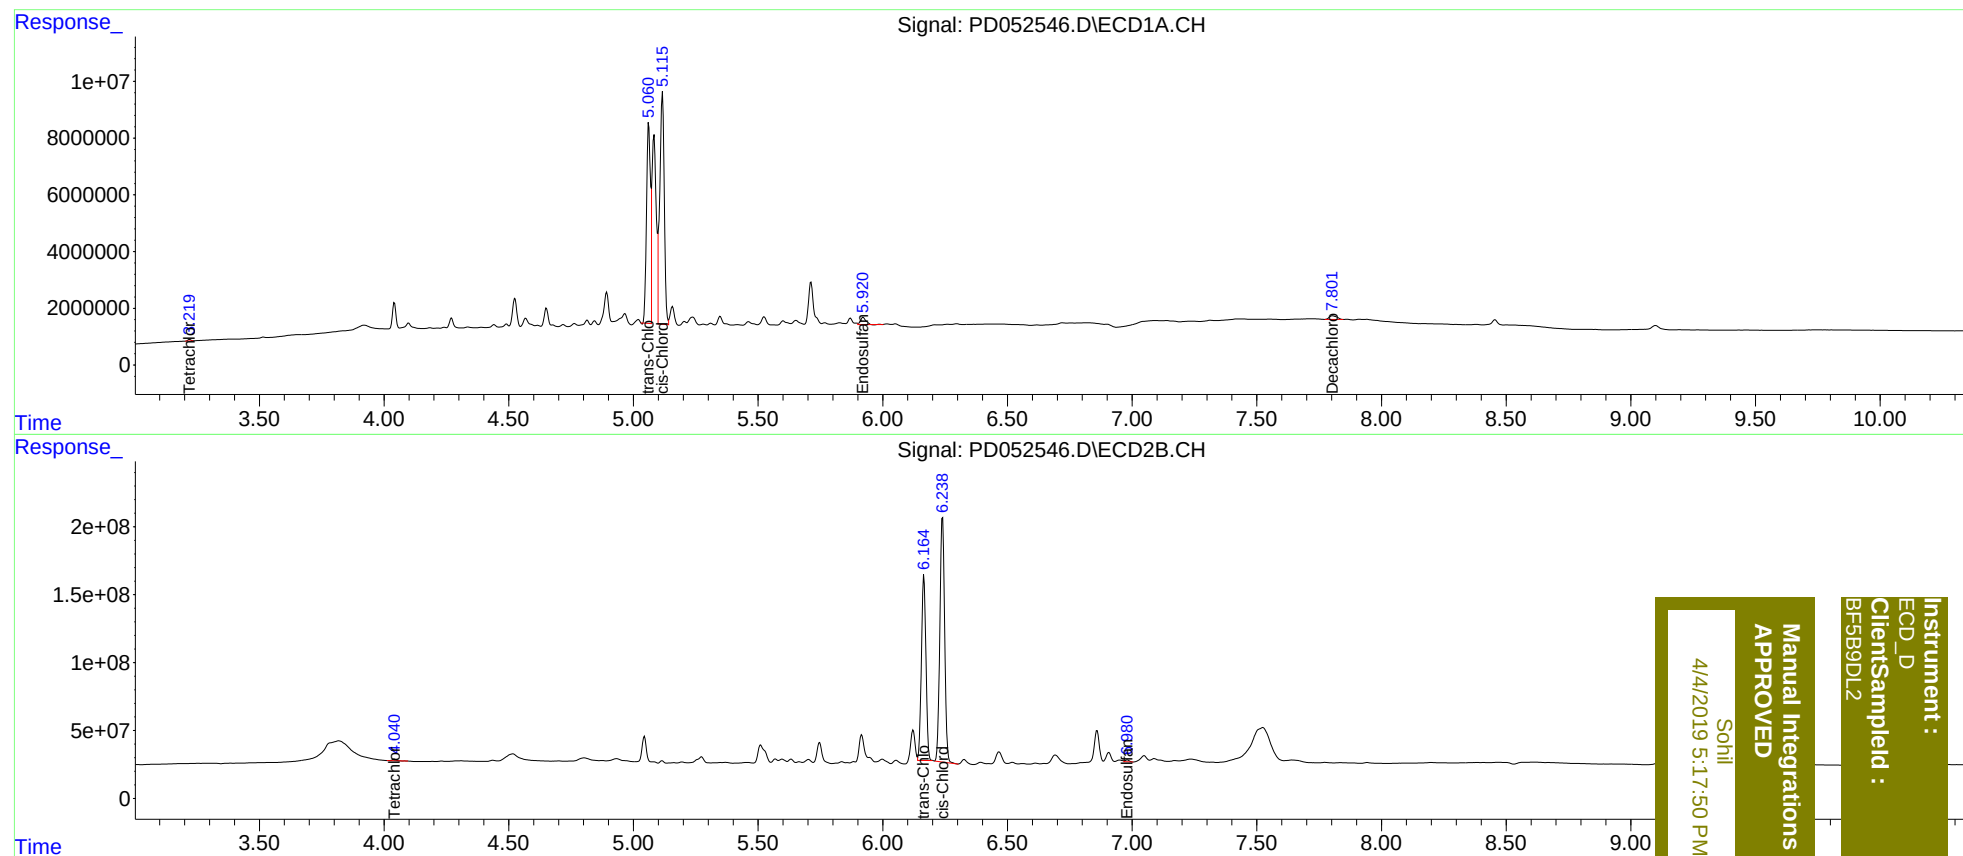

4/4/2019 5:17:50 PM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampleId :
BF5B9DL2