

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040422\
 Data File : PD068931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2022 17:52
 Operator : AR\AJ
 Sample : N2207-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-098-21-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:37:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.173	22552554	187.8E6	18.574	19.645
28)	SA Decachlor...	8.204	9.369	24524744	120.2E6	19.412	21.203

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040422\
Data File : PD068931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2022 17:52
Operator : AR\AJ
Sample : N2207-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SPLP-LEACHATE-AMENDED-098-21-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:37:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

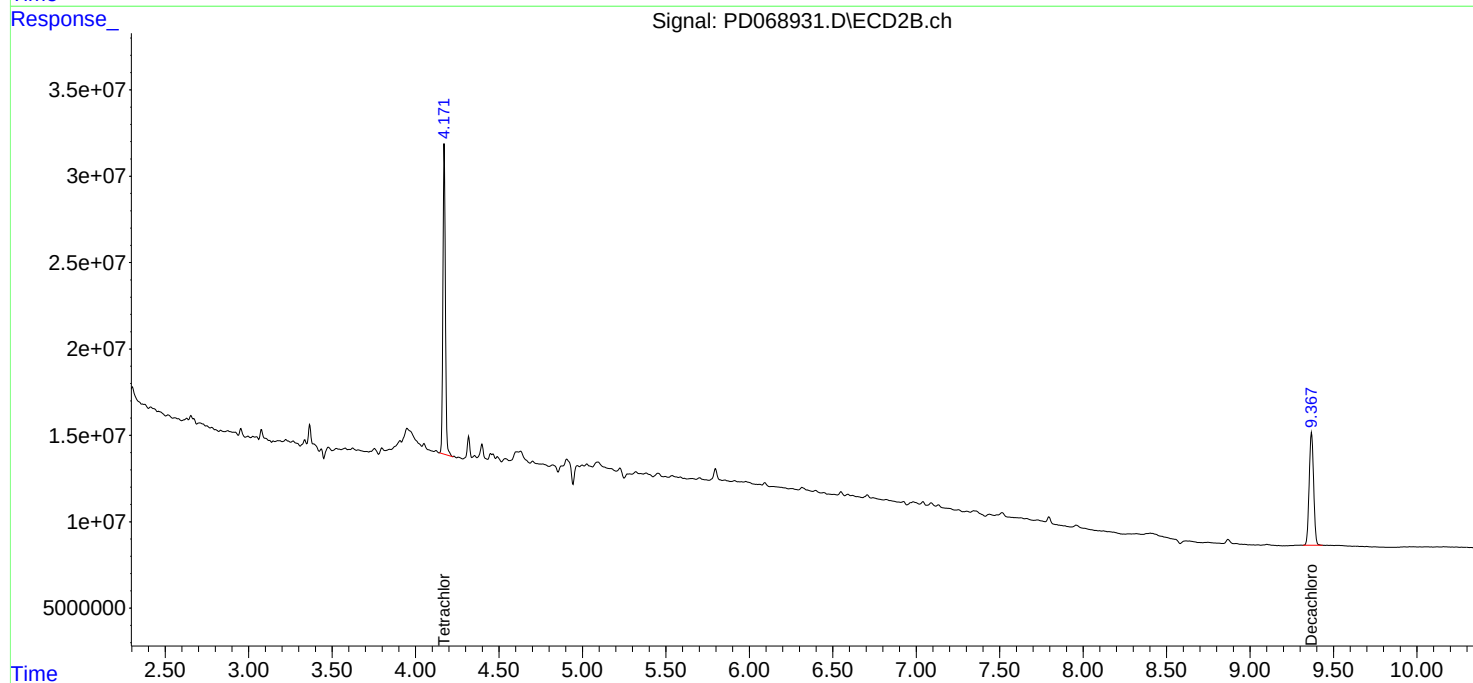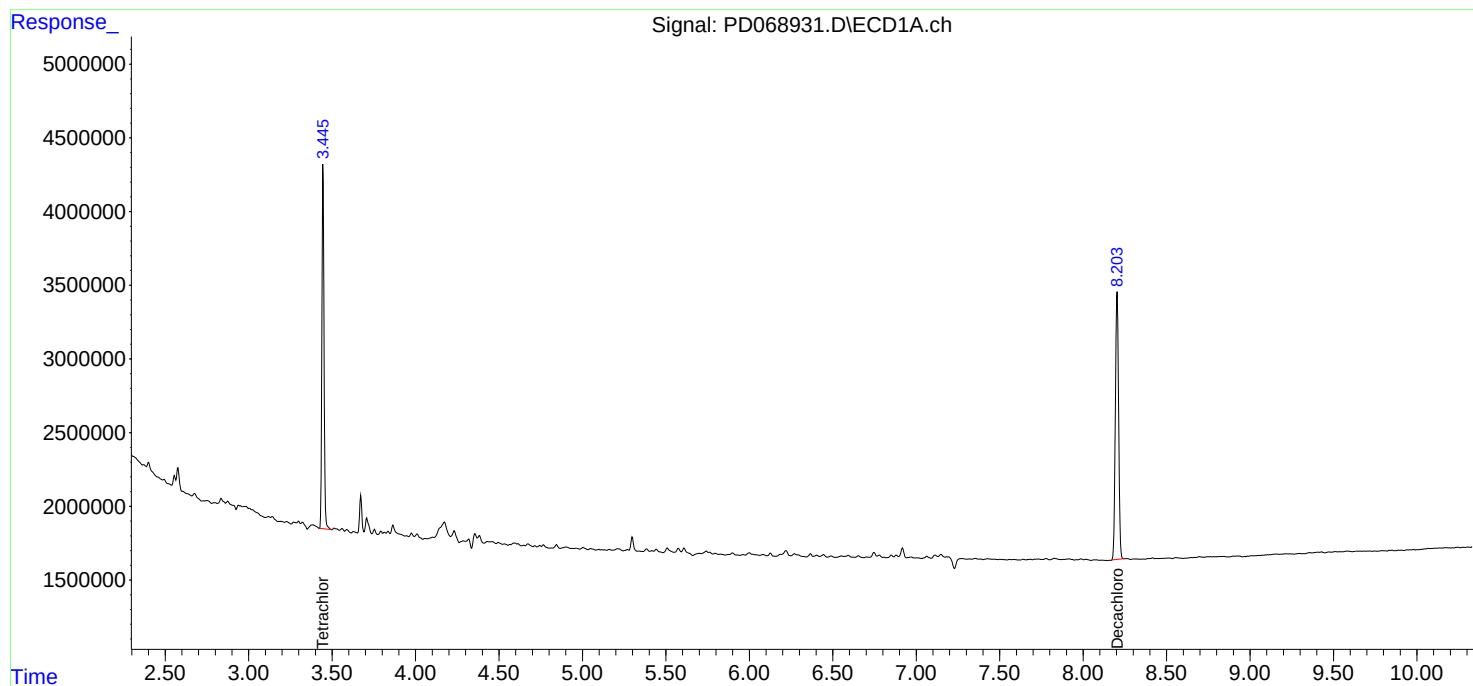

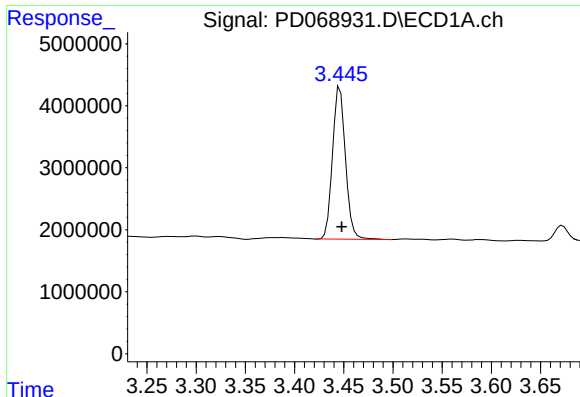

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 22552554
Conc: 18.57 ng/ml

Instrument :

ECD_D


ClientSampleId :

SPLP-LEACHATE-AMENDED-098-21-01

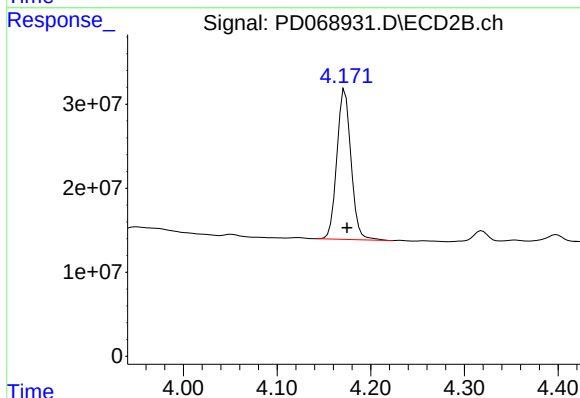


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.002 min
Response: 187824495
Conc: 19.65 ng/ml

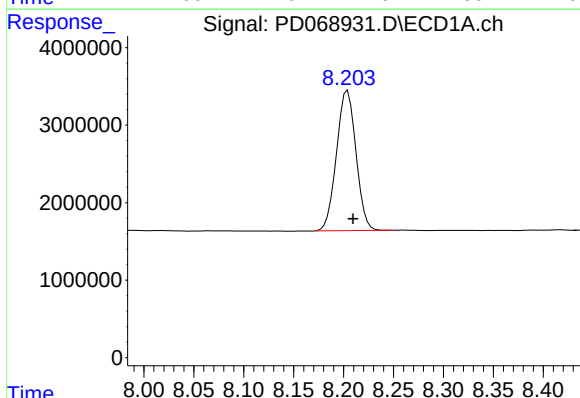

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.006 min
Response: 24524744
Conc: 19.41 ng/ml

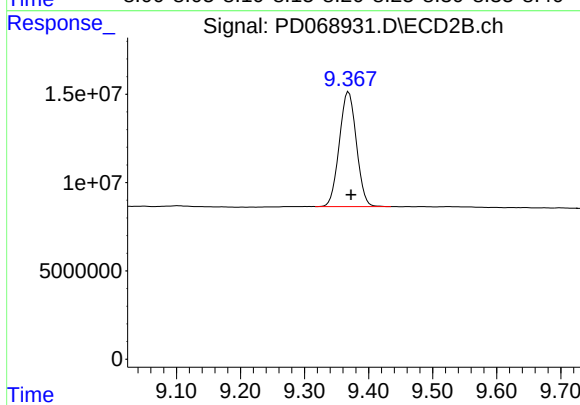

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.004 min
Response: 120152074
Conc: 21.20 ng/ml