

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052596.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 11:34
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:49:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28) SA	Decachlor...	0.000	9.160	0	7120648	N.D.	0.458 #
Target Compounds							
2) A	alpha-BHC	3.663f	4.425	398254	6212523	0.175	0.138
3) MA	gamma-BHC...	3.912	4.737	5311060	2440868	2.429	0.061 #
4) MA	Heptachlor	0.000	5.249	0	2780419	N.D.	0.070 #
9) A	Endosulfan I	0.000	6.290	0	7155189	N.D.	0.245 #
10) B	gamma-Chl...	0.000	6.188f	0	20419143	N.D.	0.638 #
11) B	alpha-Chl...	0.000	6.230	0	9068632	N.D.	0.289 #
17) MA	4,4'-DDT	0.000	7.203	0	7003893	N.D.	0.376 #
18) B	Endrin al...	0.000	7.095	0	14599712	N.D.	0.709 #
25)	Chlordane-3	0.000	6.188f	0	20419143	N.D.	4.627 #
26)	Chlordane-4	0.000	6.250	0	11512817	N.D.	2.264 #
27)	Chlordane-5	0.000	7.048	0	19475359	N.D.	21.109 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052596.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 11:34
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:49:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

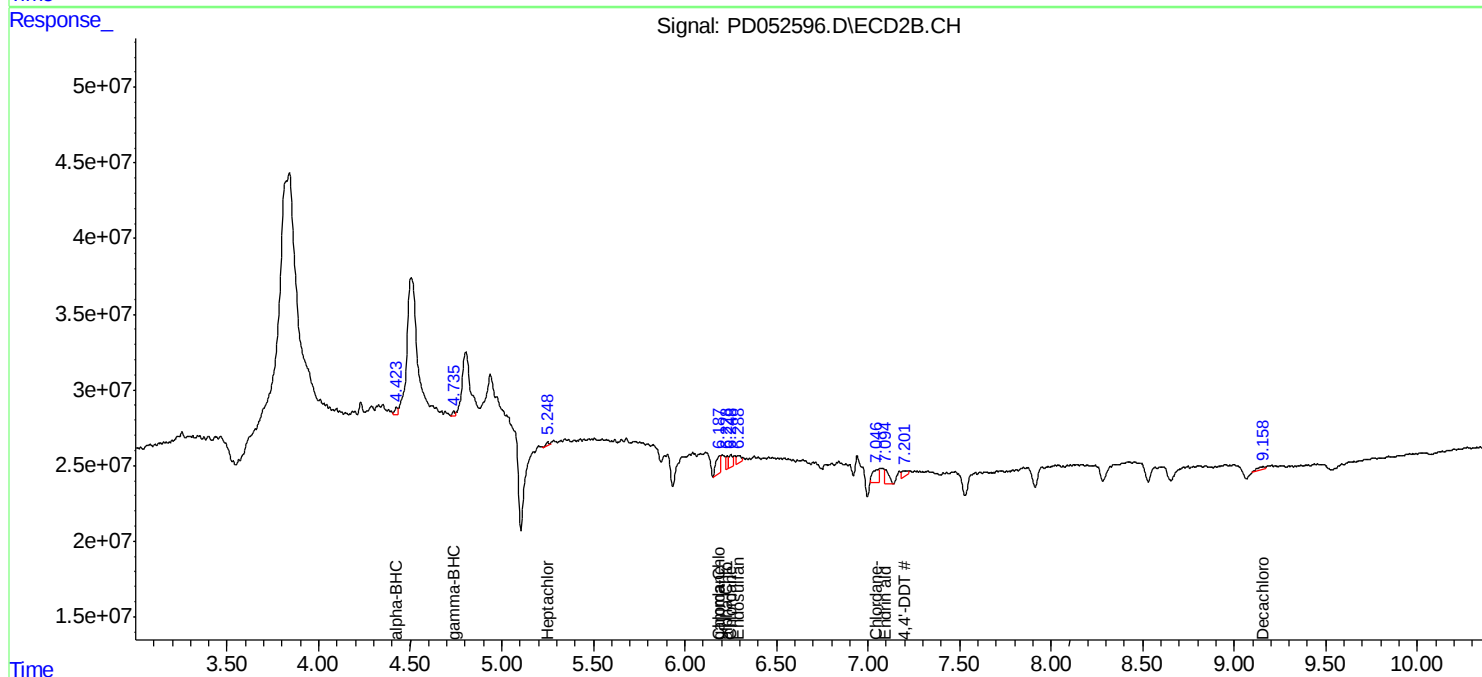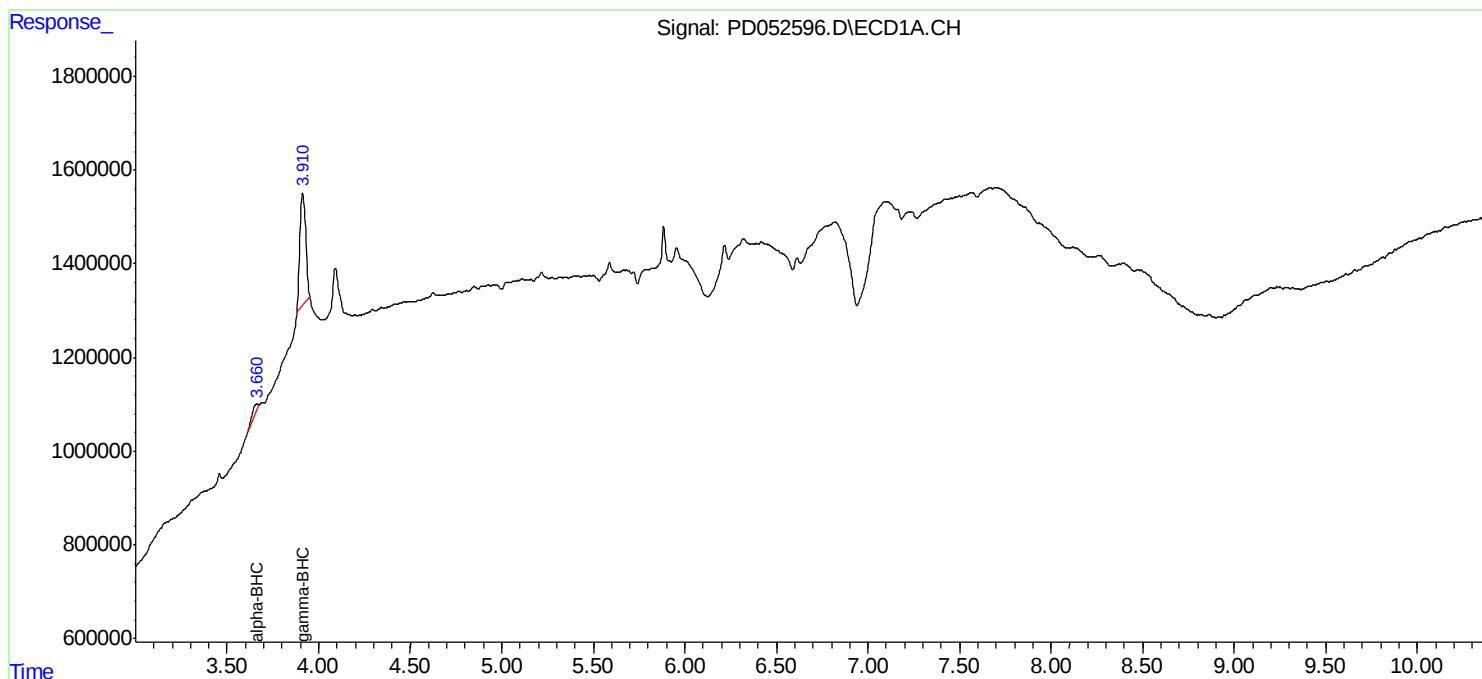


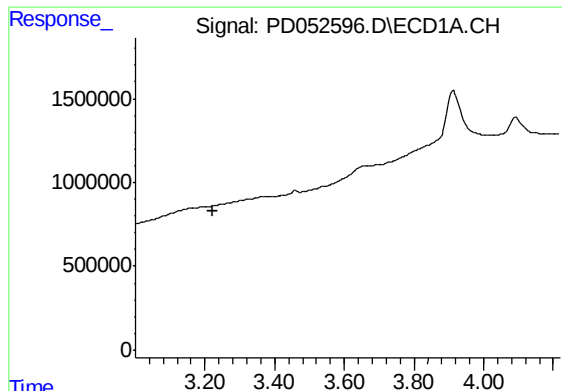

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

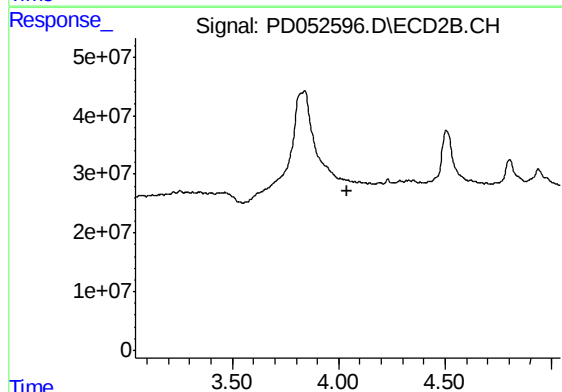


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.043 min
Response: 0
Conc: N.D.

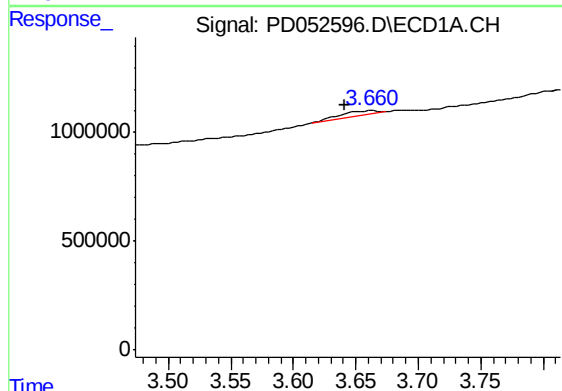


#2 alpha-BHC

R.T.: 3.663 min
Delta R.T.: 0.021 min
Response: 398254
Conc: 0.18 ng/ml

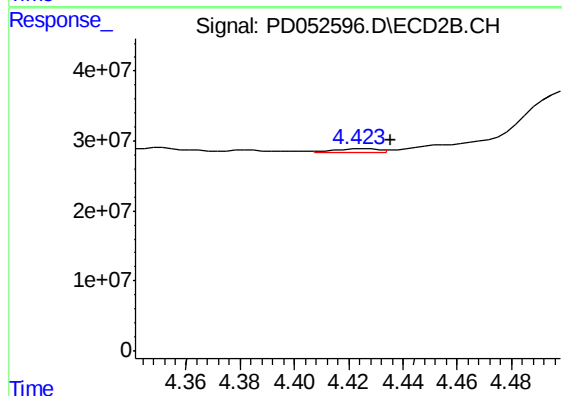

#2 alpha-BHC


R.T.: 4.425 min
Delta R.T.: -0.011 min
Response: 6212523
Conc: 0.14 ng/ml

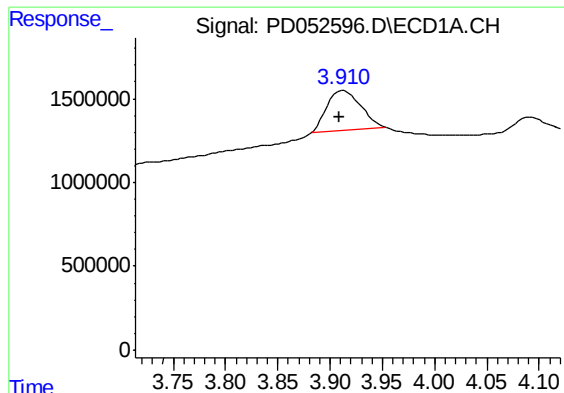

#3 gamma-BHC (Lindane)


R.T.: 3.912 min
Delta R.T.: 0.003 min
Response: 5311060
Conc: 2.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

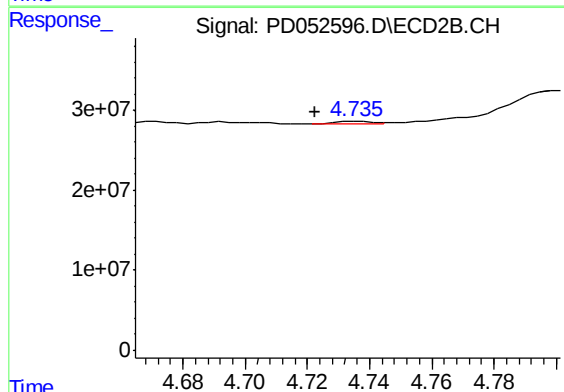


#3 gamma-BHC (Lindane)

R.T.: 4.737 min
Delta R.T.: 0.014 min
Response: 2440868
Conc: 0.06 ng/ml

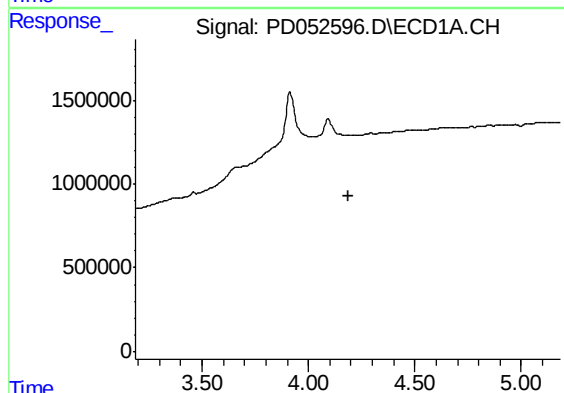


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

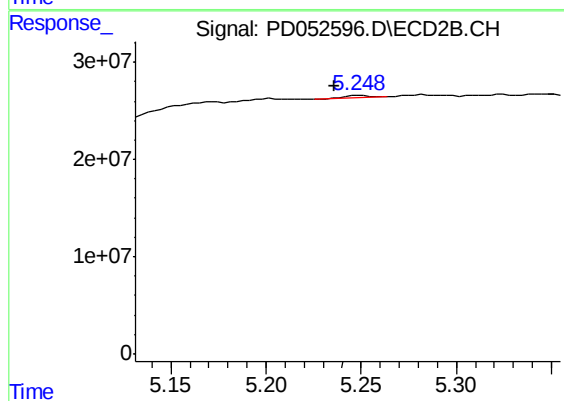

#4 Heptachlor


R.T.: 5.249 min
Delta R.T.: 0.013 min
Response: 2780419
Conc: 0.07 ng/ml

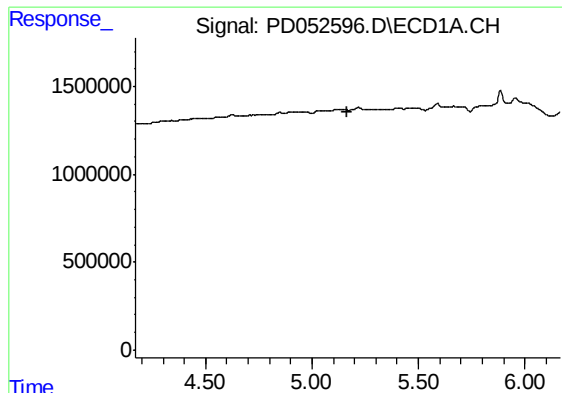

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

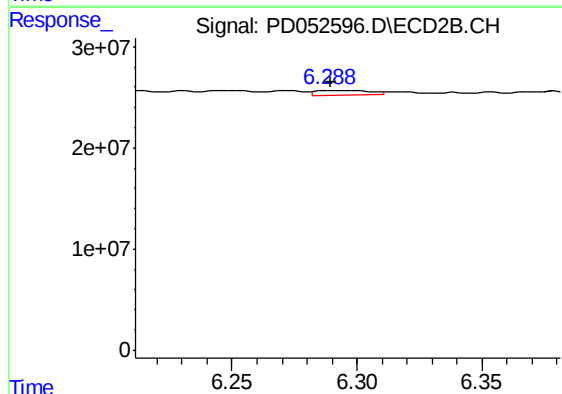


#9 Endosulfan I

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 7155189
Conc: 0.24 ng/ml

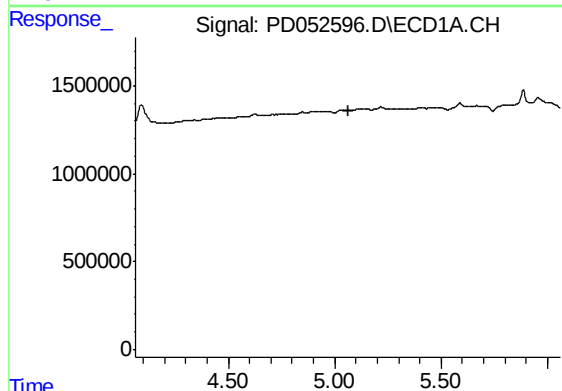


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

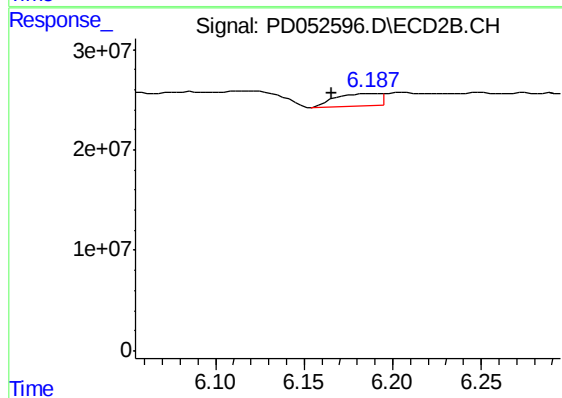

#10 gamma-Chlordane


R.T.: 6.188 min
Delta R.T.: 0.023 min
Response: 20419143
Conc: 0.64 ng/ml

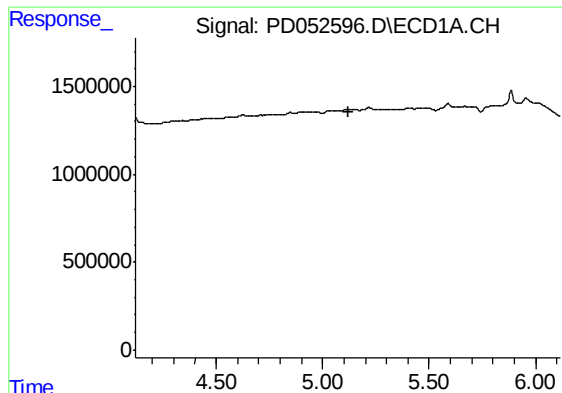

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

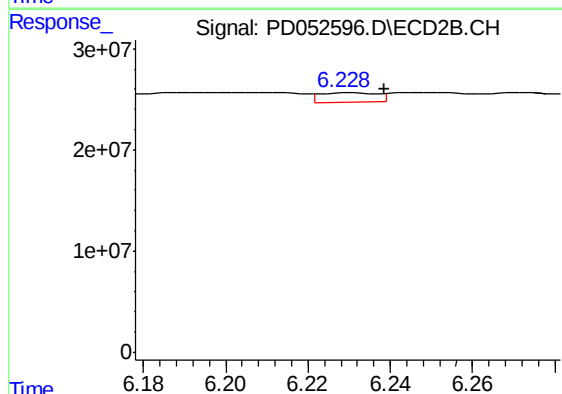


#11 alpha-Chlordane

R.T.: 6.230 min
Delta R.T.: -0.008 min
Response: 9068632
Conc: 0.29 ng/ml

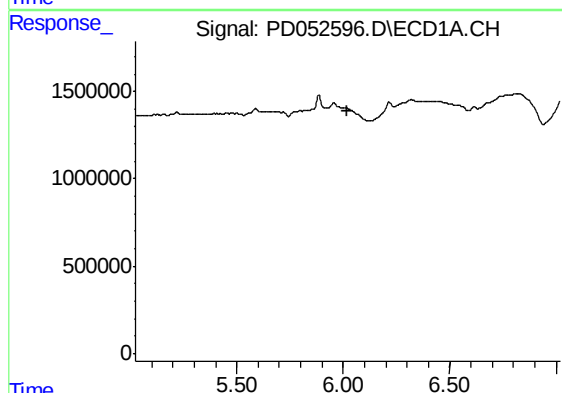


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.021 min
Response: 0
Conc: N.D.

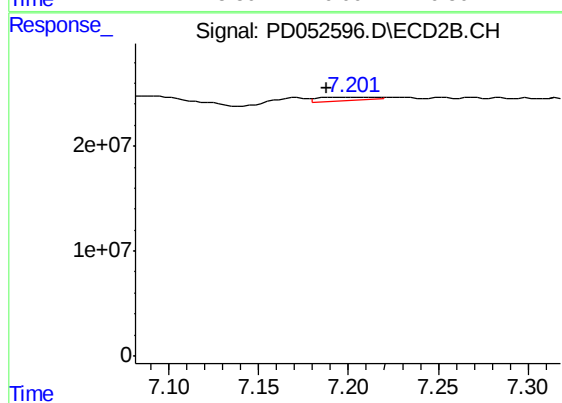

#17 4,4'-DDT


R.T.: 7.203 min
Delta R.T.: 0.015 min
Response: 7003893
Conc: 0.38 ng/ml

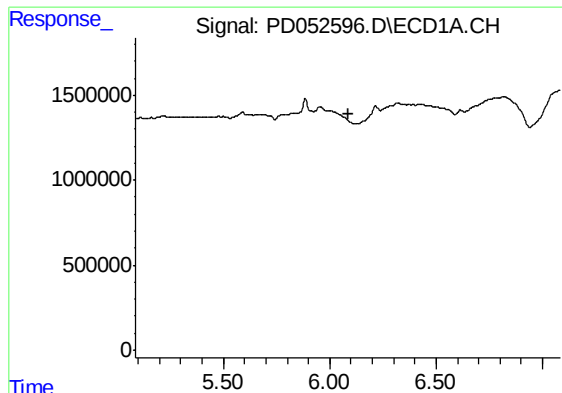

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

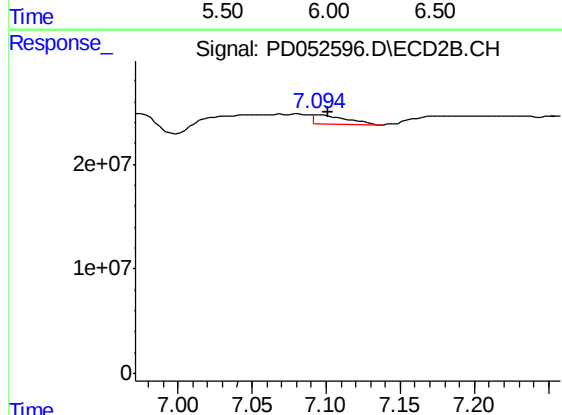


#18 Endrin aldehyde

R.T.: 7.095 min
Delta R.T.: -0.006 min
Response: 14599712
Conc: 0.71 ng/ml

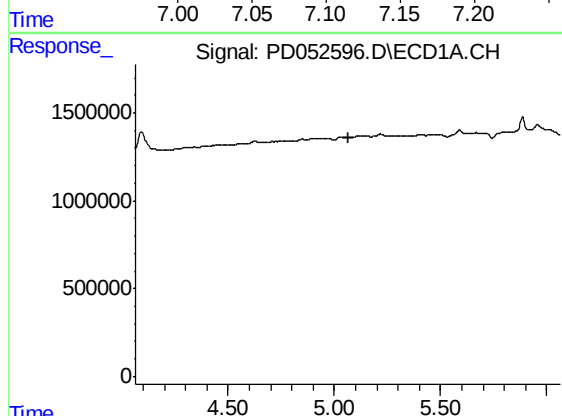


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

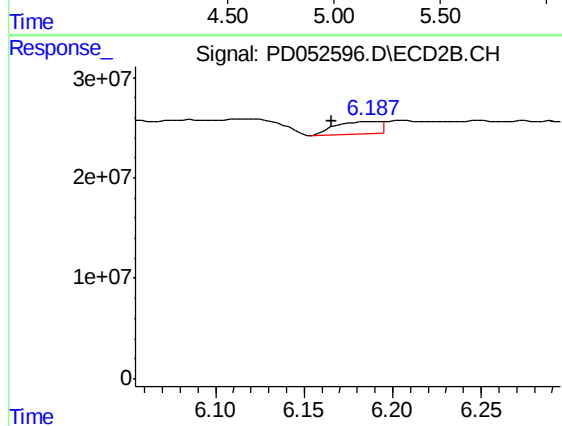

#25 Chlordane-3


R.T.: 6.188 min
Delta R.T.: 0.023 min
Response: 20419143
Conc: 4.63 ng/ml

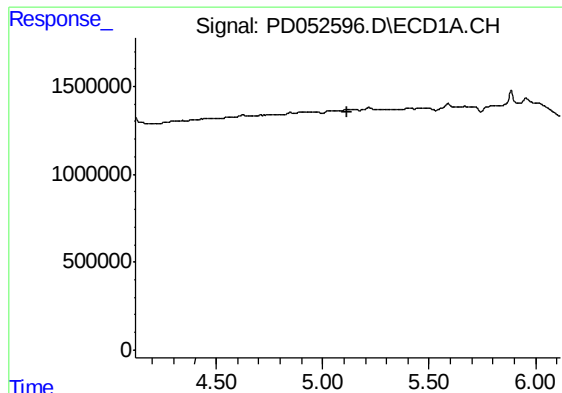

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

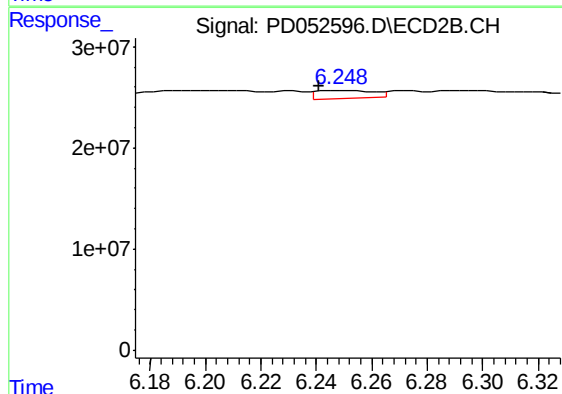


#26 Chlordane-4

R.T.: 6.250 min
Delta R.T.: 0.009 min
Response: 11512817
Conc: 2.26 ng/ml

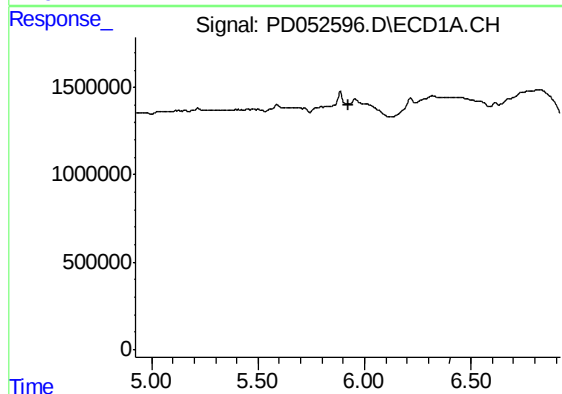


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

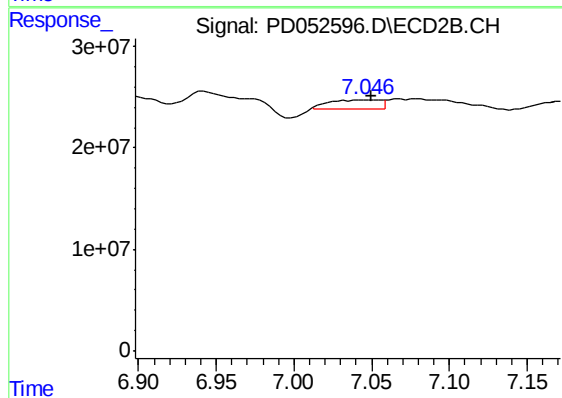

#27 Chlordane-5


R.T.: 7.048 min
Delta R.T.: -0.002 min
Response: 19475359
Conc: 21.11 ng/ml

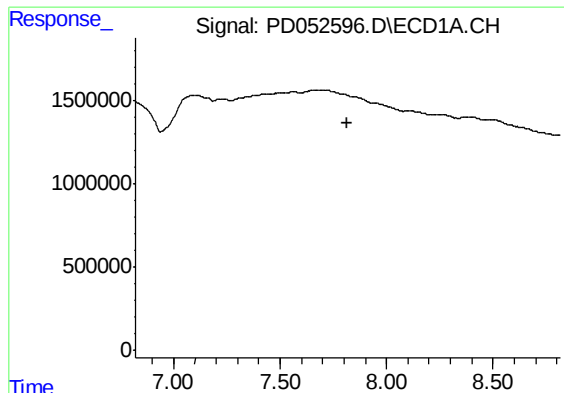

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

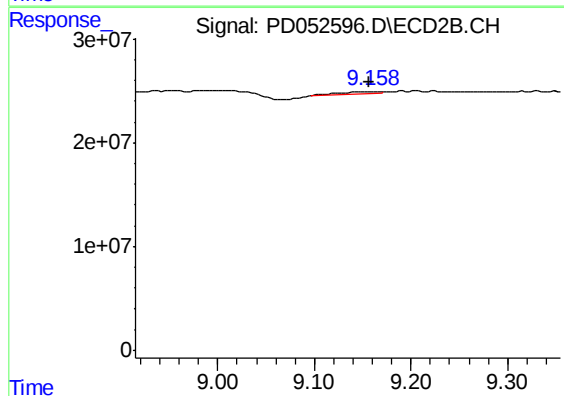

#28 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.004 min
Response: 7120648
Conc: 0.46 ng/ml