

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052609.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 14:36
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:53:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	28761297	628.4E6	20.611	21.682
28)	SA Decachlor...	7.818	9.162	31044567	393.4E6	23.293	25.295
Target Compounds							
3)	MA gamma-BHC...	3.918	0.000	3664351	0	1.676	N.D. #
4)	MA Heptachlor	0.000	5.260f	0	1470546	N.D.	0.037 #
8)	B Heptachlo...	4.869f	5.922	555895	11810568	0.292	0.366 #
10)	B gamma-Chl...	0.000	6.170	0	17187428	N.D.	0.537 #
14)	MA Endrin	0.000	6.758	0	22593332	N.D.	0.902 #
17)	MA 4,4'-DDT	0.000	7.177	0	9699493	N.D.	0.521 #
18)	B Endrin a...	0.000	7.092	0	8877360	N.D.	0.431 #
25)	Chlordane-3	0.000	6.170	0	17187428	N.D.	3.895 #
27)	Chlordane-5	0.000	7.056	0	13480514	N.D.	14.611 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052609.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 14:36
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:53:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

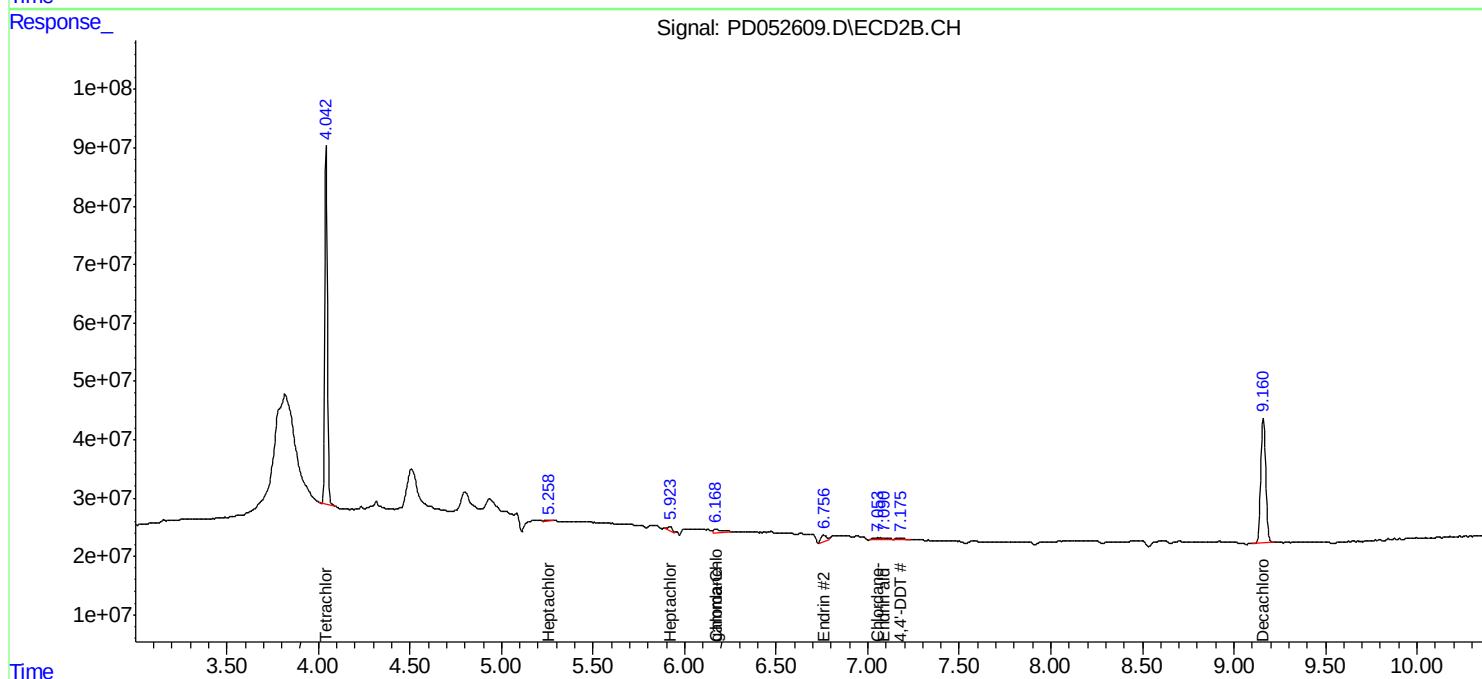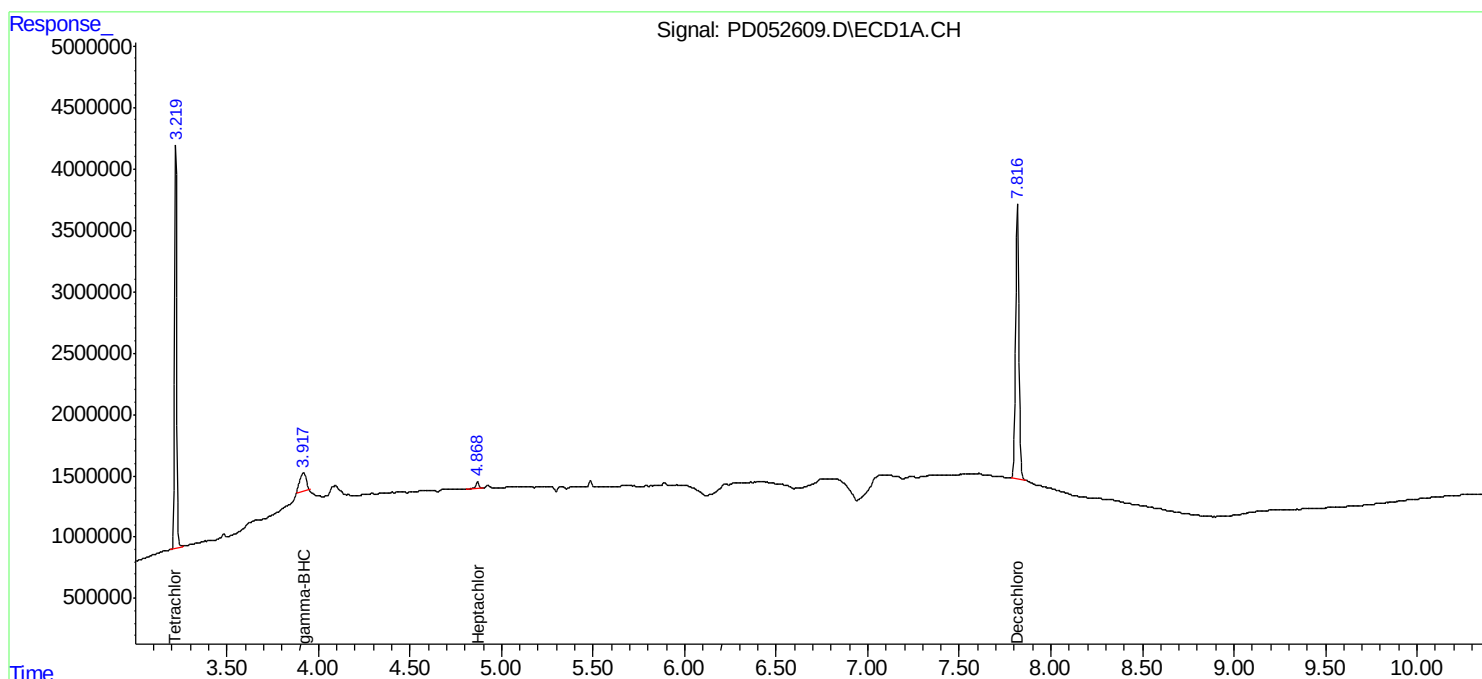


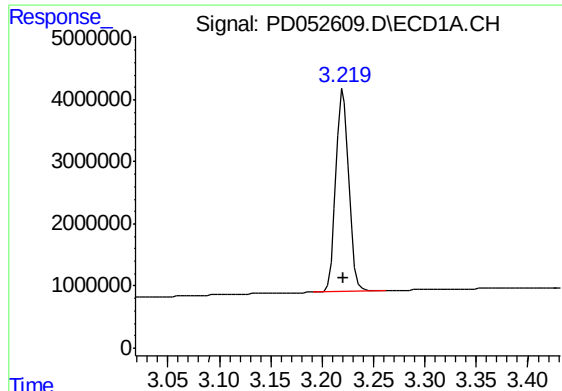

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28761297
Conc: 20.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

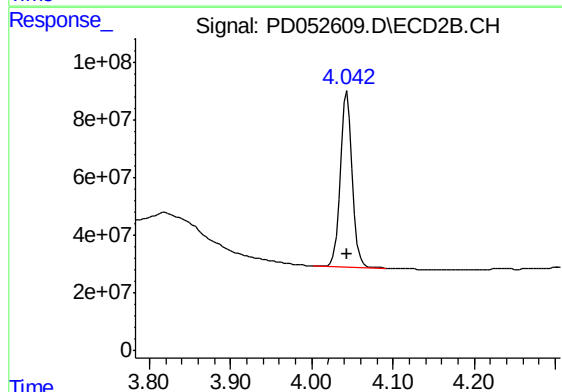


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 628437730
Conc: 21.68 ng/ml

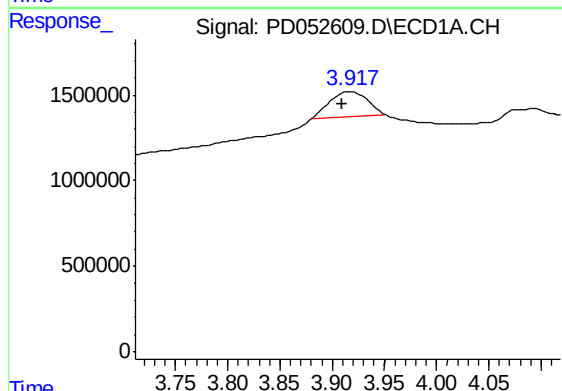


#3 gamma-BHC (Lindane)

R.T.: 3.918 min
Delta R.T.: 0.009 min
Response: 3664351
Conc: 1.68 ng/ml

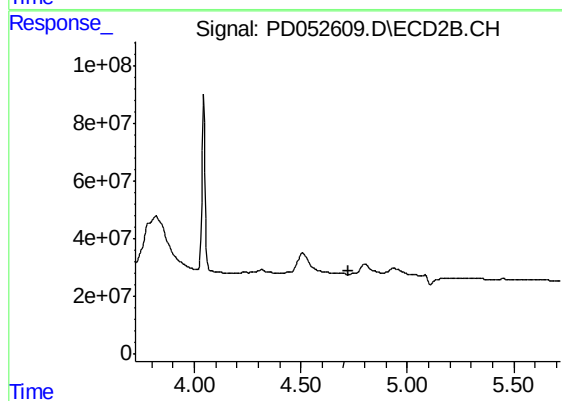

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

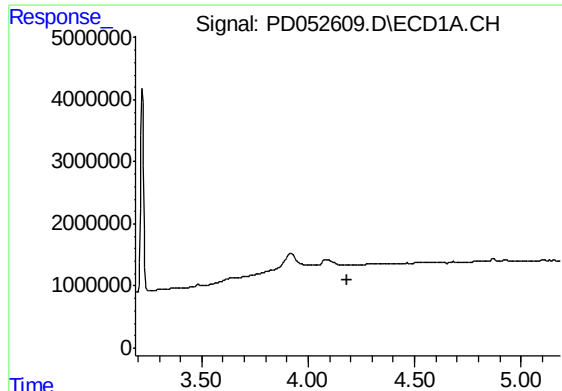

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

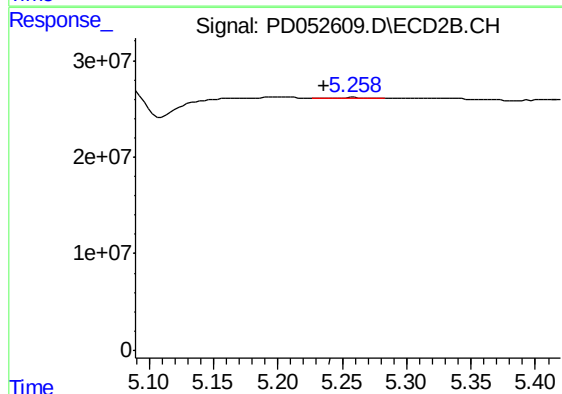


#4 Heptachlor

R.T.: 5.260 min
Delta R.T.: 0.024 min
Response: 1470546
Conc: 0.04 ng/ml

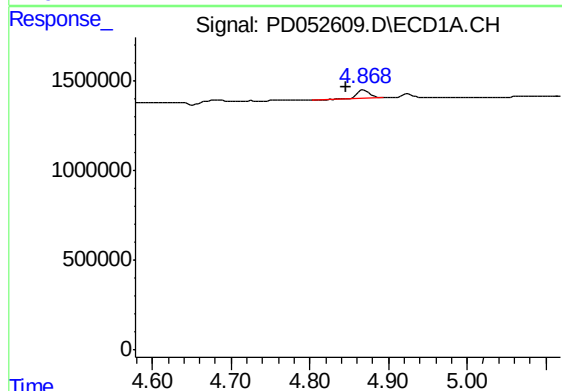


#8 Heptachlor epoxide

R.T.: 4.869 min
Delta R.T.: 0.024 min
Response: 555895
Conc: 0.29 ng/ml

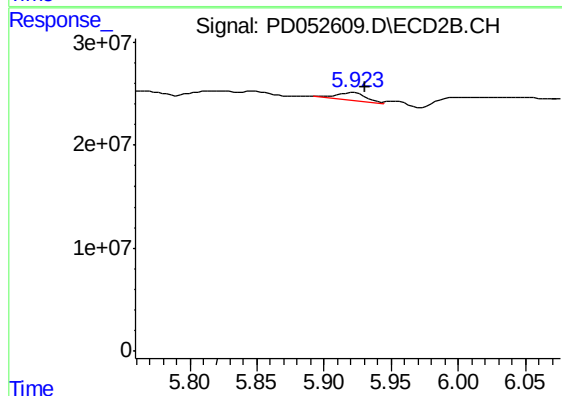

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 11810568
Conc: 0.37 ng/ml

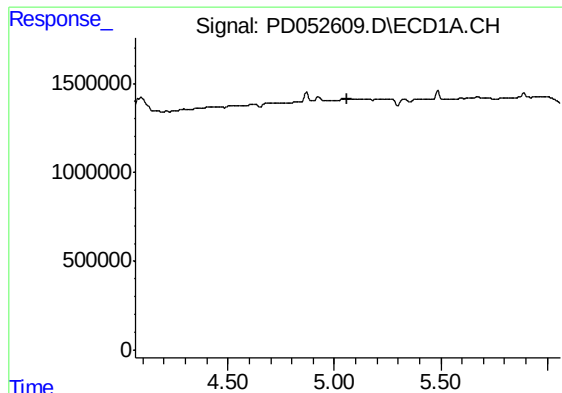

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

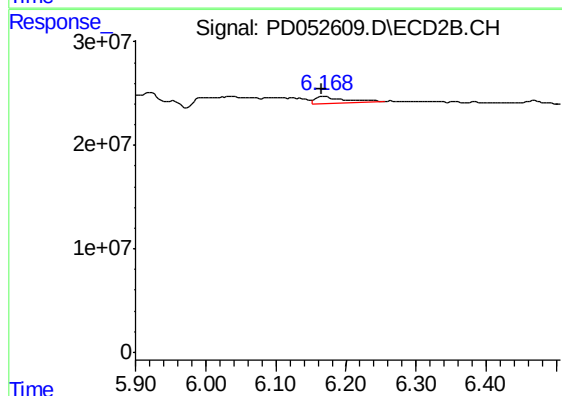


#10 gamma-Chlordane

R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 17187428
Conc: 0.54 ng/ml

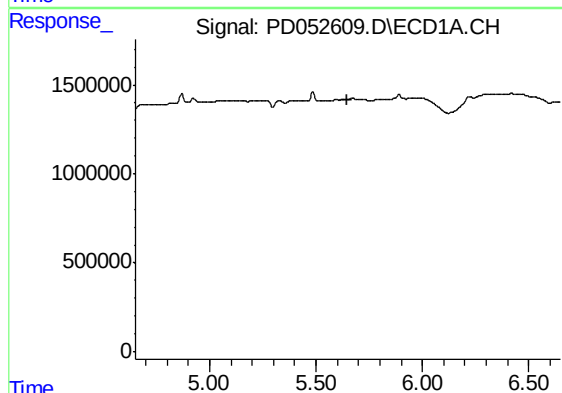


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.650 min
Response: 0
Conc: N.D.

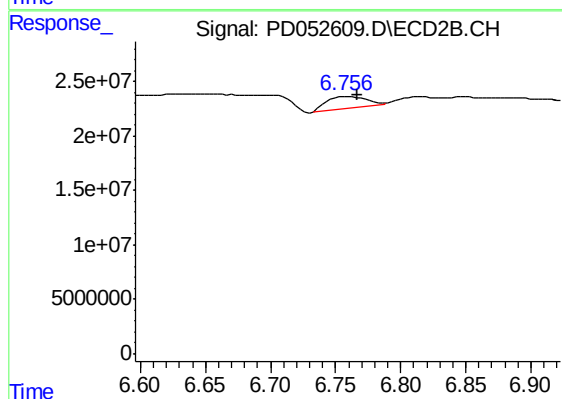

#14 Endrin


R.T.: 6.758 min
Delta R.T.: -0.009 min
Response: 22593332
Conc: 0.90 ng/ml

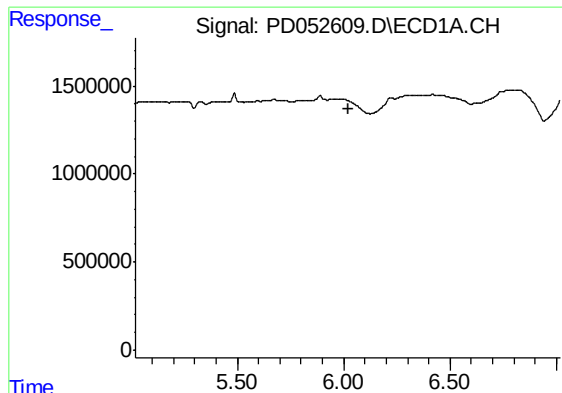

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

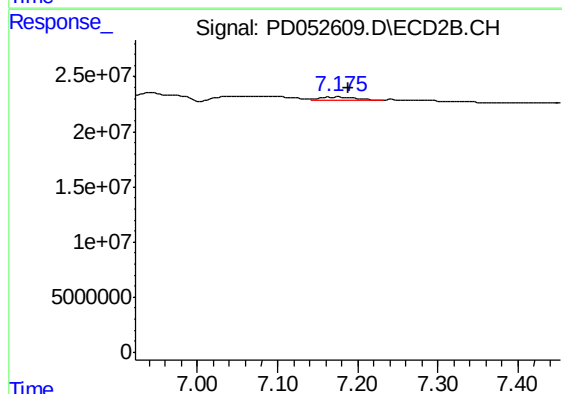


#17 4,4'-DDT

R.T.: 7.177 min
Delta R.T.: -0.012 min
Response: 9699493
Conc: 0.52 ng/ml

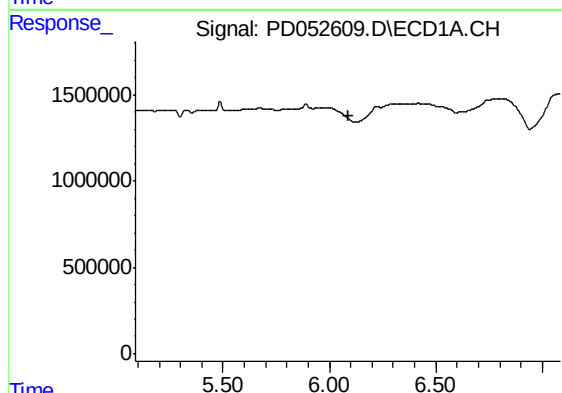


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

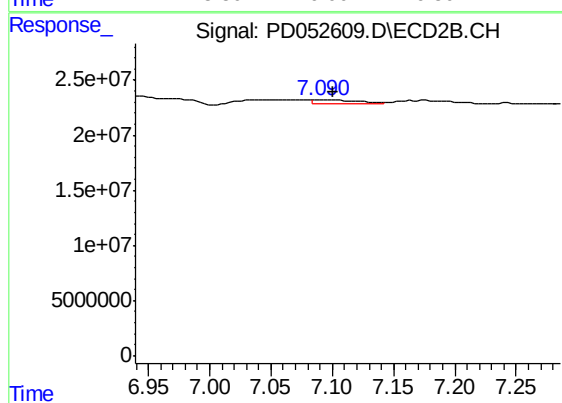

#18 Endrin aldehyde


R.T.: 7.092 min
Delta R.T.: -0.009 min
Response: 8877360
Conc: 0.43 ng/ml

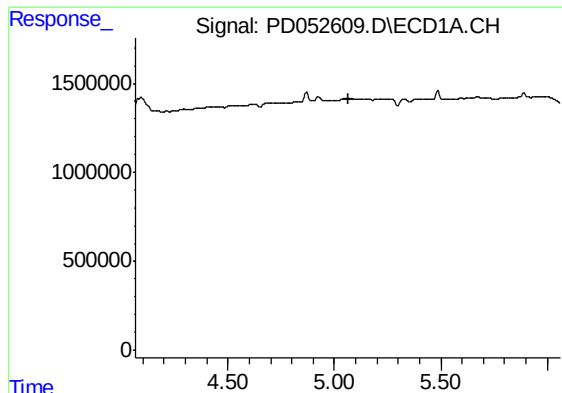

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

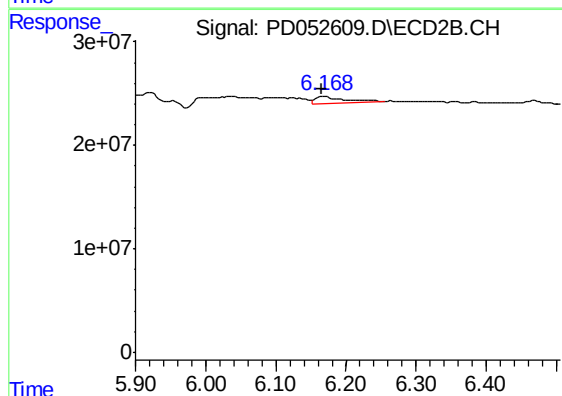


#25 Chlordane-3

R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 17187428
Conc: 3.89 ng/ml

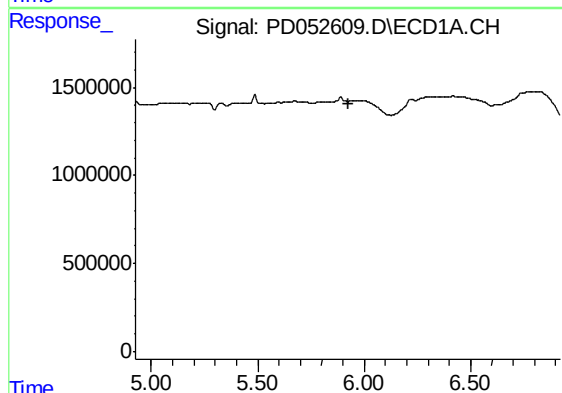


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.924 min
Response: 0
Conc: N.D.

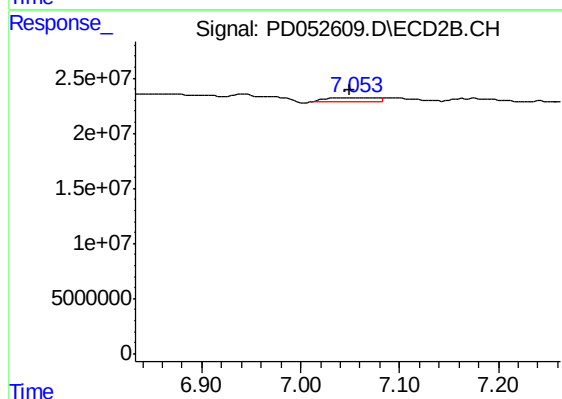

#27 Chlordane-5


R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 13480514
Conc: 14.61 ng/ml

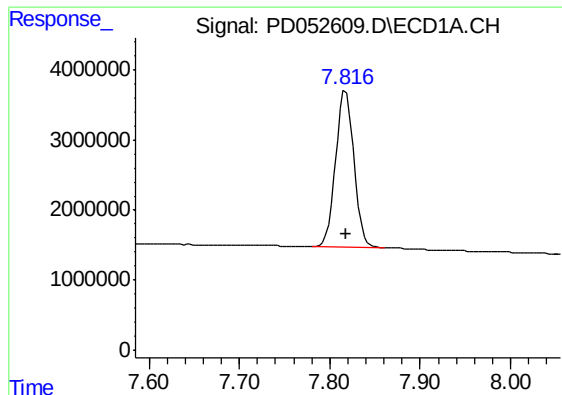

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 31044567
Conc: 23.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

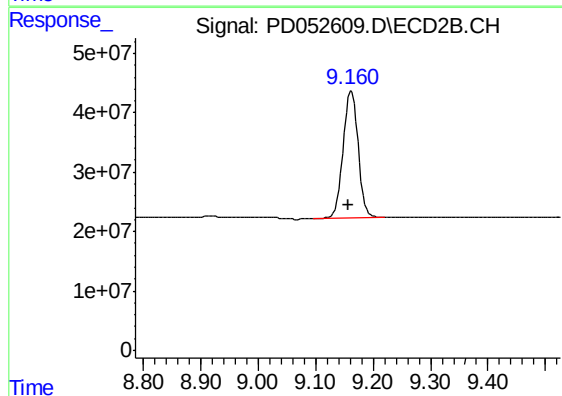

#28 Decachlorobiphenyl

R.T.: 9.162 min
Delta R.T.: 0.005 min
Response: 393378587
Conc: 25.30 ng/ml