

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052612.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 15:18
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:54:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	28718289	632.6E6	20.580	21.827
28)	SA Decachlor...	7.817	9.161	31502993	400.4E6	23.637	25.750
Target Compounds							
3)	MA gamma-BHC...	3.920	0.000	3586212	0	1.640	N.D. #
4)	MA Heptachlor	0.000	5.247	0	1155663	N.D.	0.029 #
8)	B Heptachlo...	4.869f	5.924	663591	40548105	0.349	1.256 #
10)	B gamma-Chl...	0.000	6.168	0	26119483	N.D.	0.816 #
11)	B alpha-Chl...	0.000	6.222f	0	6420686	N.D.	0.205 #
14)	MA Endrin	0.000	6.760	0	40490138	N.D.	1.616 #
25)	Chlordane-3	0.000	6.168	0	26119483	N.D.	5.919 #
26)	Chlordane-4	0.000	6.222f	0	6420686	N.D.	1.263 #
27)	Chlordane-5	0.000	7.047	0	2960724	N.D.	3.209 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052612.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 15:18
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:54:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

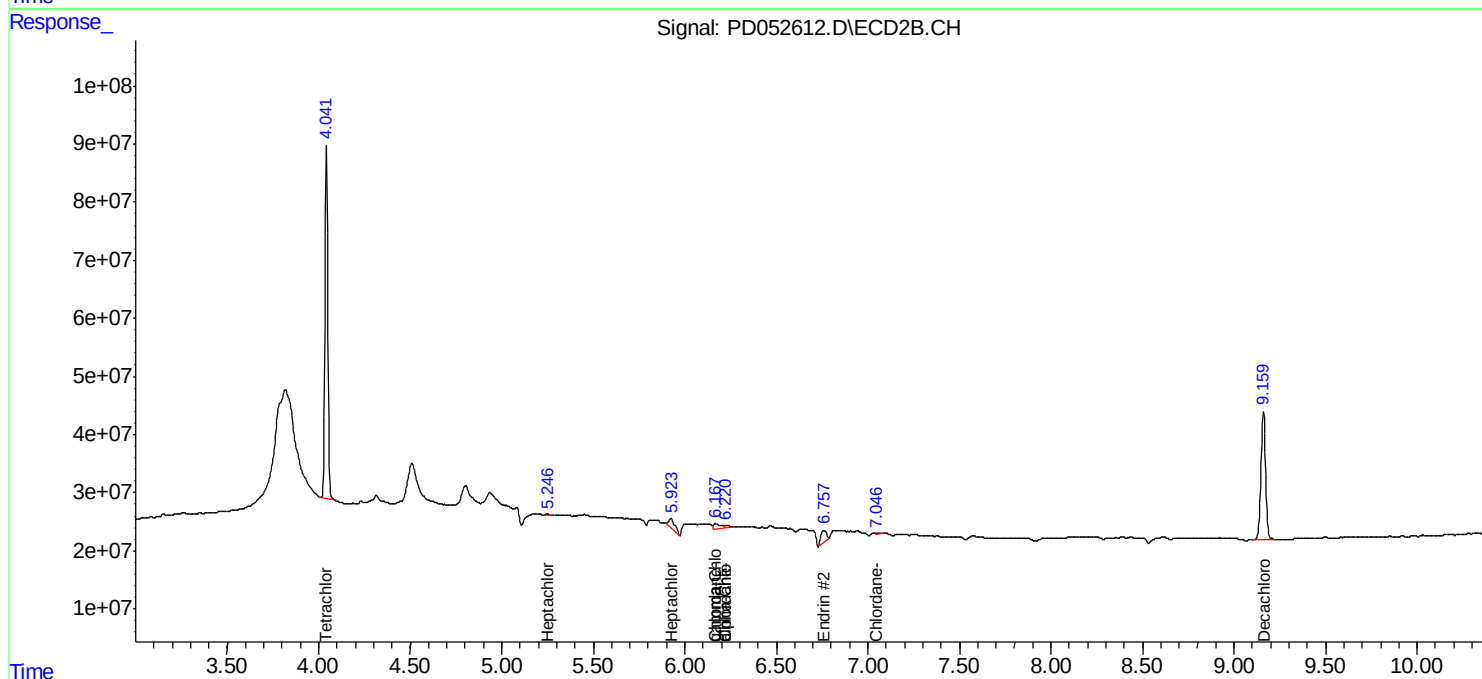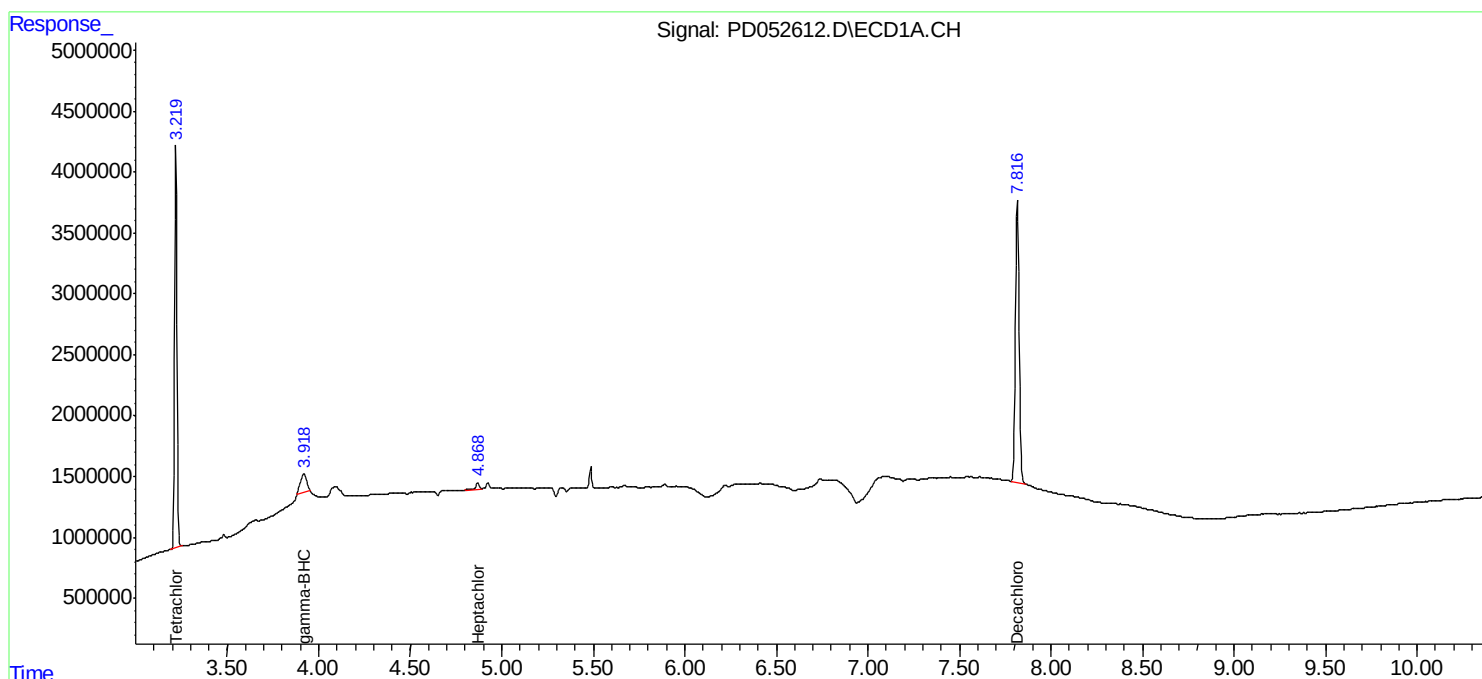


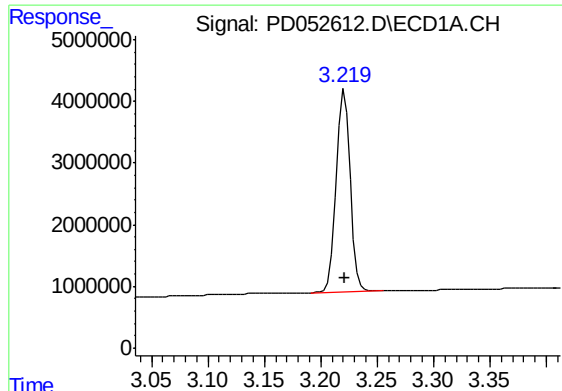

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28718289
Conc: 20.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

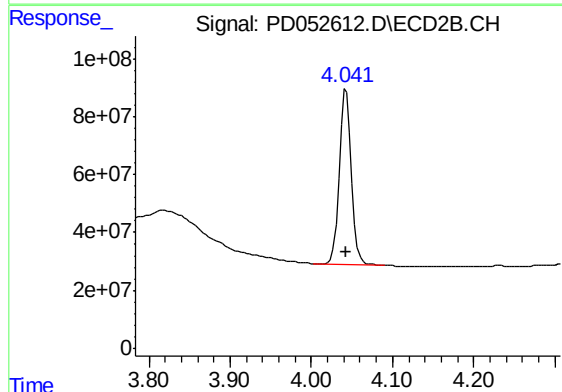


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 632621397
Conc: 21.83 ng/ml

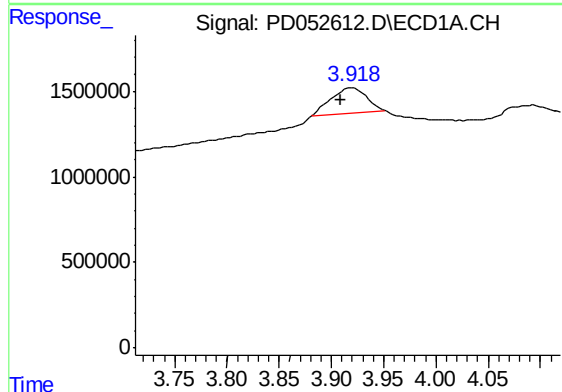


#3 gamma-BHC (Lindane)

R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 3586212
Conc: 1.64 ng/ml

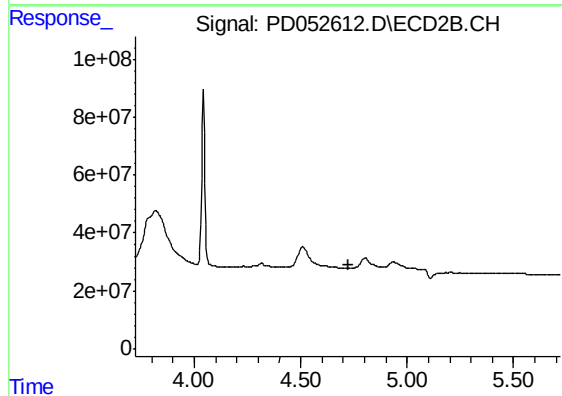

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

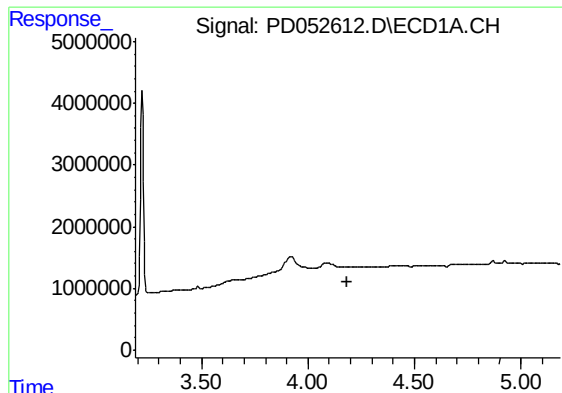

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

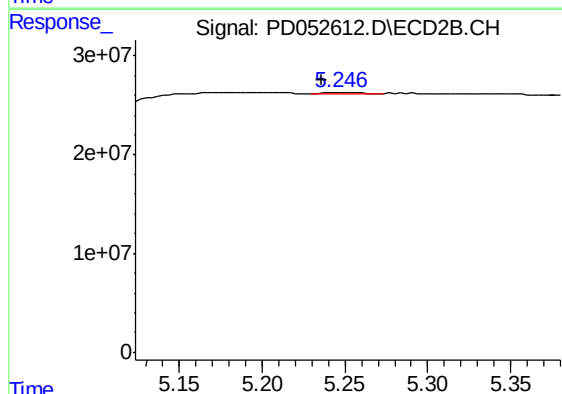


#4 Heptachlor

R.T.: 5.247 min
Delta R.T.: 0.011 min
Response: 1155663
Conc: 0.03 ng/ml

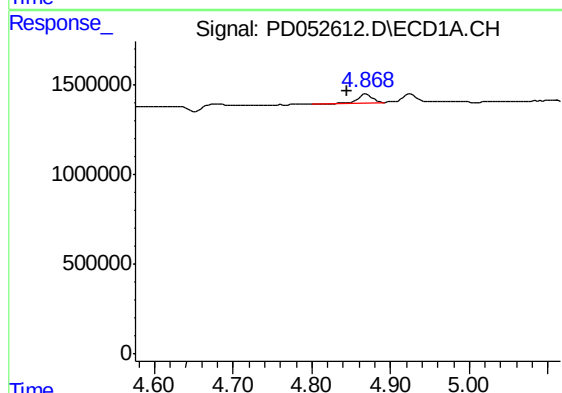


#8 Heptachlor epoxide

R.T.: 4.869 min
Delta R.T.: 0.024 min
Response: 663591
Conc: 0.35 ng/ml

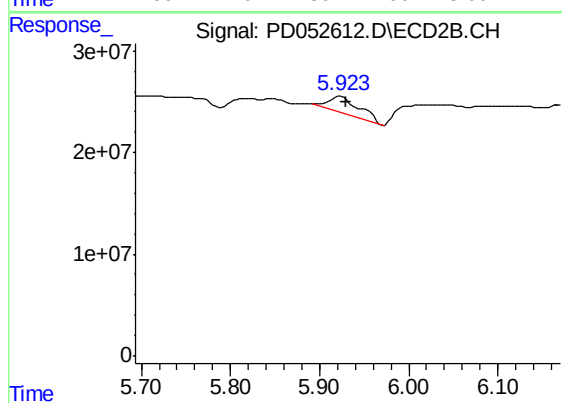

#8 Heptachlor epoxide


R.T.: 5.924 min
Delta R.T.: -0.006 min
Response: 40548105
Conc: 1.26 ng/ml

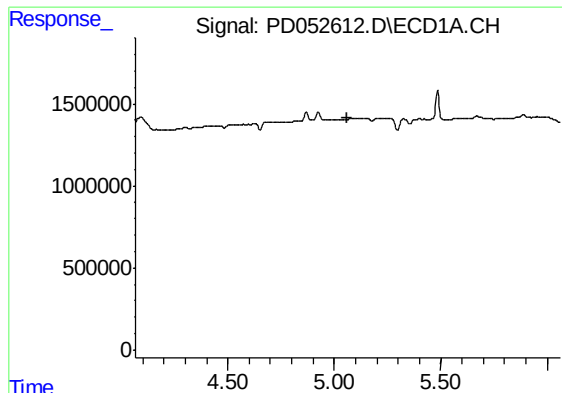

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

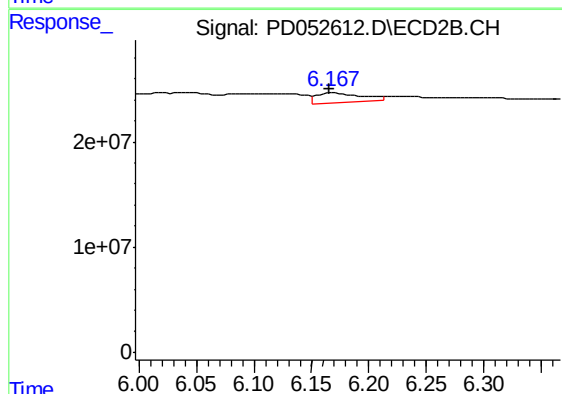


#10 gamma-Chlordane

R.T.: 6.168 min
Delta R.T.: 0.003 min
Response: 26119483
Conc: 0.82 ng/ml

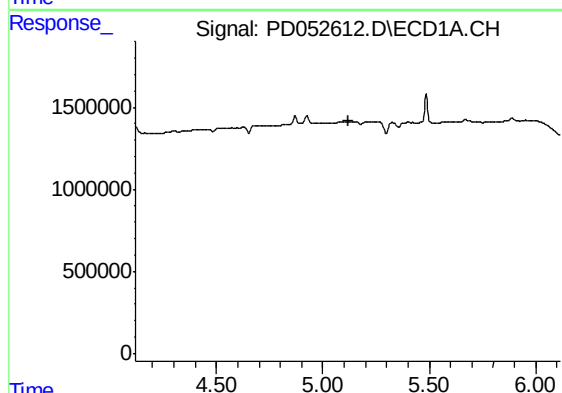


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

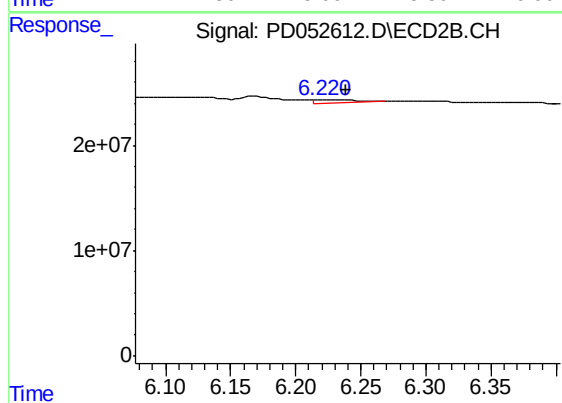

#11 alpha-Chlordane


R.T.: 6.222 min
Delta R.T.: -0.017 min
Response: 6420686
Conc: 0.20 ng/ml

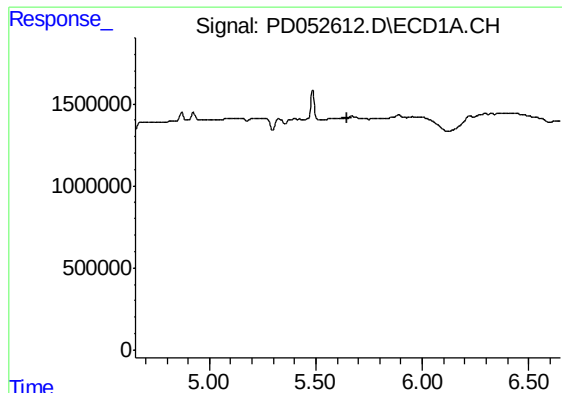

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

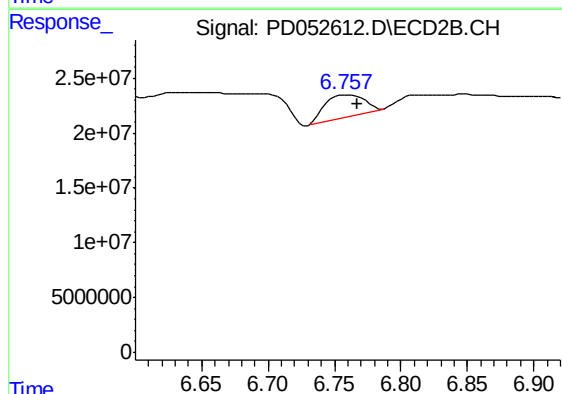


#14 Endrin

R.T.: 6.760 min
Delta R.T.: -0.008 min
Response: 40490138
Conc: 1.62 ng/ml

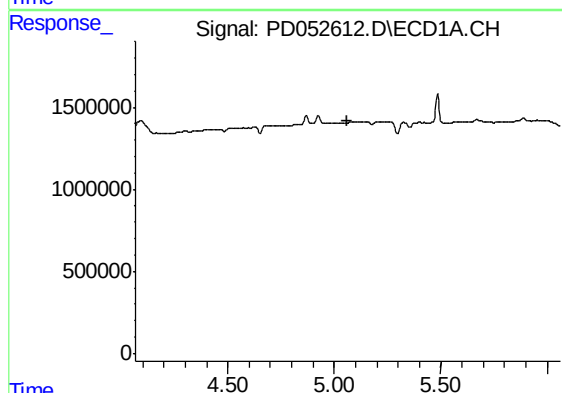


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.064 min
Response: 0
Conc: N.D.

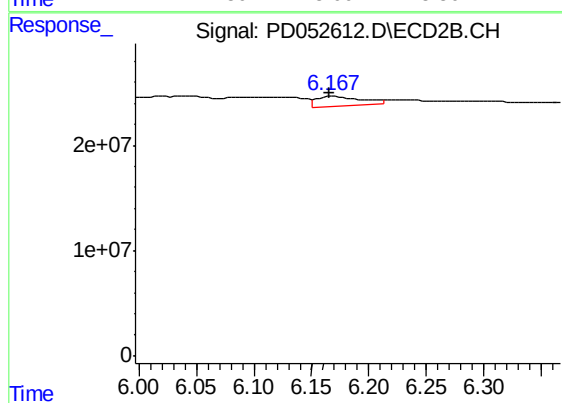

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: 0.002 min
Response: 26119483
Conc: 5.92 ng/ml

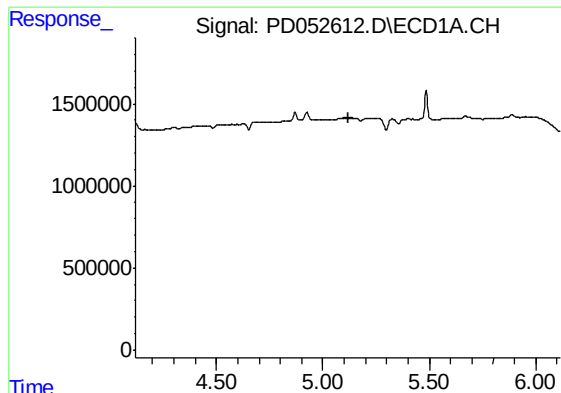

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

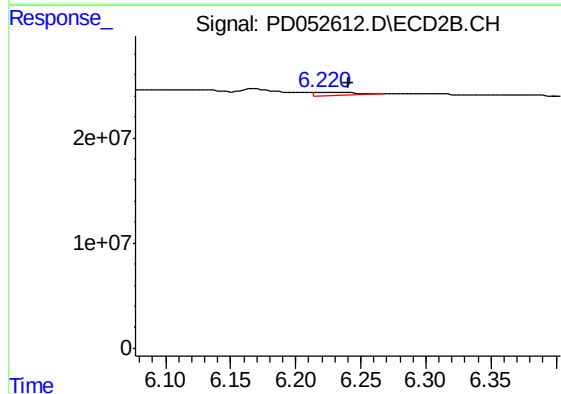


#26 Chlordane-4

R.T.: 6.222 min
Delta R.T.: -0.019 min
Response: 6420686
Conc: 1.26 ng/ml

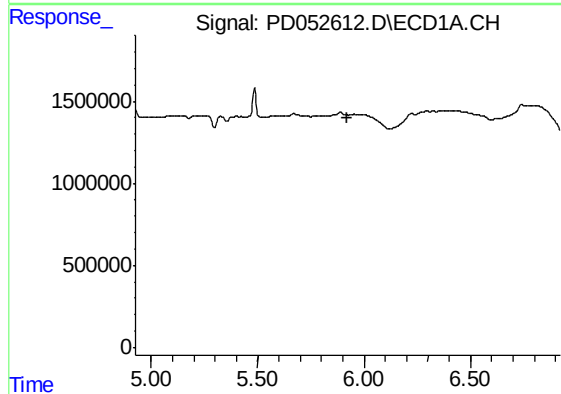


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.924 min
Response: 0
Conc: N.D.

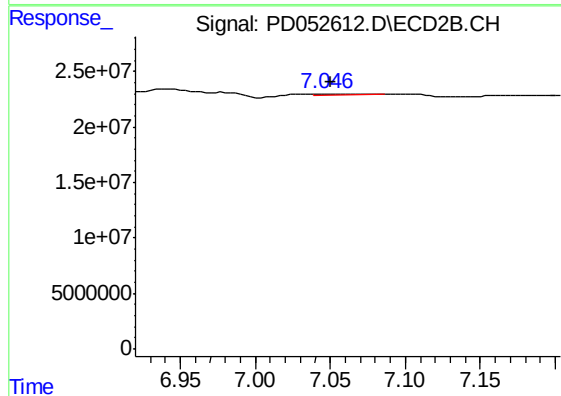

#27 Chlordane-5


R.T.: 7.047 min
Delta R.T.: -0.003 min
Response: 2960724
Conc: 3.21 ng/ml

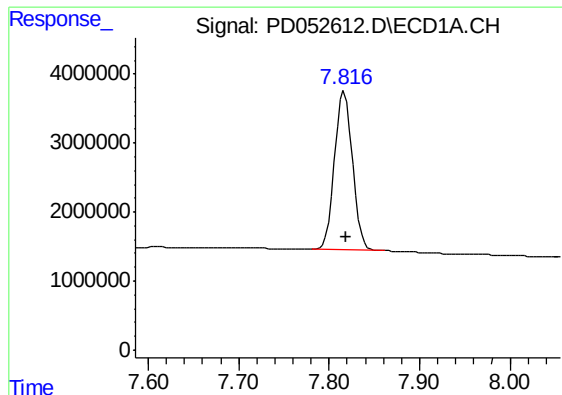

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 31502993
Conc: 23.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

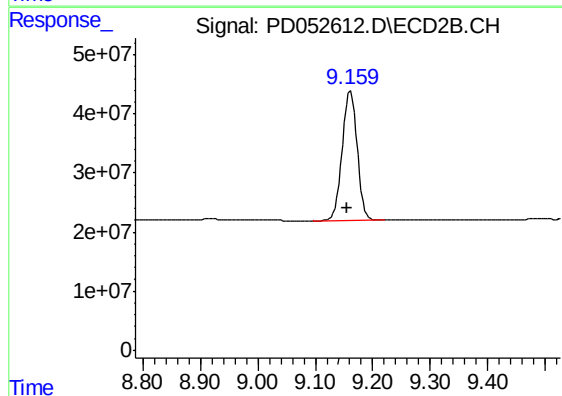

#28 Decachlorobiphenyl

R.T.: 9.161 min
Delta R.T.: 0.004 min
Response: 400444221
Conc: 25.75 ng/ml