

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052620.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 17:10
 Operator : AJ\SJ
 Sample : PB118397BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB118397BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:58:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	25769360	555.2E6	18.467	19.156
28)	SA Decachlor...	7.819	9.161	27664174	356.3E6	20.757	22.910
Target Compounds							
3)	MA gamma-BHC...	3.922	0.000	5140175	0	2.351	N.D. #
4)	MA Heptachlor	0.000	5.258f	0	2005775	N.D.	0.051 #
8)	B Heptachlo...	0.000	5.917	0	8356559	N.D.	0.259 #
10)	B gamma-Chl...	0.000	6.187f	0	6674275	N.D.	0.209 #
15)	B Endosulfa...	0.000	6.983	0	16793495	N.D.	0.674 #
25)	Chlordane-3	0.000	6.187f	0	6674275	N.D.	1.512 #
27)	Chlordane-5	0.000	7.054	0	2082272	N.D.	2.257 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052620.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 17:10
Operator : AJ\SJ
Sample : PB118397BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB118397BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:58:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

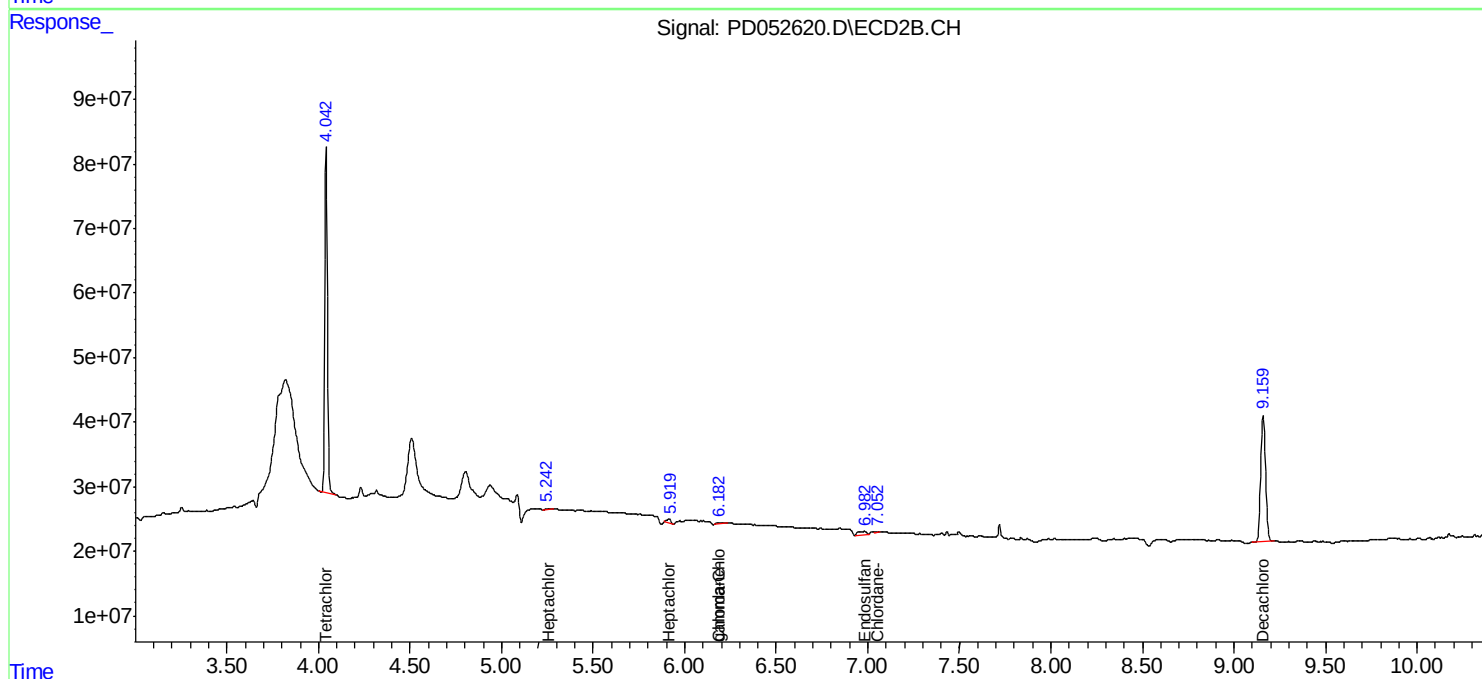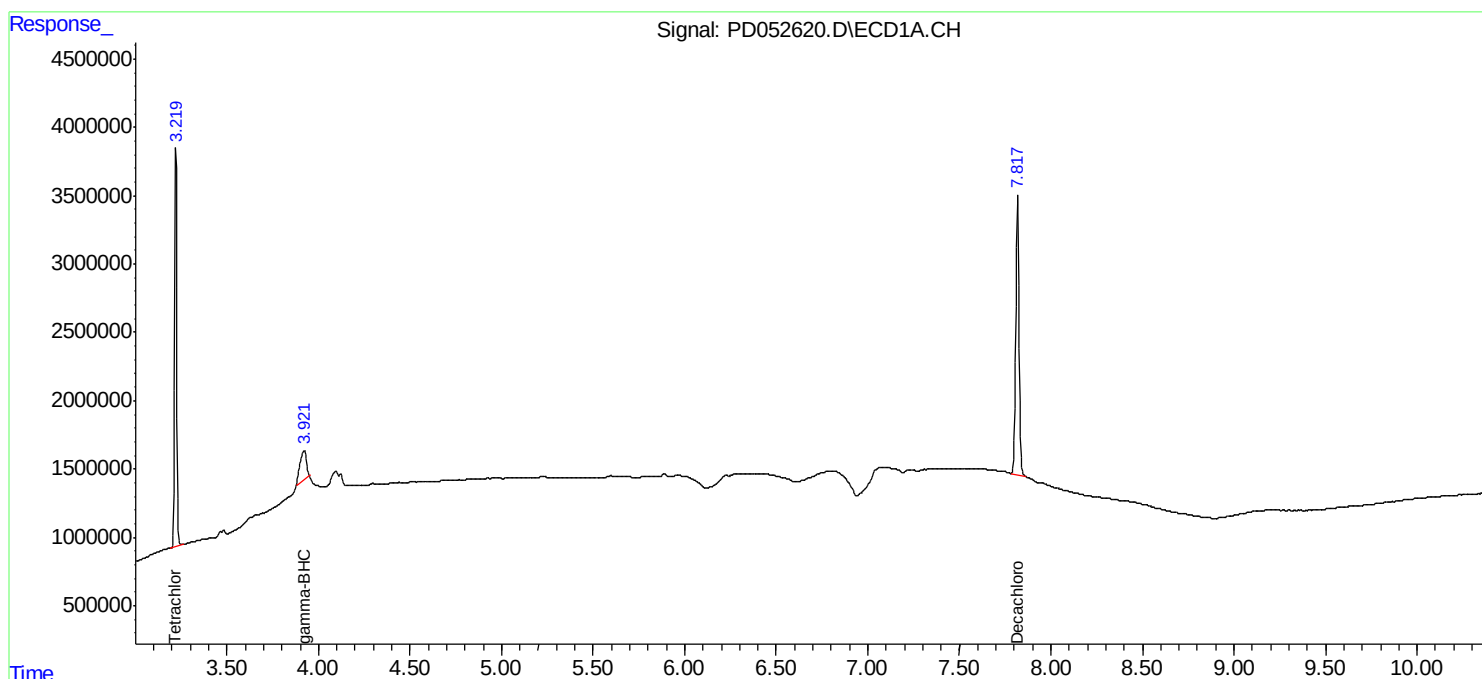


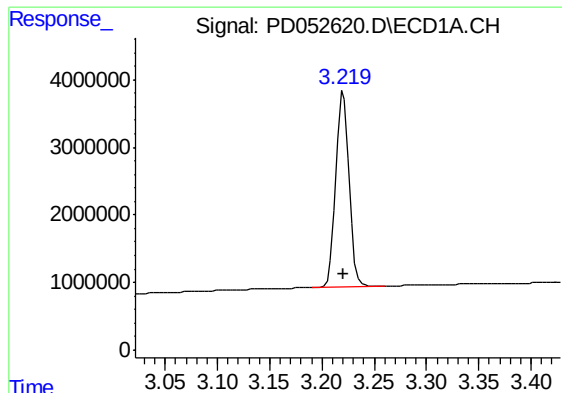

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 25769360
Conc: 18.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB118397BL

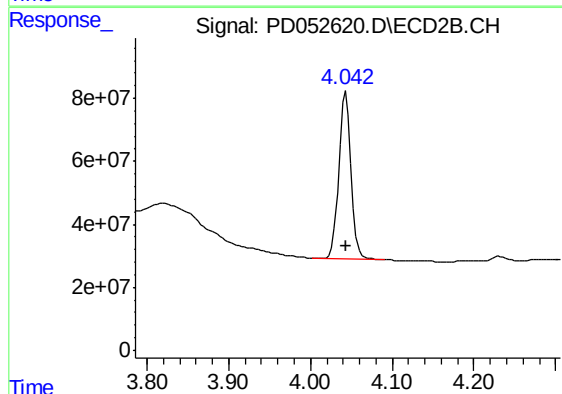


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 555205464
Conc: 19.16 ng/ml

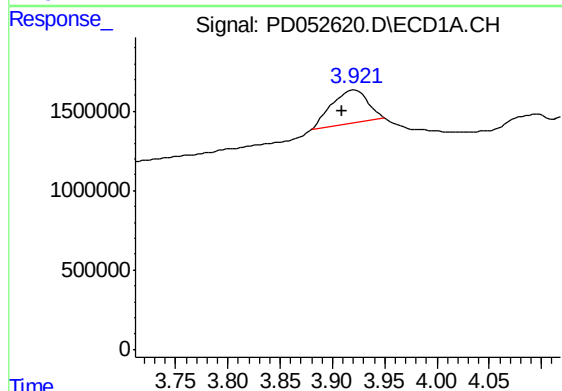


#3 gamma-BHC (Lindane)

R.T.: 3.922 min
Delta R.T.: 0.012 min
Response: 5140175
Conc: 2.35 ng/ml

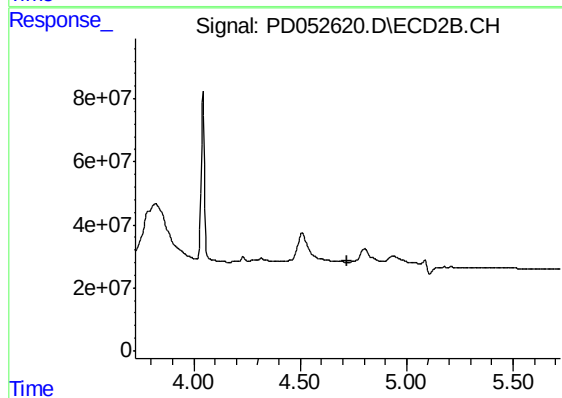

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

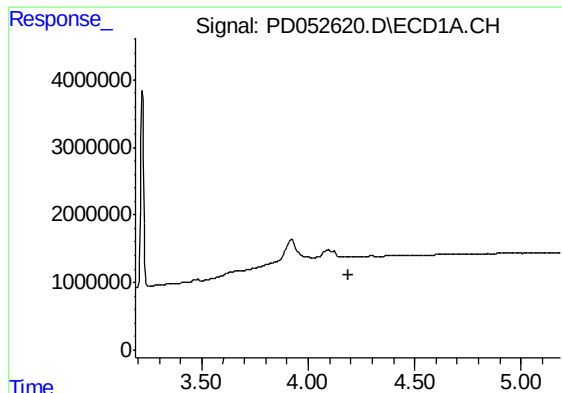

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118397BL

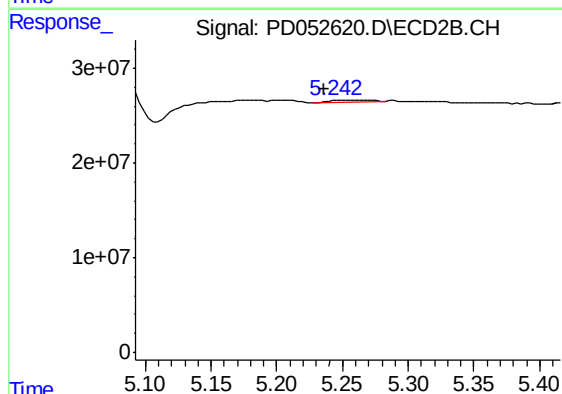


#4 Heptachlor

R.T.: 5.258 min
Delta R.T.: 0.023 min
Response: 2005775
Conc: 0.05 ng/ml

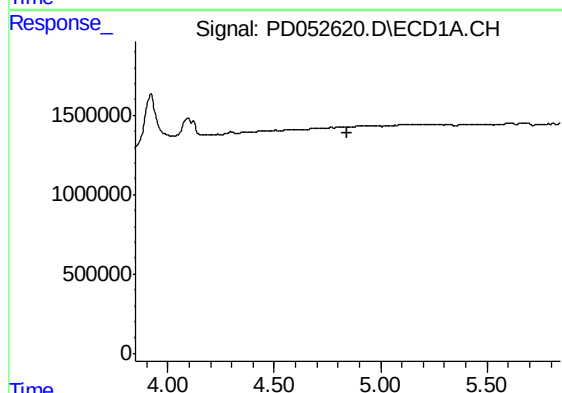


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

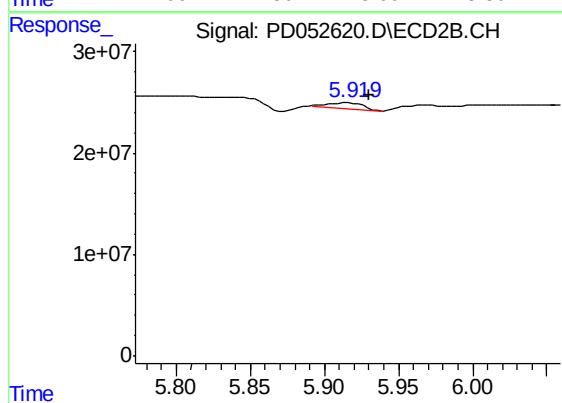

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.013 min
Response: 8356559
Conc: 0.26 ng/ml

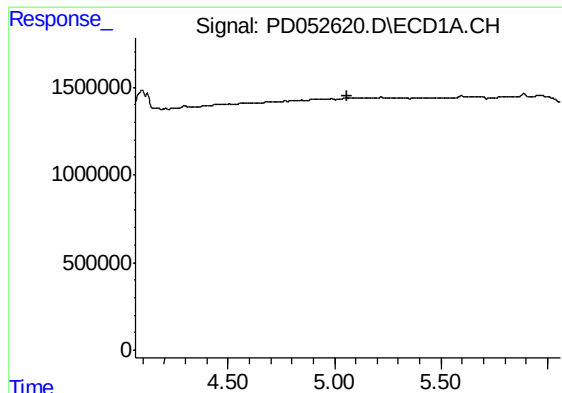

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118397BL

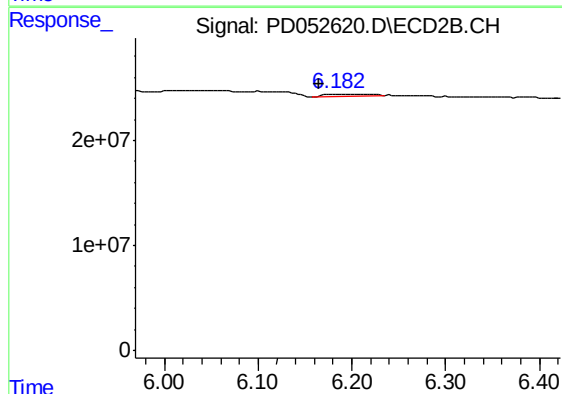


#10 gamma-Chlordane

R.T.: 6.187 min
Delta R.T.: 0.021 min
Response: 6674275
Conc: 0.21 ng/ml

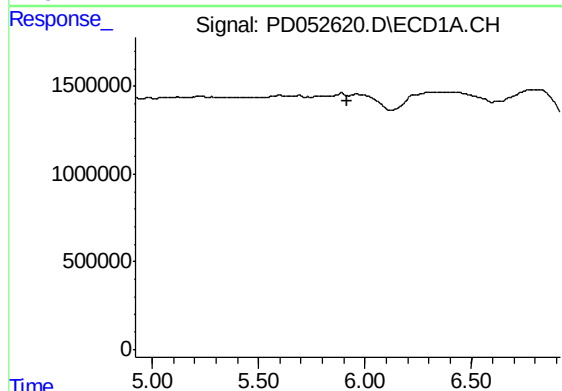


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

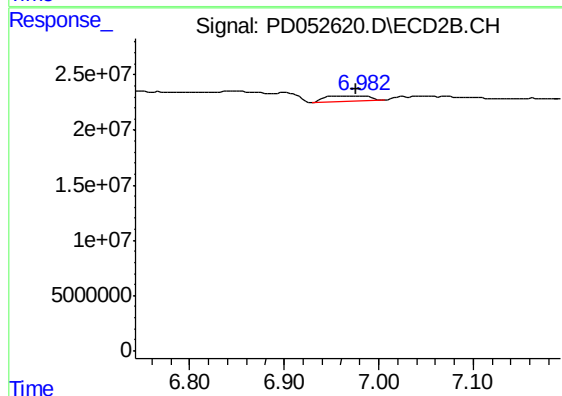

#15 Endosulfan II


R.T.: 6.983 min
Delta R.T.: 0.007 min
Response: 16793495
Conc: 0.67 ng/ml

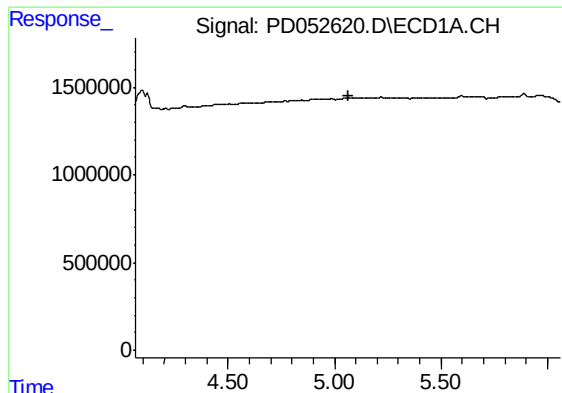

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118397BL

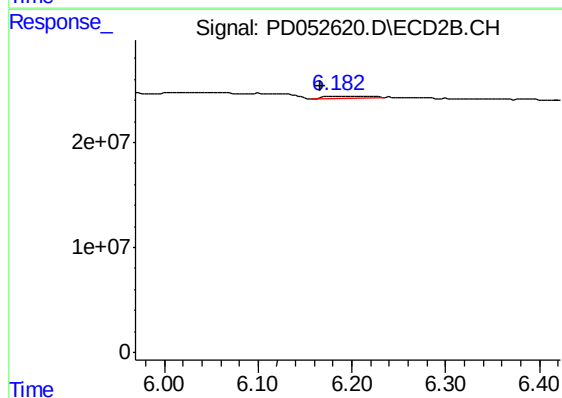


#25 Chlordane-3

R.T.: 6.187 min
Delta R.T.: 0.021 min
Response: 6674275
Conc: 1.51 ng/ml

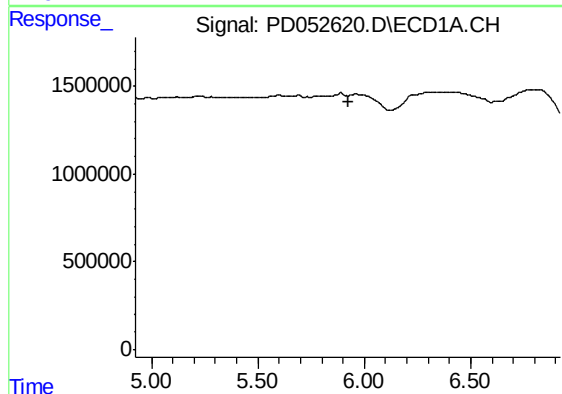


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

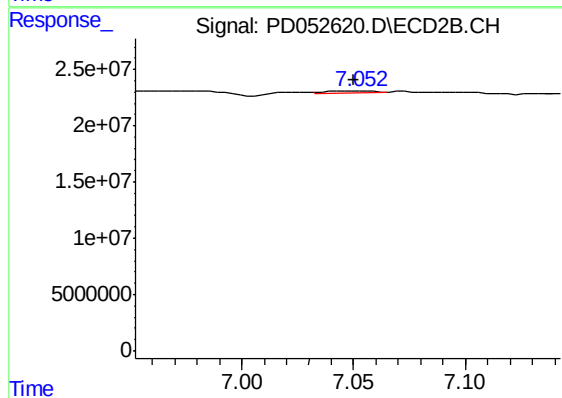

#27 Chlordane-5


R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 2082272
Conc: 2.26 ng/ml

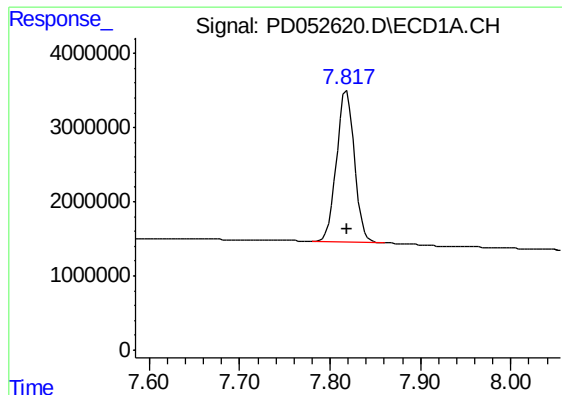

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 27664174
Conc: 20.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB118397BL

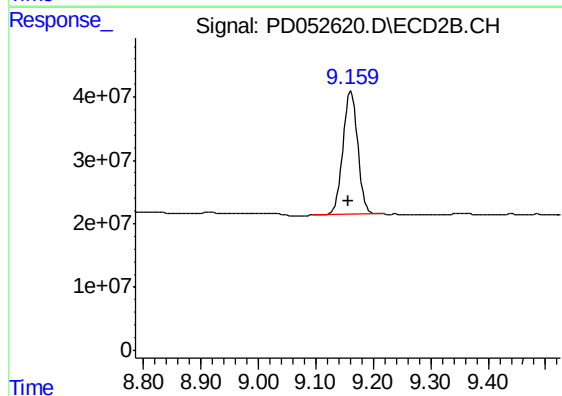

#28 Decachlorobiphenyl

R.T.: 9.161 min
Delta R.T.: 0.004 min
Response: 356277582
Conc: 22.91 ng/ml