

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 17:24
 Operator : AJ\SJ
 Sample : PB118406BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB118406BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:58:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.043	25638942	553.3E6	18.374	19.088
28)	SA Decachlor...	7.817	9.162	27569548	355.8E6	20.686	22.880
Target Compounds							
3)	MA gamma-BHC...	3.918	0.000	4845240	0	2.216	N.D. #
4)	MA Heptachlor	0.000	5.245	0	1745467	N.D.	0.044 #
8)	B Heptachlo...	0.000	5.916	0	7804807	N.D.	0.242 #
10)	B gamma-Chl...	0.000	6.176	0	3854518	N.D.	0.120 #
15)	B Endosulfa...	0.000	6.984	0	8268065	N.D.	0.332 #
18)	B Endrin al...	0.000	7.079f	0	9408877	N.D.	0.457 #
25)	Chlordane-3	0.000	6.176	0	3854518	N.D.	0.873 #
27)	Chlordane-5	0.000	7.079f	0	9408877	N.D.	10.198 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 17:24
Operator : AJ\SJ
Sample : PB118406BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB118406BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:58:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

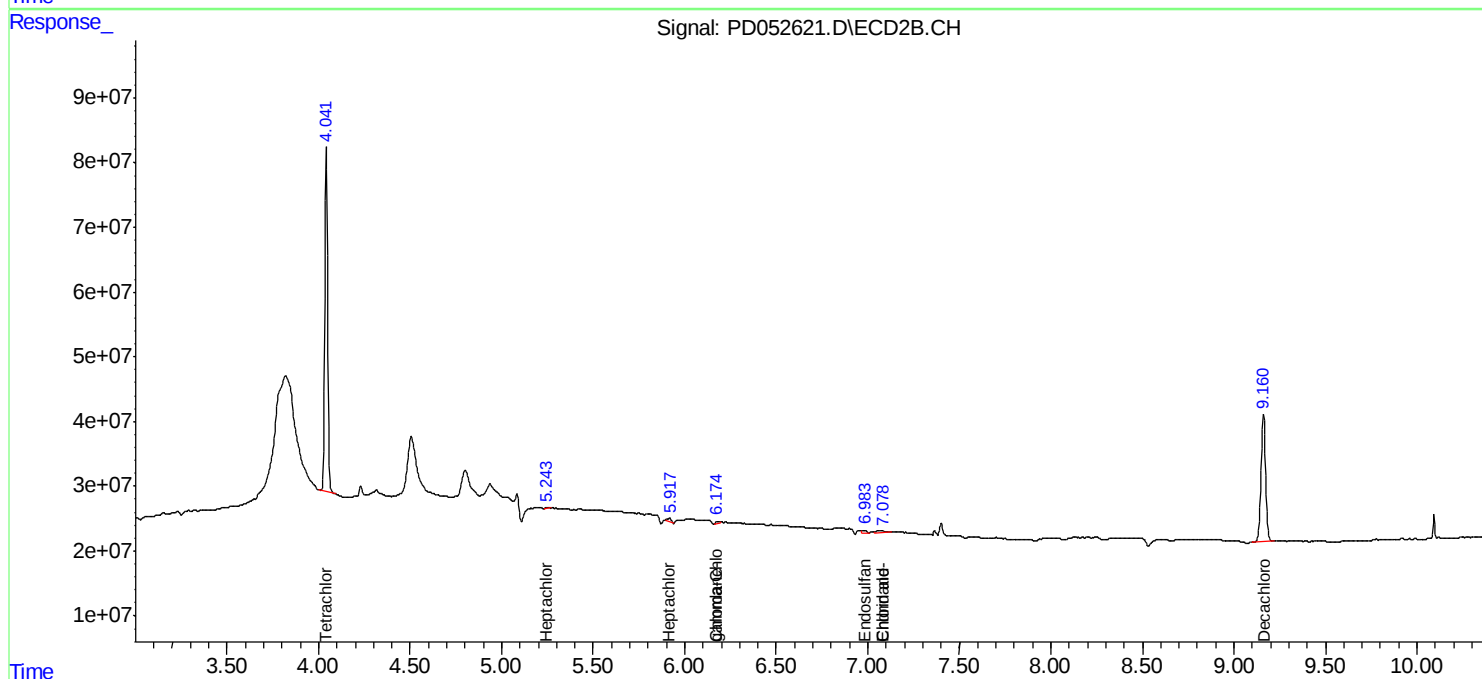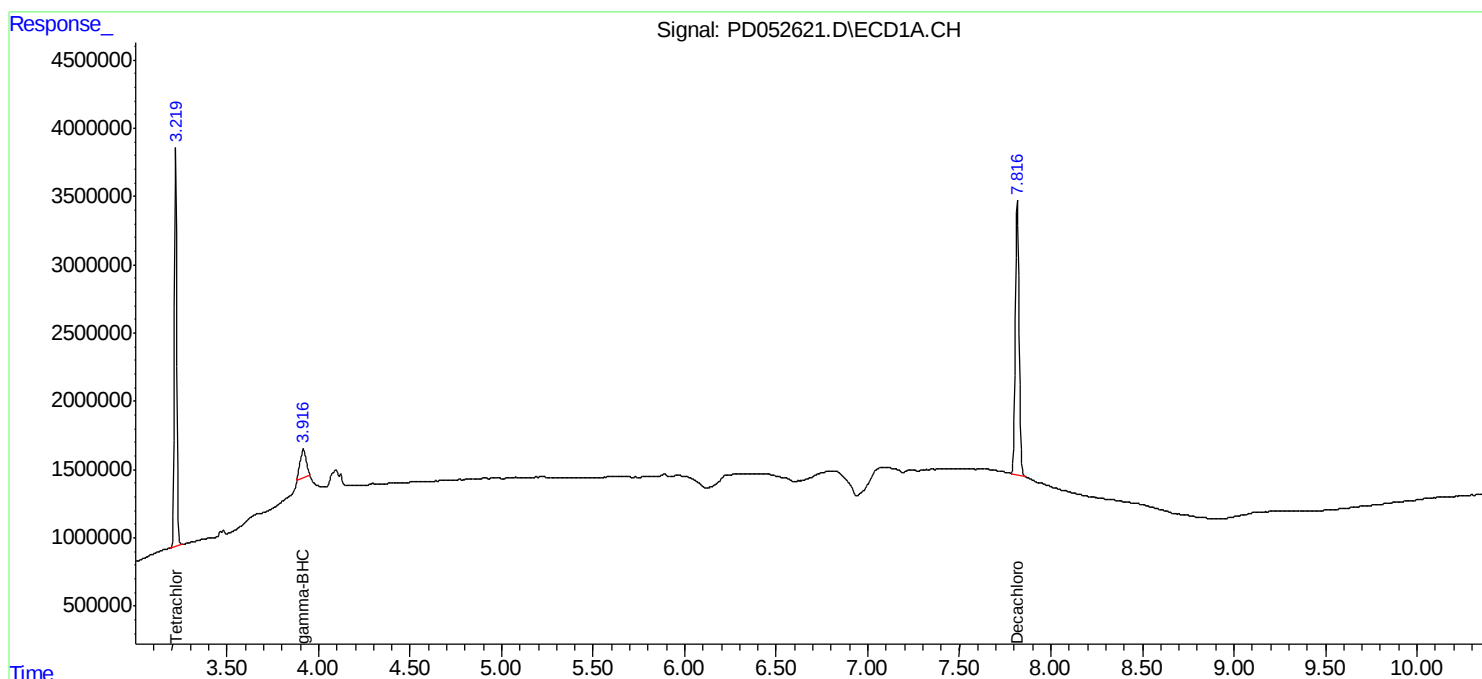


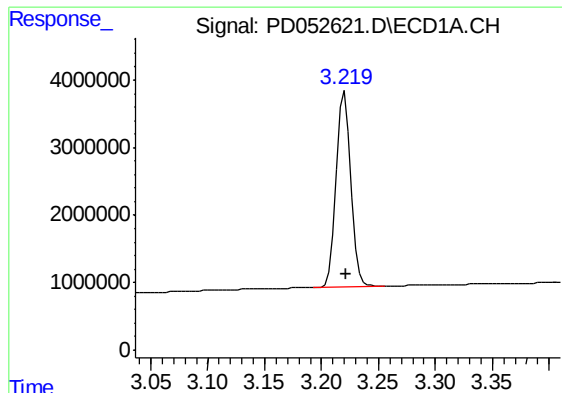

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 25638942
Conc: 18.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB118406BL

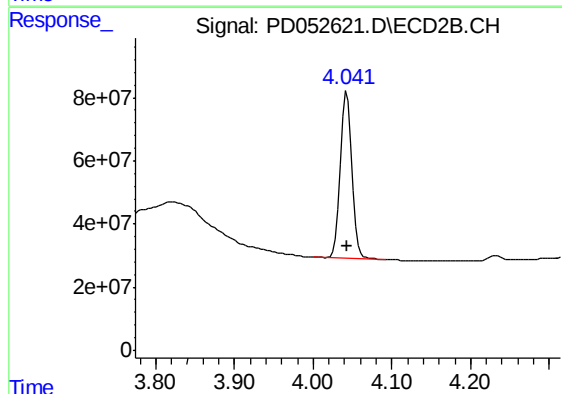


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 553258100
Conc: 19.09 ng/ml

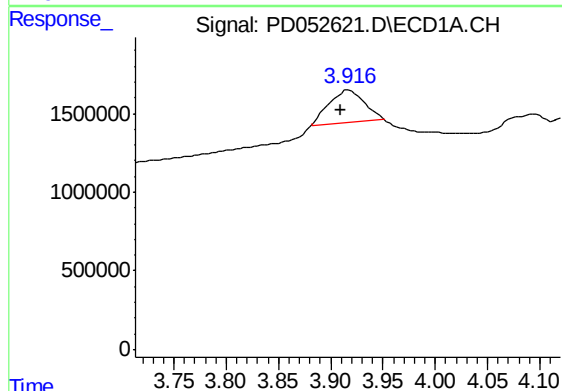


#3 gamma-BHC (Lindane)

R.T.: 3.918 min
Delta R.T.: 0.008 min
Response: 4845240
Conc: 2.22 ng/ml

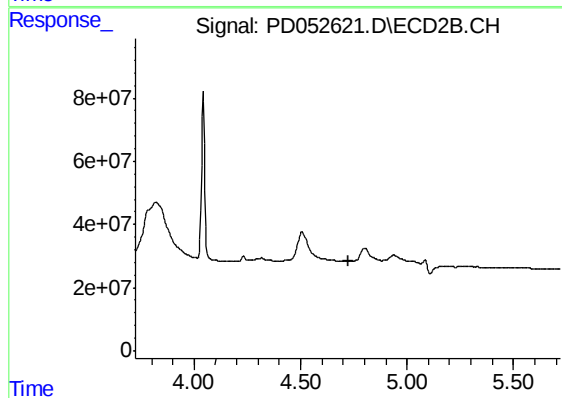

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

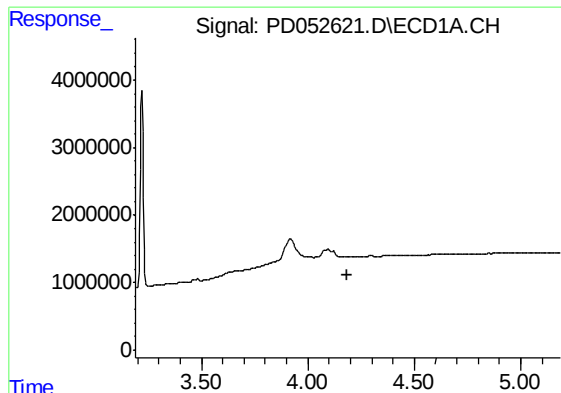

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118406BL

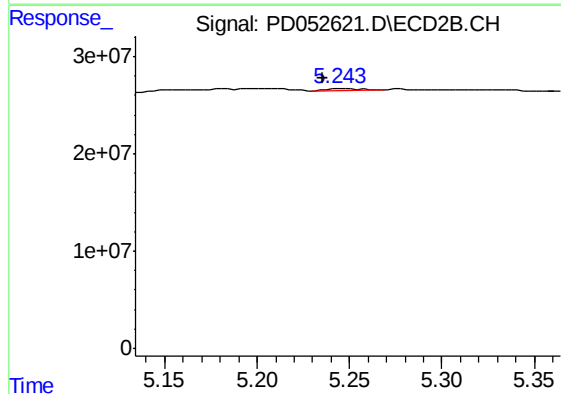


#4 Heptachlor

R.T.: 5.245 min
Delta R.T.: 0.009 min
Response: 1745467
Conc: 0.04 ng/ml

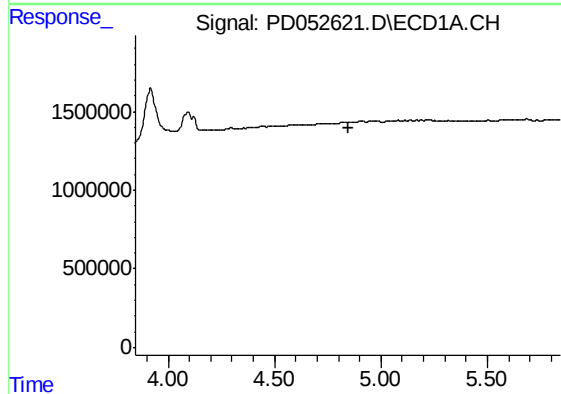


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

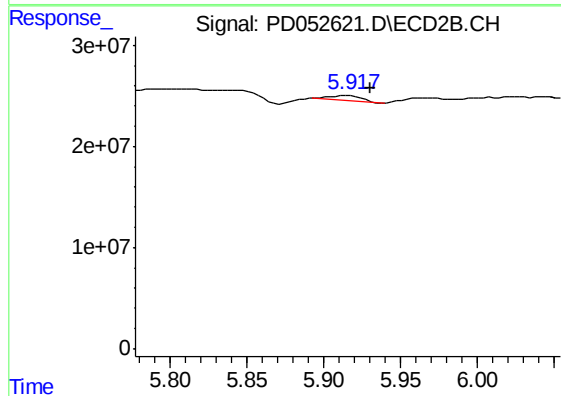

#8 Heptachlor epoxide


R.T.: 5.916 min
Delta R.T.: -0.014 min
Response: 7804807
Conc: 0.24 ng/ml

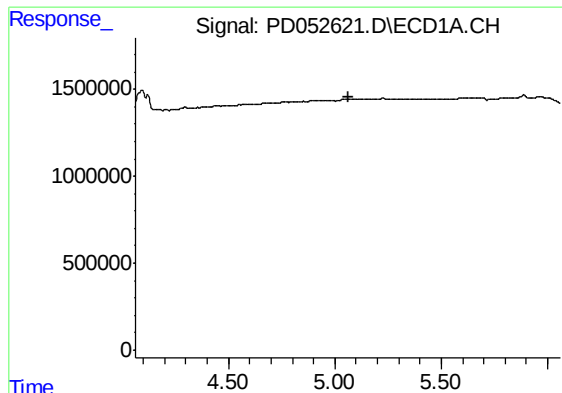

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118406BL

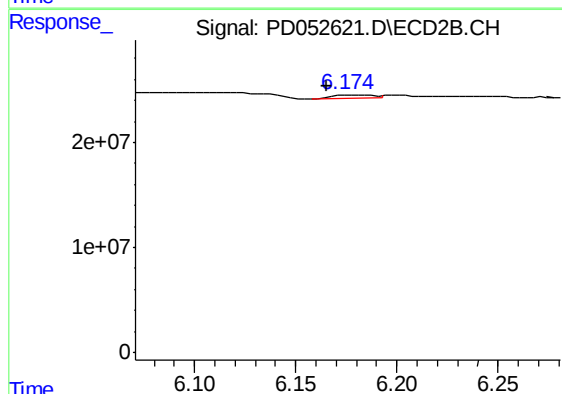


#10 gamma-Chlordane

R.T.: 6.176 min
Delta R.T.: 0.011 min
Response: 3854518
Conc: 0.12 ng/ml

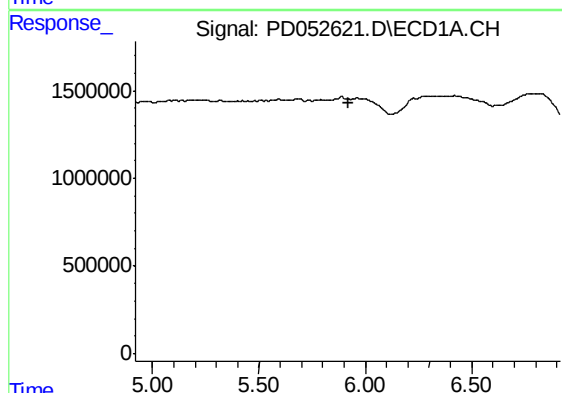


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

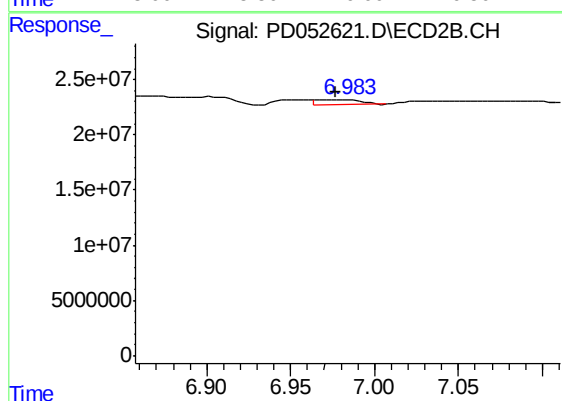

#15 Endosulfan II


R.T.: 6.984 min
Delta R.T.: 0.008 min
Response: 8268065
Conc: 0.33 ng/ml

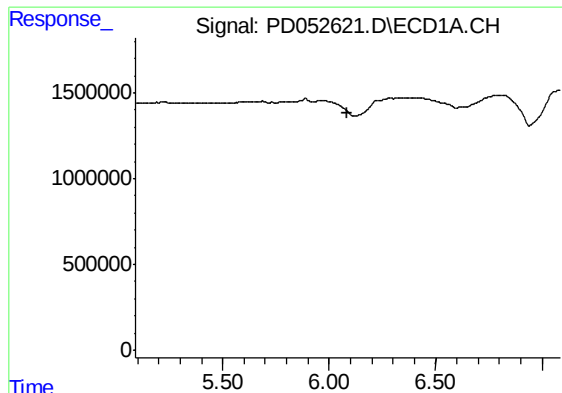

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118406BL

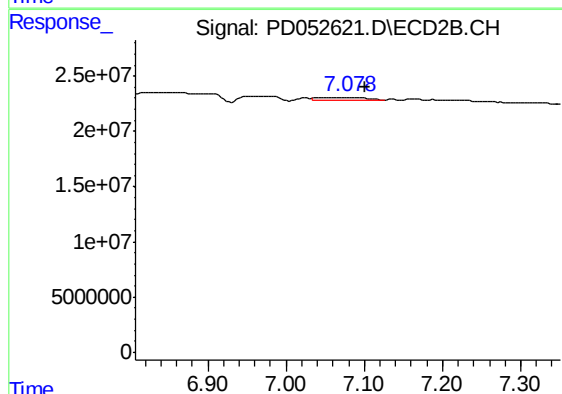


#18 Endrin aldehyde

R.T.: 7.079 min
Delta R.T.: -0.022 min
Response: 9408877
Conc: 0.46 ng/ml

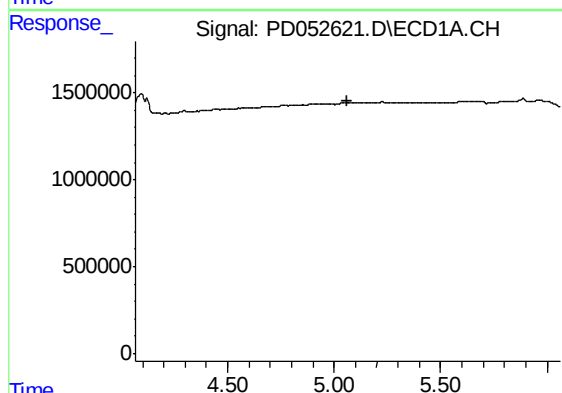


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

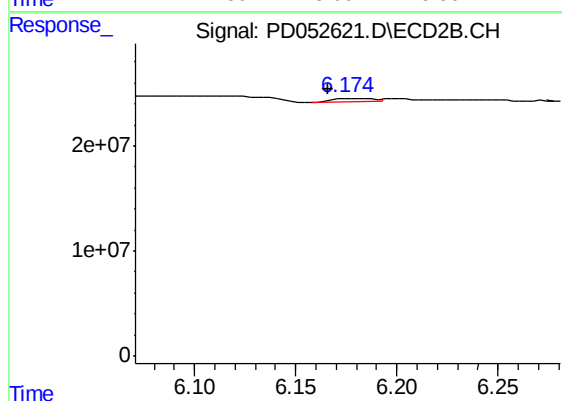

#25 Chlordane-3


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 3854518
Conc: 0.87 ng/ml

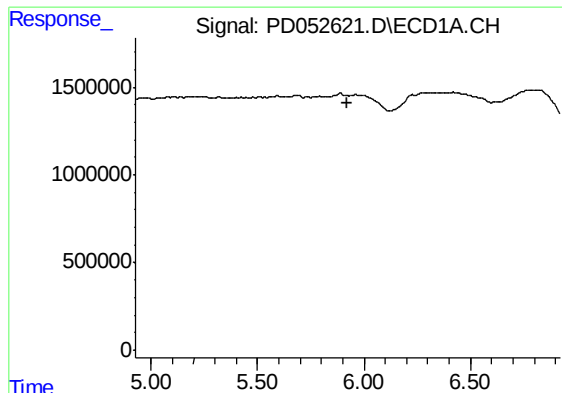

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB118406BL

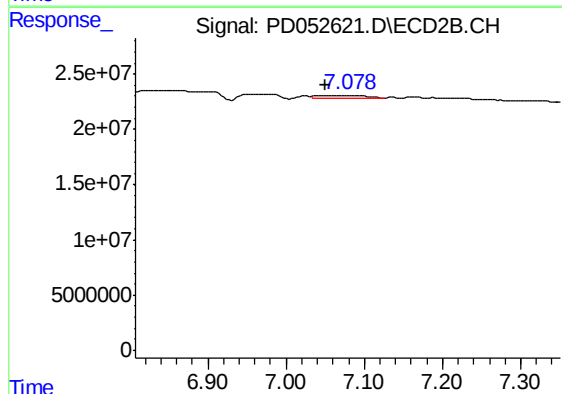


#27 Chlordane-5

R.T.: 7.079 min
Delta R.T.: 0.029 min
Response: 9408877
Conc: 10.20 ng/ml

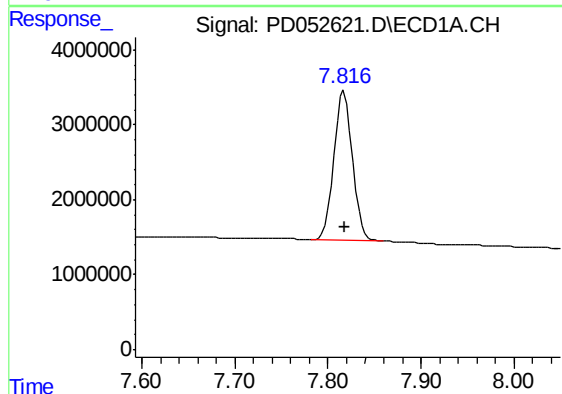

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.001 min
Response: 27569548
Conc: 20.69 ng/ml

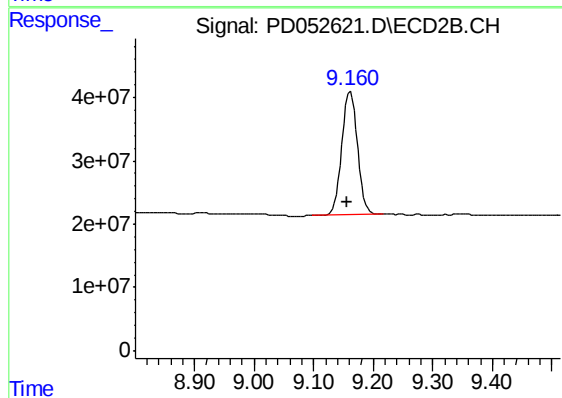

#28 Decachlorobiphenyl

R.T.: 9.162 min
Delta R.T.: 0.005 min
Response: 355810597
Conc: 22.88 ng/ml