

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052624.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 1:26
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:59:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.241	0	7452611	N.D.	0.188 #
8) B	Heptachlo...	0.000	5.924	0	6961649	N.D.	0.216 #
10) B	gamma-Chl...	0.000	6.169	0	15193769	N.D.	0.475 #
13) MA	Dieldrin	0.000	6.571f	0	6145141	N.D.	0.205 #
14) MA	Endrin	0.000	6.752f	0	22120209	N.D.	0.883 #
17) MA	4,4'-DDT	0.000	7.164f	0	30462127	N.D.	1.635 #
25)	Chlordane-3	0.000	6.169	0	15193769	N.D.	3.443 #
27)	Chlordane-5	0.000	7.031f	0	8373839	N.D.	9.076 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052624.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 1:26
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:59:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

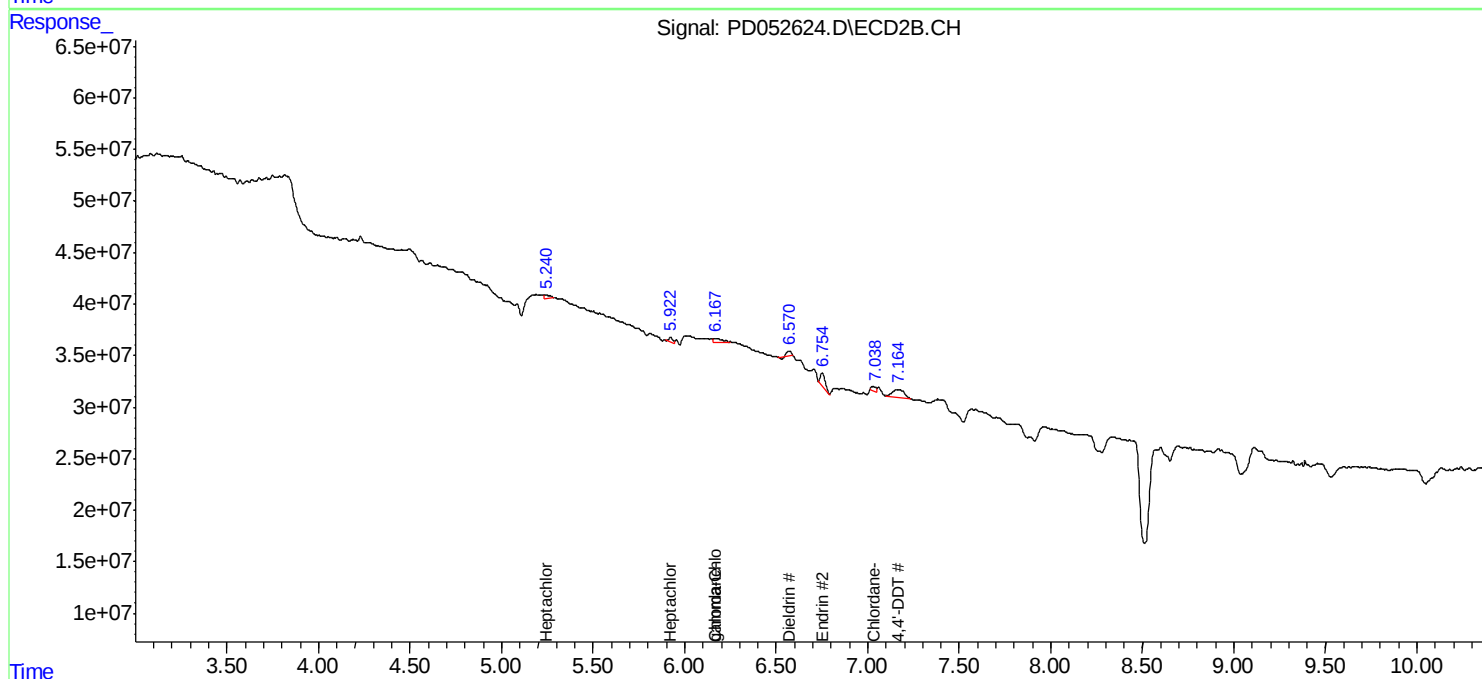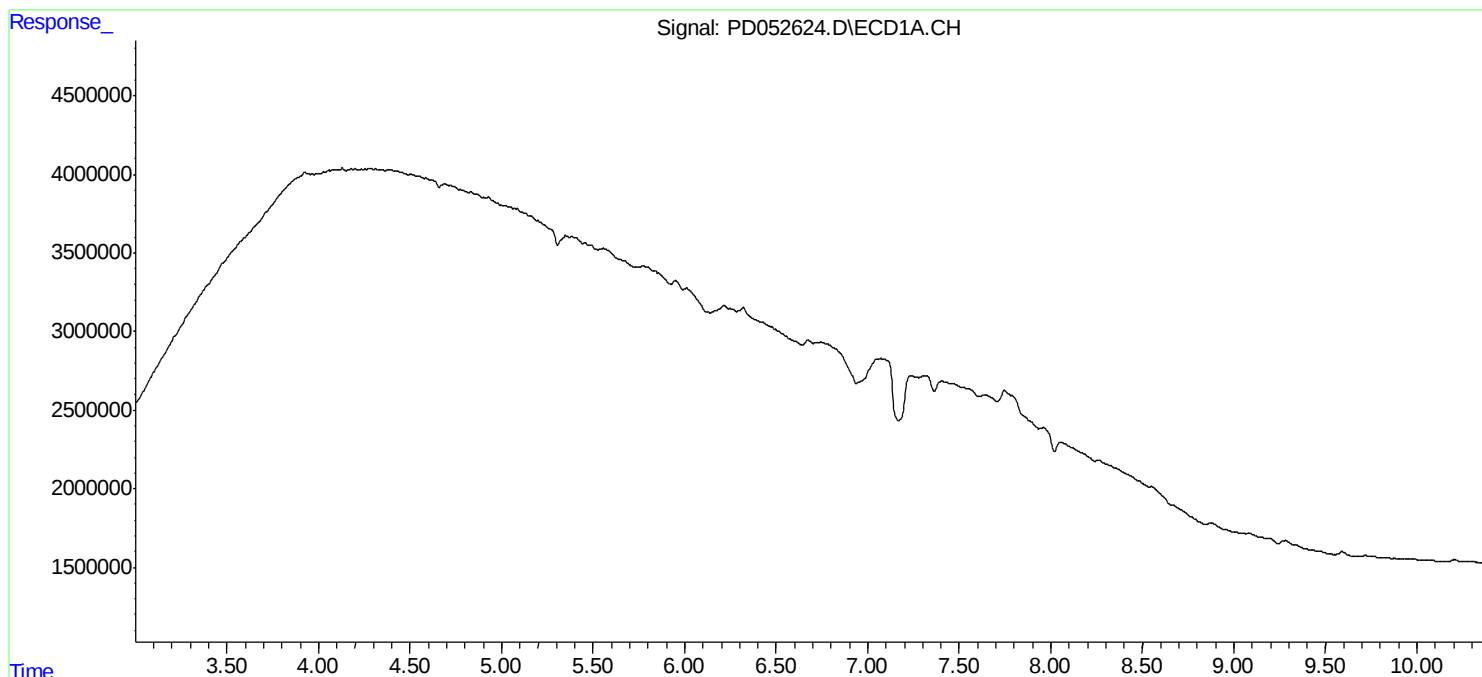


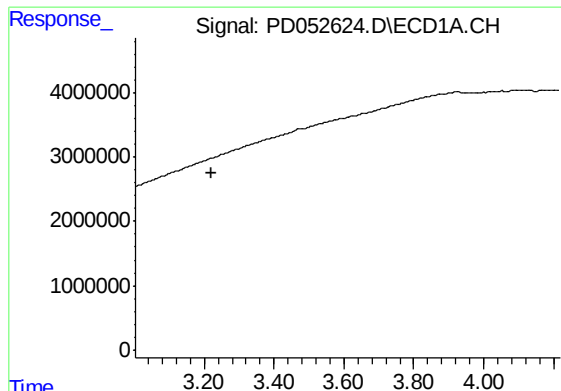

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

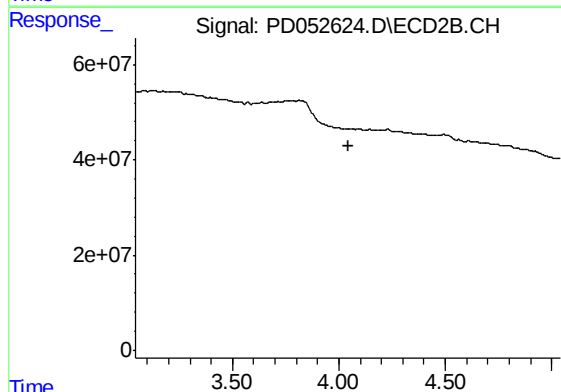


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

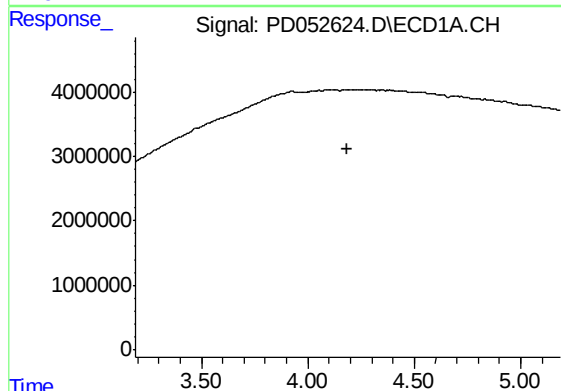


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

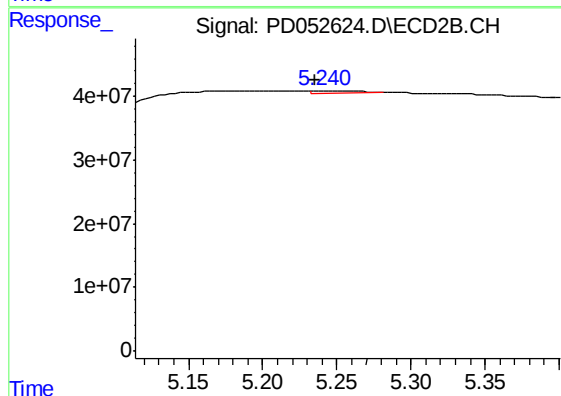

#4 Heptachlor


R.T.: 5.241 min
Delta R.T.: 0.005 min
Response: 7452611
Conc: 0.19 ng/ml

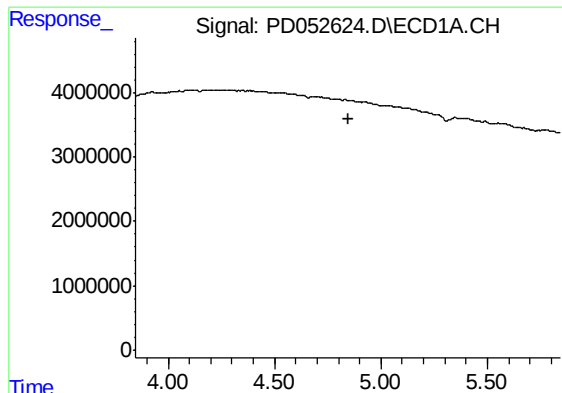

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

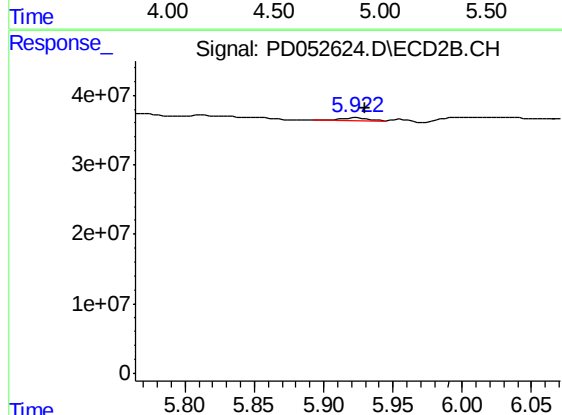


#8 Heptachlor epoxide

R.T.: 5.924 min
Delta R.T.: -0.006 min
Response: 6961649
Conc: 0.22 ng/ml

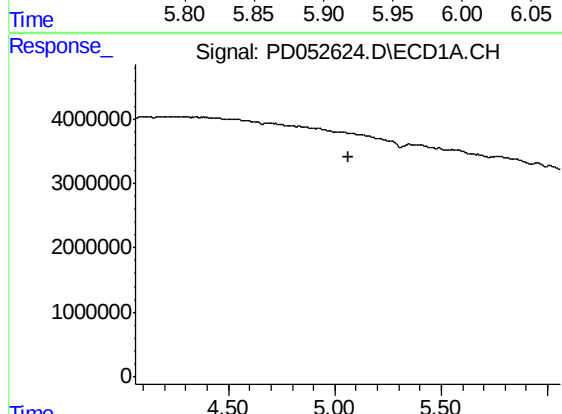


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

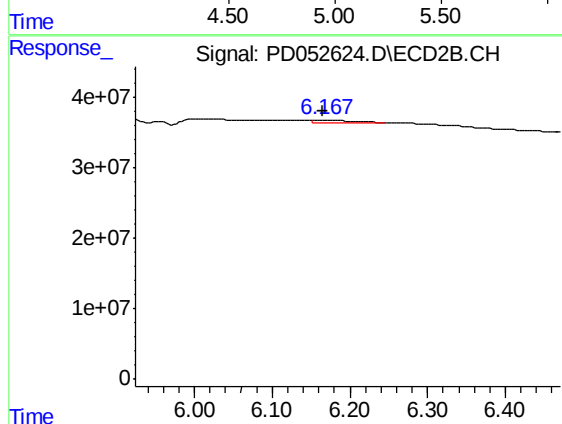

#10 gamma-Chlordane


R.T.: 6.169 min
Delta R.T.: 0.003 min
Response: 15193769
Conc: 0.47 ng/ml

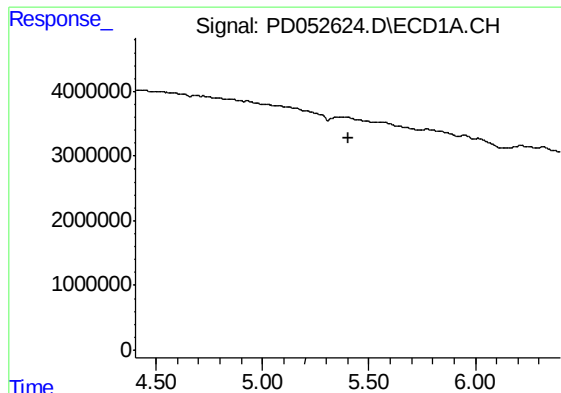

#13 Dielddrin


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

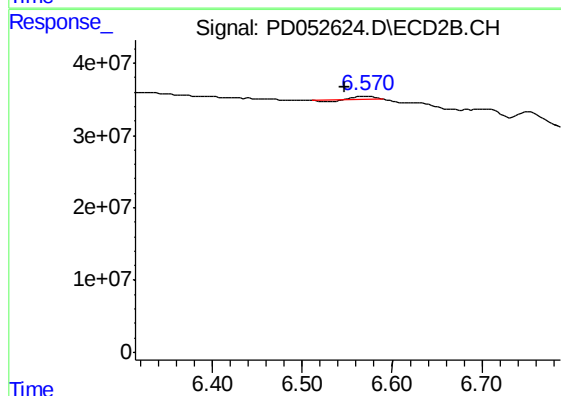


#13 Dielddrin

R.T.: 6.571 min
Delta R.T.: 0.023 min
Response: 6145141
Conc: 0.21 ng/ml

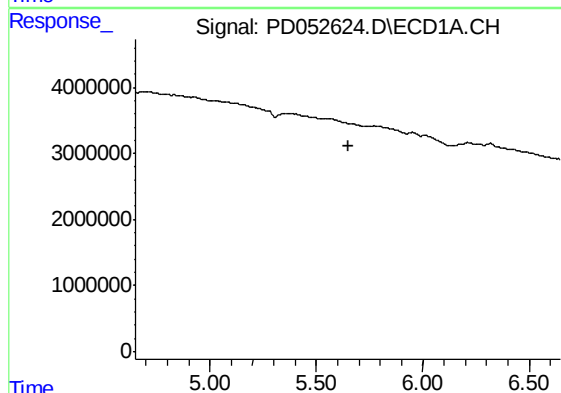


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.650 min
Response: 0
Conc: N.D.

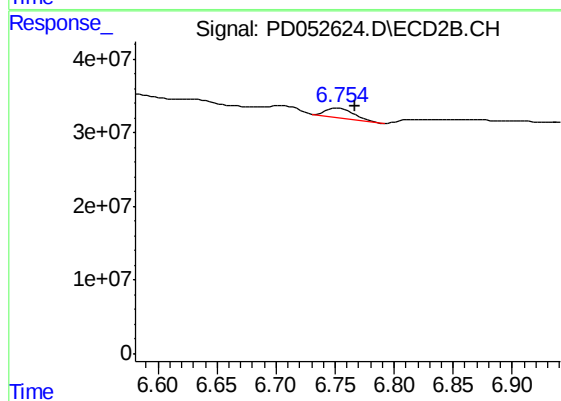

#14 Endrin


R.T.: 6.752 min
Delta R.T.: -0.015 min
Response: 22120209
Conc: 0.88 ng/ml

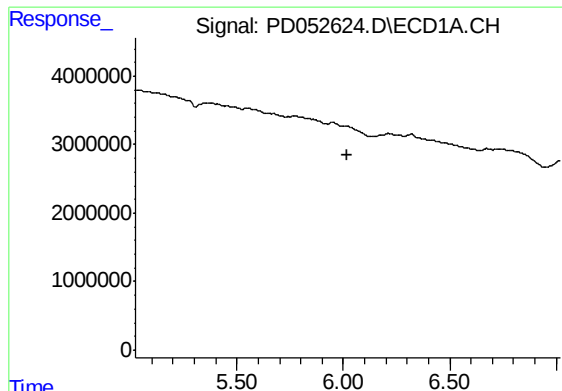

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

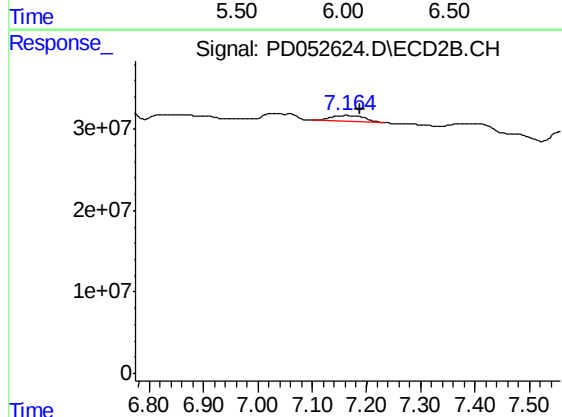


#17 4,4'-DDT

R.T.: 7.164 min
Delta R.T.: -0.024 min
Response: 30462127
Conc: 1.63 ng/ml

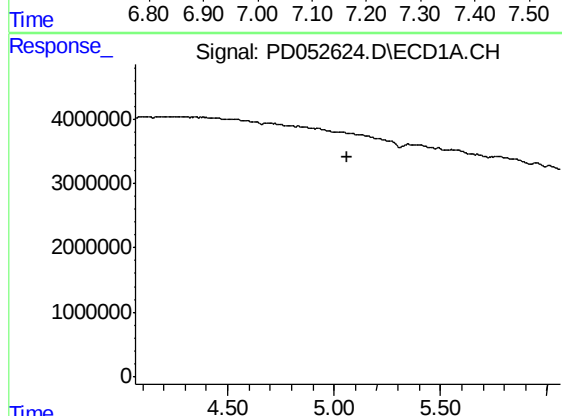


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

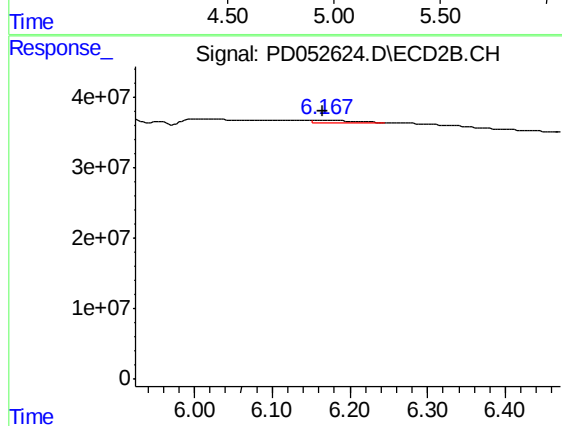

#25 Chlordane-3


R.T.: 6.169 min
Delta R.T.: 0.003 min
Response: 15193769
Conc: 3.44 ng/ml

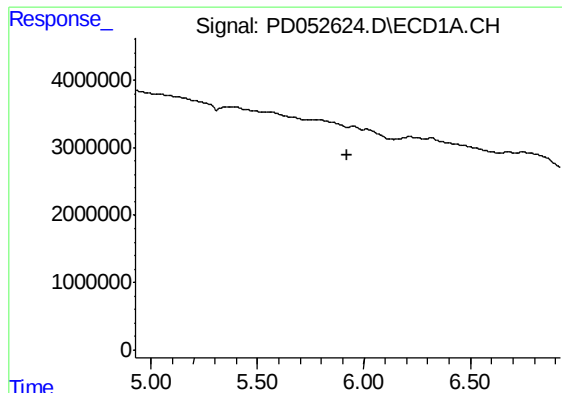

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 5.924 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

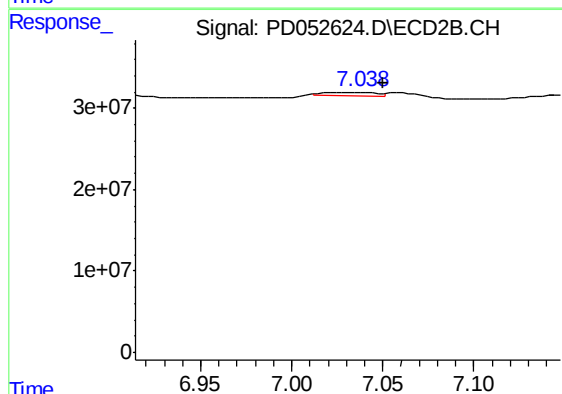


#27 Chlordane-5

R.T.: 7.031 min
Delta R.T.: -0.020 min
Response: 8373839
Conc: 9.08 ng/ml

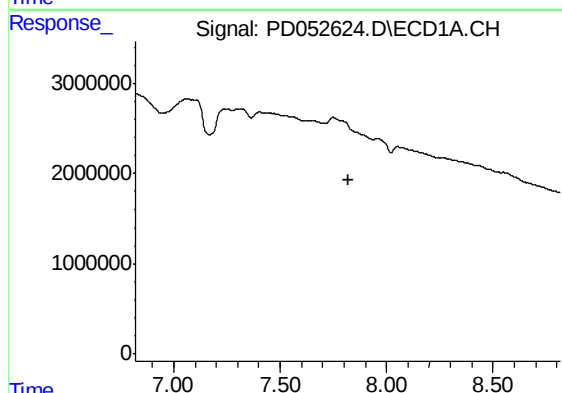

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.819 min
Response: 0
Conc: N.D.

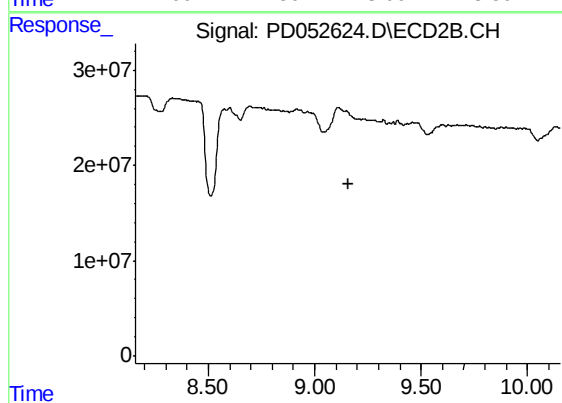

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.156 min
Response: 0
Conc: N.D.