

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052638.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 5:27
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 07:04:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.042	29602448	630.3E6	21.214	21.746
28)	SA Decachlor...	7.815	9.158	31127107	407.4E6	23.355	26.194
Target Compounds							
3)	MA gamma-BHC...	3.923	0.000	2020849	0	0.924	N.D. #
8)	B Heptachlo...	4.868f	5.925	790574	90065049	0.416	2.790 #
10)	B gamma-Chl...	0.000	6.166	0	39370549	N.D.	1.231 #
11)	B alpha-Chl...	0.000	6.245	0	1089241	N.D.	0.035 #
14)	MA Endrin	0.000	6.758	0	62475478	N.D.	2.493 #
17)	MA 4,4'-DDT	0.000	7.168f	0	21156621	N.D.	1.135 #
25)	Chlordane-3	0.000	6.166	0	39370549	N.D.	8.922 #
26)	Chlordane-4	0.000	6.245	0	1089241	N.D.	0.214 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 5:27
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 07:04:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

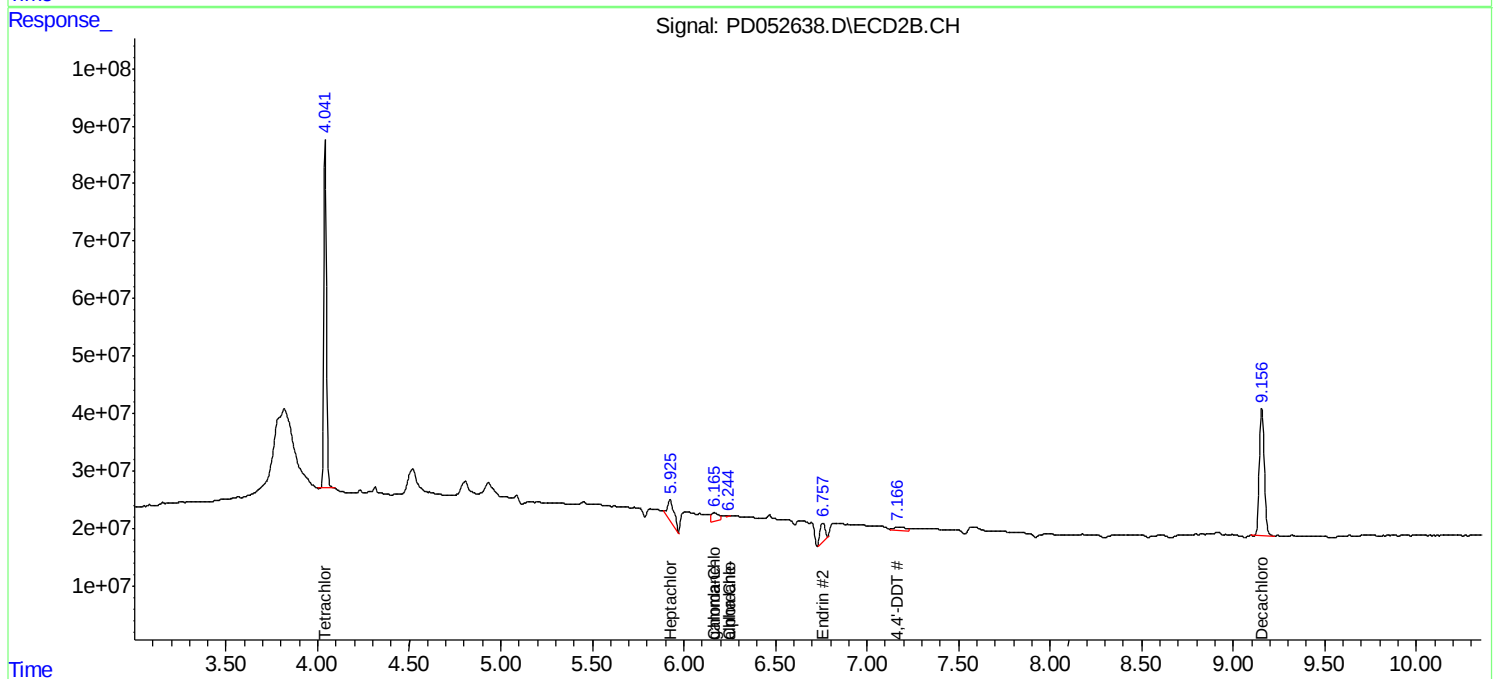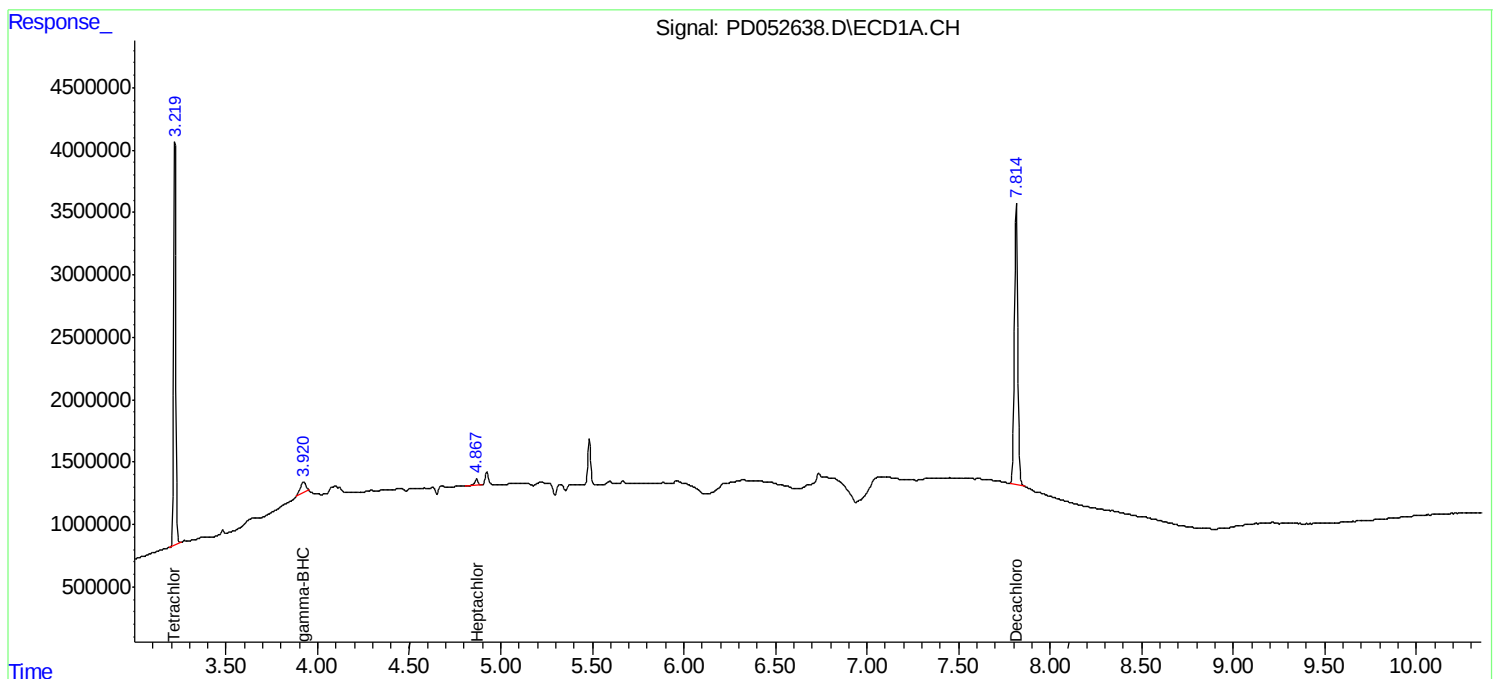


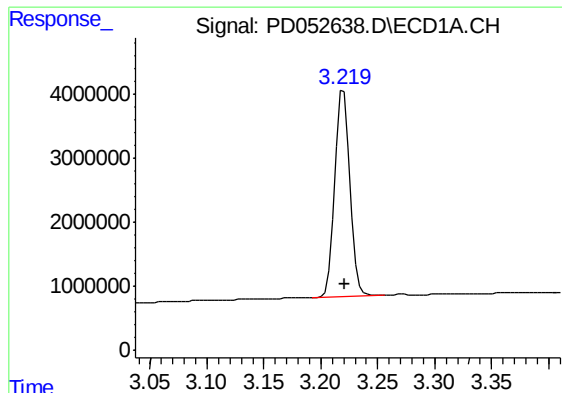

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 29602448
Conc: 21.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

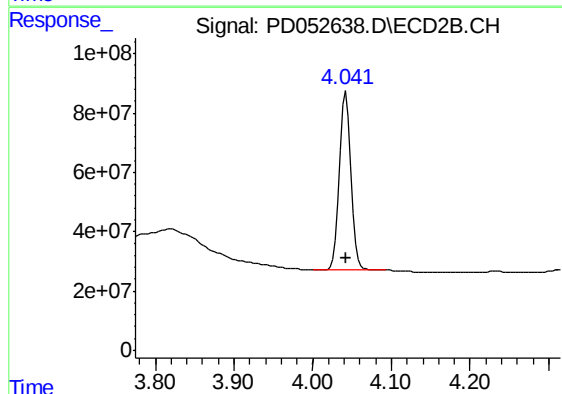


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 630291131
Conc: 21.75 ng/ml

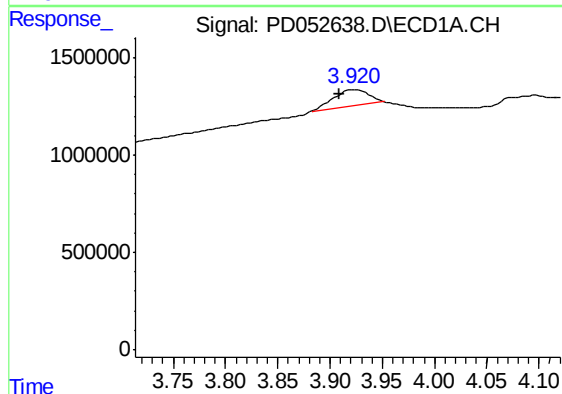


#3 gamma-BHC (Lindane)

R.T.: 3.923 min
Delta R.T.: 0.013 min
Response: 2020849
Conc: 0.92 ng/ml

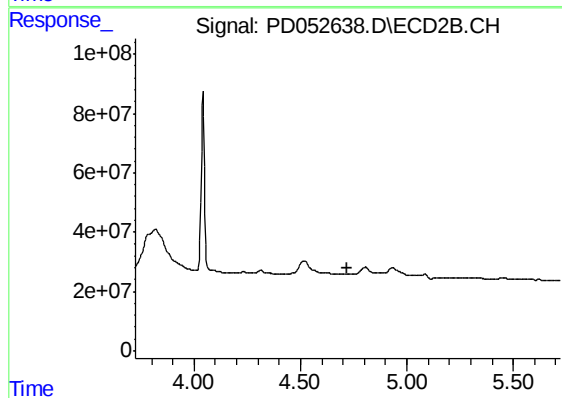

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

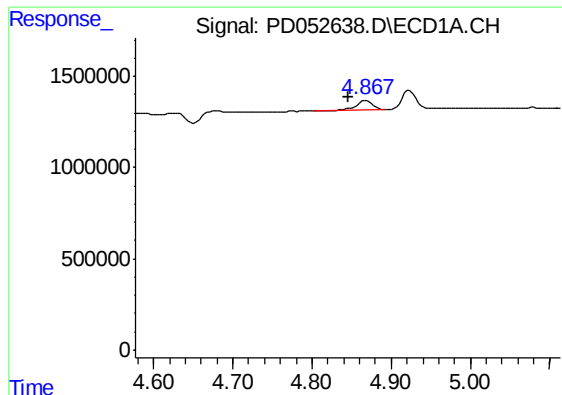

#8 Heptachlor epoxide


R.T.: 4.868 min
Delta R.T.: 0.023 min
Response: 790574
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

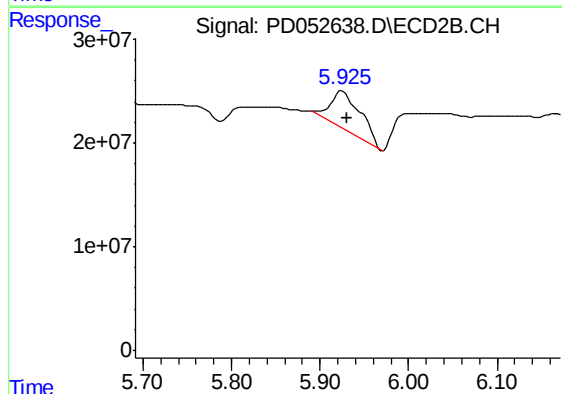


#8 Heptachlor epoxide

R.T.: 5.925 min
Delta R.T.: -0.005 min
Response: 90065049
Conc: 2.79 ng/ml

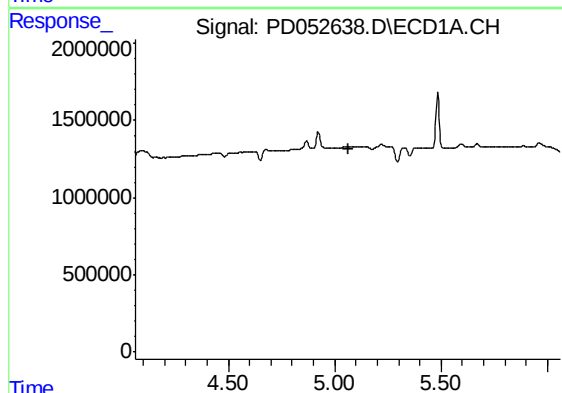


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

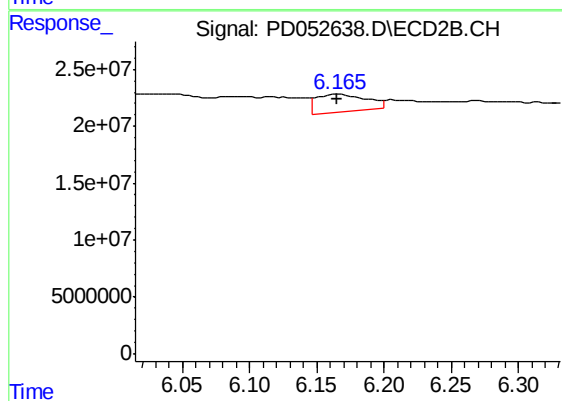

#10 gamma-Chlordane


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 39370549
Conc: 1.23 ng/ml

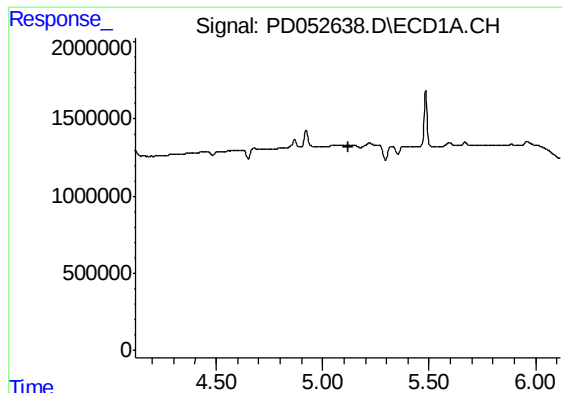

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

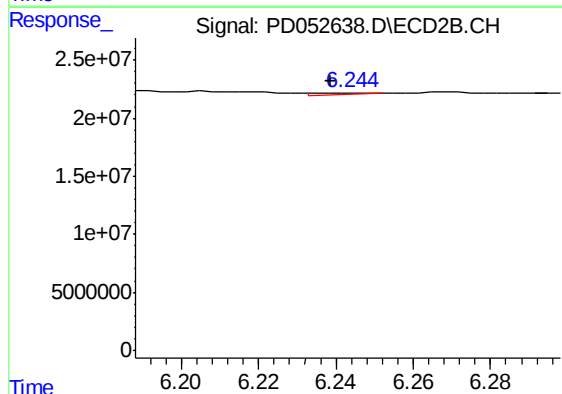


#11 alpha-Chlordane

R.T.: 6.245 min
Delta R.T.: 0.006 min
Response: 1089241
Conc: 0.03 ng/ml

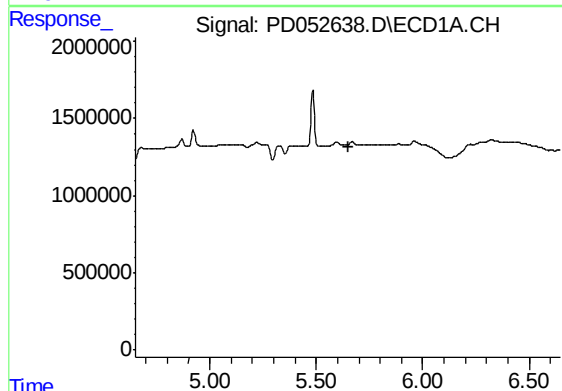


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.650 min
Response: 0
Conc: N.D.

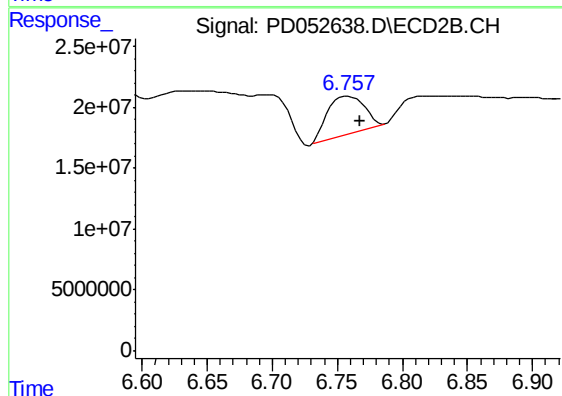

#14 Endrin


R.T.: 6.758 min
Delta R.T.: -0.009 min
Response: 62475478
Conc: 2.49 ng/ml

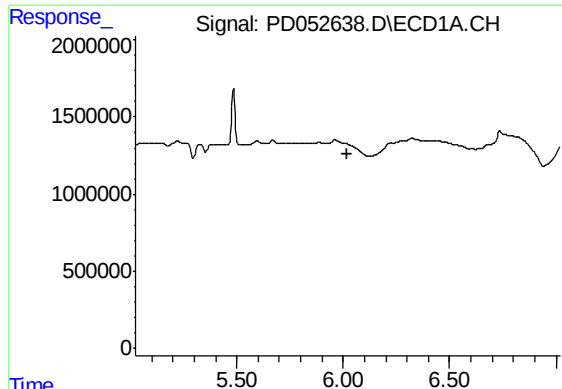

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

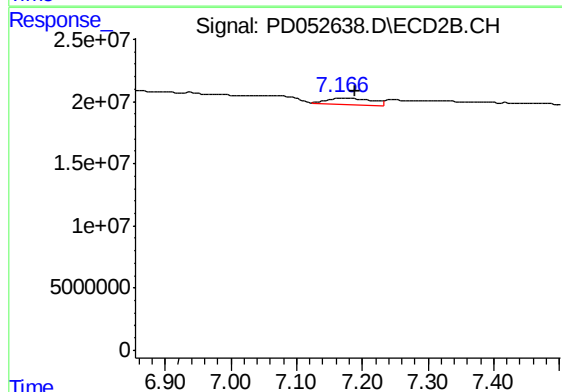


#17 4,4'-DDT

R.T.: 7.168 min
Delta R.T.: -0.020 min
Response: 21156621
Conc: 1.14 ng/ml

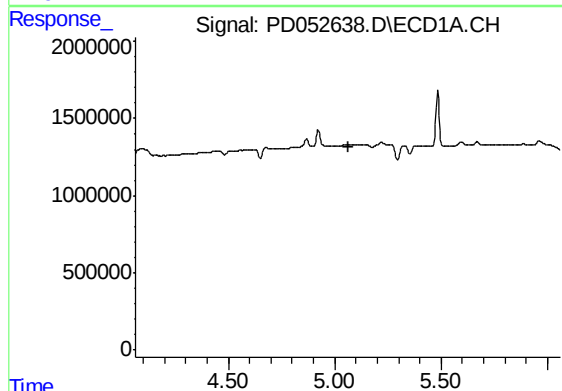


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

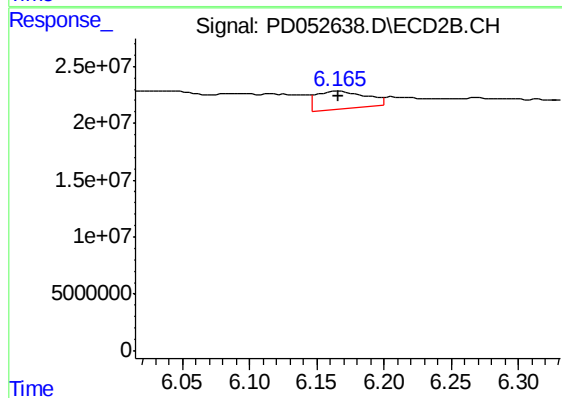

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 39370549
Conc: 8.92 ng/ml

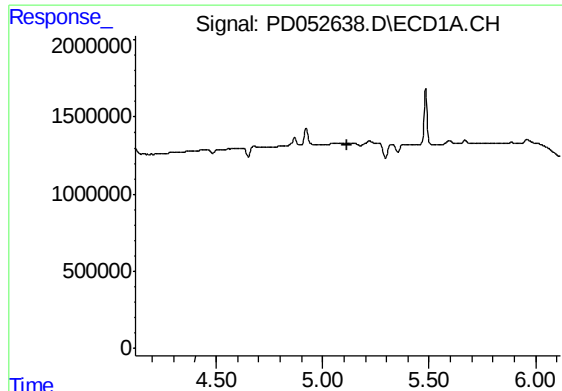

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

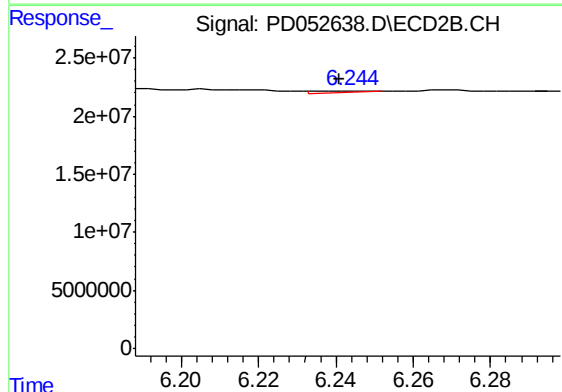


#26 Chlordane-4

R.T.: 6.245 min
Delta R.T.: 0.004 min
Response: 1089241
Conc: 0.21 ng/ml

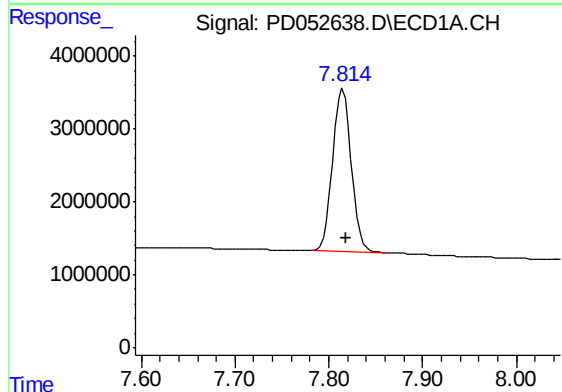

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: -0.003 min
Response: 31127107
Conc: 23.36 ng/ml

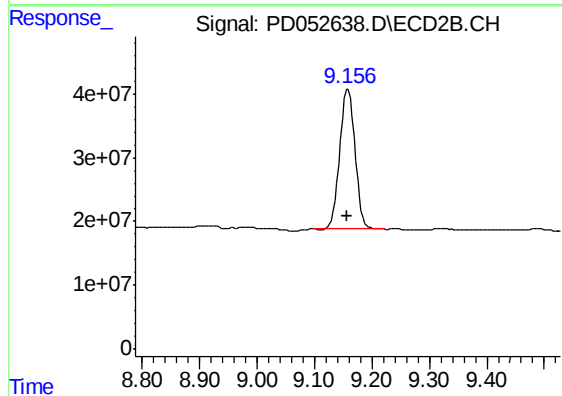

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.001 min
Response: 407358541
Conc: 26.19 ng/ml