

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
 Data File : PD052628.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 2:37
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 07:01:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.042	70747172	1340.9E6	50.699	46.265
28)	SA Decachlor...	7.816	9.159	66585971	826.6E6	49.961	53.155
Target Compounds							
23)	Chlordane-1	4.042	5.045	31736400	702.2E6	505.405	457.705
24)	Chlordane-2	4.521	5.515	37139757	636.1E6	499.082	454.180
25)	Chlordane-3	5.061	6.165	112.6E6	2039.5E6	509.263	462.175
26)	Chlordane-4	5.117	6.240	107.9E6	2316.5E6	508.805	455.550
27)	Chlordane-5	5.921	7.049	33551670	472.2E6	515.917	511.824



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040519\
Data File : PD052628.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 2:37
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 07:01:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

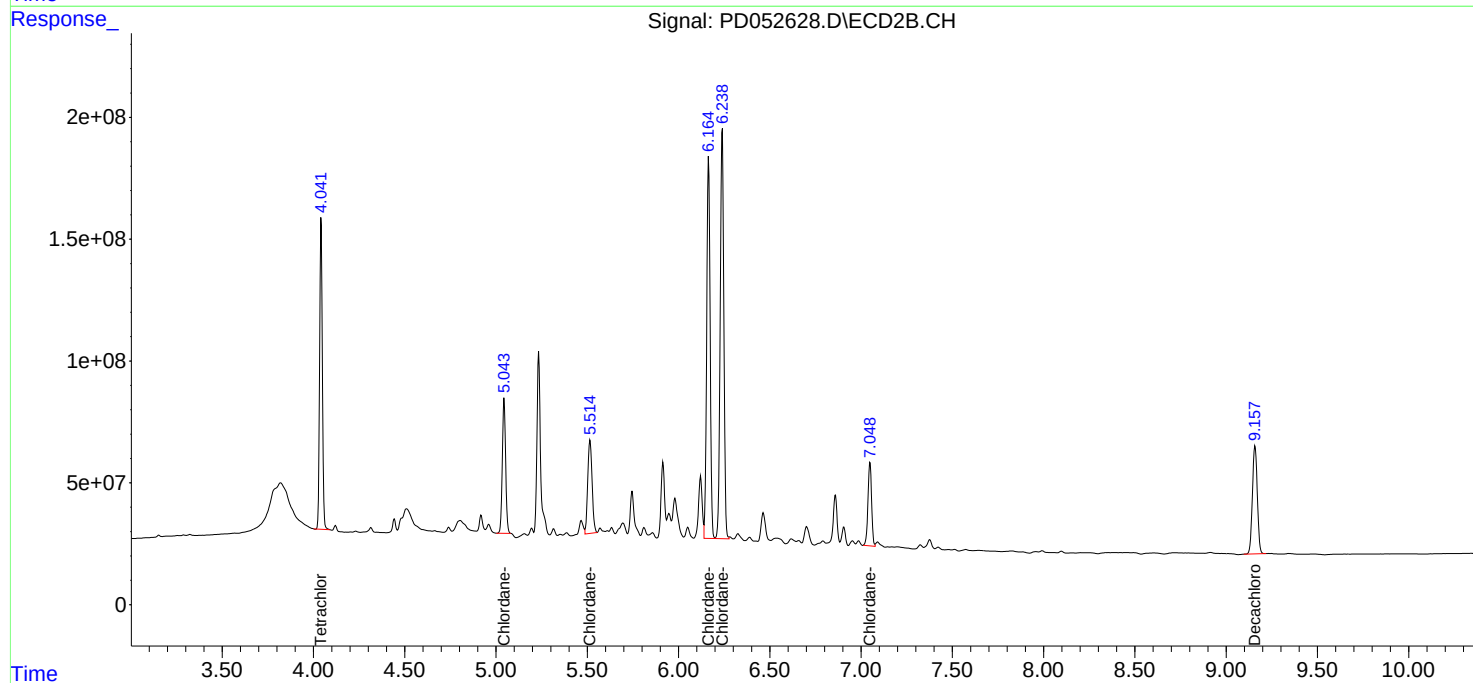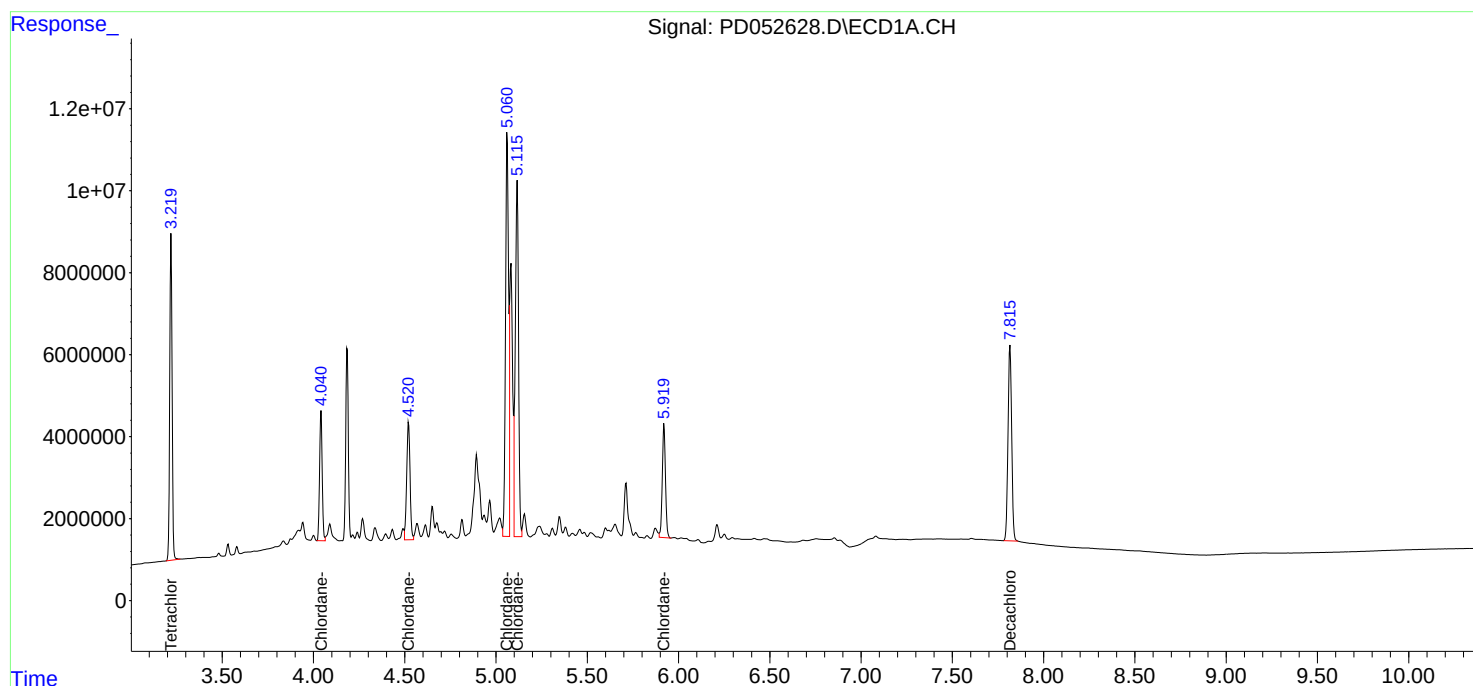


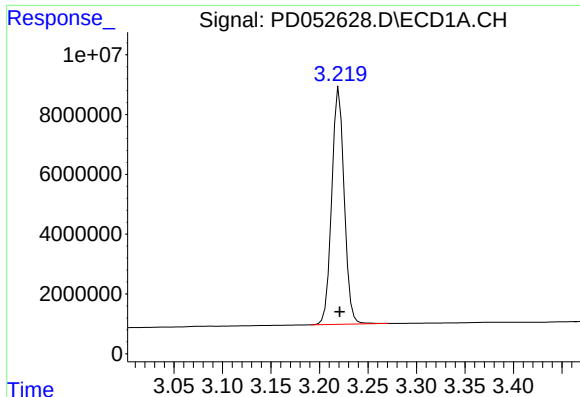

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 70747172
Conc: 50.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

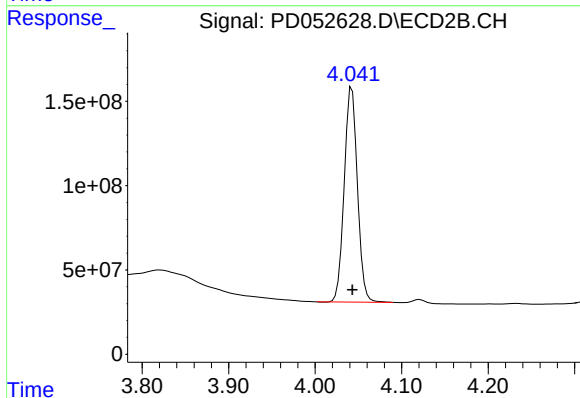


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 1340930925
Conc: 46.26 ng/ml

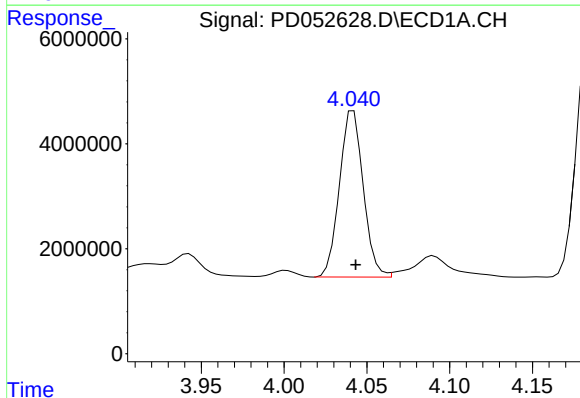


#23 Chlordane-1

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 31736400
Conc: 505.41 ng/ml

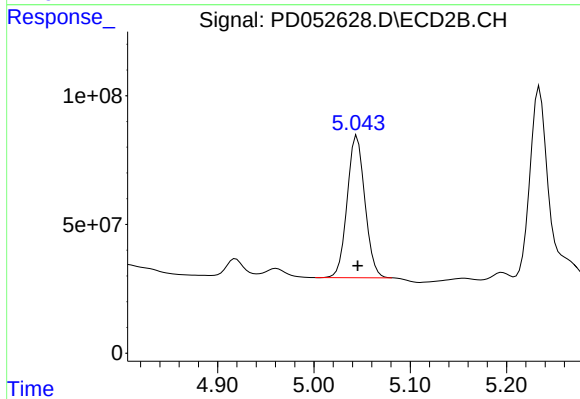

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 702164031
Conc: 457.70 ng/ml

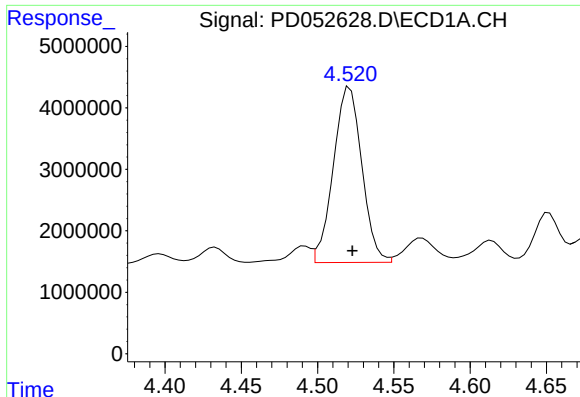

#24 Chlordane-2


R.T.: 4.521 min
Delta R.T.: -0.002 min
Response: 37139757
Conc: 499.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

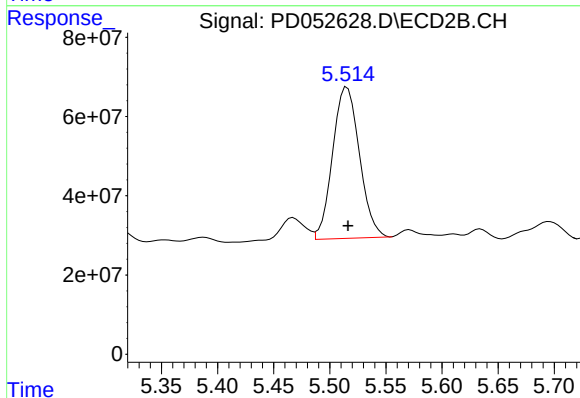


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 636065925
Conc: 454.18 ng/ml

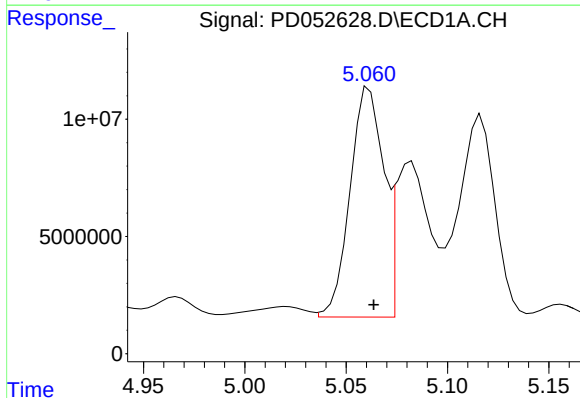


#25 Chlordane-3

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 112616955
Conc: 509.26 ng/ml

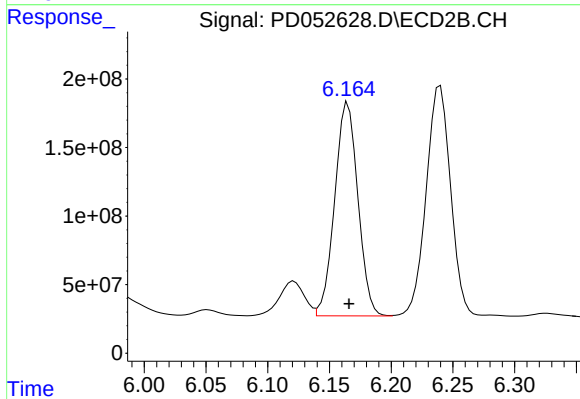

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 2039482005
Conc: 462.17 ng/ml

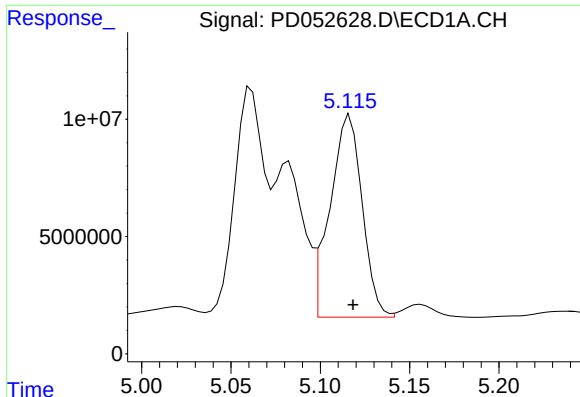

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: -0.002 min
Response: 107913850
Conc: 508.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

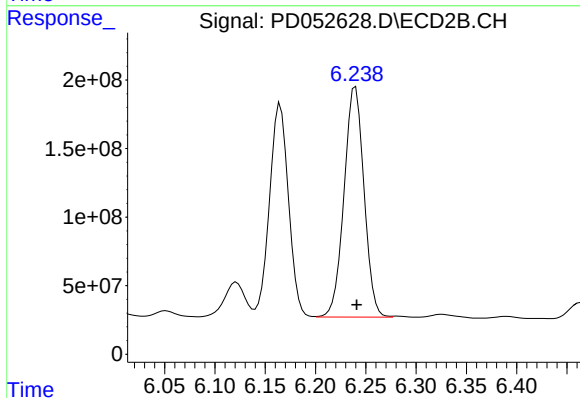


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: -0.001 min
Response: 2316538064
Conc: 455.55 ng/ml

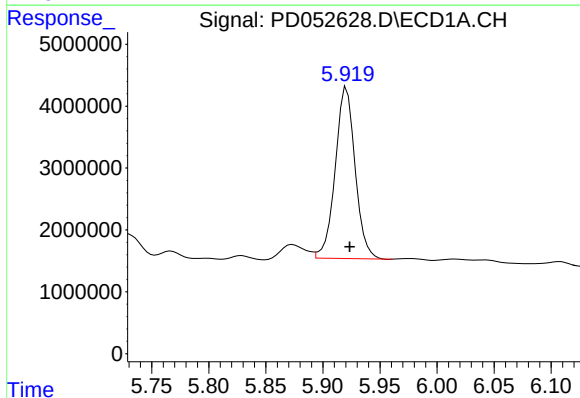


#27 Chlordane-5

R.T.: 5.921 min
Delta R.T.: -0.003 min
Response: 33551670
Conc: 515.92 ng/ml

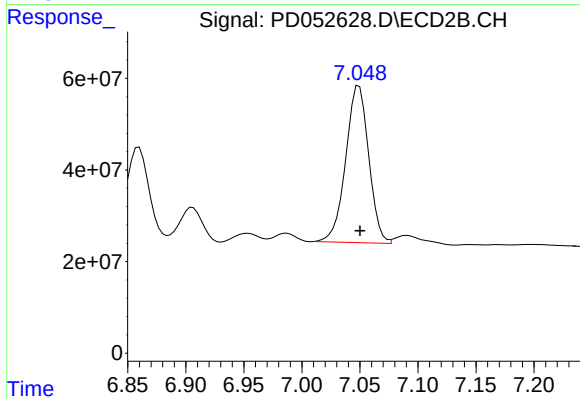

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 472213488
Conc: 511.82 ng/ml

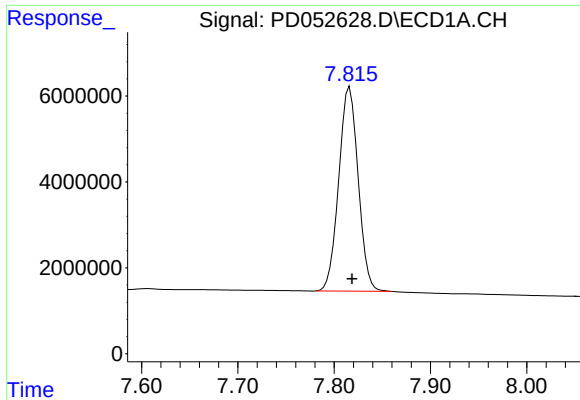

#28 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.002 min
Response: 66585971
Conc: 49.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

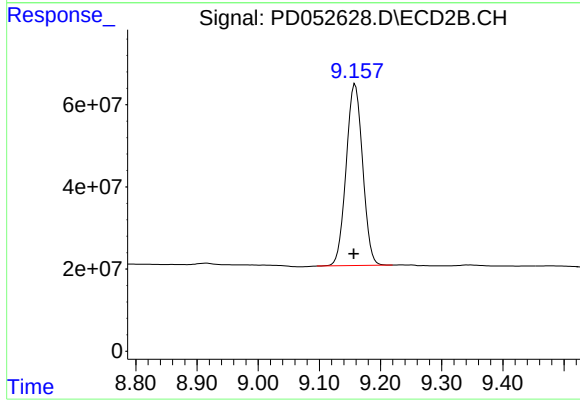

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 826630319
Conc: 53.15 ng/ml