

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
 Data File : PD068935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 08:49
 Operator : AR\AJ
 Sample : PIBLK256
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 06:55:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.172	27488605	241.4E6	20.186	22.051
27)	SA Decachlor...	8.205	9.367	56065825	274.6E6	40.319	43.533
Target Compounds							
2)	A alpha-BHC	0.000	4.604f	0	945949	N.D.	<MDL
7)	B delta-BHC	0.000	5.228	0	2253150	N.D.	0.159
8)	B Heptachlo...	0.000	6.149f	0	1275807	N.D.	0.106


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
Data File : PD068935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 08:49
Operator : AR\AJ
Sample : PIBLK256
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 06:55:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

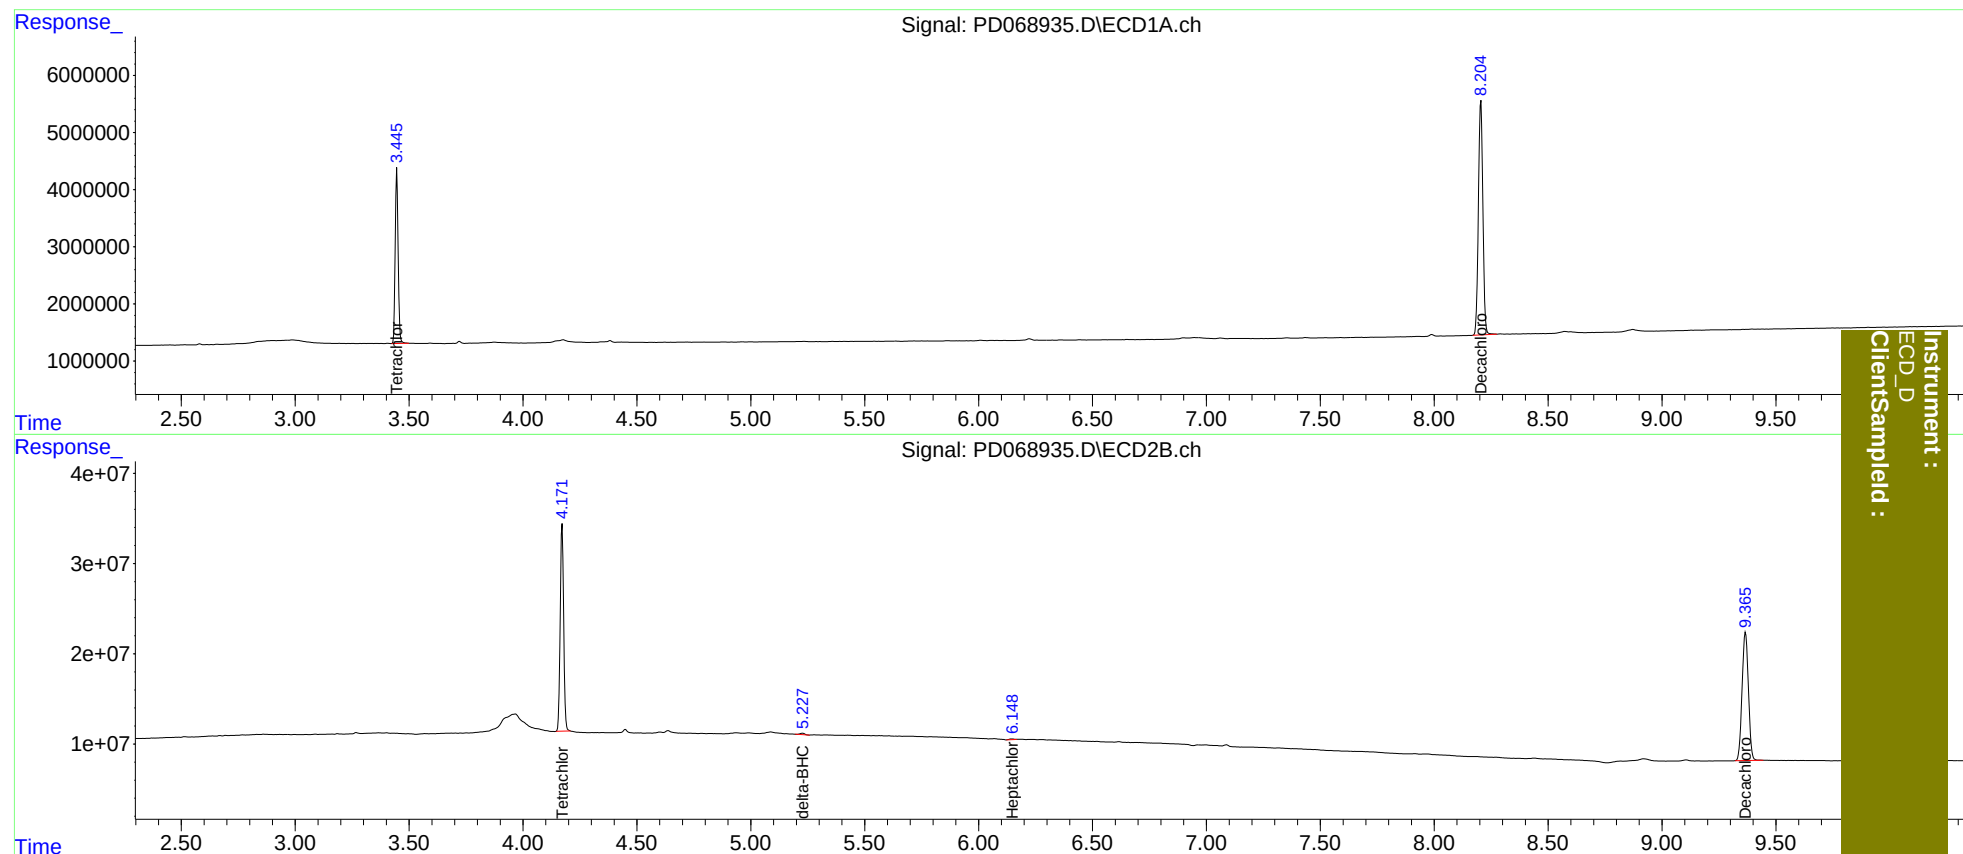


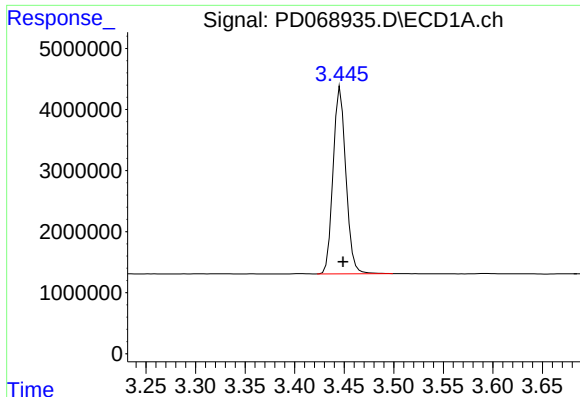

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.003 min
Response: 27488605
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

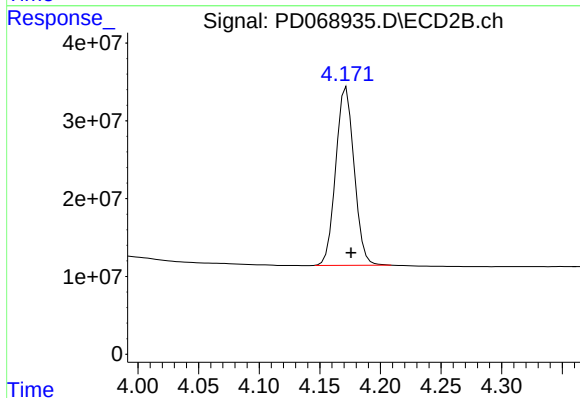


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.004 min
Response: 241358994
Conc: 22.05 ng/ml

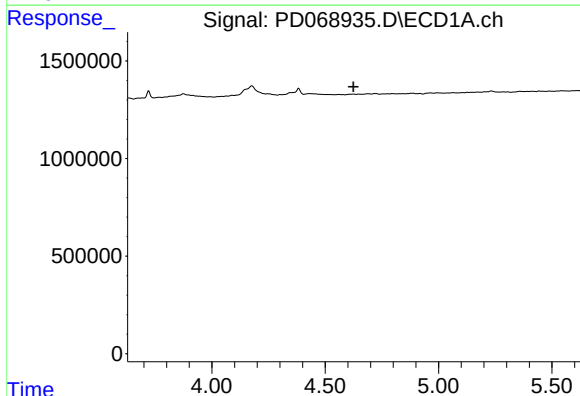


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.625 min
Response: 0
Conc: N.D.

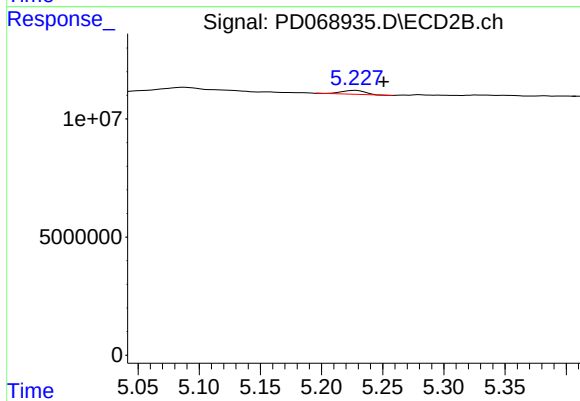

#7 delta-BHC


R.T.: 5.228 min
Delta R.T.: -0.023 min
Response: 2253150
Conc: 0.16 ng/ml

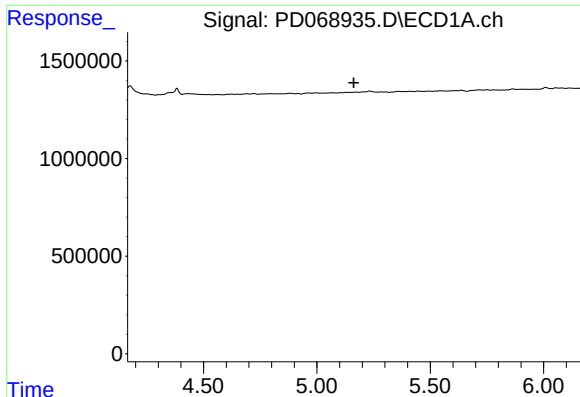

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

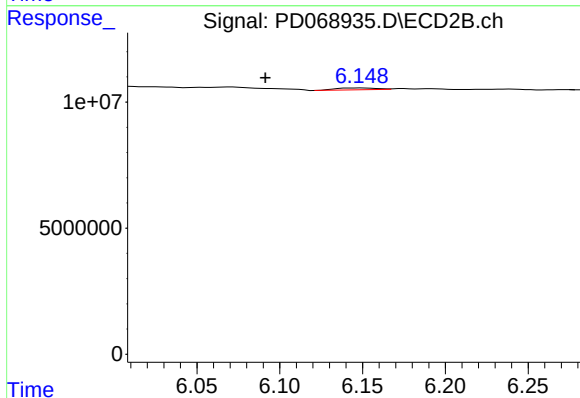


#8 Heptachlor epoxide

R.T.: 6.149 min
Delta R.T.: 0.058 min
Response: 1275807
Conc: 0.11 ng/ml

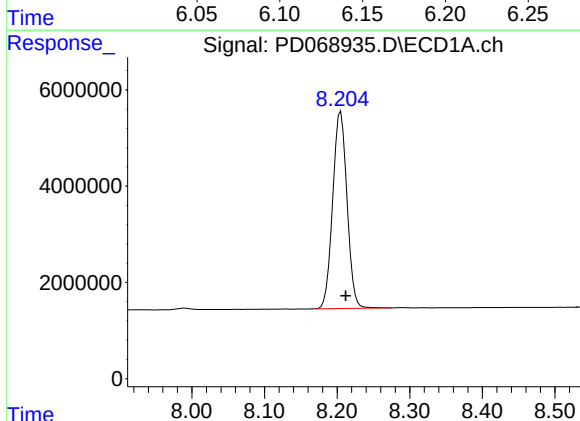

#27 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.007 min
Response: 56065825
Conc: 40.32 ng/ml

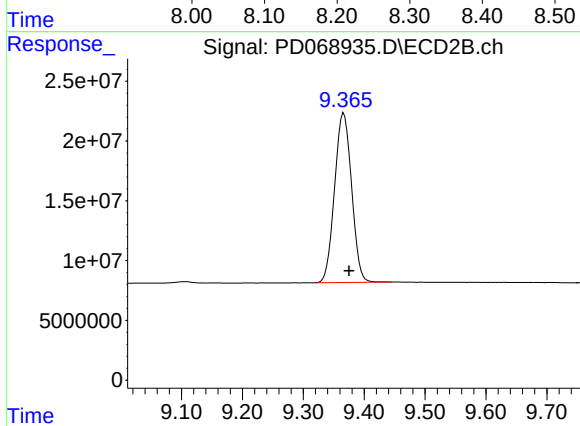

#27 Decachlorobiphenyl

R.T.: 9.367 min
Delta R.T.: -0.008 min
Response: 274568856
Conc: 43.53 ng/ml