

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
 Data File : PD068938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 09:52
 Operator : AR\AJ
 Sample : PB143814BS
 Misc : 1
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS814

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2022
 Supervised By : mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 06:56:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	22648764	196.4E6	16.632	17.943
27)	SA Decachlor...	8.205	9.368	47342792	231.1E6	34.046	36.636
Target Compounds							
2)	A alpha-BHC	3.886	4.568	7360208	68023406	3.845	4.351
3)	MA gamma-BHC...	4.169	4.859	8198941	67945077	4.517	4.686
4)	MA Heptachlor	4.467	5.386	7708251	69552722	4.303	5.053
5)	MB Aldrin	4.715	5.699	7407295	68118406	4.212	5.048
6)	B beta-BHC	4.420	5.023	3934636	31971339	4.722	5.006
7)	B delta-BHC	4.623	5.248	6033499	61057712	3.412	4.313 #
8)	B Heptachlo...	5.159	6.087	7357408	62444974	4.530	5.184
9)	A Endosulfan I	5.498	6.450	6905322	55600017	4.485	5.109
10)	B trans-Chl...	5.385	6.324	7521020	60386988	4.507	5.077
11)	B cis-Chlor...	5.444	6.399	7418722	59444914	4.519	5.183
12)	B 4,4'-DDE	5.610	6.548	12913846	107.0E6	8.681	10.478
13)	MA Dieldrin	5.742	6.708	14080638	112.3E6	8.429	10.108
14)	MA Endrin	6.000	6.928	12625392	90181186	8.930	10.666
15)	B Endosulfa...	6.273	7.132	12826460	91645075	8.843	10.241m
16)	A 4,4'-DDD	6.127	7.039	11293228	85969469	8.592	10.246
17)	MA 4,4'-DDT	6.368	7.342	10565537	78768861	7.912	9.994 #
18)	B Endrin al...	6.443	7.257	11604792	78924783	10.582	11.886
19)	B Endosulfa...	6.655	7.482	11804028	79099628	8.446	9.658
20)	A Methoxychlor	6.918	7.796	32127423	191.0E6	45.389	54.514
21)	B Endrin ke...	7.149	7.958	14845316	91905156	9.304	10.764

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
Data File : PD068938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 09:52
Operator : AR\AJ
Sample : PB143814BS
Misc : 1
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 06:56:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

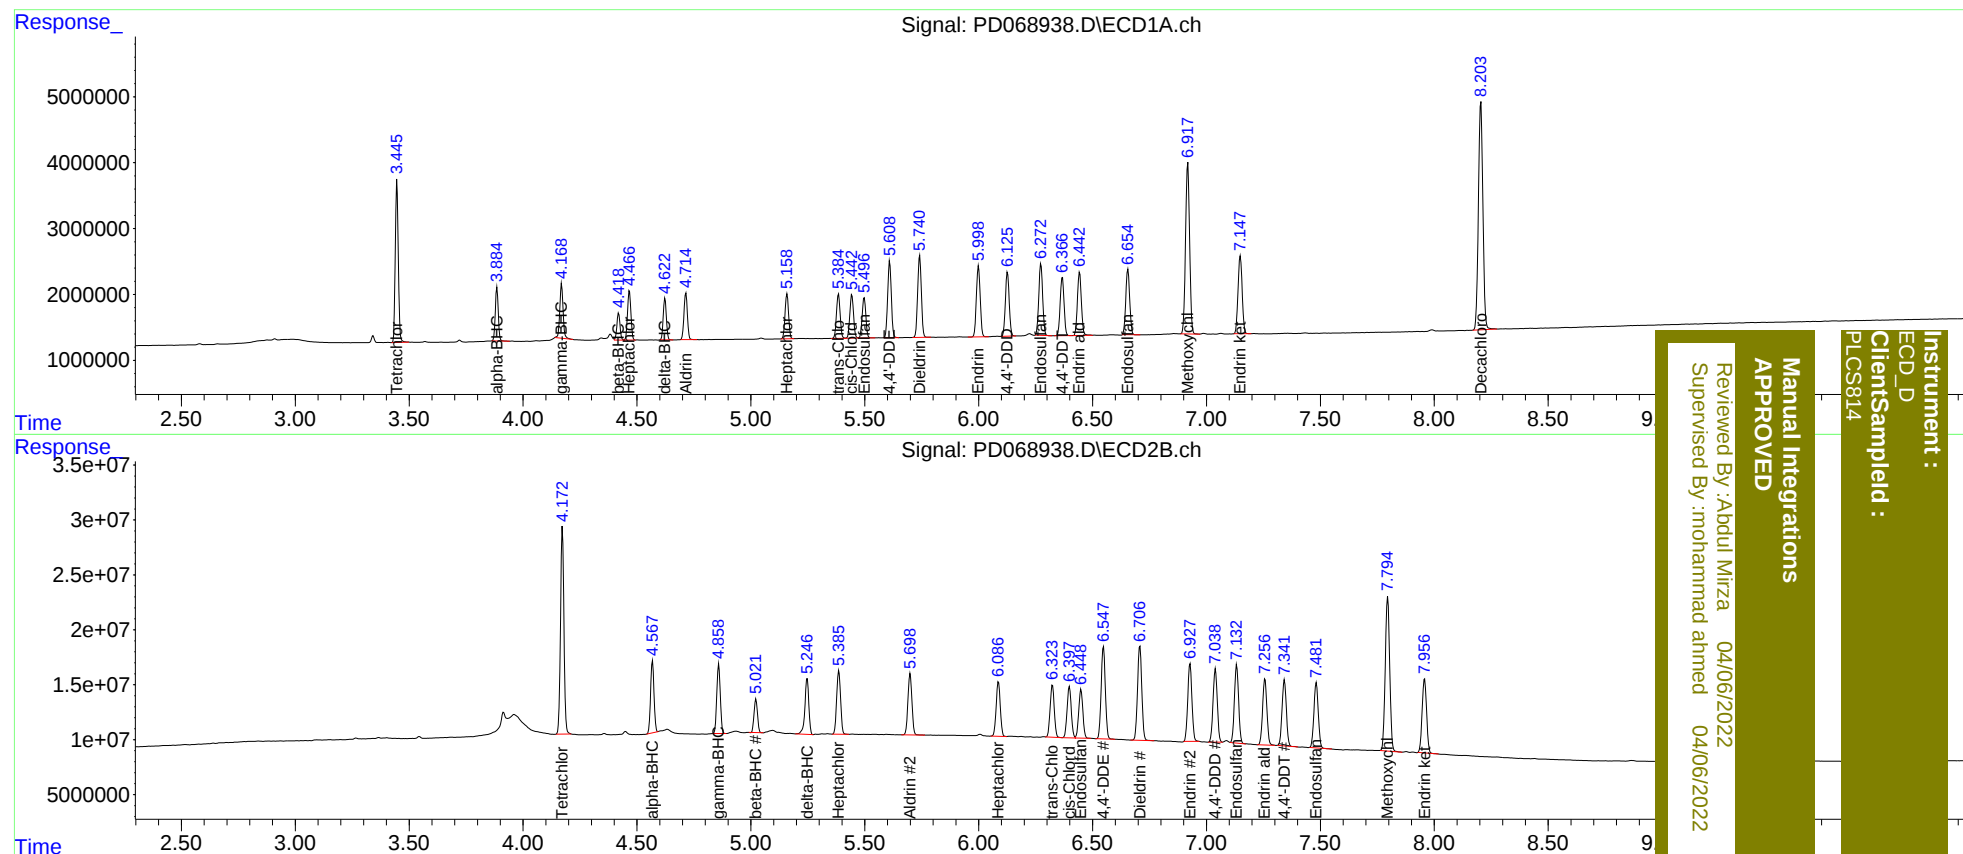

Reviewed By: Abdul Mirza 04/06/2022
Supervised By: mohammad ahmed 04/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS814