

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
 Data File : PD068952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 15:00
 Operator : AR\AJ
 Sample : N2183-02MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COR30MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/06/2022
 Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 07:00:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.172	19706873	183.9E6	14.471	16.804
27)	SA Decachlor...	8.204	9.367	36302740	179.1E6	26.107	28.393
Target Compounds							
2)	A alpha-BHC	3.886	4.568	92546032	696.9E6	48.345	44.573
3)	MA gamma-BHC...	4.169	4.859	89432452	664.5E6	49.268	45.833
4)	MA Heptachlor	4.467	5.386	87779126	625.6E6	49.002	45.453
5)	MB Aldrin	4.713	5.699	82718975	632.4E6	47.033m	46.866
6)	B beta-BHC	4.419	5.022	35361904	297.7E6	42.435	46.615
7)	B delta-BHC	4.624	5.246	48431244	306.4E6	27.391	21.646m
8)	B Heptachlo...	5.159	6.087	79538483	539.5E6	48.977	44.789
9)	A Endosulfan I	5.498	6.450	74165131	503.3E6	48.172	46.245
10)	B trans-Chl...	5.385	6.323	82578952	540.7E6	49.481	45.466
11)	B cis-Chlor...	5.443	6.398	80885974	522.0E6	49.273	45.515
12)	B 4,4'-DDE	5.610	6.548	158.7E6	1009.2E6	106.661	98.781
13)	MA Dieldrin	5.742	6.708	171.9E6	1060.0E6	102.928	95.399
14)	MA Endrin	6.000	6.929	150.8E6	851.6E6	106.676	100.730
15)	B Endosulfa...	6.273	7.133	143.0E6	836.8E6	98.566	93.505
16)	A 4,4'-DDD	6.126	7.039	130.8E6	788.2E6	99.489	93.936
17)	MA 4,4'-DDT	6.367	7.342	139.3E6	836.8E6	104.321	106.168
18)	B Endrin al...	6.443	7.257	106.6E6	617.6E6	97.248	93.012
19)	B Endosulfa...	6.656	7.482	122.9E6	711.0E6	87.946	86.814
20)	A Methoxychlor	6.918	7.796	358.8E6	1799.9E6	506.933	513.809
21)	B Endrin ke...	7.150	7.957	164.8E6	835.9E6	103.306	97.901

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
Data File : PD068952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 15:00
Operator : AR\AJ
Sample : N2183-02MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 07:00:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

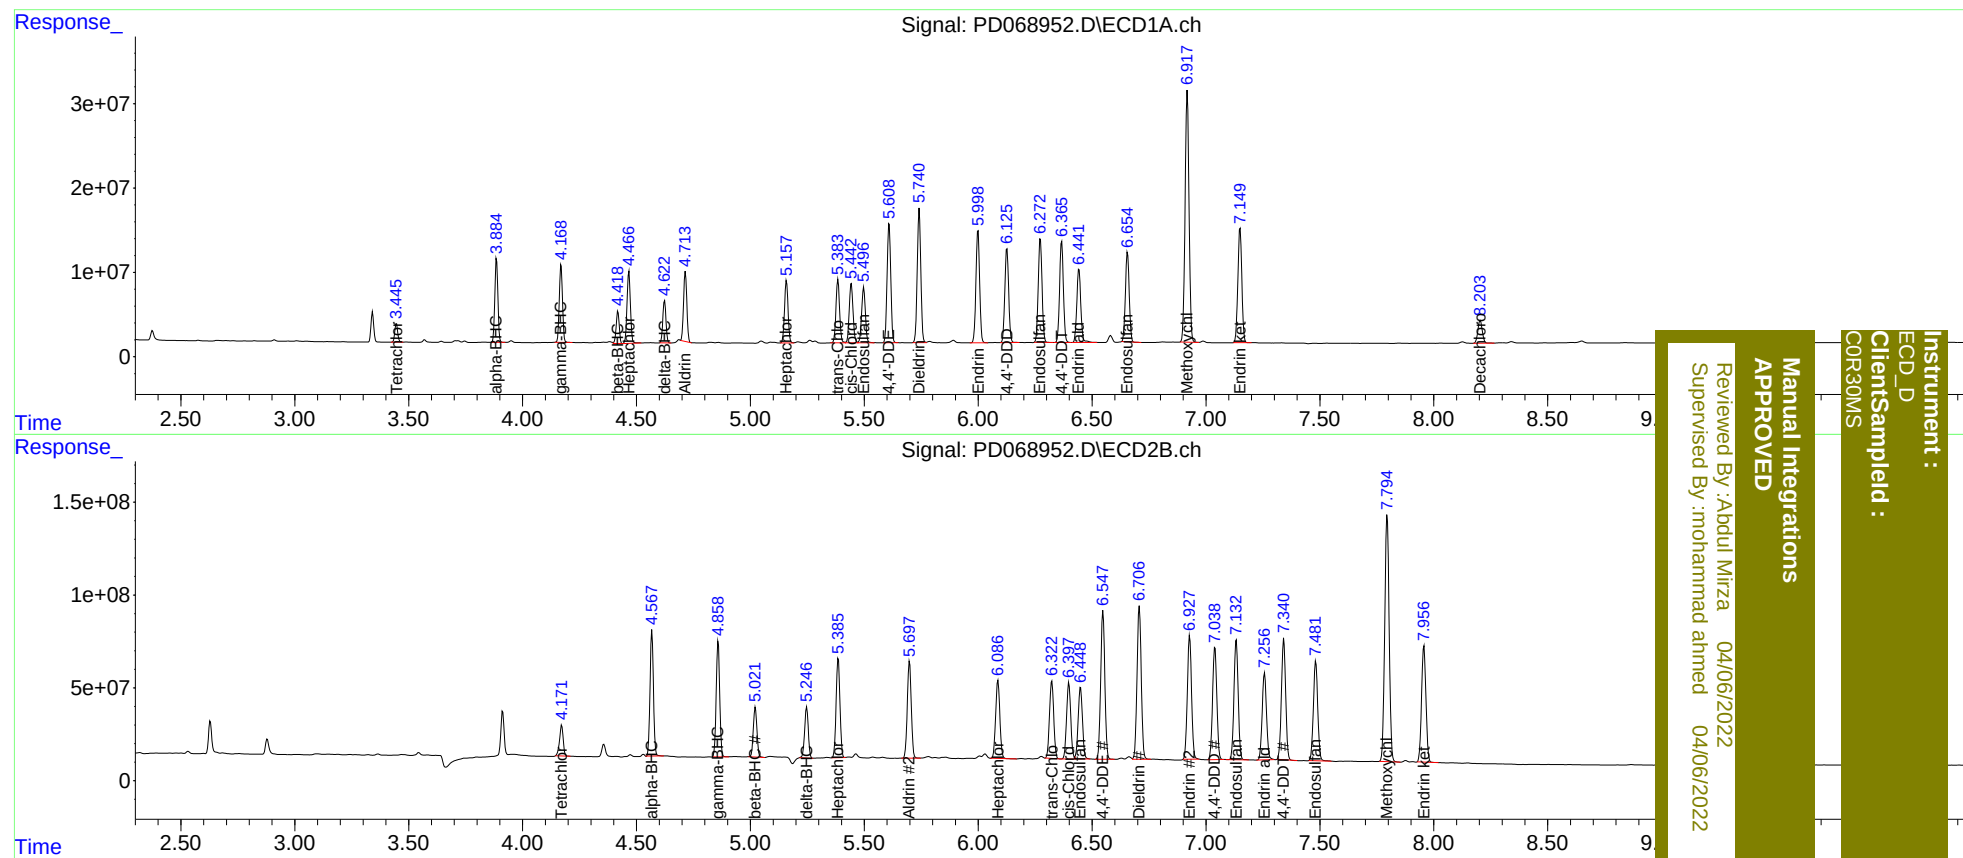

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/06/2022
Supervised By: mohammad ahmed 04/06/2022

Instrument :
ECD_D
ClientSampled :
COR30MS