

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
 Data File : PD068940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 10:45
 Operator : AR\AJ
 Sample : N2166-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0R39MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2022
 Supervised By : mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 06:57:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.170	22219492	214.2E6	16.317	19.568m
2)	SA Decachlor...	8.204	9.367	45805536	223.0E6	32.941	35.351
Target Compounds							
2)	A alpha-BHC	3.885	4.568	96796105	745.1E6	50.566	47.654
3)	MA gamma-BHC...	4.169	4.858	93537090	707.2E6	51.529	48.775
4)	MA Heptachlor	4.467	5.386	87826945	657.5E6	49.029	47.770
5)	MB Aldrin	4.715	5.698	87543957	654.0E6	49.777	48.468
6)	B beta-BHC	4.419	5.021	40534706	307.7E6	48.643	48.173
7)	B delta-BHC	4.623	5.247	53573060	414.5E6	30.299	29.279
8)	B Heptachlo...	5.159	6.087	82902708	585.1E6	51.048	48.580
9)	A Endosulfan I	5.497	6.449	77616948	528.0E6	50.414	48.518
10)	B trans-Chl...	5.385	6.323	84923415	575.5E6	50.886	48.388
11)	B cis-Chlor...	5.444	6.398	82495847	559.0E6	50.254	48.737
12)	B 4,4'-DDE	5.610	6.548	163.7E6	1054.7E6	110.037	103.237
13)	MA Dieldrin	5.741	6.707	178.9E6	1120.9E6	107.112	100.877
14)	MA Endrin	5.999	6.926	155.5E6	904.7E6	109.981	107.009m
15)	B Endosulfa...	6.272	7.133	148.9E6	887.8E6	102.683	99.215
16)	A 4,4'-DDD	6.126	7.039	135.5E6	826.8E6	103.065	98.547
17)	MA 4,4'-DDT	6.367	7.342	141.9E6	867.3E6	106.267	110.047
18)	B Endrin al...	6.443	7.256	108.4E6	644.6E6	98.849	97.076
19)	B Endosulfa...	6.655	7.481	126.6E6	744.1E6	90.557	90.848
20)	A Methoxychlor	6.918	7.795	364.4E6	1844.5E6	514.867	526.543
21)	B Endrin ke...	7.149	7.957	171.0E6	876.9E6	107.183	102.696

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
Data File : PD068940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 10:45
Operator : AR\AJ
Sample : N2166-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 06:57:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

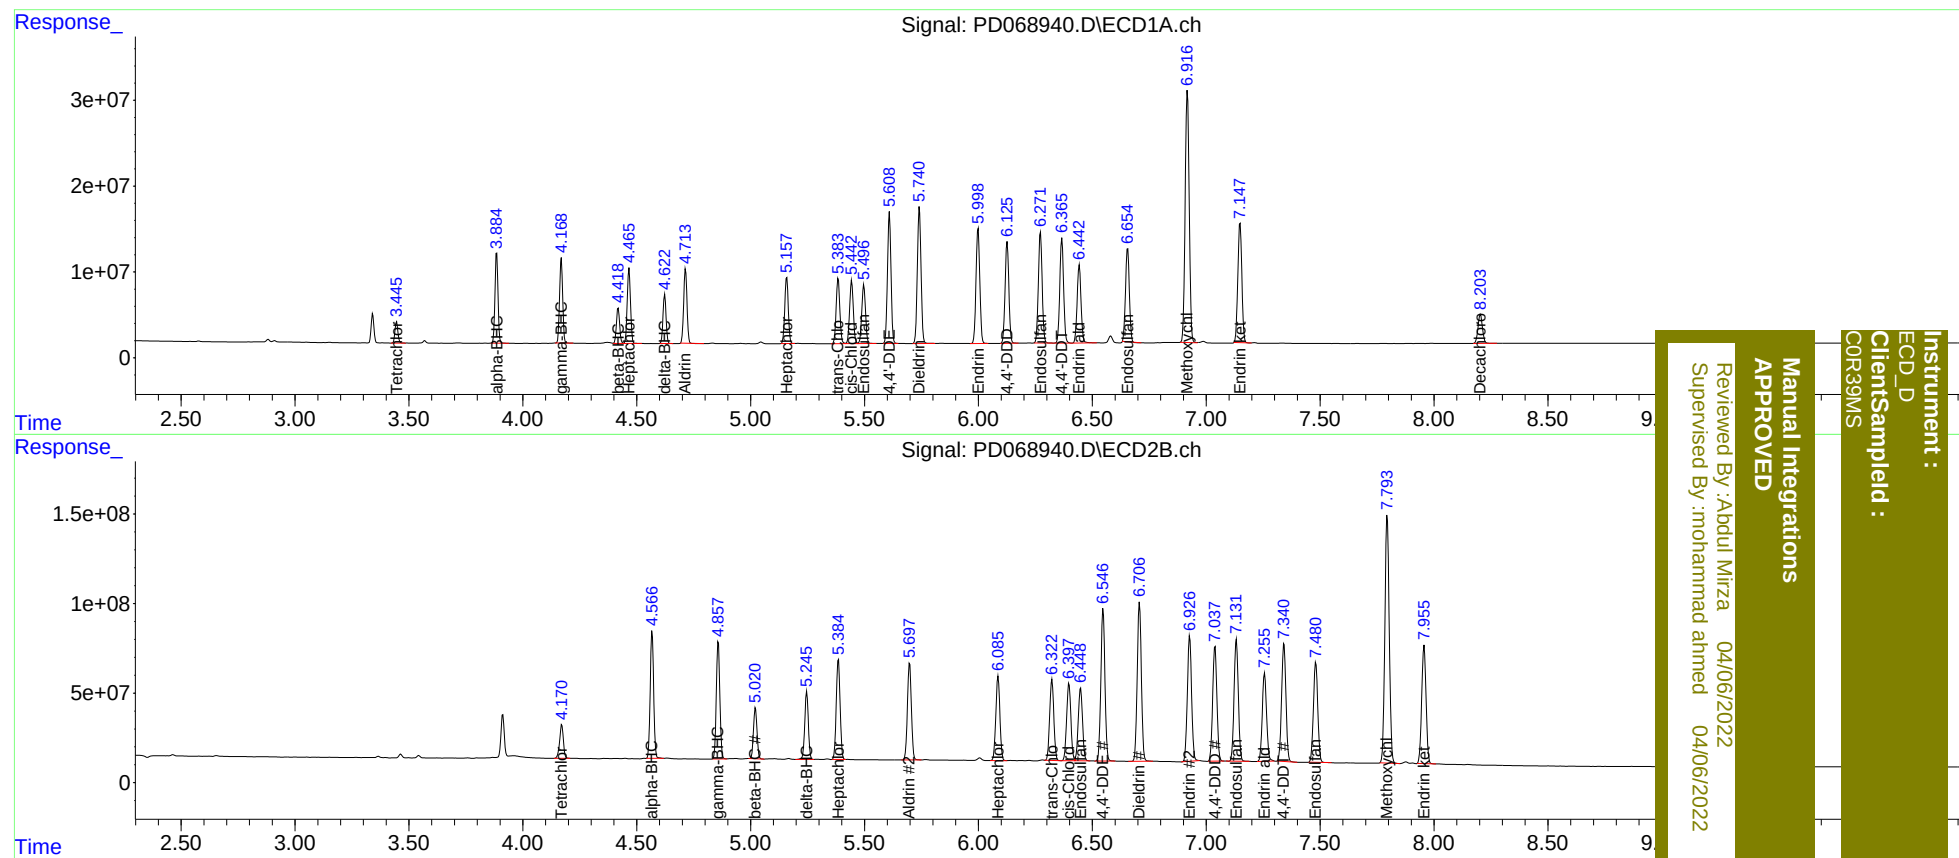

Reviewed By: Abdul Mirza 04/06/2022
Supervised By: mohammad ahmed 04/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COR39MS