

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
 Data File : PD068956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 16:10
 Operator : AR\AJ
 Sample : N2183-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0R33

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2022
 Supervised By : mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 07:01:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.466	4.173	14693653	119.0E6	10.790	10.872
2) SA Decachlor...	8.223	9.366	27200116	136.6E6	19.561	21.661
Target Compounds						
13) MA Dieldrin	5.735	6.727	5695766	7216170	3.410m	0.649 #
16) A 4,4'-DDD	6.147	7.038	1054306	15263154	0.802m	1.819m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040522\
Data File : PD068956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 16:10
Operator : AR\AJ
Sample : N2183-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 07:01:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

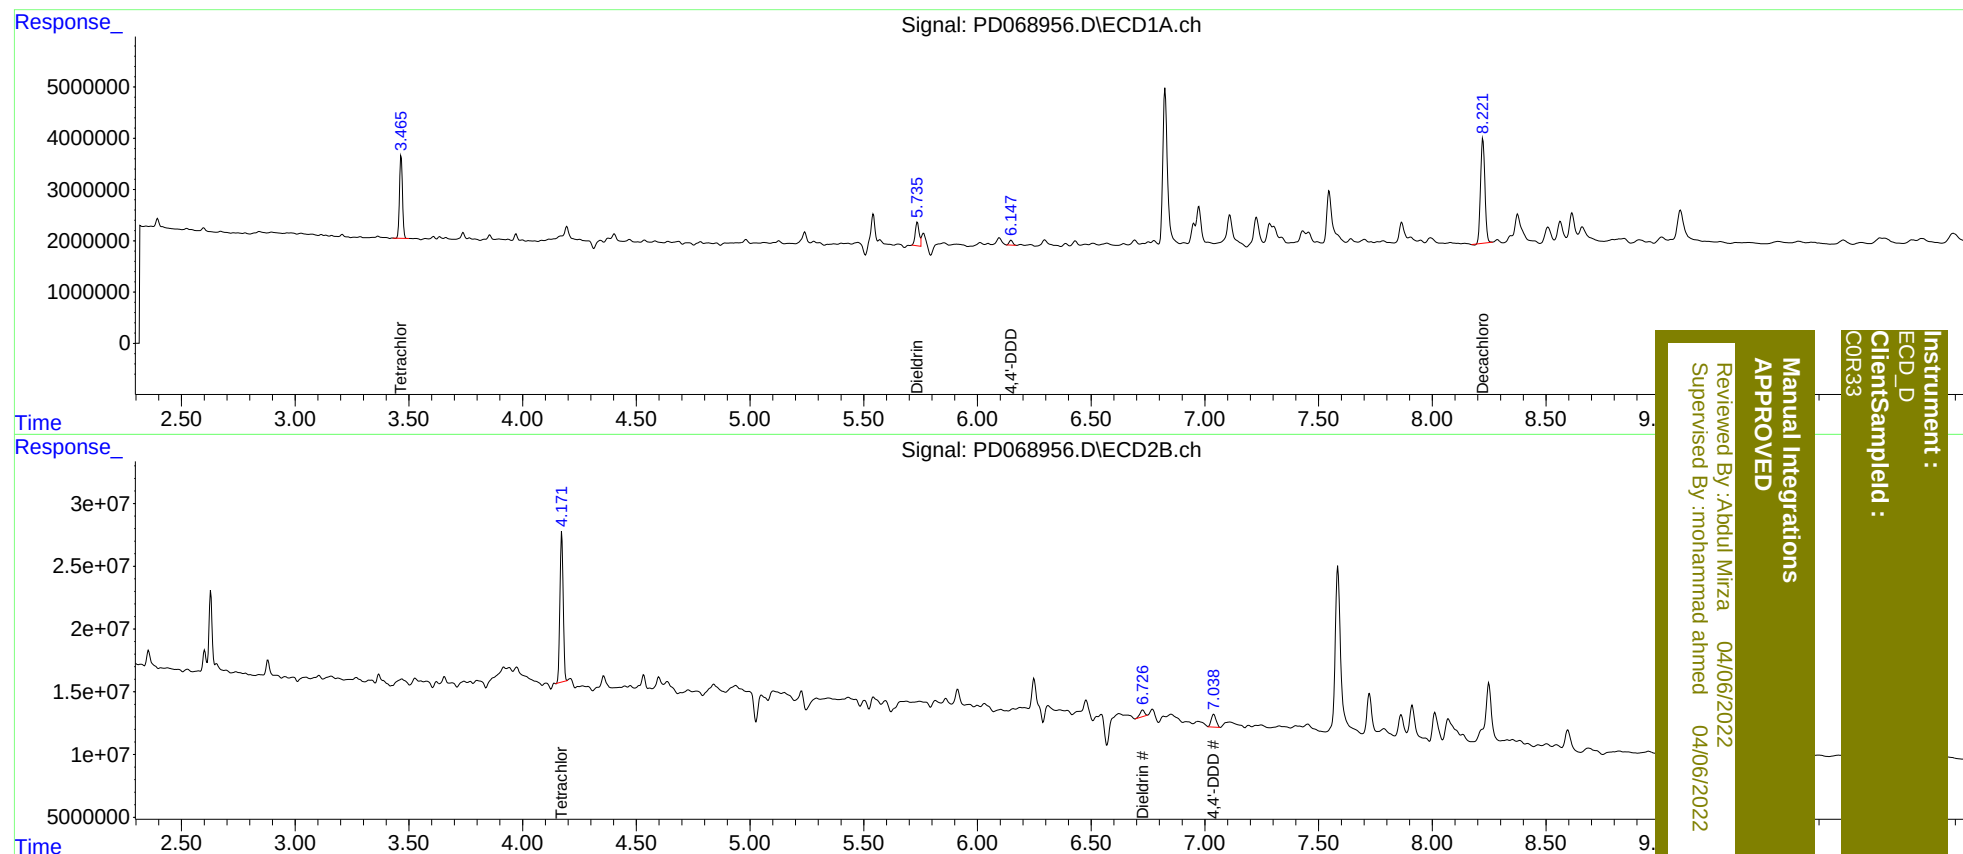

Reviewed By :Abdul Mirza 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COR33