

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
 Data File : PD074598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2023 11:03
 Operator : AR\AJ
 Sample : 02115-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9C7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2023
 Supervised By : Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 08:54:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.772	15588856	7762129	6.275	6.170
2)	SA Decachlor...	9.088	7.918	29984619	11298324	10.955m	9.436m
Target Compounds							
10)	B trans-Chl...	5.955	4.978	6139514	2554327	1.914m	1.651m
11)	B cis-Chlor...	6.039	5.042	7783856	1558572	2.375	0.985m#
13)	MA Dieldrin	6.362	5.363	11064673	7390845	3.488m	4.767m#
17)	MA 4,4'-DDT	7.039	6.036	3765735	2266909	1.501m	1.809m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
Data File : PD074598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2023 11:03
Operator : AR\AJ
Sample : 02115-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 08:54:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

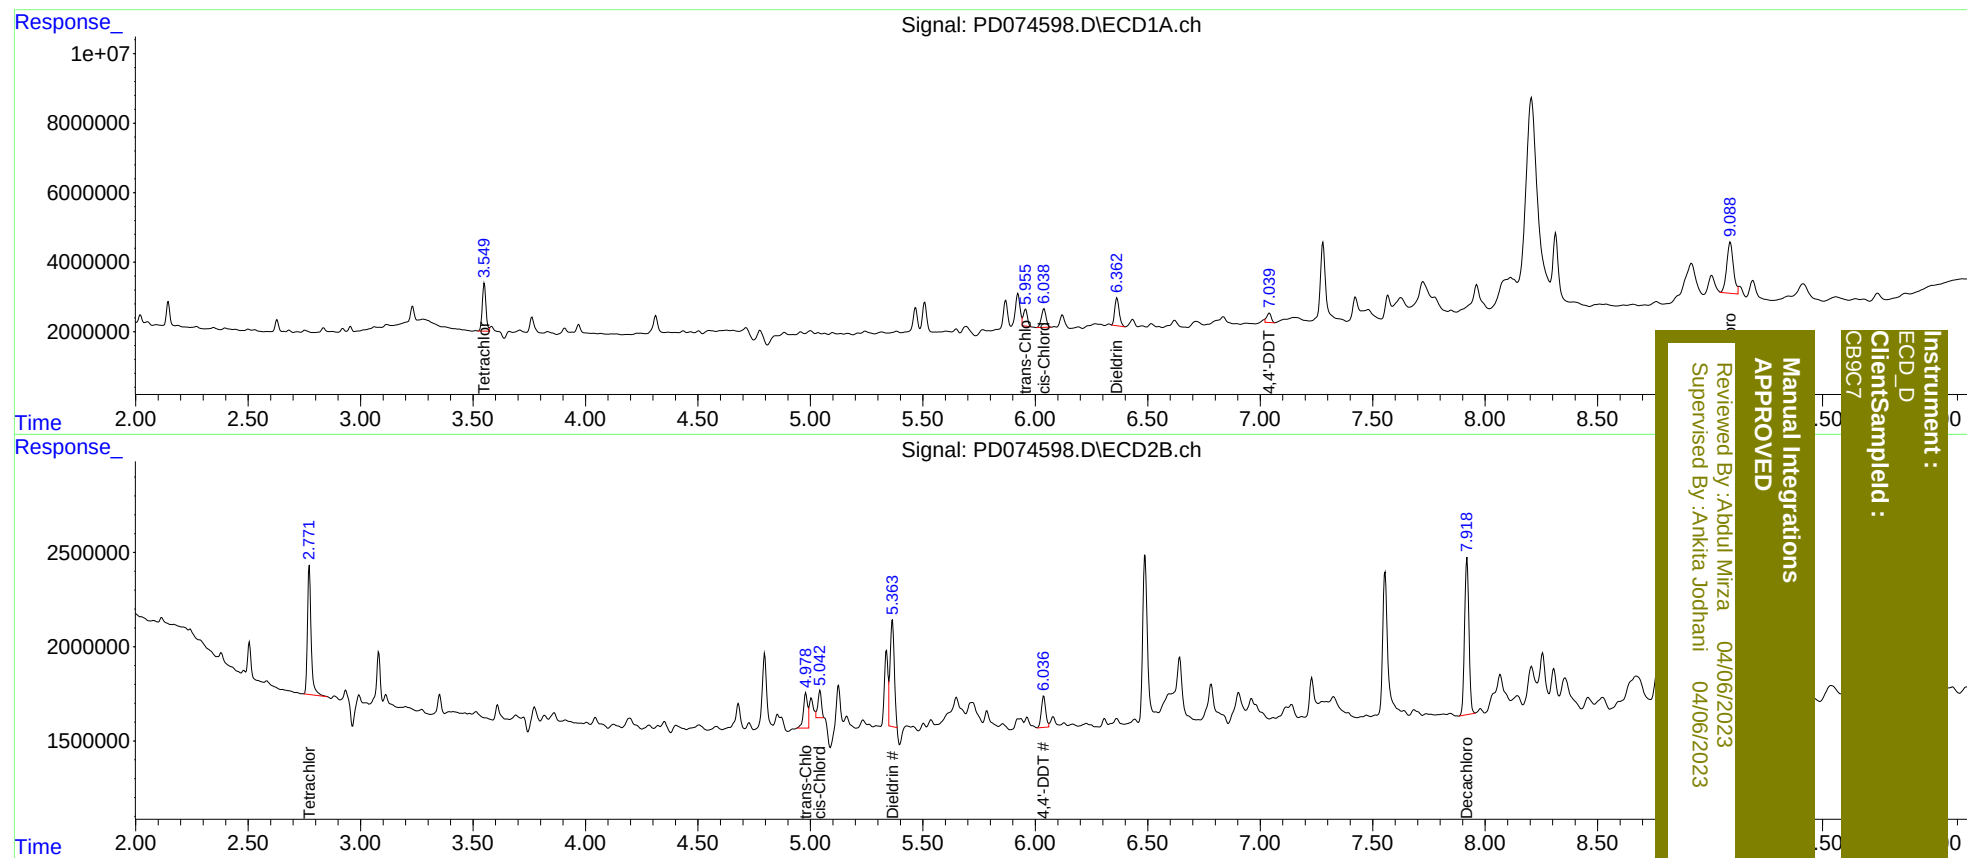

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/06/2023
Supervised By: Ankita Jodhani 04/06/2023

Instrument :
ECD_D
ClientSampled :
CB9C7