

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
 Data File : PD074599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2023 11:17
 Operator : AR\AJ
 Sample : 02115-06MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9C7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2023
 Supervised By : Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 22:26:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.772	14567957	7174831	5.864	5.703
27)	SA Decachlor...	9.090	7.919	25998676	10702105	9.499	8.938
Target Compounds							
2)	A alpha-BHC	4.006	3.274	135.6E6	59224134	34.741	33.140
3)	MA gamma-BHC...	4.339	3.604	124.2E6	54987823	33.637	32.194
4)	MA Heptachlor	4.931	3.946	127.3E6	53464417	33.627	32.245
5)	MB Aldrin	5.275	4.226	127.1E6	56509440	34.770	33.005
6)	B beta-BHC	4.534	3.899	50377059	24930871	29.799	30.773
7)	B delta-BHC	4.783	4.131	116.8E6	55686997	32.098	31.484
8)	B Heptachlo...	5.701	4.728	111.2E6	47853339	33.862	30.207
9)	A Endosulfan I	6.088	5.099	100.9E6	41869282	33.808	29.860
10)	B trans-Chl...	5.956	4.979	115.9E6	52151416	36.126m	33.711
11)	B cis-Chlor...	6.037	5.043	117.3E6	51648485	35.782	32.651
12)	B 4,4'-DDE	6.209	5.233	202.0E6	93834878	67.423	64.600
13)	MA Dieldrin	6.364	5.363	247.1E6	109.7E6	77.895	70.752m
14)	MA Endrin	6.594	5.639	196.2E6	90454808	74.451	67.238
15)	B Endosulfa...	6.813	5.933	193.1E6	84721261	69.967	63.014
16)	A 4,4'-DDD	6.727	5.787	177.1E6	76911027	74.954	65.322
17)	MA 4,4'-DDT	7.042	6.039	196.4E6	83182409	78.266	66.398
18)	B Endrin al...	6.943	6.112	140.3E6	62517778	62.305	56.871
19)	B Endosulfa...	7.178	6.335	178.7E6	77449126	68.624	61.527
20)	A Methoxychlor	7.518	6.615	506.2E6	204.0E6	368.712	331.589
21)	B Endrin ke...	7.664	6.841	205.8E6	93133798	69.408	61.207

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
Data File : PD074599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2023 11:17
Operator : AR\AJ
Sample : 02115-06MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 22:26:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

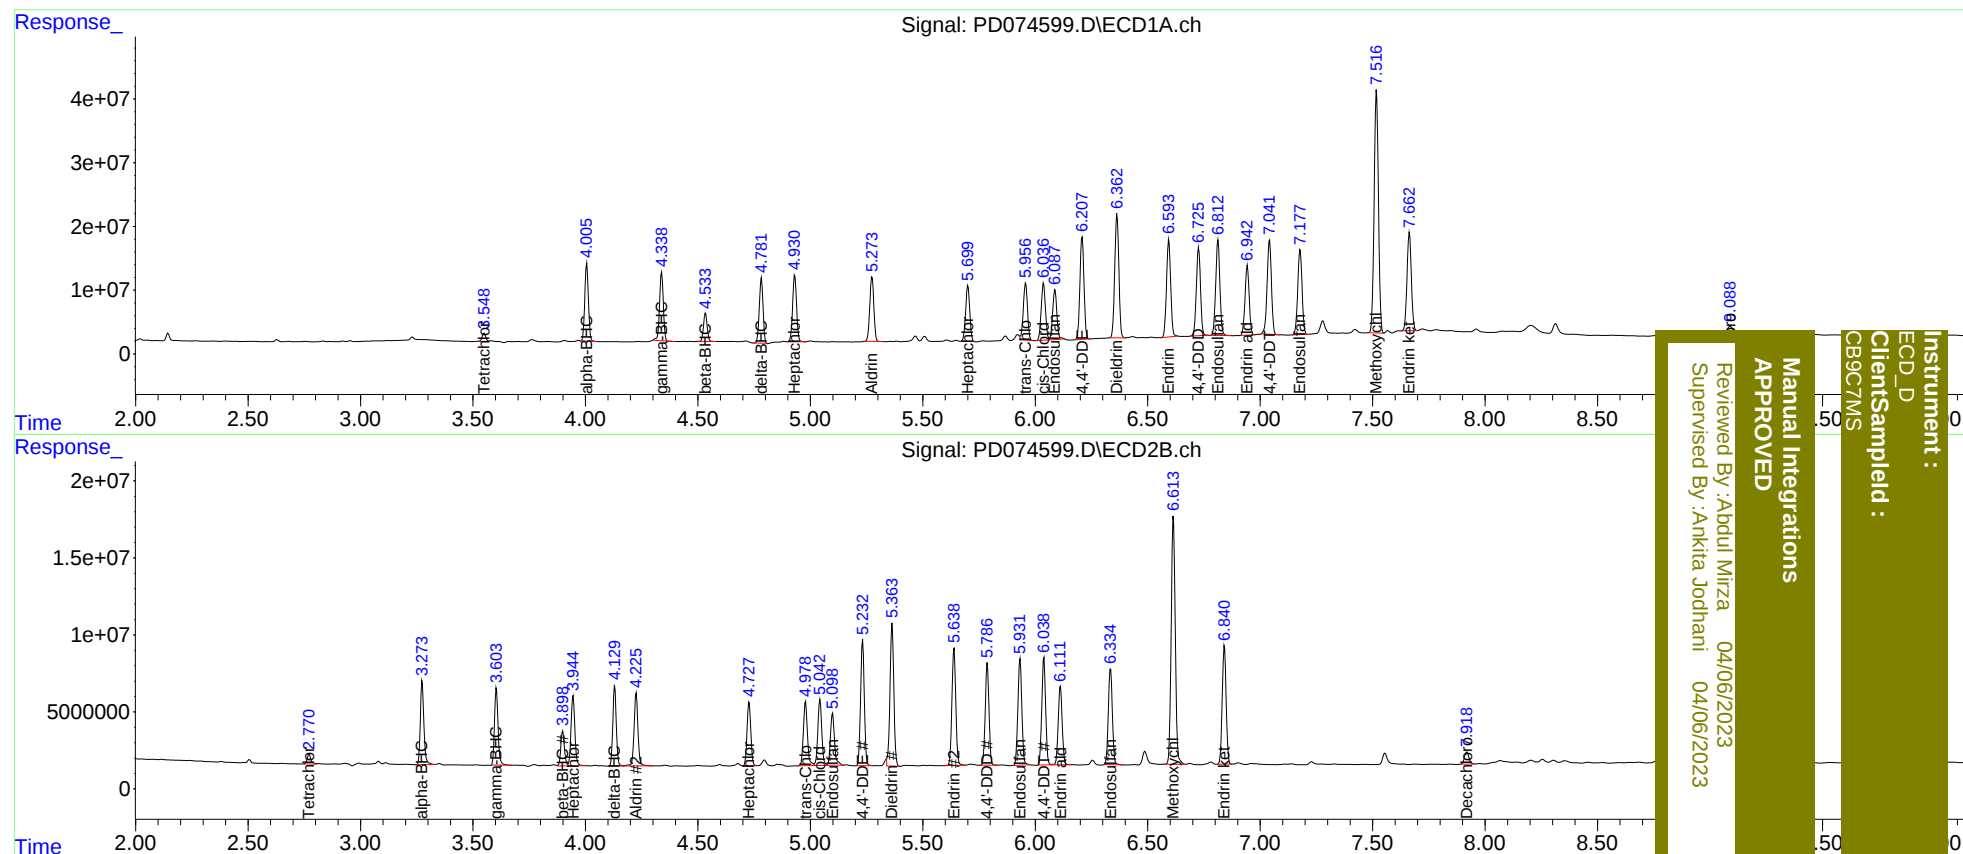

Reviewed By: Abdul Mirza 04/06/2023
Supervised By: Ankita Jodhani 04/06/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CB9C7MS