

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
 Data File : PD074600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2023 11:30
 Operator : AR\AJ
 Sample : 02115-07MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9C7MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/06/2023
 Supervised By : Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 22:27:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.772	14316501	7031922	5.763	5.589
27)	SA Decachlor...	9.090	7.919	25574395	10370322	9.344	8.661
Target Compounds							
2)	A alpha-BHC	4.007	3.275	133.3E6	58275393	34.151	32.609
3)	MA gamma-BHC...	4.340	3.605	122.6E6	54566144	33.204	31.947
4)	MA Heptachlor	4.932	3.946	126.2E6	52798191	33.325	31.843
5)	MB Aldrin	5.275	4.226	125.9E6	55812463	34.446	32.598
6)	B beta-BHC	4.535	3.900	49746557	24538943	29.426	30.289
7)	B delta-BHC	4.783	4.131	114.7E6	54966749	31.507	31.077
8)	B Heptachlo...	5.701	4.728	110.7E6	47120145	33.711	29.744
9)	A Endosulfan I	6.088	5.099	99296109	41438692	33.286	29.553
10)	B trans-Chl...	5.957	4.979	114.4E6	51426296	35.656m	33.242
11)	B cis-Chlor...	6.038	5.043	116.2E6	51012999	35.467	32.249
12)	B 4,4'-DDE	6.209	5.233	200.1E6	92426273	66.795	63.630
13)	MA Dieldrin	6.365	5.363	245.8E6	108.4E6	77.476	69.901m
14)	MA Endrin	6.595	5.639	195.1E6	89350270	74.035	66.417
15)	B Endosulfa...	6.813	5.933	192.6E6	83832051	69.784	62.353
16)	A 4,4'-DDD	6.727	5.787	174.3E6	75956421	73.773	64.512
17)	MA 4,4'-DDT	7.042	6.037	193.3E6	82038306	77.032	65.484m
18)	B Endrin al...	6.943	6.113	139.4E6	61462577	61.877	55.911
19)	B Endosulfa...	7.178	6.335	177.5E6	76943433	68.136	61.125
20)	A Methoxychlor	7.518	6.615	503.4E6	202.8E6	366.669	329.730
21)	B Endrin ke...	7.664	6.842	204.6E6	92174173	69.006	60.576

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040523\
Data File : PD074600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2023 11:30
Operator : AR\AJ
Sample : 02115-07MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 22:27:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

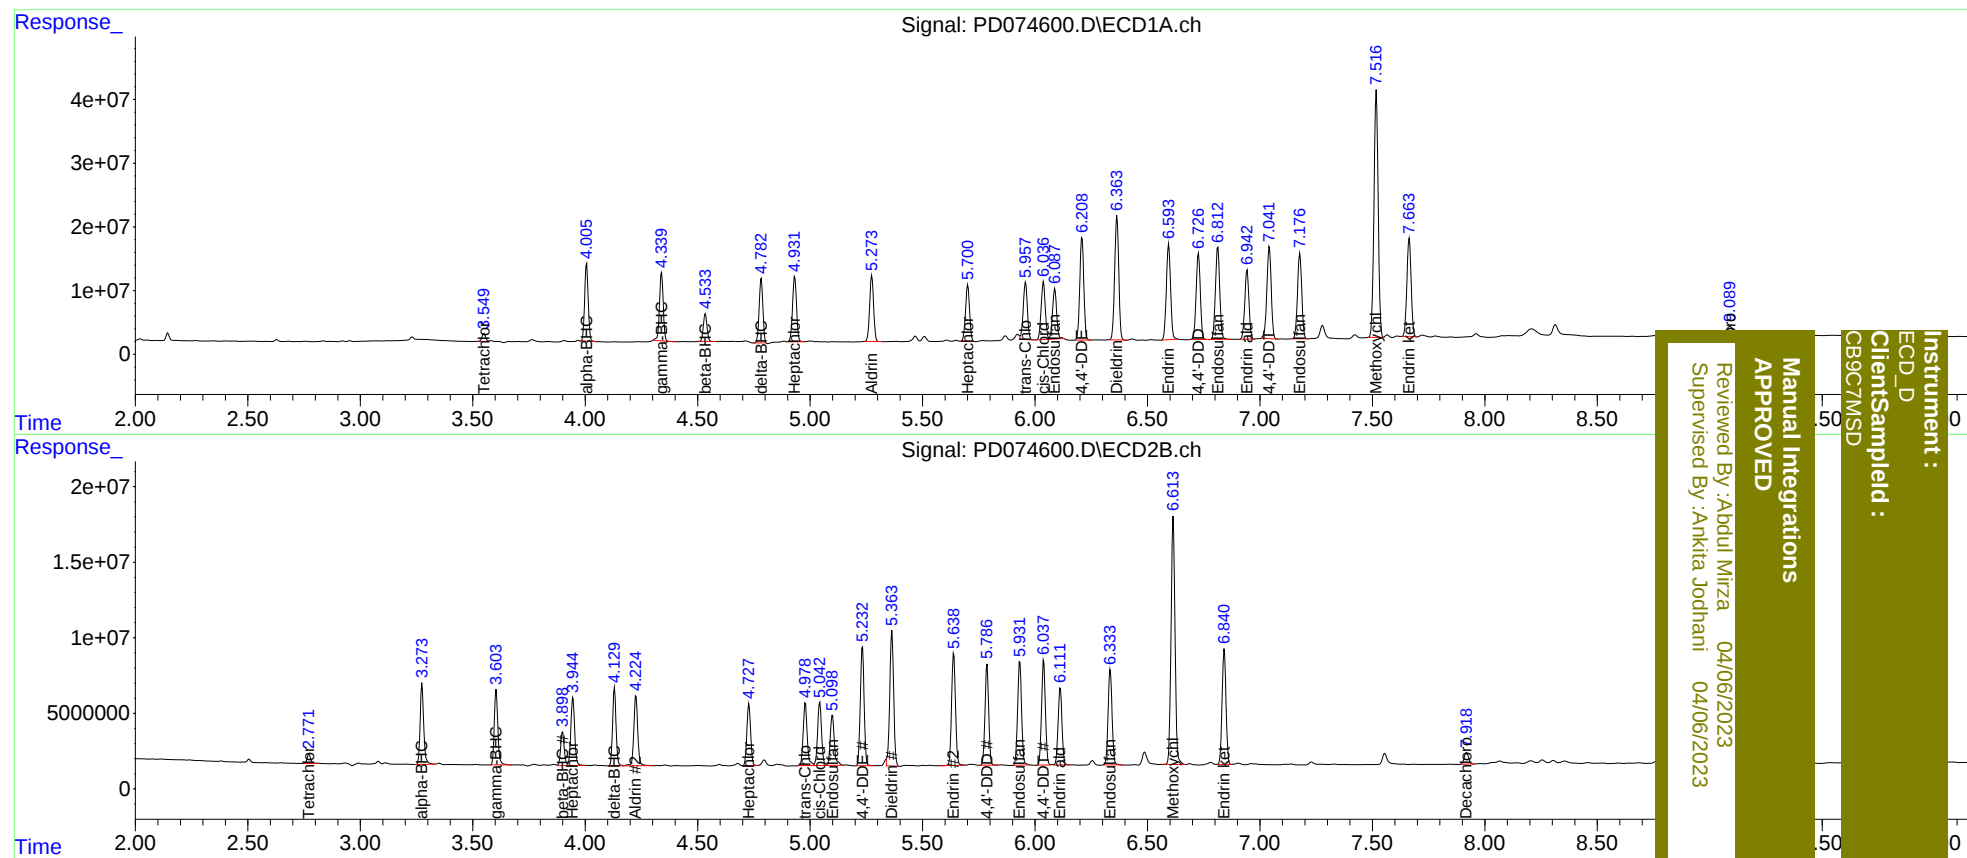

Instrument :
ECD_D
ClientSampled :
CB9C7MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023