

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040623\
 Data File : PD074609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2023 10:45
 Operator : AR\AJ
 Sample : 02115-06MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9C7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/07/2023
 Supervised By : Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 00:55:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.770	18899967	8779114	7.607	6.978
27)	SA Decachlor...	9.098	7.921	31245043	13947750	11.416	11.648
Target Compounds							
2)	A alpha-BHC	4.011	3.273	122.5E6	54173376	31.392m	30.314
3)	MA gamma-BHC...	4.346	3.603	114.5E6	50721835	31.007	29.696
4)	MA Heptachlor	4.937	3.945	115.8E6	49121480	30.597	29.625
5)	MB Aldrin	5.281	4.225	115.9E6	51797458	31.715	30.253
6)	B beta-BHC	4.540	3.899	45997851	22894154	27.209	28.259
7)	B delta-BHC	4.788	4.130	106.0E6	50632743	29.138m	28.626
8)	B Heptachlo...	5.707	4.728	94261767	43808408	28.711	27.654
9)	A Endosulfan I	6.094	5.099	87938869	38927911	29.478	27.763
10)	B trans-Chl...	5.962	4.979	106.4E6	47921750	33.172m	30.977
11)	B cis-Chlor...	6.044	5.043	106.1E6	47575115	32.374	30.076
12)	B 4,4'-DDE	6.215	5.233	184.4E6	85724210	61.558	59.016
13)	MA Dieldrin	6.370	5.363	226.2E6	99156154	71.292	63.960m
14)	MA Endrin	6.600	5.639	177.0E6	82585657	67.174	61.389
15)	B Endosulfa...	6.819	5.933	176.5E6	77876972	63.939	57.924
16)	A 4,4'-DDD	6.733	5.788	160.5E6	70641833	67.893	59.998
17)	MA 4,4'-DDT	7.048	6.039	178.5E6	76294317	71.119	60.900
18)	B Endrin al...	6.949	6.112	128.5E6	57918286	57.049	52.687
19)	B Endosulfa...	7.184	6.335	162.6E6	71939642	62.432	57.150
20)	A Methoxychlor	7.524	6.615	459.4E6	186.9E6	334.643	303.782
21)	B Endrin ke...	7.670	6.843	189.2E6	86293828	63.807	56.712

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040623\
Data File : PD074609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2023 10:45
Operator : AR\AJ
Sample : 02115-06MS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 00:55:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

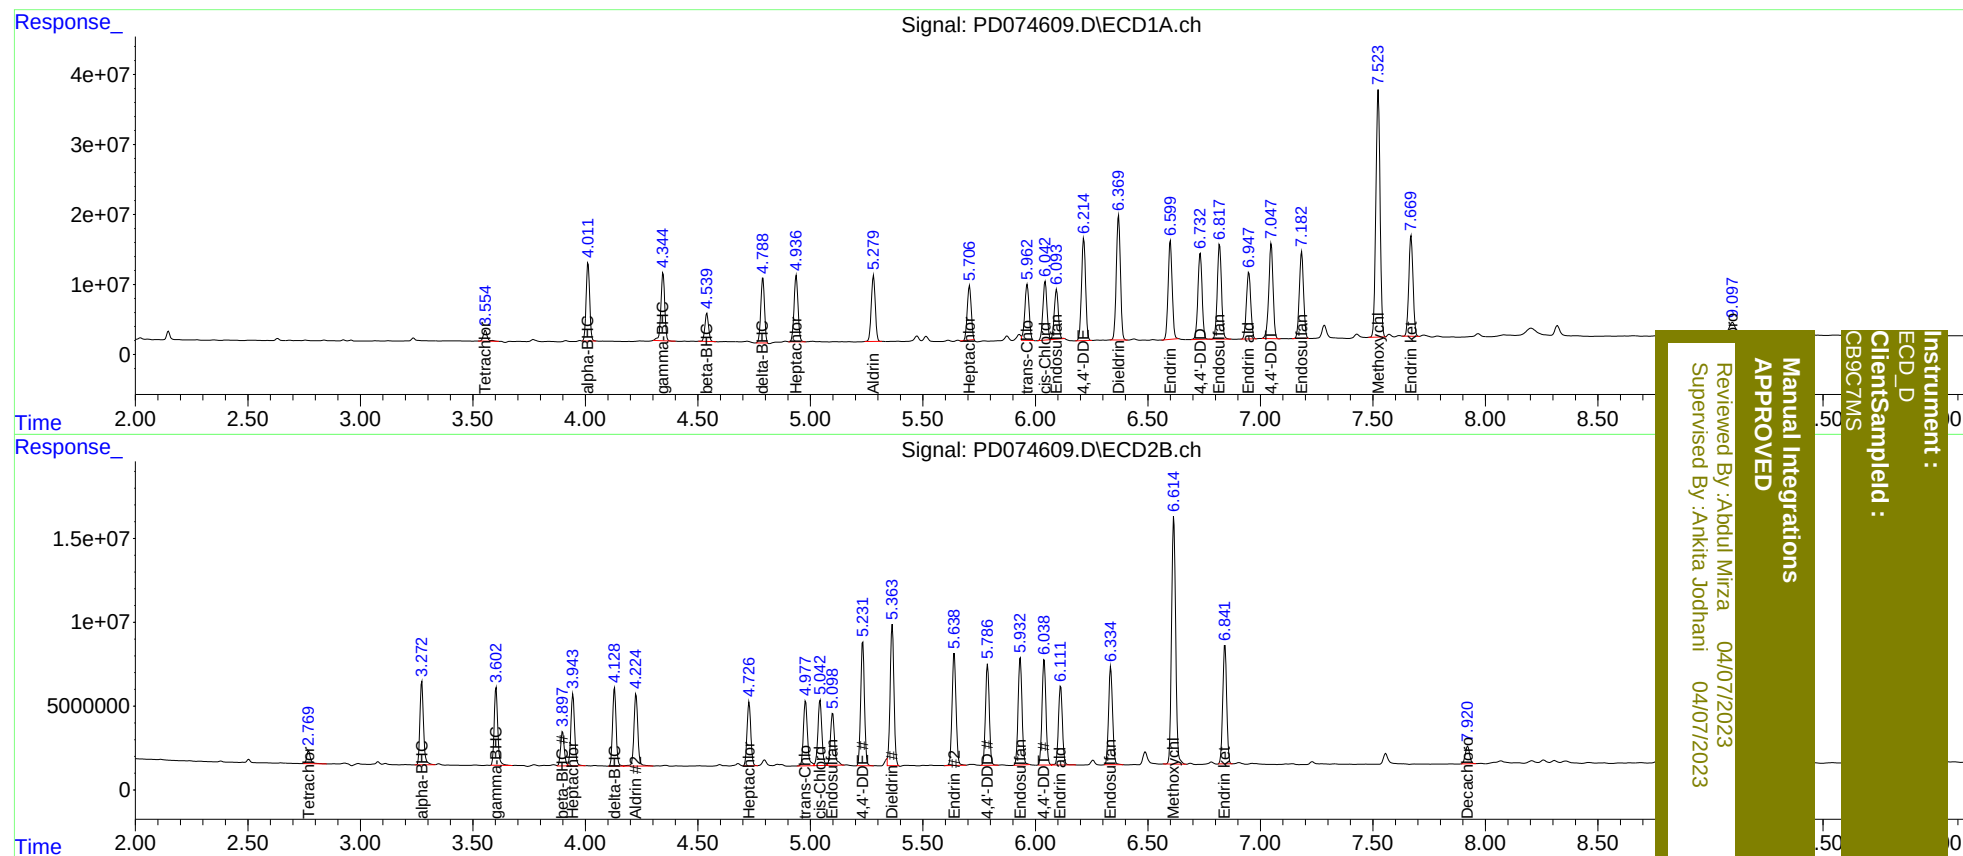

Instrument :
ECD_D
ClientSampled :
CB9C7MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/07/2023
Supervised By: Ankita Jodhani 04/07/2023