

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040623\
 Data File : PD074610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2023 11:00
 Operator : AR\AJ
 Sample : 02115-07MSD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9C7MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 00:56:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.771	19010134	8795987	7.652	6.991
27)	SA Decachlor...	9.094	7.921	31981559	13769345	11.685	11.499
Target Compounds							
2)	A alpha-BHC	4.008	3.274	123.3E6	53699873	31.596m	30.049
3)	MA gamma-BHC...	4.341	3.604	113.4E6	50601697	30.716m	29.626
4)	MA Heptachlor	4.934	3.946	116.6E6	48739686	30.807	29.395
5)	MB Aldrin	5.277	4.226	116.0E6	51711831	31.734	30.203
6)	B beta-BHC	4.537	3.900	46125924	22788171	27.285	28.128
7)	B delta-BHC	4.785	4.130	105.4E6	50488786	28.963m	28.545
8)	B Heptachlo...	5.704	4.728	99831917	43535363	30.407	27.481
9)	A Endosulfan I	6.091	5.099	91234290	38392437	30.583	27.381
10)	B trans-Chl...	5.959	4.979	107.0E6	47484735	33.353m	30.694
11)	B cis-Chlor...	6.041	5.043	107.0E6	47121425	32.663	29.789
12)	B 4,4'-DDE	6.212	5.234	185.0E6	84950681	61.769	58.484
13)	MA Dieldrin	6.367	5.363	225.8E6	98857549	71.172	63.767m
14)	MA Endrin	6.597	5.639	178.4E6	82011787	67.698	60.962
15)	B Endosulfa...	6.816	5.933	177.1E6	77138223	64.162	57.374
16)	A 4,4'-DDD	6.730	5.787	160.9E6	70127784	68.098	59.561
17)	MA 4,4'-DDT	7.045	6.037	178.7E6	75006689	71.216	59.872m
18)	B Endrin al...	6.946	6.112	128.5E6	56618378	57.063	51.505
19)	B Endosulfa...	7.180	6.335	163.2E6	71007648	62.675	56.409
20)	A Methoxychlor	7.520	6.615	458.9E6	186.5E6	334.288	303.216
21)	B Endrin ke...	7.666	6.842	188.2E6	85291270	63.483	56.053

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040623\
Data File : PD074610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2023 11:00
Operator : AR\AJ
Sample : 02115-07MSD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 00:56:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

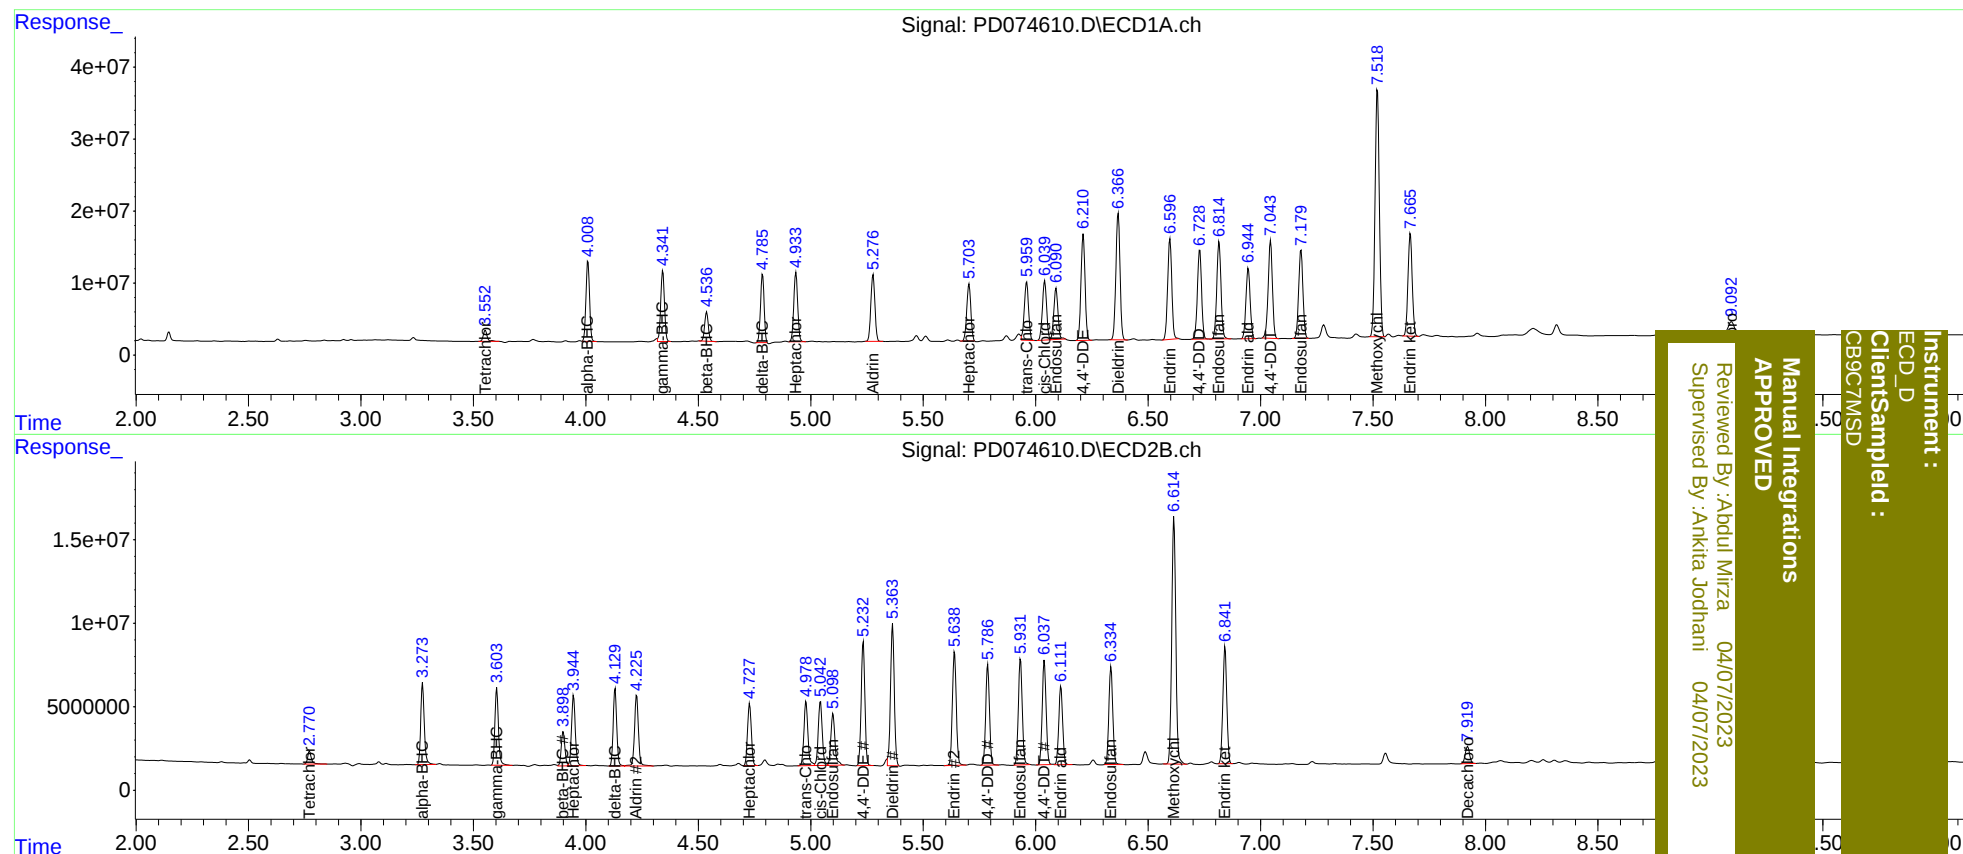

Instrument :
ECD_D
ClientSampled :
CB9C7MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/07/2023
Supervised By: Ankita Jodhani 04/07/2023