

Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
 Data File : PD046827.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2018 3:36
 Operator : UA/AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:30:59 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 07 04:23:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.431	4.042	137.2E6	1980.0E6	101.923	97.723
28) SA Decachlor...	8.156	9.121	132.7E6	1606.6E6	99.855	96.699
Target Compounds						
23) Chlordane-1	4.292	5.043	61286051	1066.8E6	1003.683	980.773
24) Chlordane-2	4.789	5.509	61241113	989.9E6	994.802	961.136
25) Chlordane-3	5.352	6.154	200.7E6	3289.3E6	1015.944	978.129
26) Chlordane-4	5.410	6.230	171.2E6	3719.3E6	1010.509	975.814
27) Chlordane-5	6.243	7.030	60711404	815.7E6	1004.606	978.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
Data File : PD046827.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2018 3:36
Operator : UA/AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:30:59 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
Quant Title : GC Extractables
QLast Update : Sat Apr 07 04:23:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

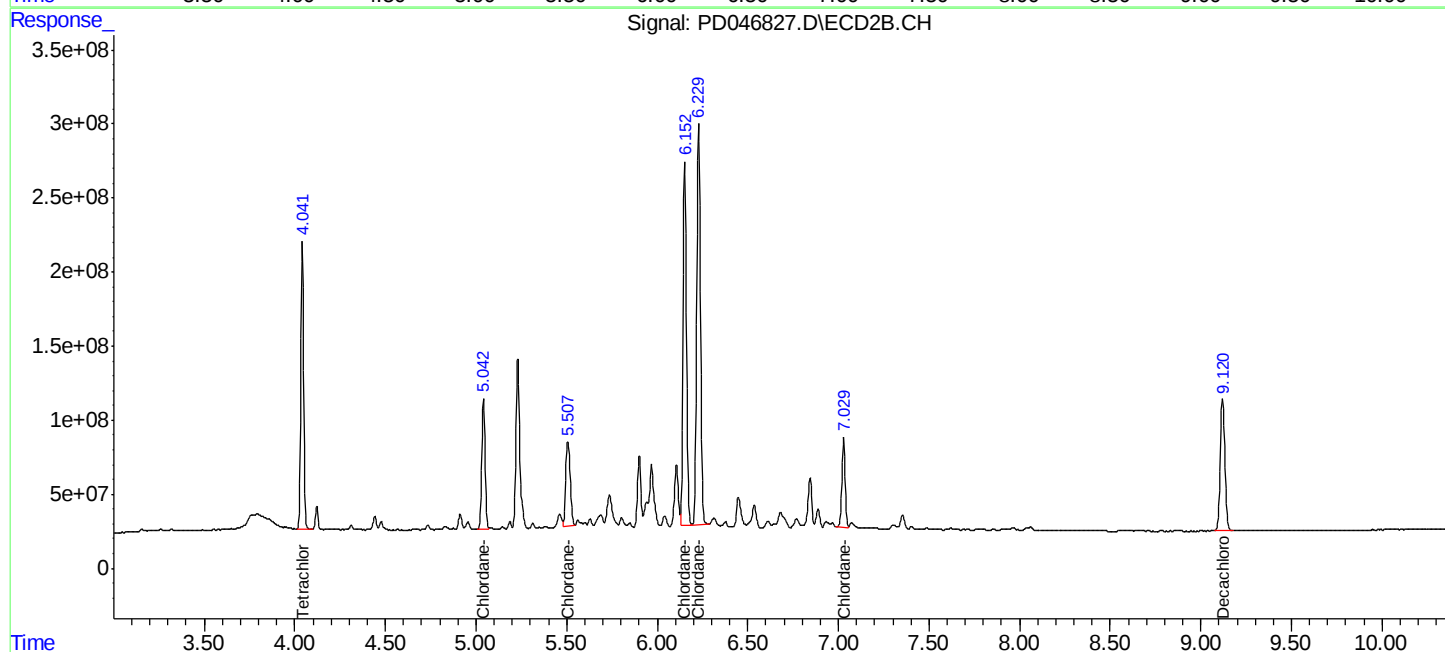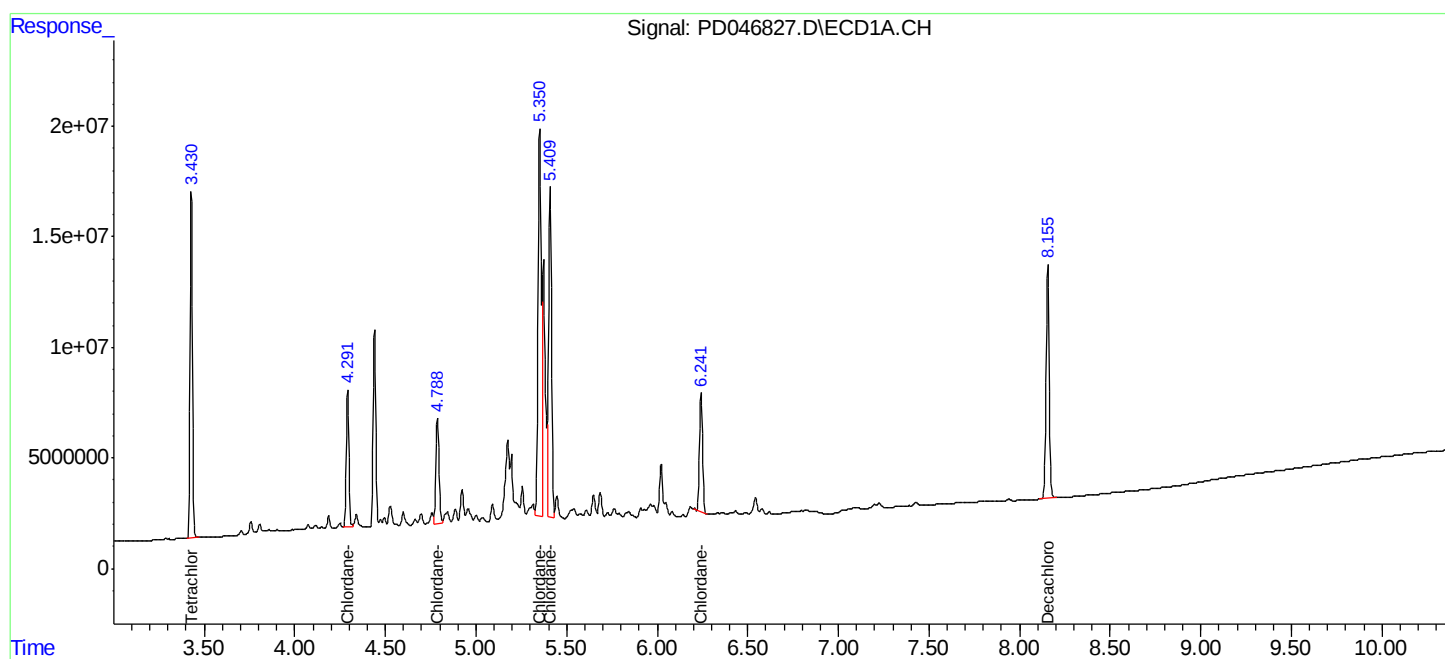


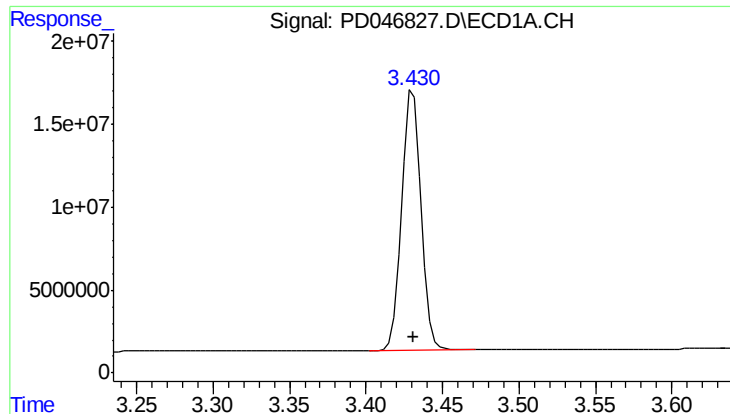

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 137249401
Conc: 101.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

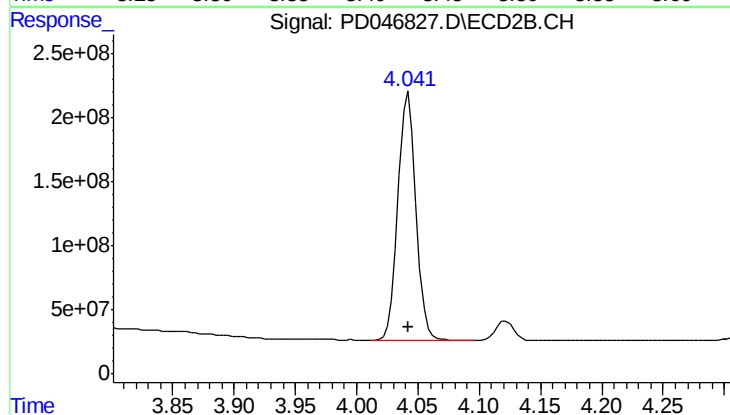


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 1979964087
Conc: 97.72 ng/ml

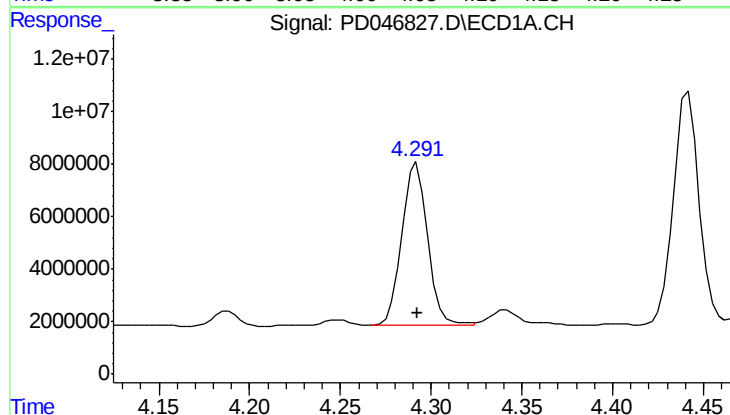


#23 Chlordane-1

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 61286051
Conc: 1003.68 ng/ml

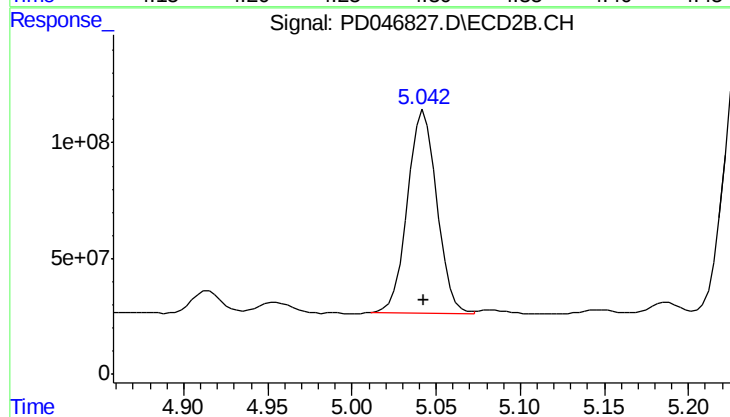

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 1066844763
Conc: 980.77 ng/ml

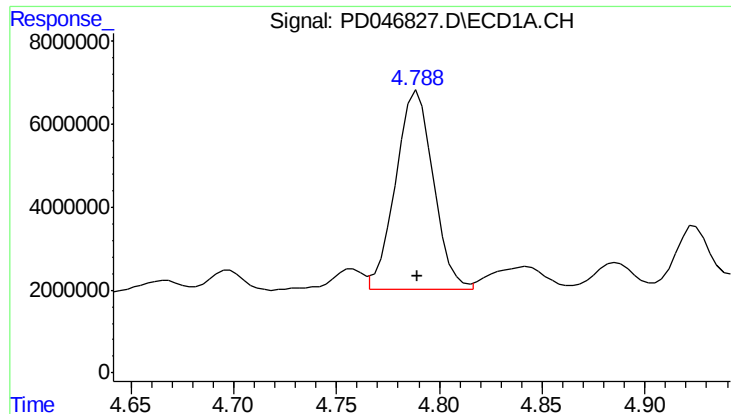

#24 Chlordane-2


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 61241113
Conc: 994.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

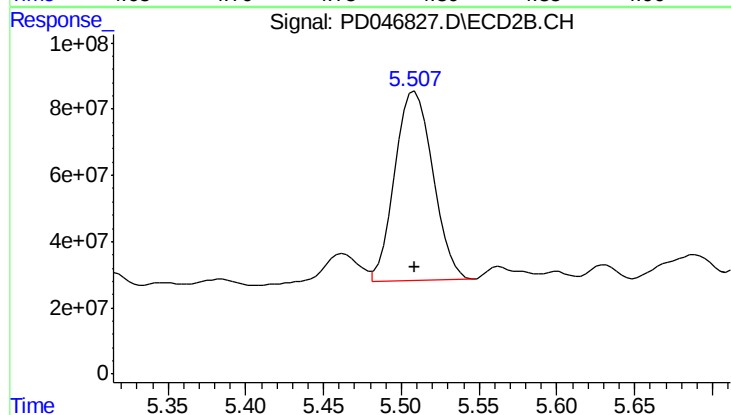


#24 Chlordane-2

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 989927261
Conc: 961.14 ng/ml

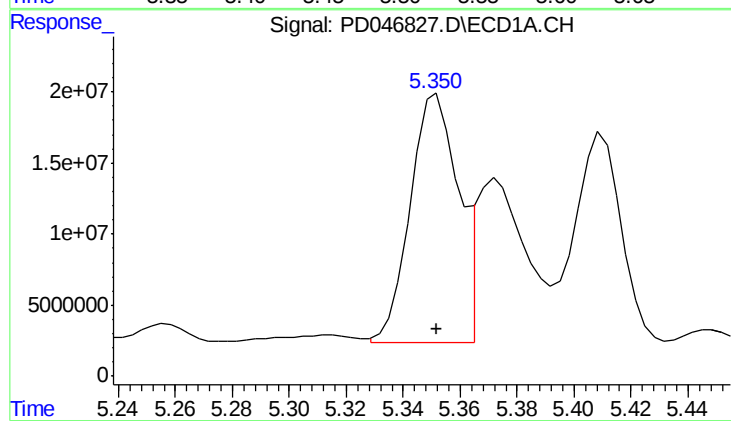


#25 Chlordane-3

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 200722198
Conc: 1015.94 ng/ml

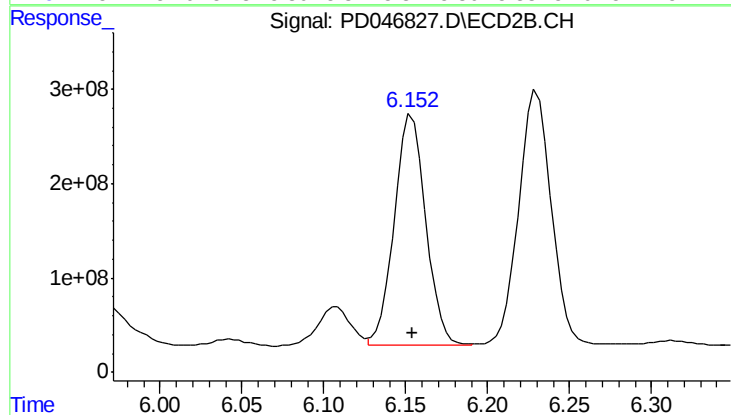

#25 Chlordane-3


R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 3289265472
Conc: 978.13 ng/ml

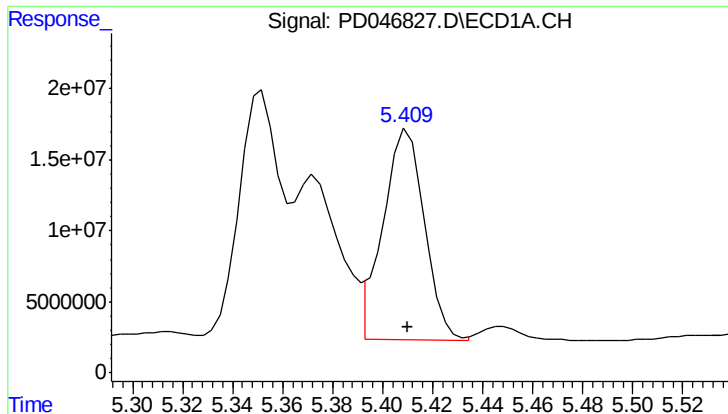

#26 Chlordane-4


R.T.: 5.410 min
Delta R.T.: 0.000 min
Response: 171195346
Conc: 1010.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

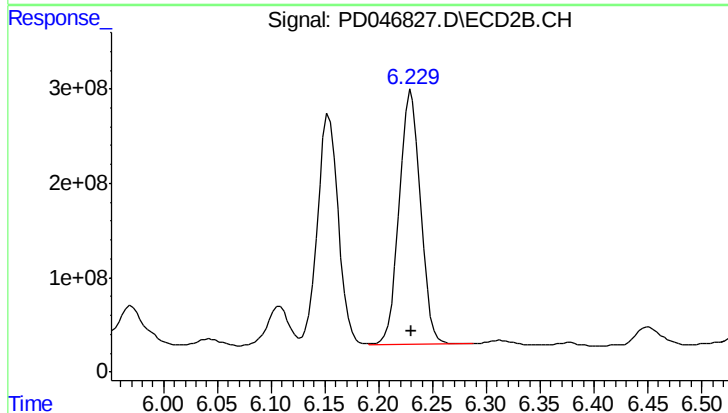


#26 Chlordane-4

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 3719348404
Conc: 975.81 ng/ml

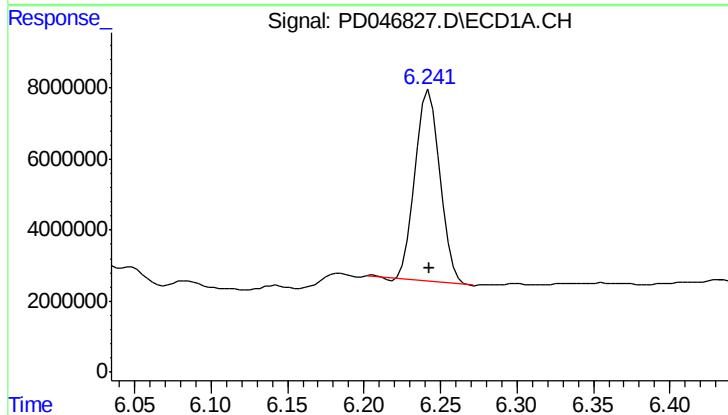


#27 Chlordane-5

R.T.: 6.243 min
Delta R.T.: 0.000 min
Response: 60711404
Conc: 1004.61 ng/ml

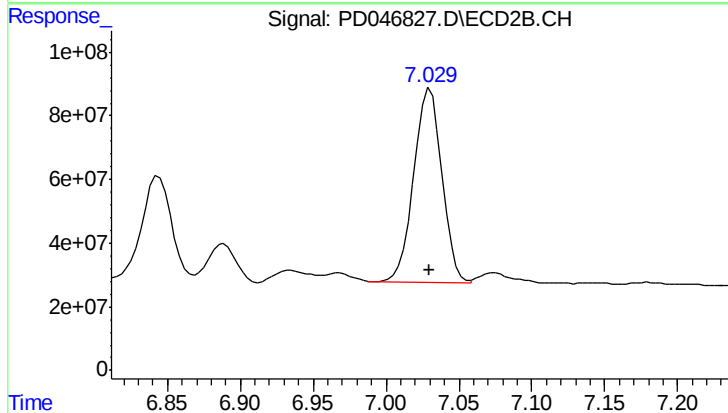

#27 Chlordane-5


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 815735154
Conc: 978.11 ng/ml

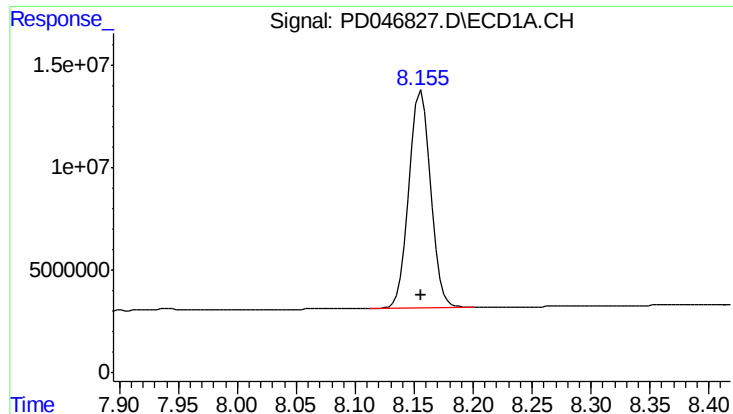

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.000 min
Response: 132669031
Conc: 99.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

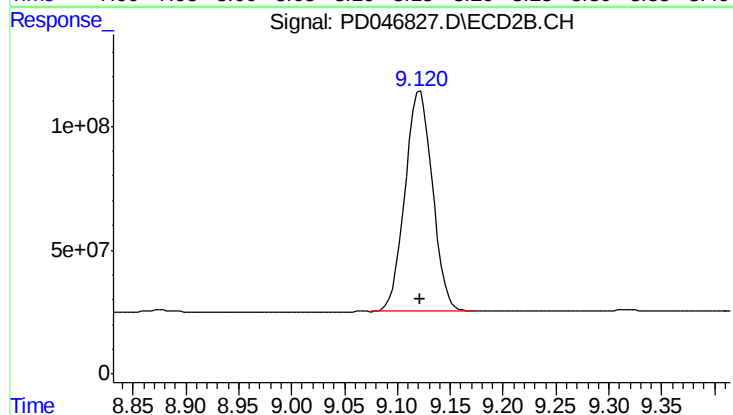

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 1606618502
Conc: 96.70 ng/ml