

Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
 Data File : PD046834.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2018 5:19
 Operator : UA/AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD040718CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 05:32:43 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 07 04:44:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	4.042	64709400	1012.9E6	51.276	47.404
28)	SA Decachlor...	8.156	9.121	65557867	851.7E6	48.731	47.340
Target Compounds							
23)	Chlordane-1	4.292	5.043	29805469	539.7E6	484.166	465.342
24)	Chlordane-2	4.789	5.509	30356575	519.9E6	492.037	471.647
25)	Chlordane-3	5.352	6.153	93546238	1671.1E6	497.599	475.255
26)	Chlordane-4	5.410	6.230	81562893	1897.7E6	492.013	471.495
27)	Chlordane-5	6.242	7.029	29305657	416.3E6	480.439	487.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
Data File : PD046834.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2018 5:19
Operator : UA/AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD040718CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 05:32:43 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
Quant Title : GC Extractables
QLast Update : Sat Apr 07 04:44:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

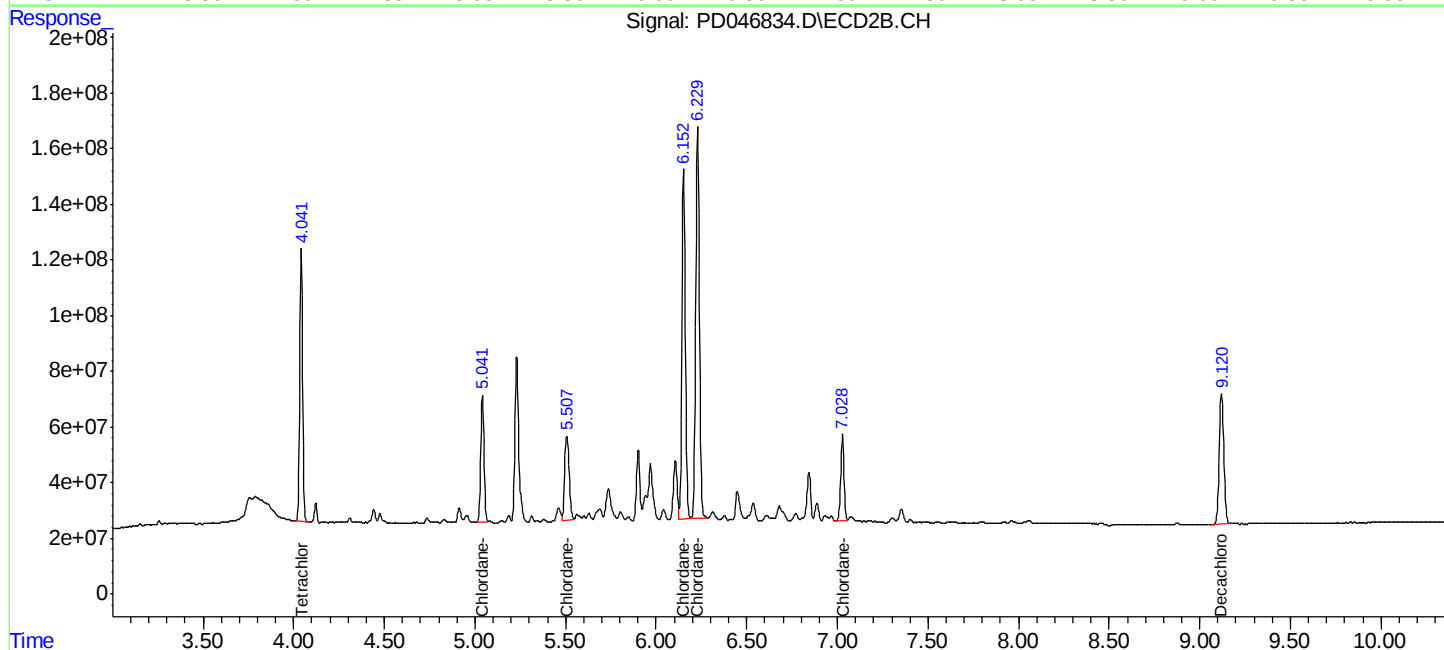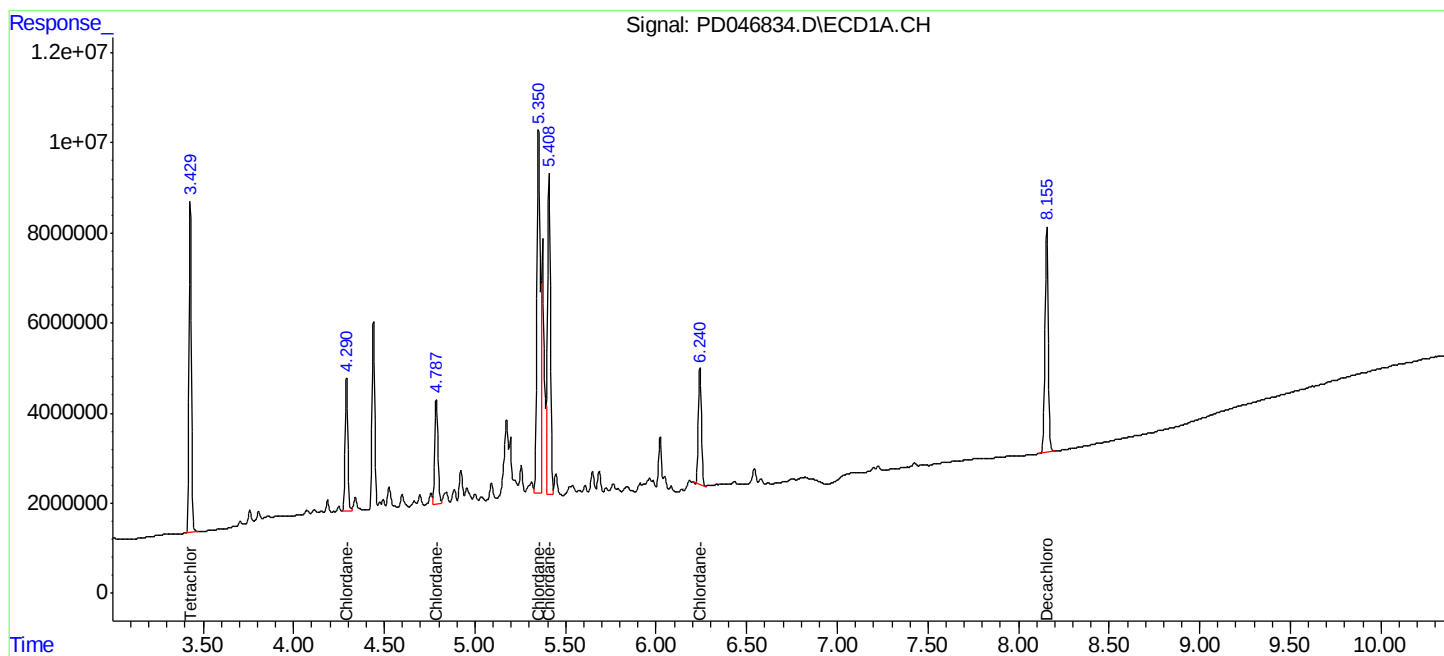


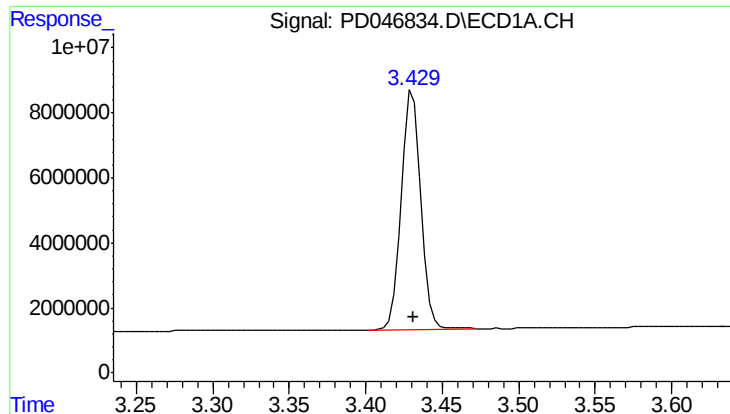

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 64709400
Conc: 51.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD040718CHLOR

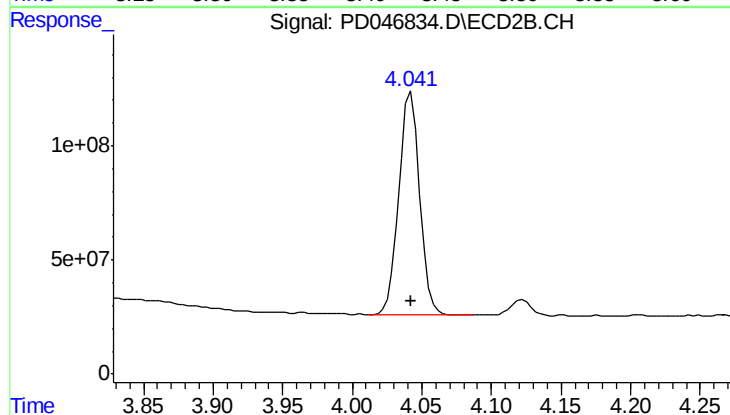


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 1012874270
Conc: 47.40 ng/ml

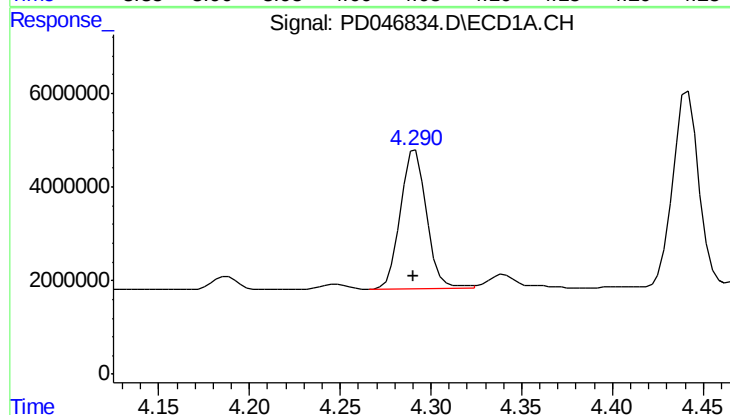


#23 Chlordane-1

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 29805469
Conc: 484.17 ng/ml

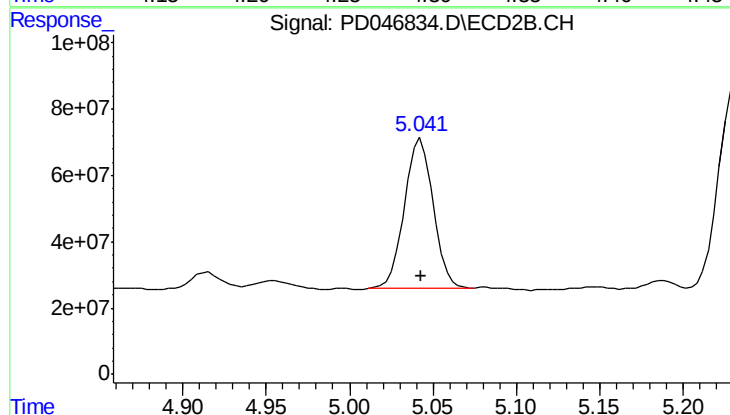

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 539678655
Conc: 465.34 ng/ml

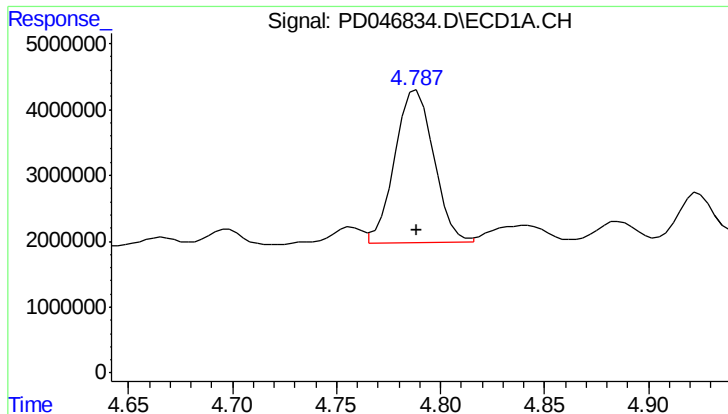

#24 Chlordane-2


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 30356575
Conc: 492.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD040718CHLOR

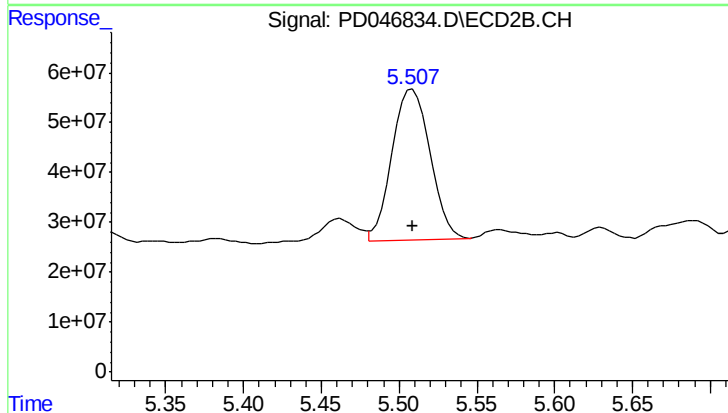


#24 Chlordane-2

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 519873456
Conc: 471.65 ng/ml

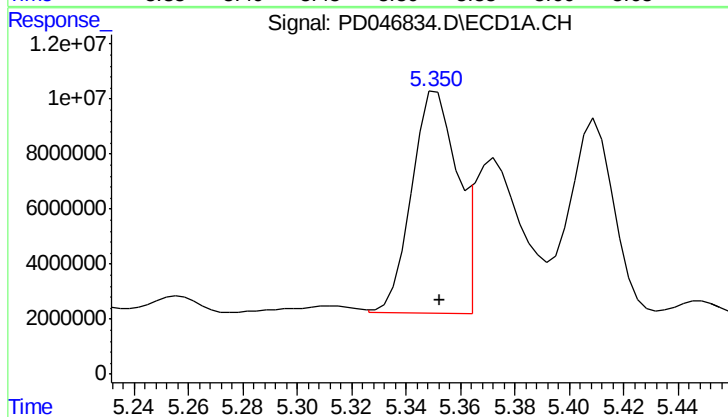


#25 Chlordane-3

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 93546238
Conc: 497.60 ng/ml

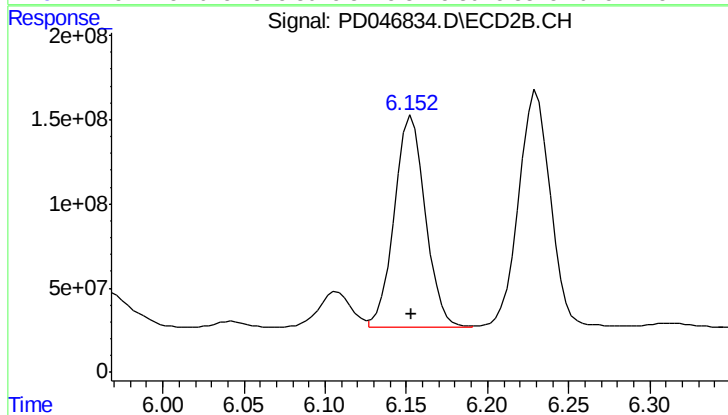

#25 Chlordane-3


R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 1671129318
Conc: 475.26 ng/ml

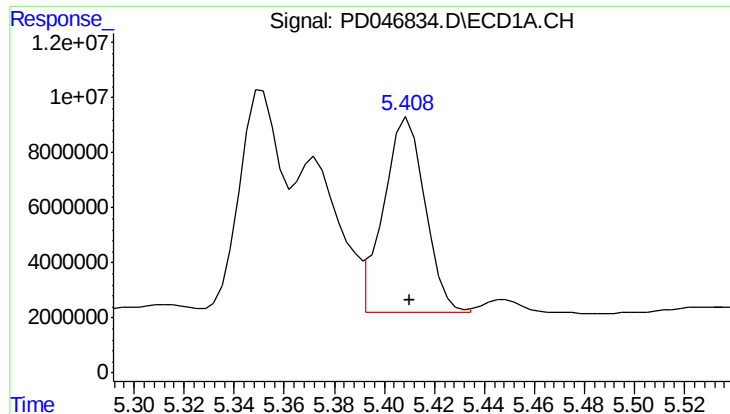

#26 Chlordane-4


R.T.: 5.410 min
Delta R.T.: 0.000 min
Response: 81562893
Conc: 492.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD040718CHLOR

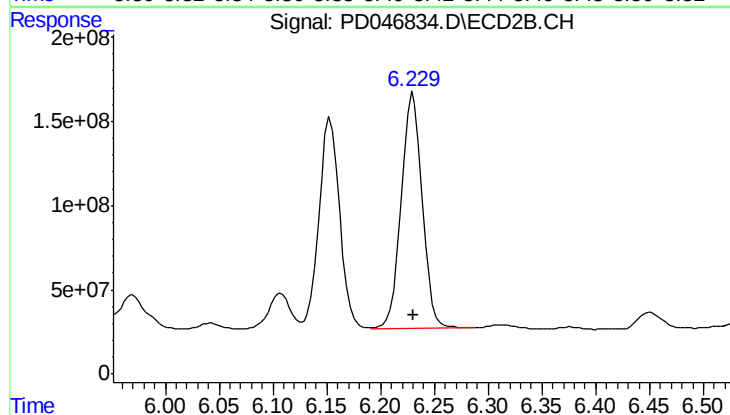


#26 Chlordane-4

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 1897686886
Conc: 471.50 ng/ml

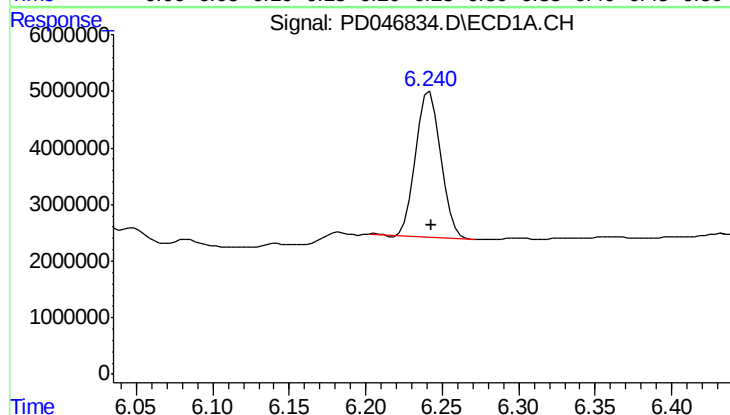


#27 Chlordane-5

R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 29305657
Conc: 480.44 ng/ml

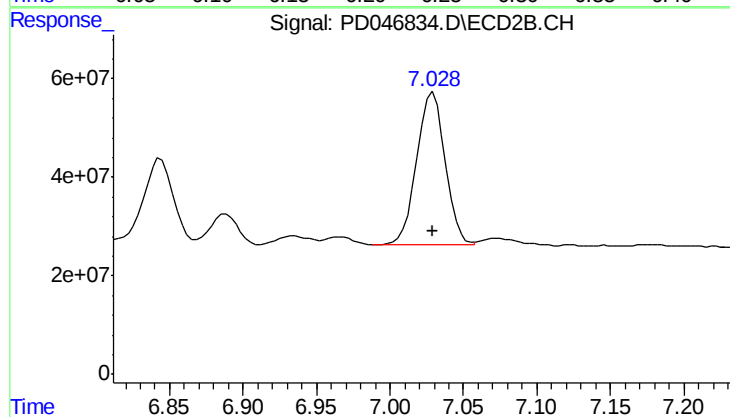

#27 Chlordane-5


R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 416318593
Conc: 487.59 ng/ml

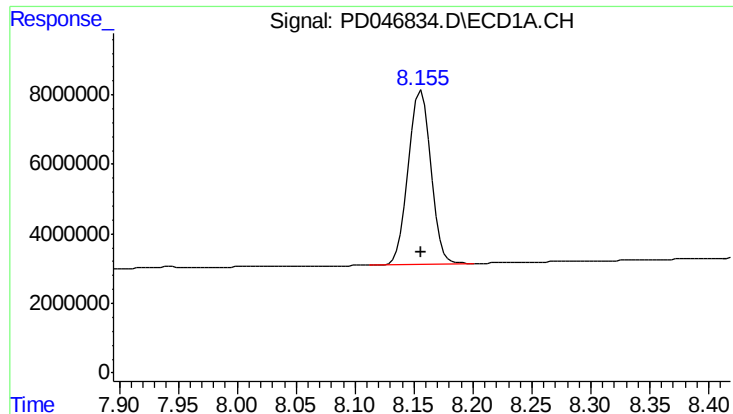

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.000 min
Response: 65557867
Conc: 48.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD040718CHLOR

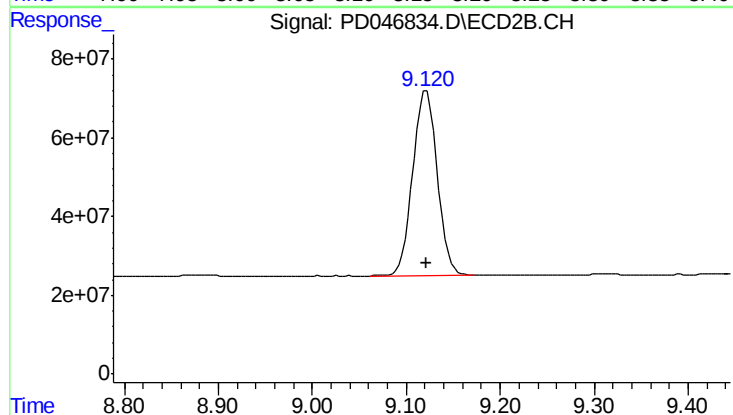

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 851745820
Conc: 47.34 ng/ml