

Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
 Data File : PD046850.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2018 10:43
 Operator : UA/AJ
 Sample : LOQ CHLOR
 Misc : ECD_D LOQ CHLOR WATER 200 PPB
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOQ CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 01:07:20 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 07 04:44:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	4.042	21541622	356.8E6	17.070	16.700
28)	SA Decachlor...	8.155	9.120	23454971	322.7E6	17.435	17.938
Target Compounds							
23)	Chlordane-1	4.291	5.042	10931661	207.7E6	177.576	179.054
24)	Chlordane-2	4.789	5.507	11110548	202.9E6	180.086	184.046
25)	Chlordane-3	5.351	6.153	33510463	621.4E6	178.252	176.734
26)	Chlordane-4	5.409	6.230	29378077	711.2E6	177.218	176.713
27)	Chlordane-5	6.242	7.029	10534417	151.7E6	172.702	177.622



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD040718\
Data File : PD046850.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2018 10:43
Operator : UA/AJ
Sample : LOQ CHLOR
Misc : ECD_D LOQ CHLOR WATER 200 PPB
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
LOQ CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 01:07:20 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD040718.M
Quant Title : GC Extractables
QLast Update : Sat Apr 07 04:44:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

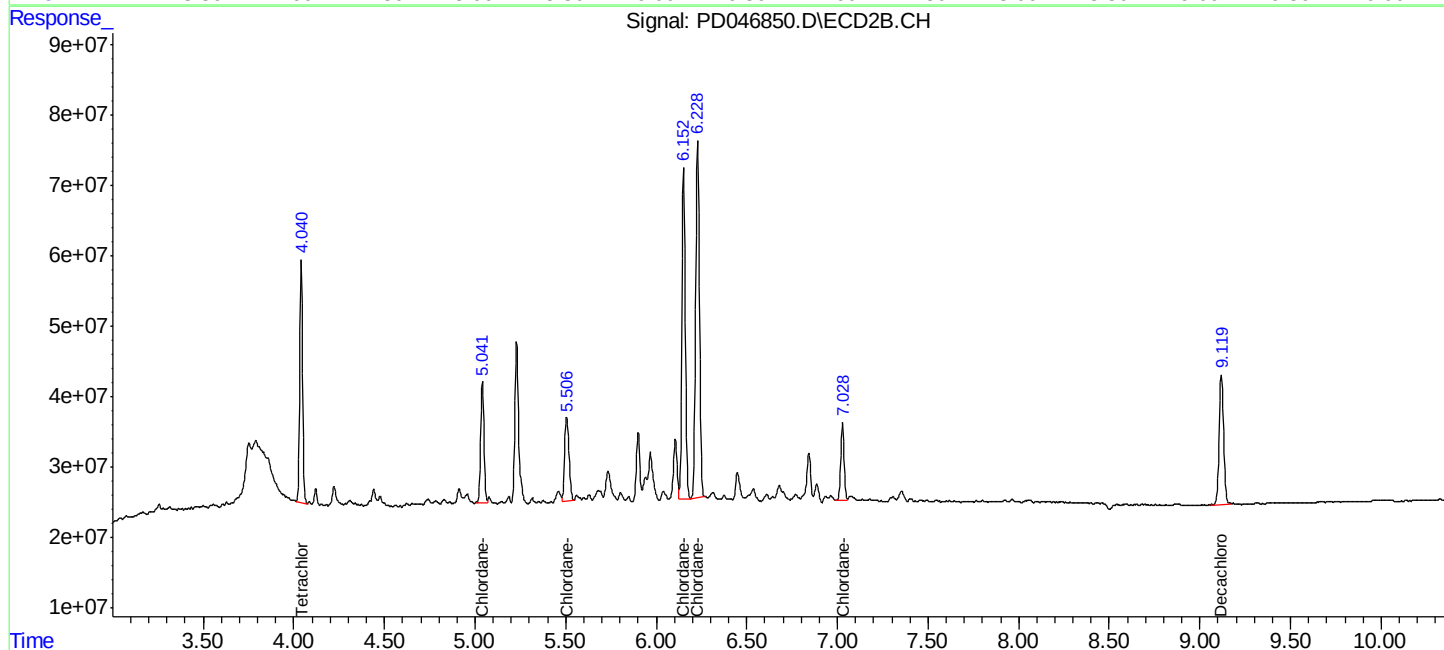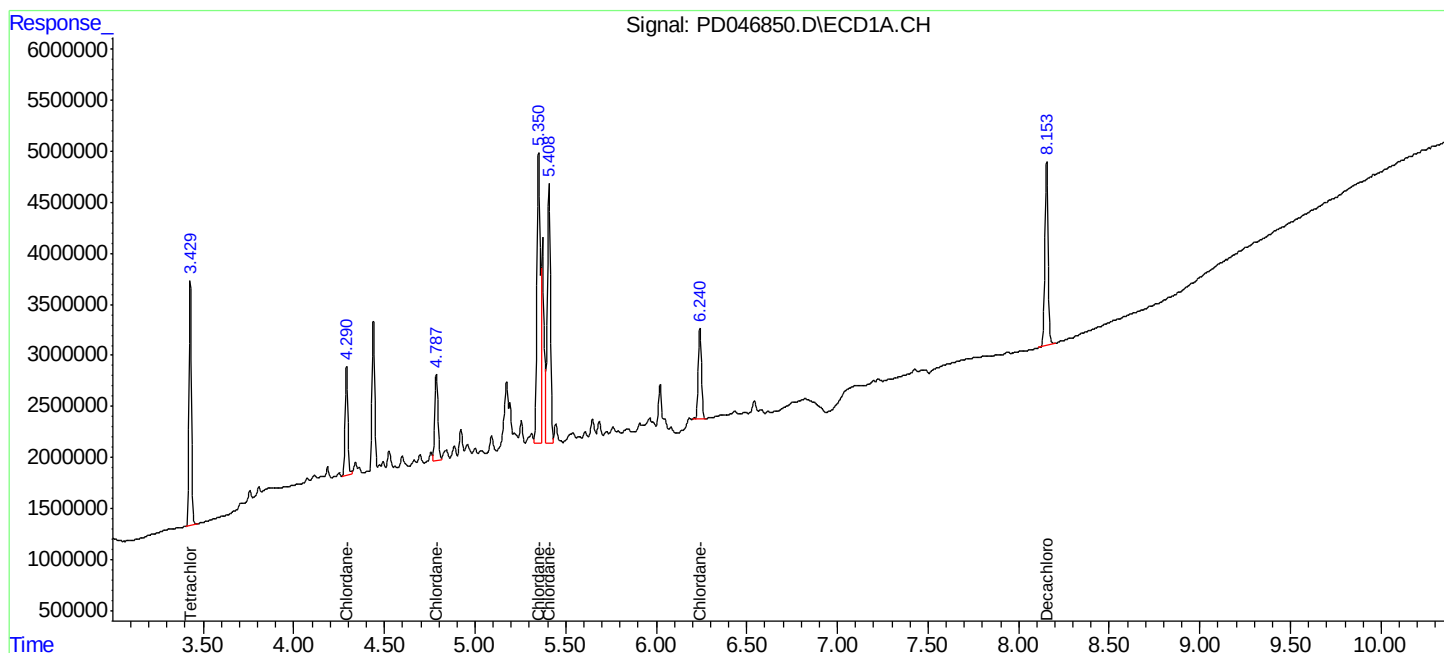


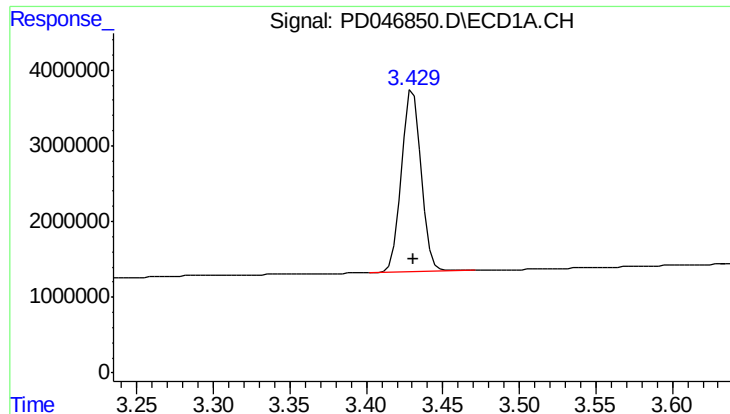

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 21541622
Conc: 17.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ CHLOR

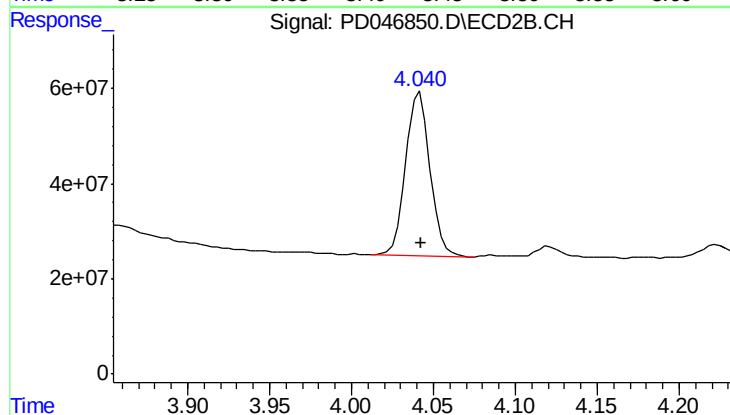


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 356823665
Conc: 16.70 ng/ml

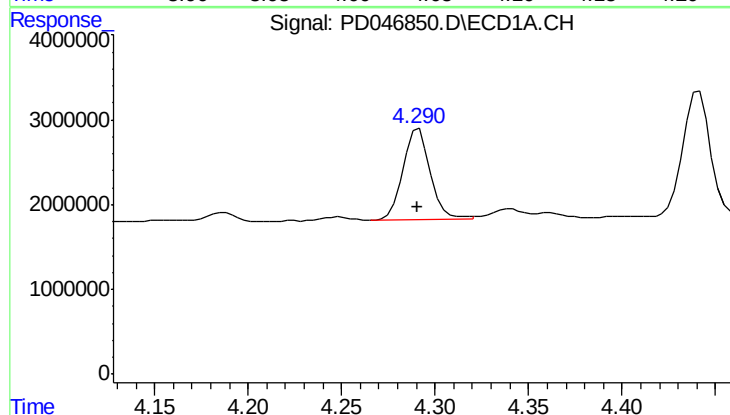


#23 Chlordane-1

R.T.: 4.291 min
Delta R.T.: 0.000 min
Response: 10931661
Conc: 177.58 ng/ml

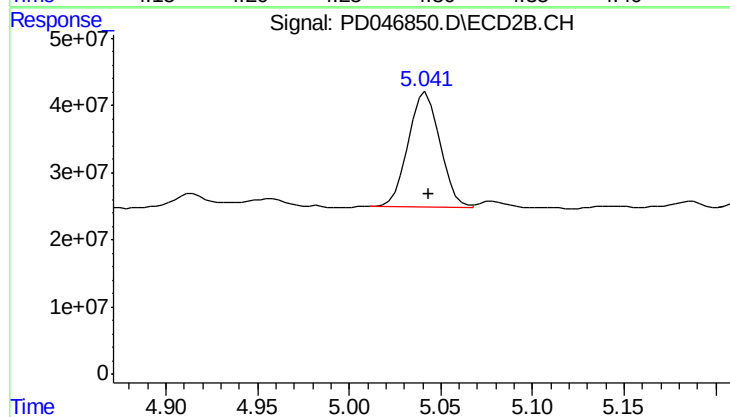

#23 Chlordane-1


R.T.: 5.042 min
Delta R.T.: -0.001 min
Response: 207657037
Conc: 179.05 ng/ml

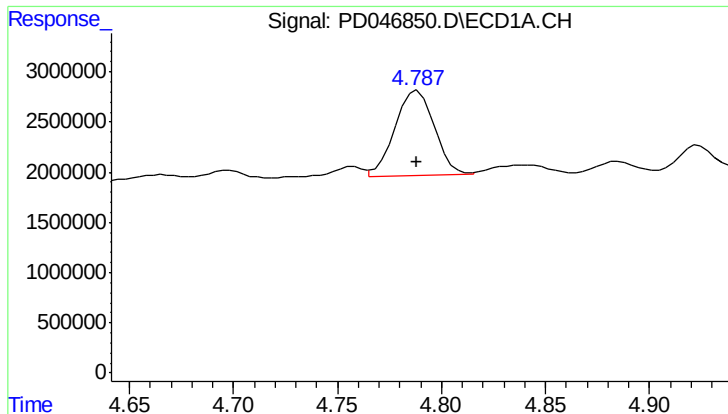

#24 Chlordane-2


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 11110548
Conc: 180.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ CHLOR

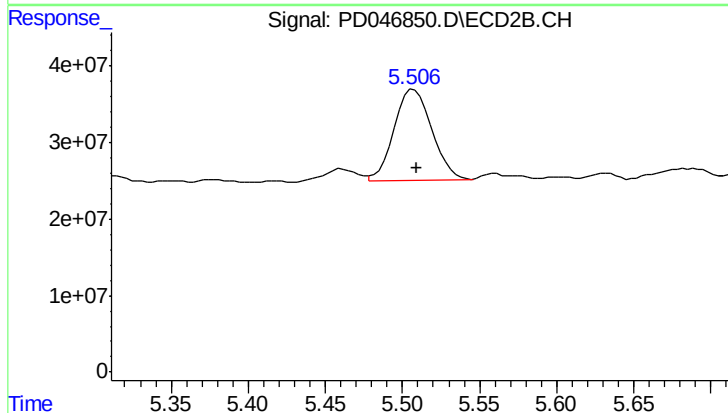


#24 Chlordane-2

R.T.: 5.507 min
Delta R.T.: -0.001 min
Response: 202864660
Conc: 184.05 ng/ml

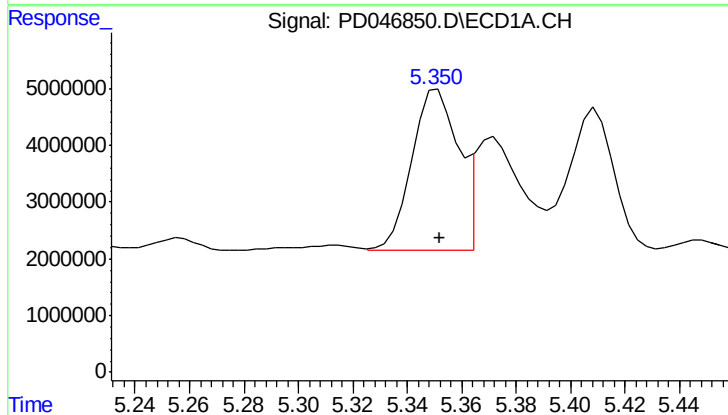


#25 Chlordane-3

R.T.: 5.351 min
Delta R.T.: 0.000 min
Response: 33510463
Conc: 178.25 ng/ml

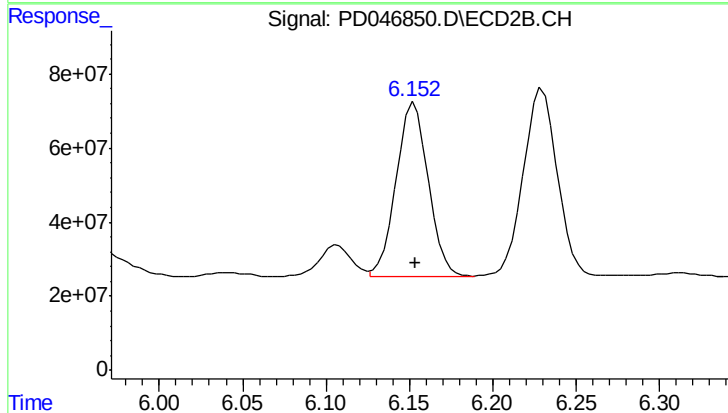

#25 Chlordane-3


R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 621446203
Conc: 176.73 ng/ml

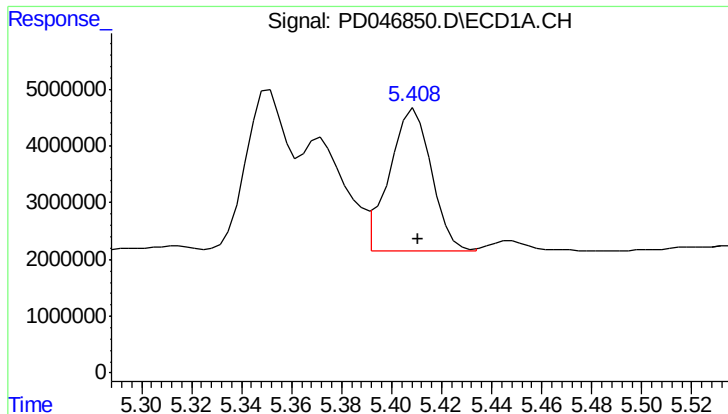

#26 Chlordane-4


R.T.: 5.409 min
Delta R.T.: -0.001 min
Response: 29378077
Conc: 177.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ CHLOR

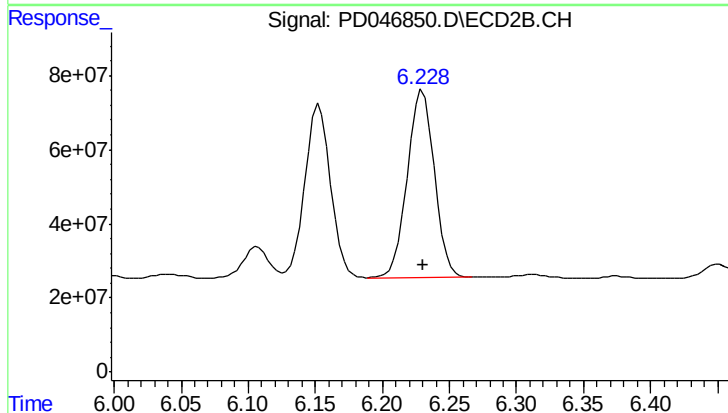


#26 Chlordane-4

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 711240071
Conc: 176.71 ng/ml

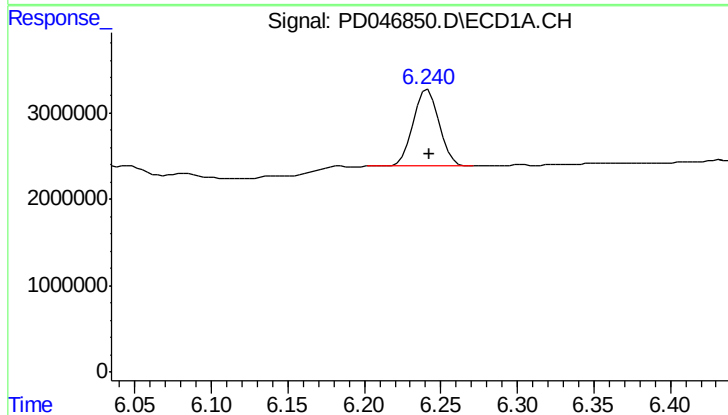


#27 Chlordane-5

R.T.: 6.242 min
Delta R.T.: -0.001 min
Response: 10534417
Conc: 172.70 ng/ml

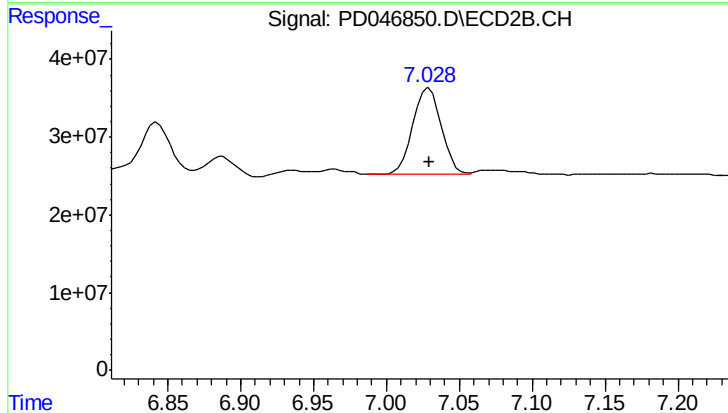

#27 Chlordane-5


R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 151658101
Conc: 177.62 ng/ml

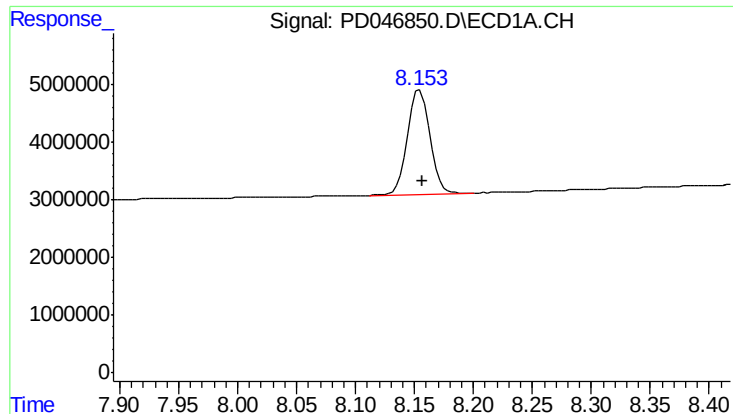

#28 Decachlorobiphenyl

R.T.: 8.155 min
Delta R.T.: -0.002 min
Response: 23454971
Conc: 17.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ CHLOR

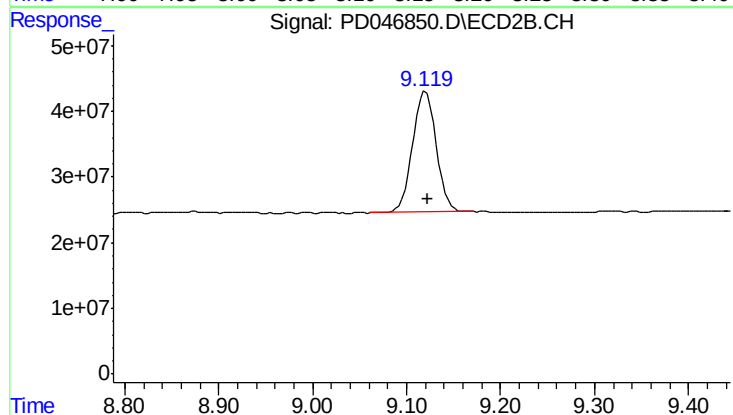

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.002 min
Response: 322735992
Conc: 17.94 ng/ml