

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
 Data File : PD052715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2019 22:59
 Operator : AJ\SJ
 Sample : PB118646BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK46

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:26:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 05 16:11:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.042	26389395	564.5E6	18.996	18.838
27)	SA Decachlor...	7.814	9.156	50183695	631.4E6	33.527	33.808
Target Compounds							
6)	B beta-BHC	0.000	4.935f	0 26799087	N.D.	1.400	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
Data File : PD052715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2019 22:59
Operator : AJ\SJ
Sample : PB118646BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK46

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:26:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 05 16:11:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

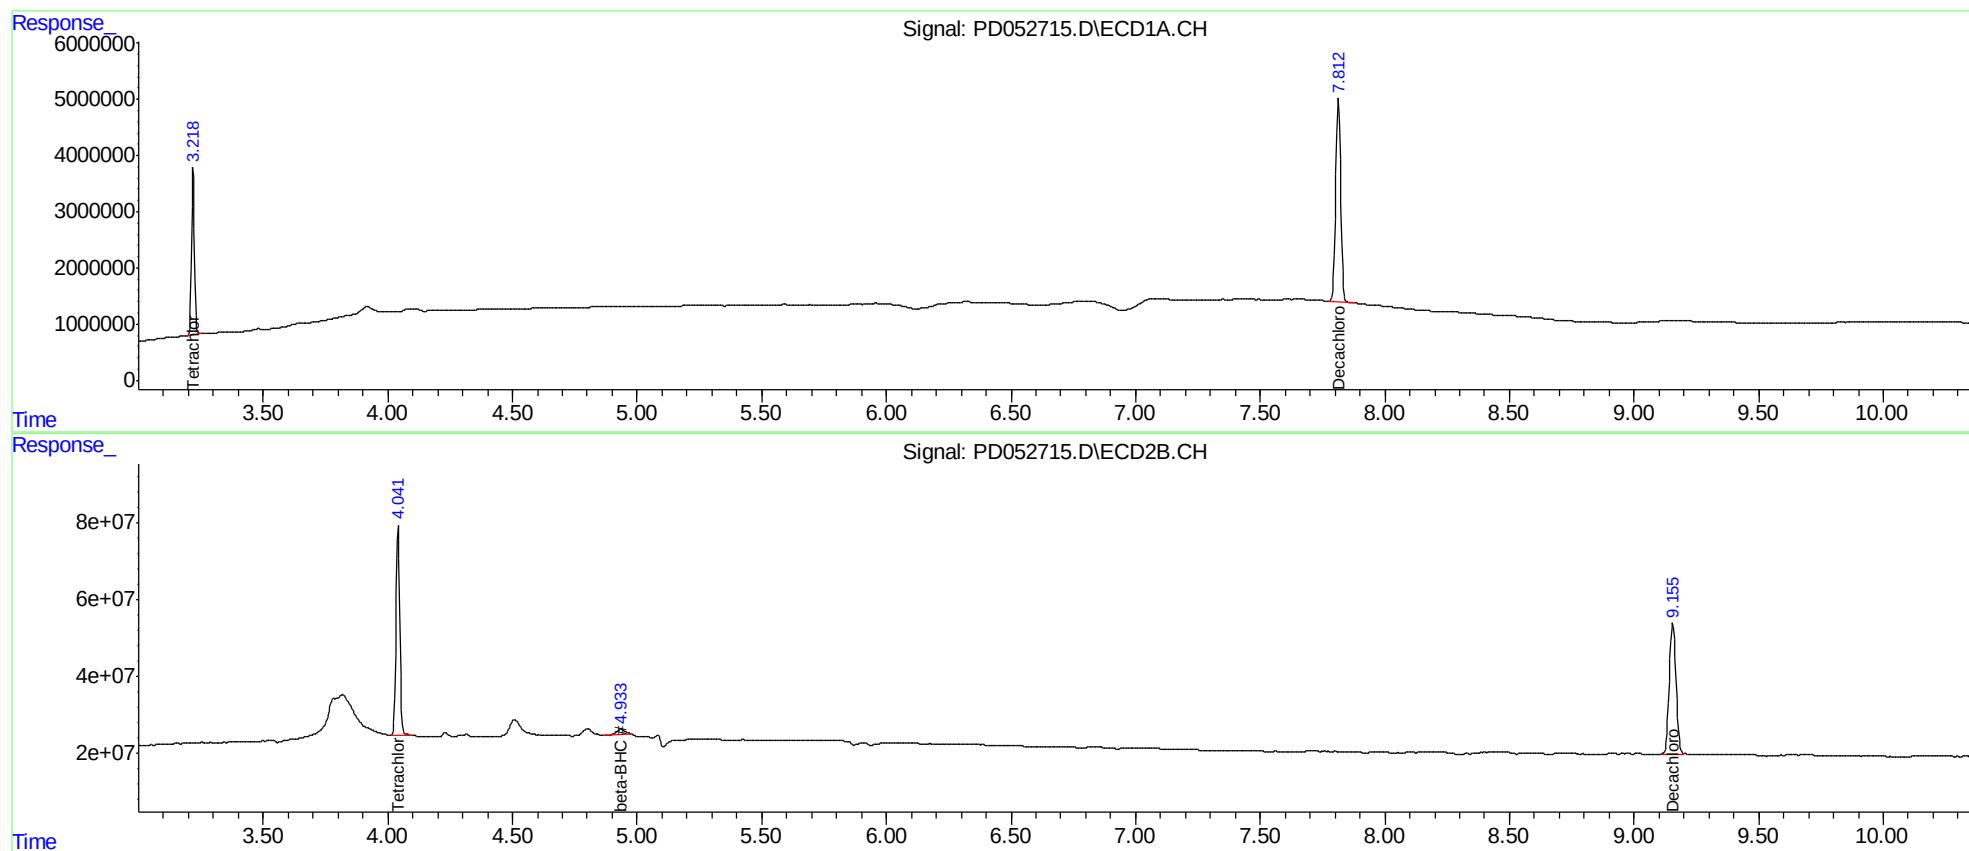


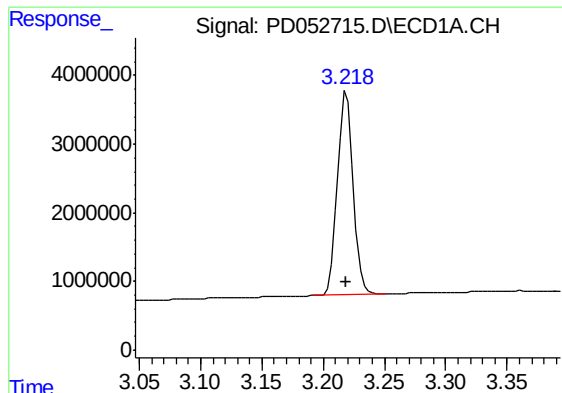

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: 0.000 min
Response: 26389395
Conc: 19.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK46

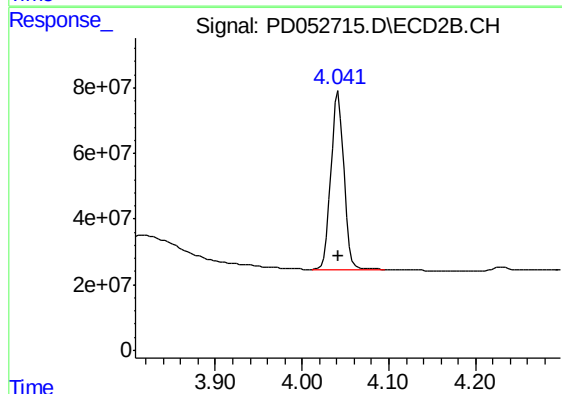


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 564544074
Conc: 18.84 ng/ml

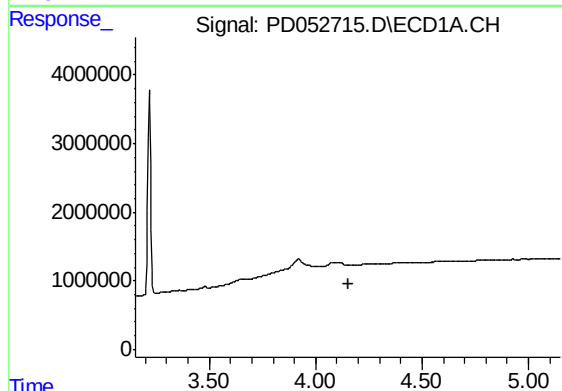


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

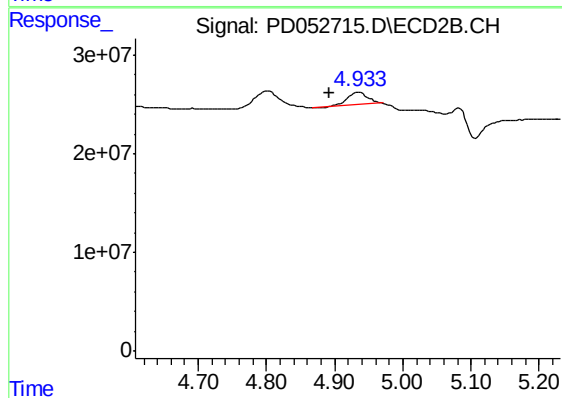

#6 beta-BHC


R.T.: 4.935 min
Delta R.T.: 0.043 min
Response: 26799087
Conc: 1.40 ng/ml

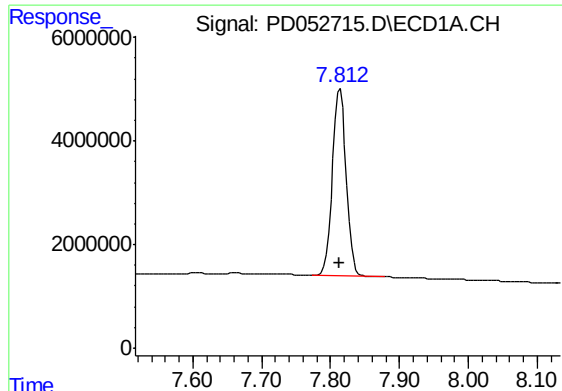

#27 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: 0.000 min
Response: 50183695
Conc: 33.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK46

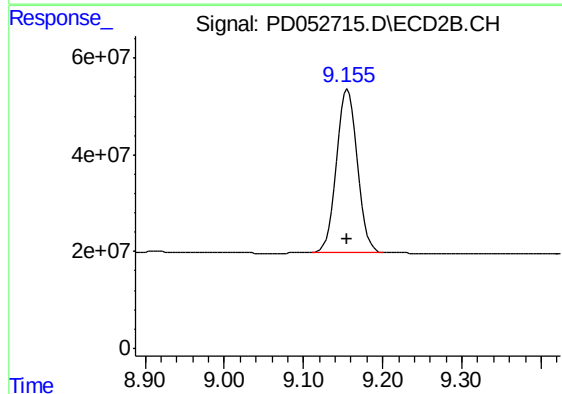

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 631372781
Conc: 33.81 ng/ml