

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
 Data File : PD052738.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 4:38
 Operator : AJ\SJ
 Sample : PIBLK27
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 05:41:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 05 16:11:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.219	4.042	29482572	626.7E6	21.222	20.913
27) SA	Decachlor...	7.814	9.156	55828178	621.5E6	37.299	33.278
Target Compounds							
6) B	beta-BHC	0.000	4.935f	0 25008461	N.D.		1.306
8) B	Heptachlo...	0.000	5.923	0 83097745	N.D.		2.304
20) A	Methoxychlor	0.000	7.590f	0 26134933	N.D.		2.412


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
Data File : PD052738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 4:38
Operator : AJ\SJ
Sample : PIBLK27
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK27

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 05:41:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 05 16:11:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

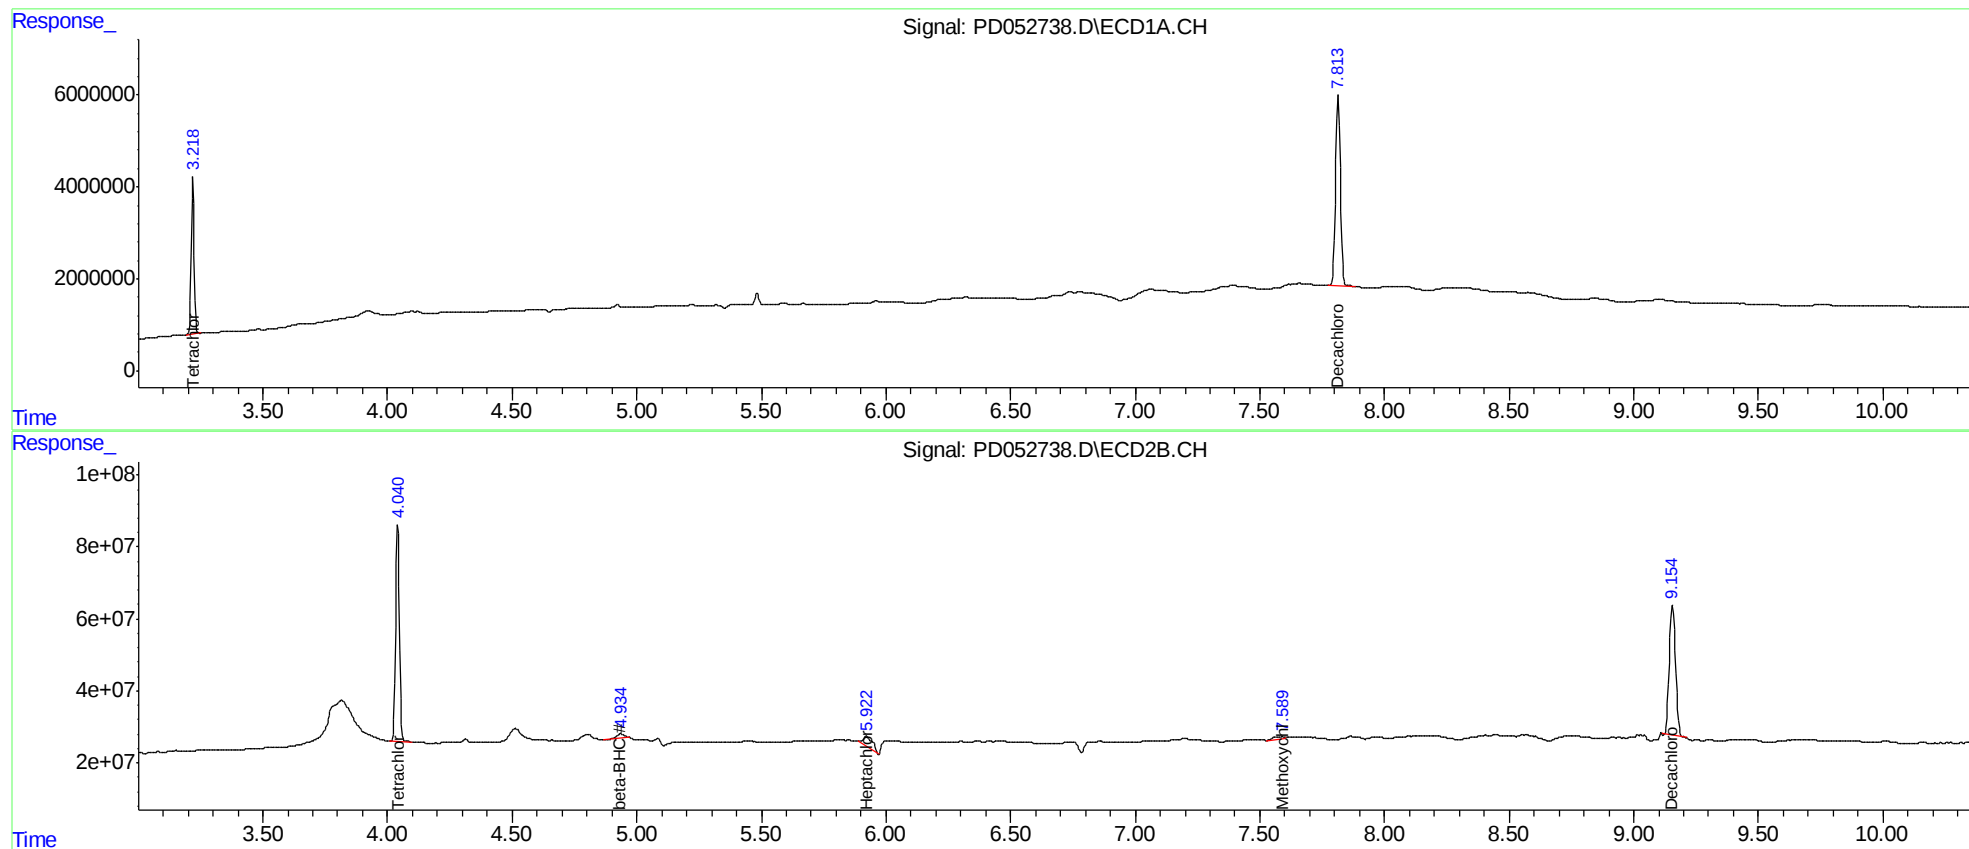


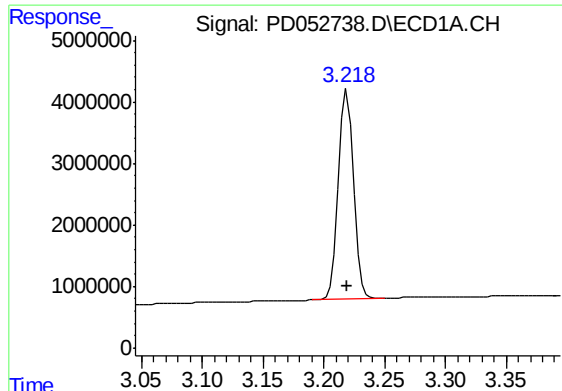

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: 0.000 min
Response: 29482572
Conc: 21.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK27

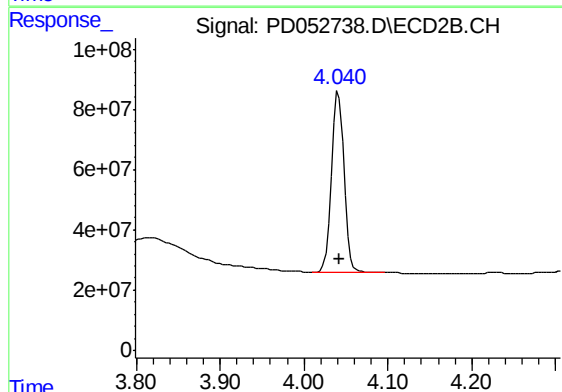


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 626725593
Conc: 20.91 ng/ml

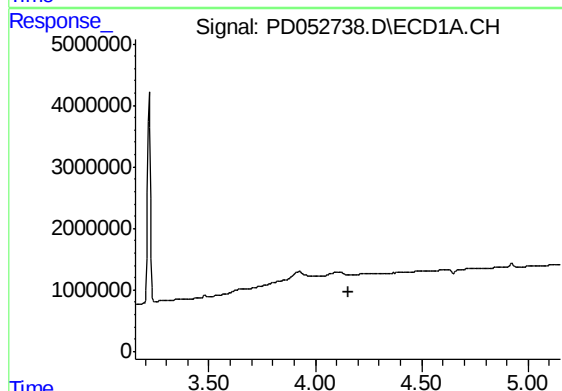


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

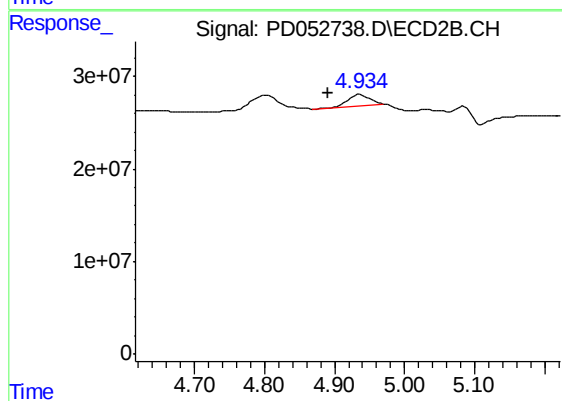

#6 beta-BHC


R.T.: 4.935 min
Delta R.T.: 0.044 min
Response: 25008461
Conc: 1.31 ng/ml

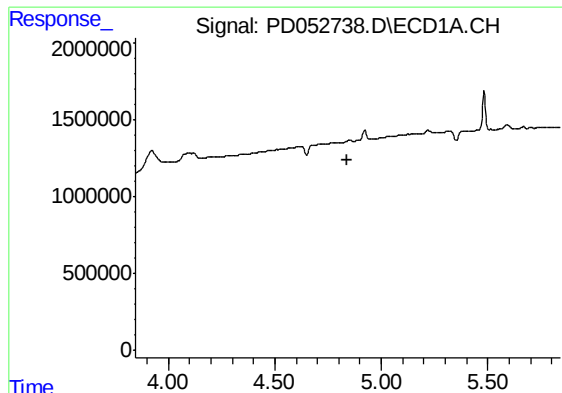

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.842 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK27

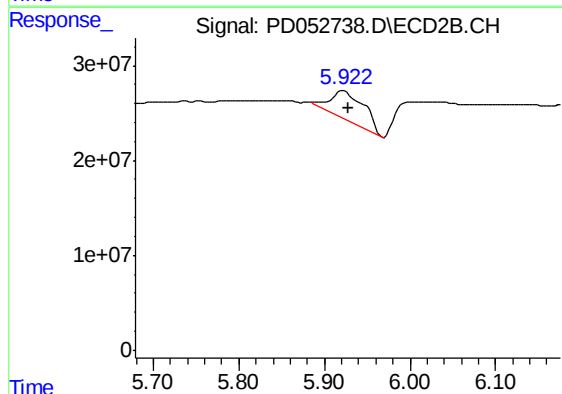


#8 Heptachlor epoxide

R.T.: 5.923 min
Delta R.T.: -0.006 min
Response: 83097745
Conc: 2.30 ng/ml

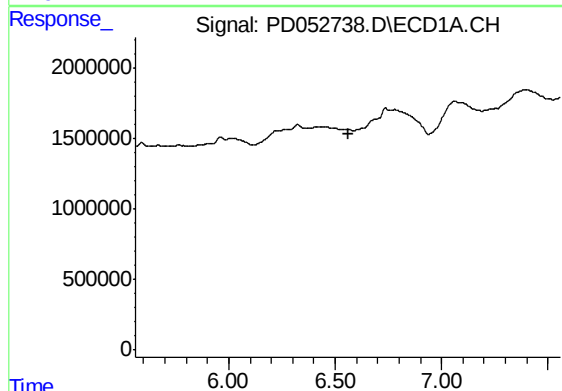


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.561 min
Response: 0
Conc: N.D.

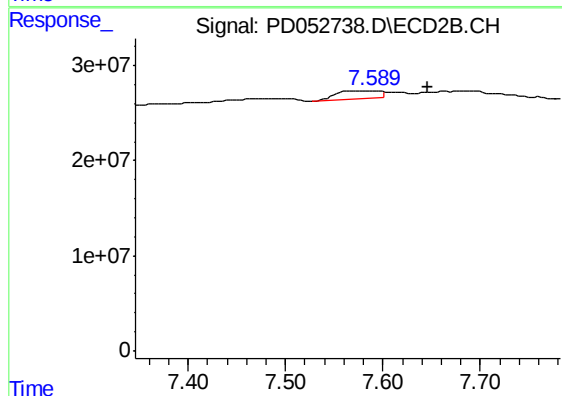

#20 Methoxychlor


R.T.: 7.590 min
Delta R.T.: -0.056 min
Response: 26134933
Conc: 2.41 ng/ml

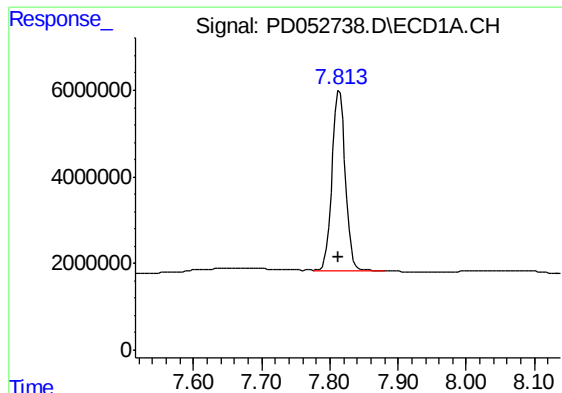

#27 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: 0.001 min
Response: 55828178
Conc: 37.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK27

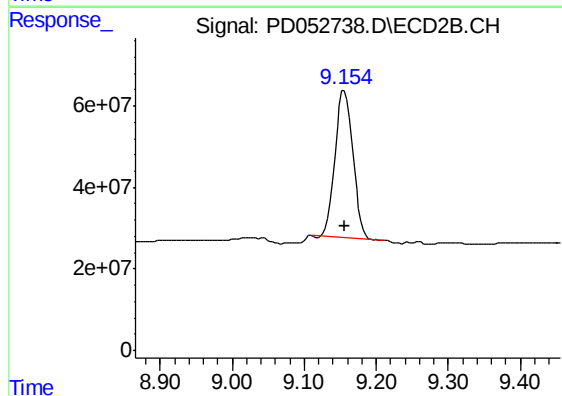

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 621482488
Conc: 33.28 ng/ml