

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
 Data File : PD052702.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2019 19:55
 Operator : AJ\SJ
 Sample : K2217-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF615

Manual Integrations
 APPROVED

Sohil
 4/18/2019 3:03:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 00:25:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 05 16:11:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	13762136	310.3E6	9.906	10.355
27)	SA Decachlor...	7.813	9.156	25717839	325.0E6	17.182	17.403
Target Compounds							
12)	B 4,4'-DDE	5.283	6.393	1984691	46549196	1.019m	1.441 #
16)	A 4,4'-DDD	5.783	6.887	789064	33586640	0.493m	1.302m#
17)	MA 4,4'-DDT	6.010	7.184	2823570	15010244	1.804m	0.686m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040719\
Data File : PD052702.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2019 19:55
Operator : AJ\SJ
Sample : K2217-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 00:25:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040719CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 05 16:11:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

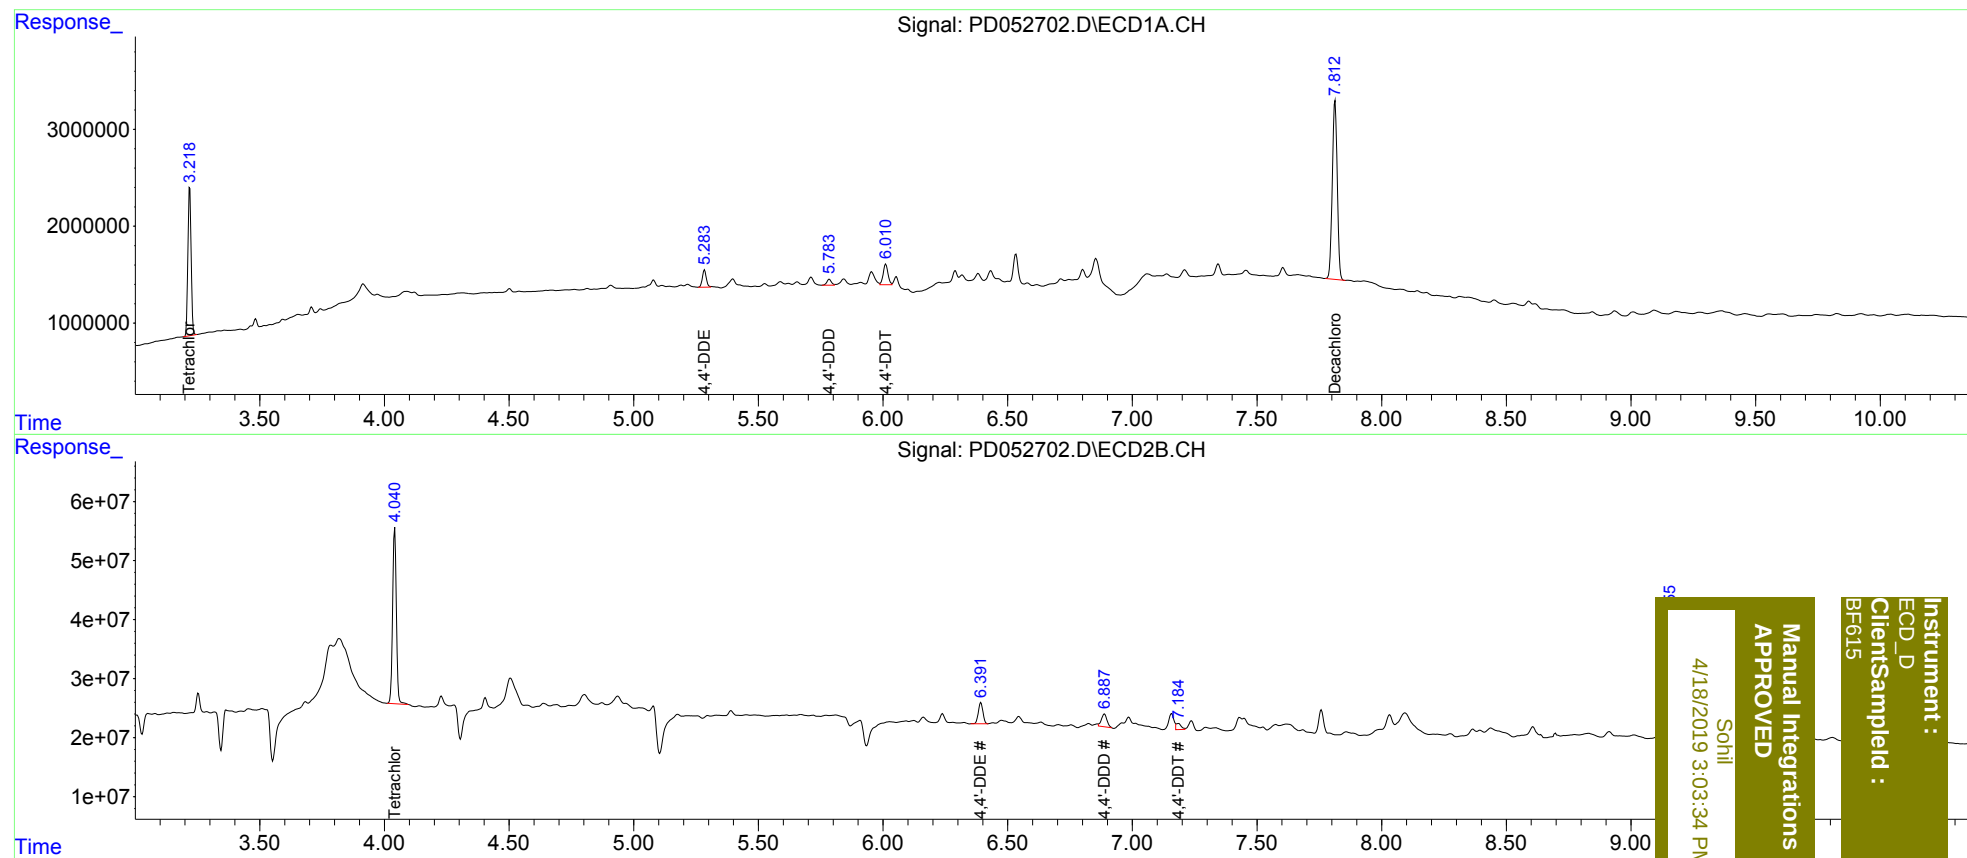

4/18/2019 3:03:34 PM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BF615