

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
 Data File : PD057741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 12:56
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 07:35:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 08 07:20:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.895	3653039	4758542	5.102	4.921
27)	SA Decachlor...	7.865	8.898	8833577	12036225	10.640	11.018
Target Compounds							
2)	A alpha-BHC	3.649	4.279	4710493	6231573	4.565	4.579
3)	MA gamma-BHC...	3.920	4.560	4986945	6053153	4.998	4.643
4)	MA Heptachlor	4.201	5.061	4421618	6402575	5.110	4.874
9)	A Endosulfan I	5.196	6.098	4011276	5757512	4.901	4.978
13)	MA Dieldrin	5.433	6.353	8752130	12146491	9.600	9.587
14)	MA Endrin	5.685	6.568	7750096	10438947	9.901	9.675
16)	A 4,4'-DDD	5.822	6.695	6666398	9829597	9.527	9.689
17)	MA 4,4'-DDT	6.056	6.992	6243299	9804622	8.969	9.454
20)	A Methoxychlor	6.603	7.451	17680614	29751567	48.902	52.407


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 12:56
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:35:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:20:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

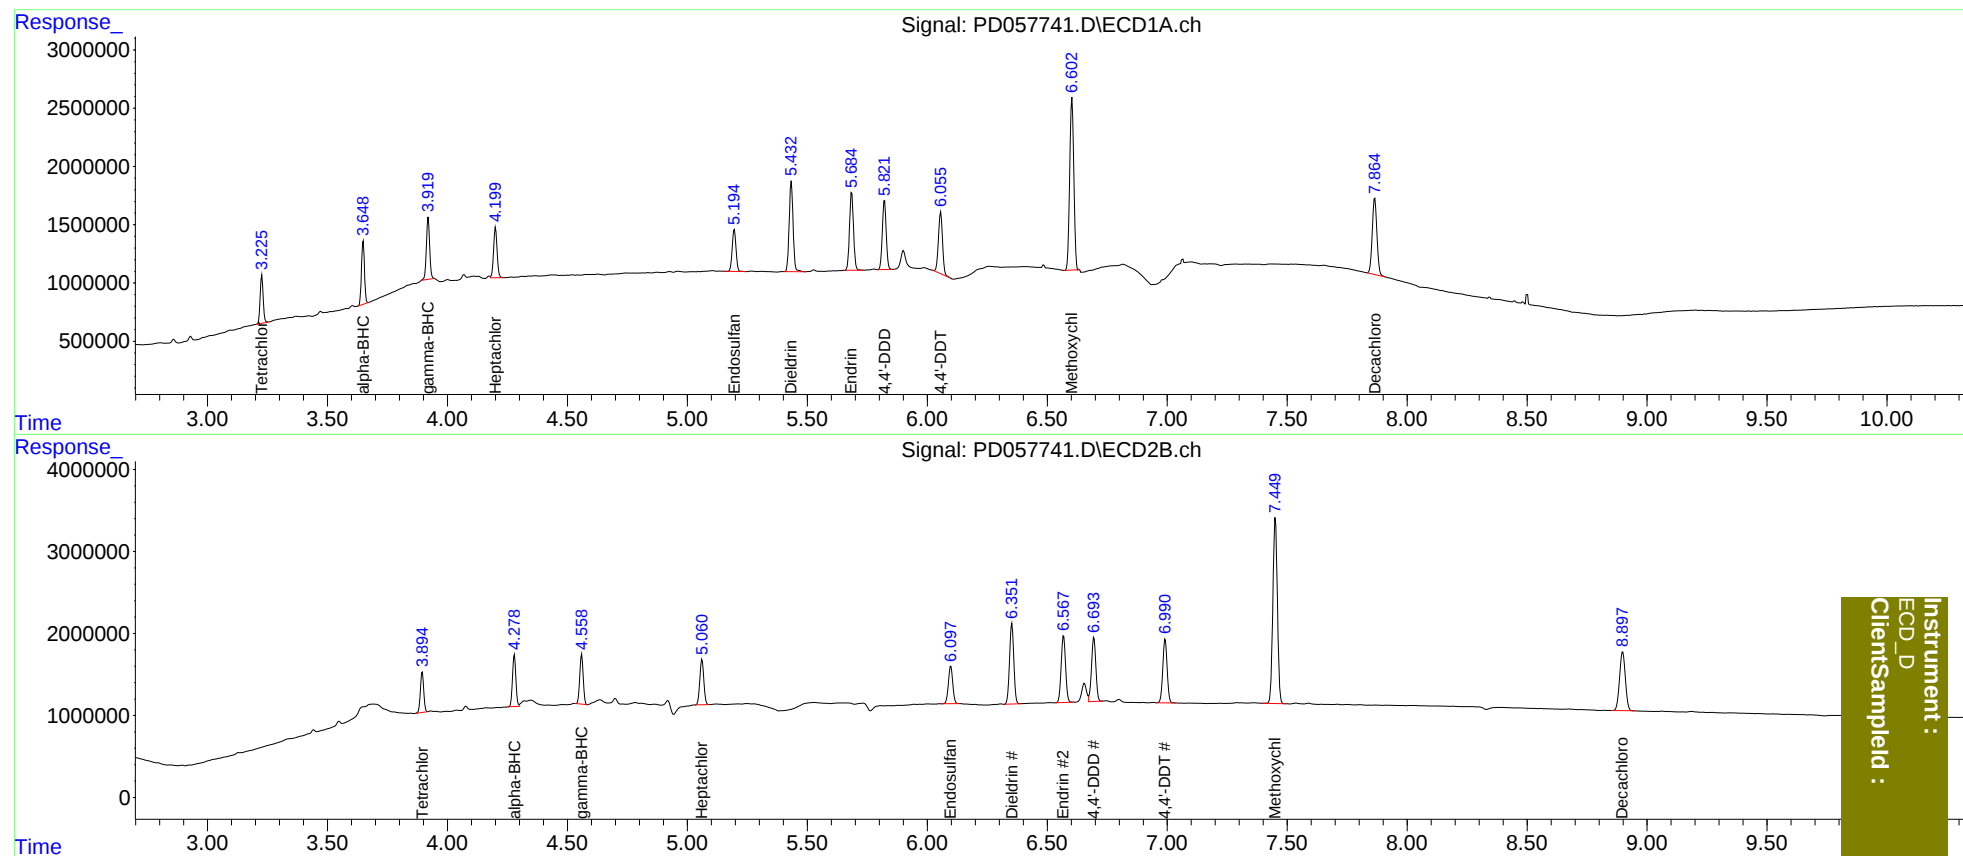


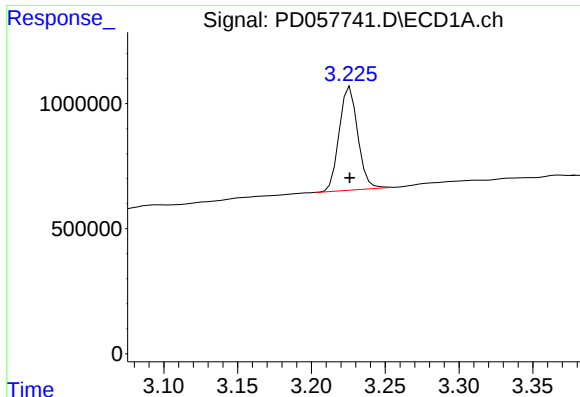

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 3653039
Conc: 5.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

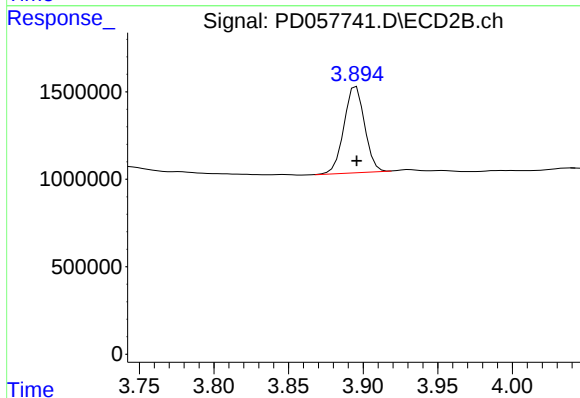


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 4758542
Conc: 4.92 ng/ml

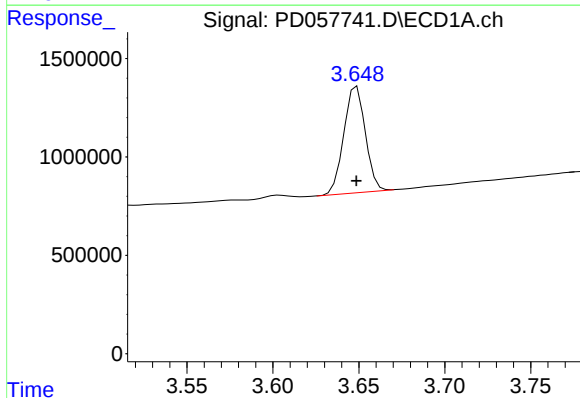


#2 alpha-BHC

R.T.: 3.649 min
Delta R.T.: 0.000 min
Response: 4710493
Conc: 4.56 ng/ml

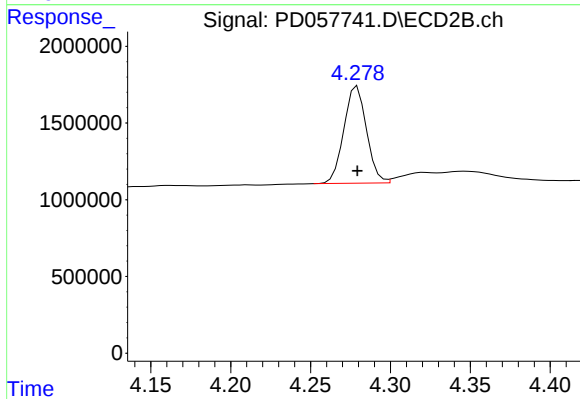

#2 alpha-BHC


R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 6231573
Conc: 4.58 ng/ml

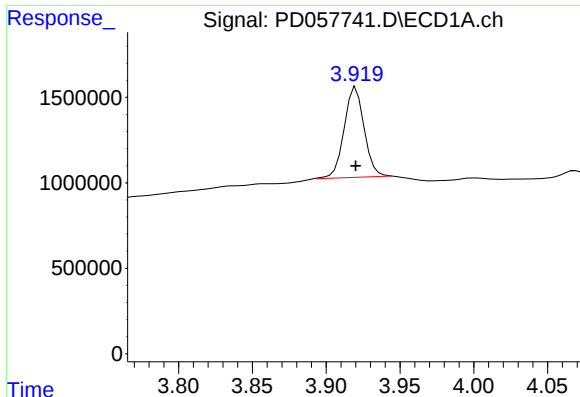

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 4986945
Conc: 5.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

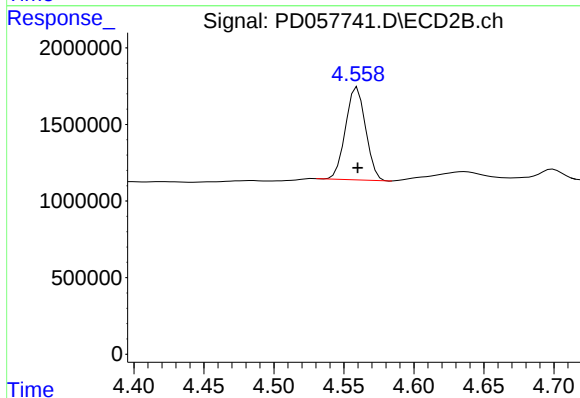


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 6053153
Conc: 4.64 ng/ml

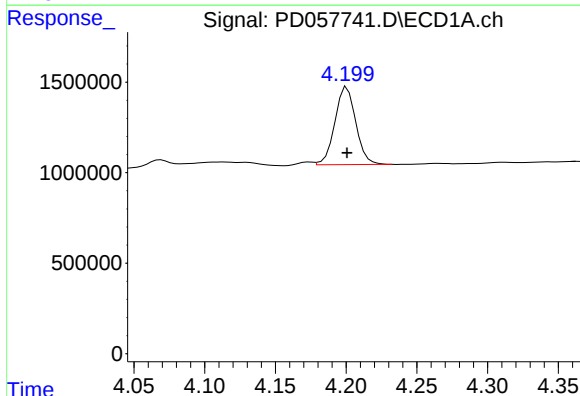


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 4421618
Conc: 5.11 ng/ml

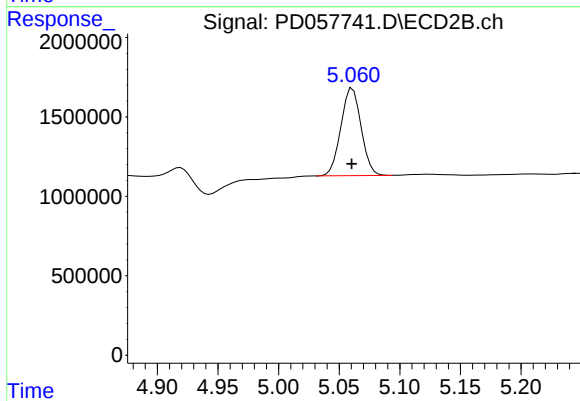

#4 Heptachlor


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 6402575
Conc: 4.87 ng/ml

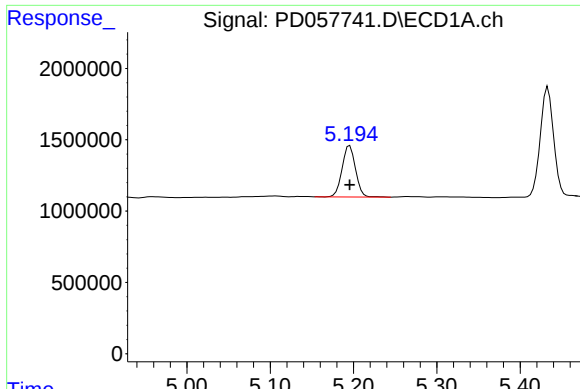

#9 Endosulfan I


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 4011276
Conc: 4.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

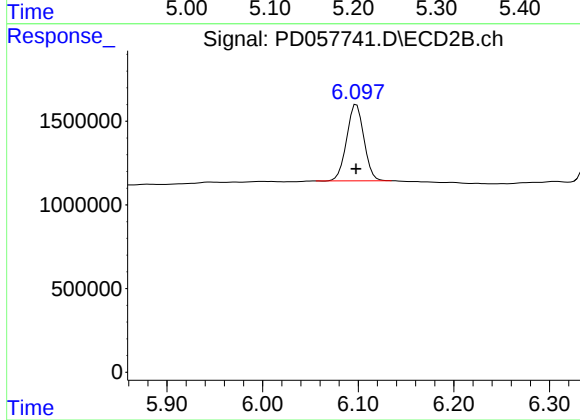


#9 Endosulfan I

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 5757512
Conc: 4.98 ng/ml

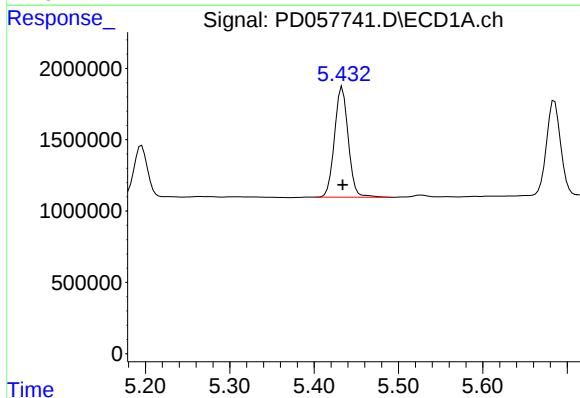


#13 Dieldrin

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 8752130
Conc: 9.60 ng/ml

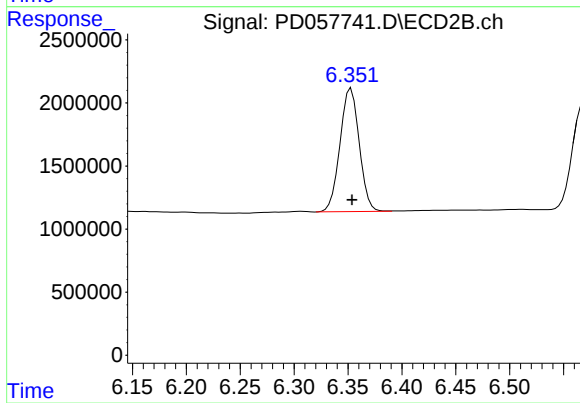

#13 Dieldrin


R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 12146491
Conc: 9.59 ng/ml

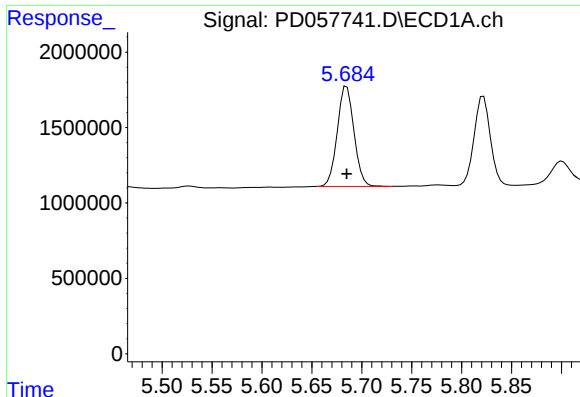

#14 Endrin


R.T.: 5.685 min
Delta R.T.: 0.000 min
Response: 7750096
Conc: 9.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

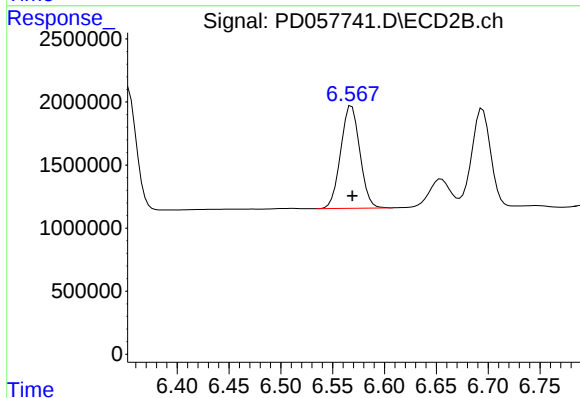


#14 Endrin

R.T.: 6.568 min
Delta R.T.: 0.000 min
Response: 10438947
Conc: 9.68 ng/ml

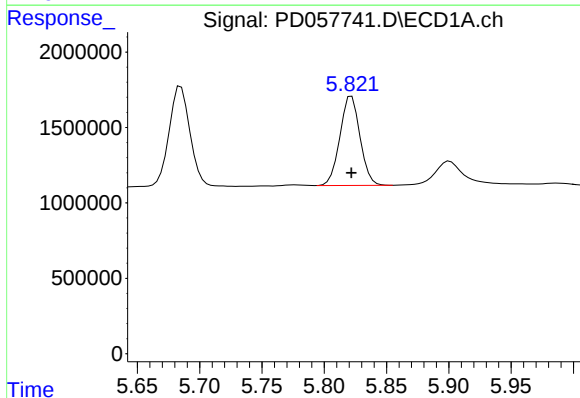


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 6666398
Conc: 9.53 ng/ml

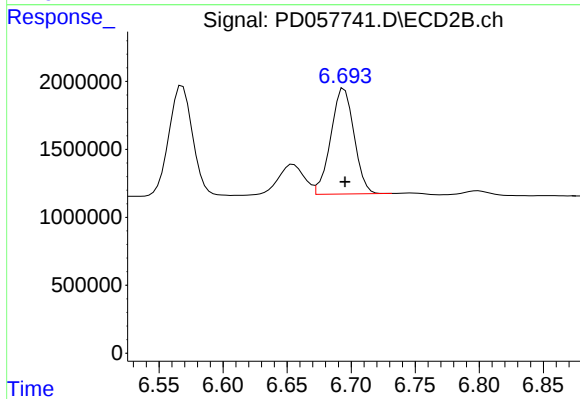

#16 4,4'-DDD


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 9829597
Conc: 9.69 ng/ml

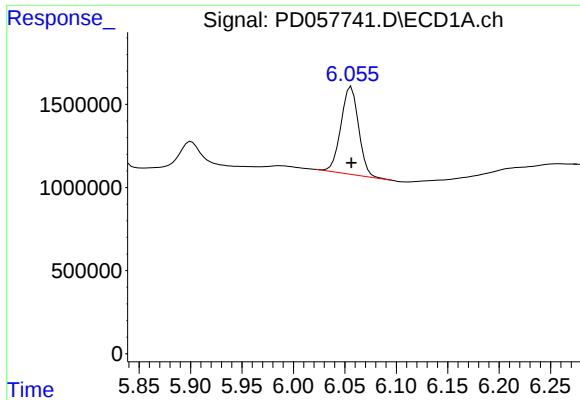

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 6243299
Conc: 8.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

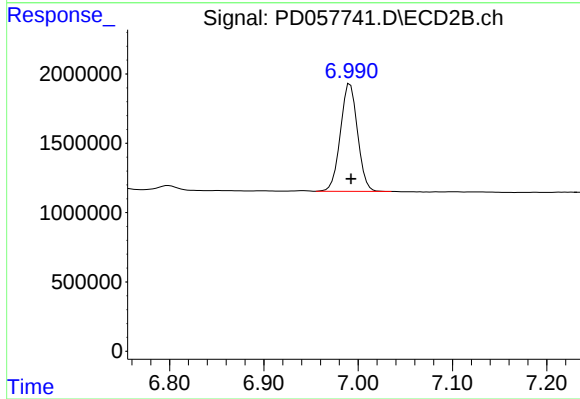


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 9804622
Conc: 9.45 ng/ml

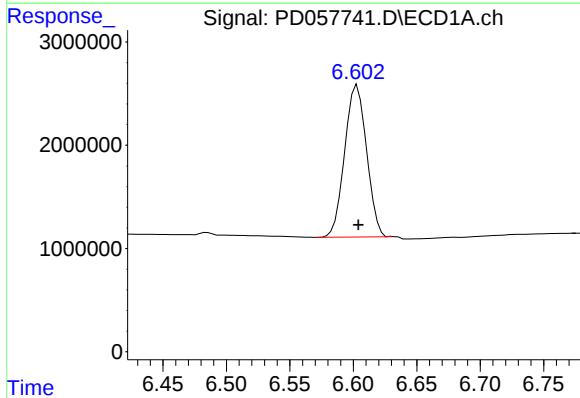


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 17680614
Conc: 48.90 ng/ml

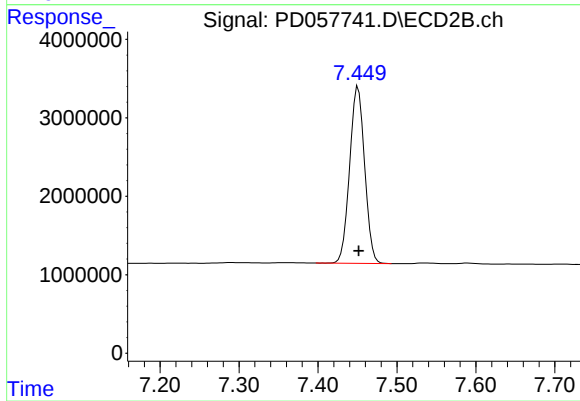

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 29751567
Conc: 52.41 ng/ml

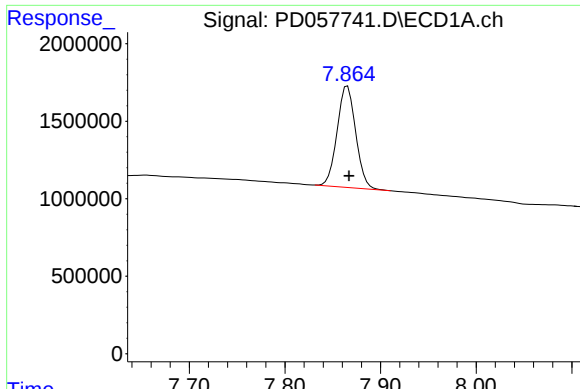

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 8833577
Conc: 10.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

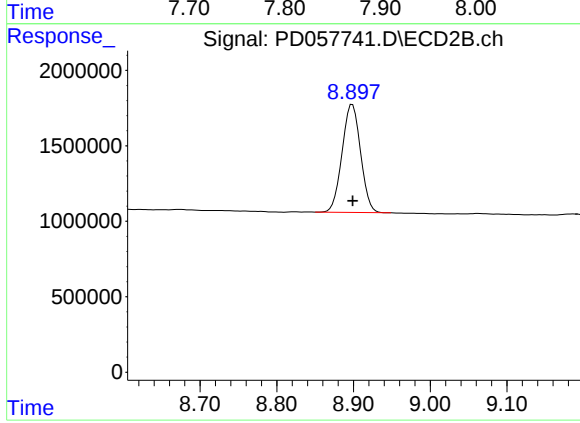

#27 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 12036225
Conc: 11.02 ng/ml