

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
 Data File : PD057743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 13:24
 Operator : AJ\MA
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 07:25:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 08 07:20:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	7443166	9889250	10.395	10.227
27)	SA Decachlor...	7.866	8.897	17824169	23540178	21.469	21.549
Target Compounds							
2)	A alpha-BHC	3.649	4.279	10176363	13357321	9.861	9.816
3)	MA gamma-BHC...	3.920	4.560	10297948	12963353	10.322	9.943
4)	MA Heptachlor	4.200	5.060	8844842	13390497	10.221	10.193
9)	A Endosulfan I	5.196	6.098	8343621	11956067	10.194	10.337
13)	MA Dieldrin	5.434	6.353	18344588	25356909	20.123	20.014
14)	MA Endrin	5.685	6.568	16066936	21840744	20.526	20.243
16)	A 4,4'-DDD	5.822	6.695	14130153	20462570	20.193	20.171
17)	MA 4,4'-DDT	6.054	6.992	13628580	20650478	19.579	19.911
20)	A Methoxychlor	6.603	7.450	36190849	59421336	100.098	104.669


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 13:24
Operator : AJ\MA
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:25:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:20:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

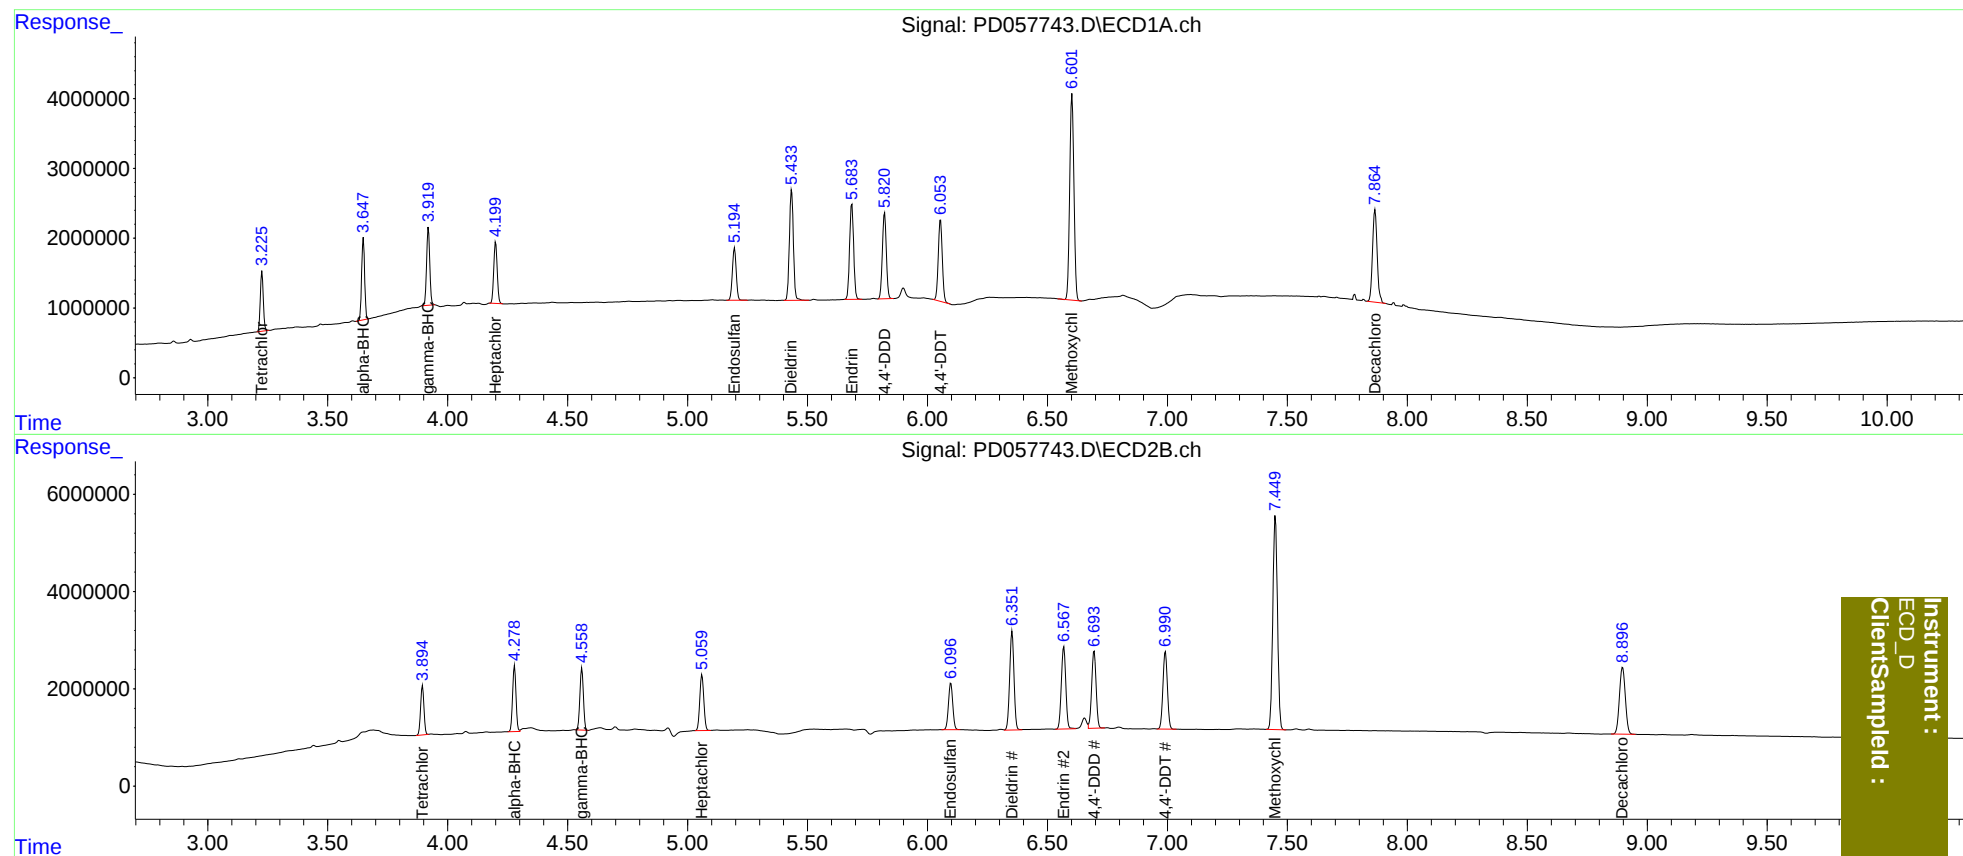


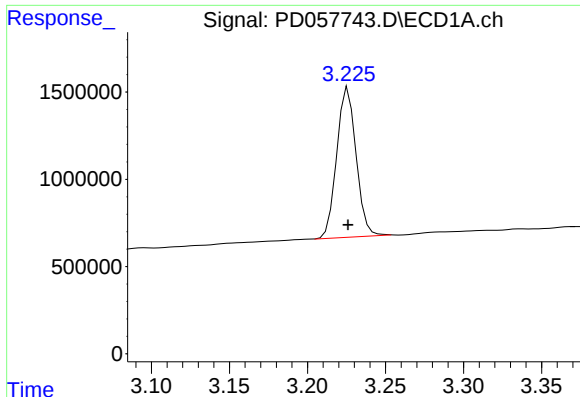

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 7443166
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

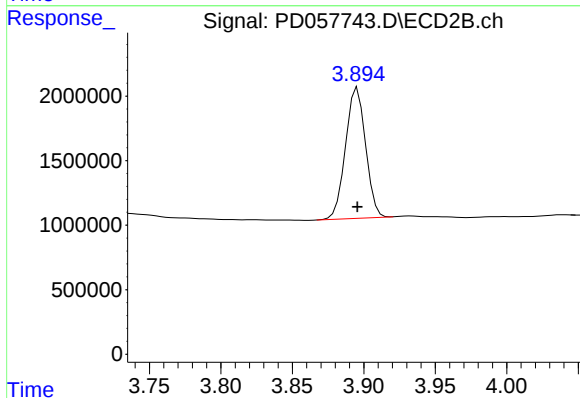


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 9889250
Conc: 10.23 ng/ml

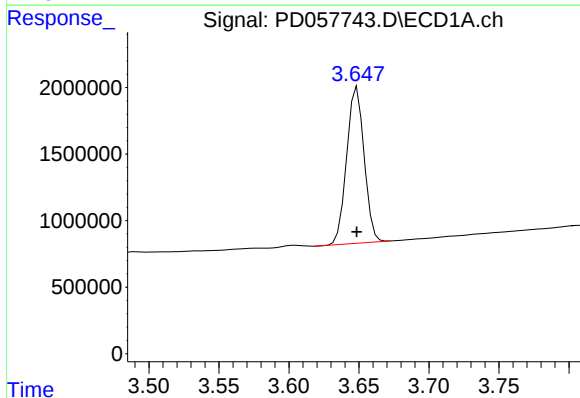


#2 alpha-BHC

R.T.: 3.649 min
Delta R.T.: 0.000 min
Response: 10176363
Conc: 9.86 ng/ml

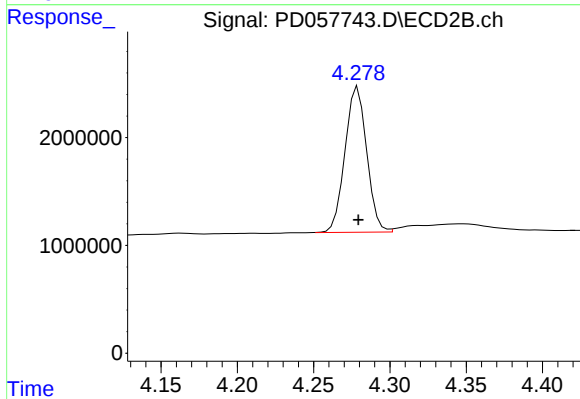

#2 alpha-BHC


R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 13357321
Conc: 9.82 ng/ml

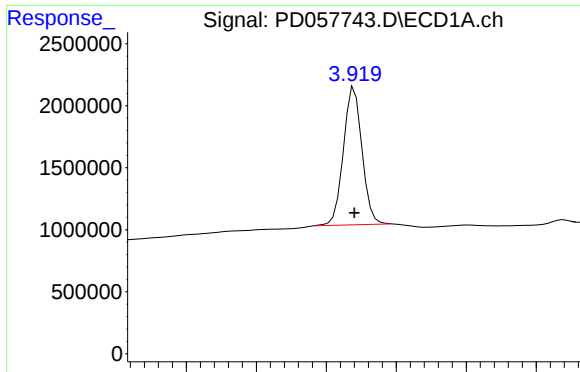

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 10297948
Conc: 10.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

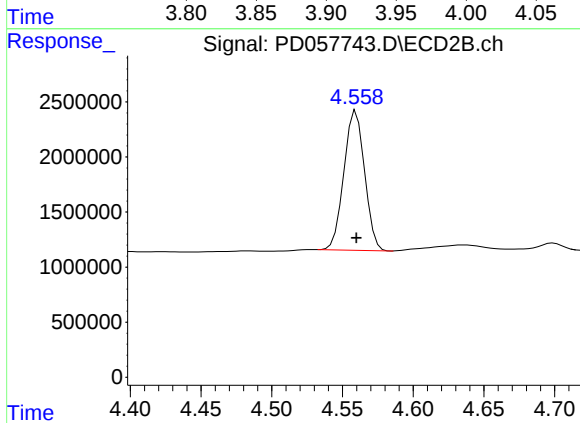


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 12963353
Conc: 9.94 ng/ml

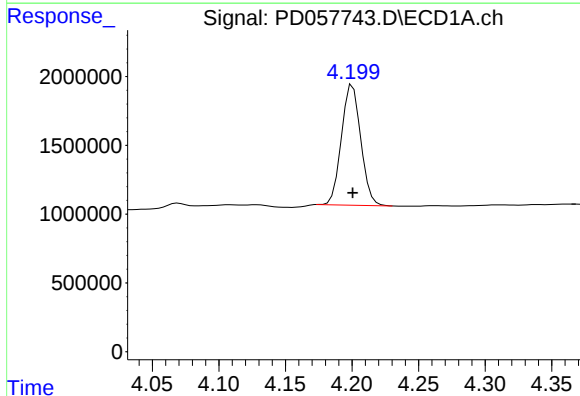


#4 Heptachlor

R.T.: 4.200 min
Delta R.T.: 0.000 min
Response: 8844842
Conc: 10.22 ng/ml

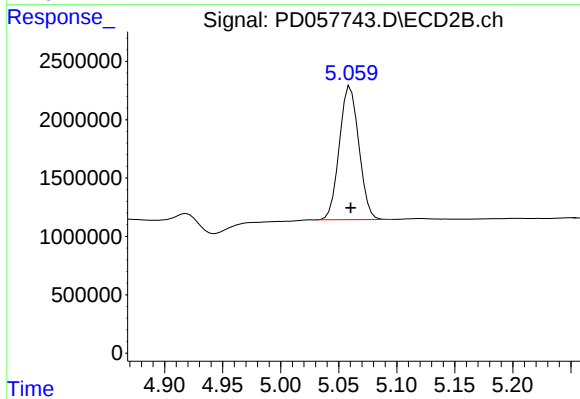

#4 Heptachlor


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 13390497
Conc: 10.19 ng/ml

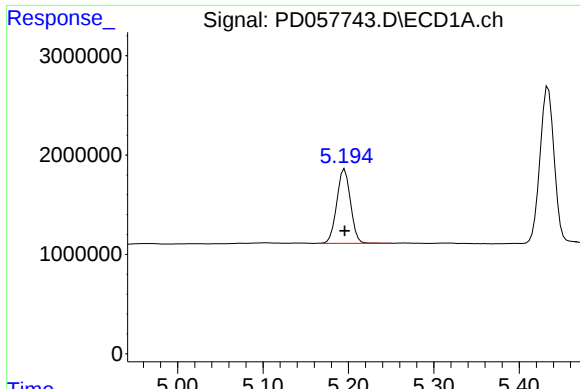

#9 Endosulfan I


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 8343621
Conc: 10.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

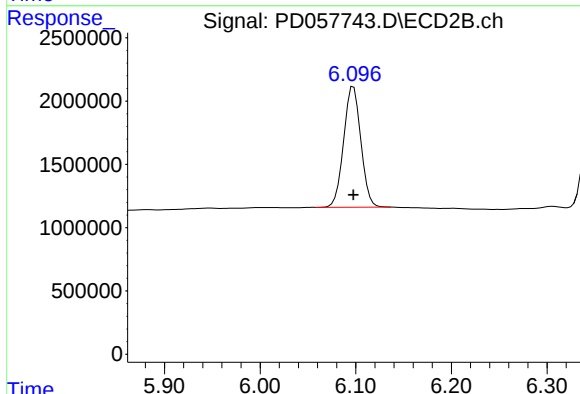


#9 Endosulfan I

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 11956067
Conc: 10.34 ng/ml

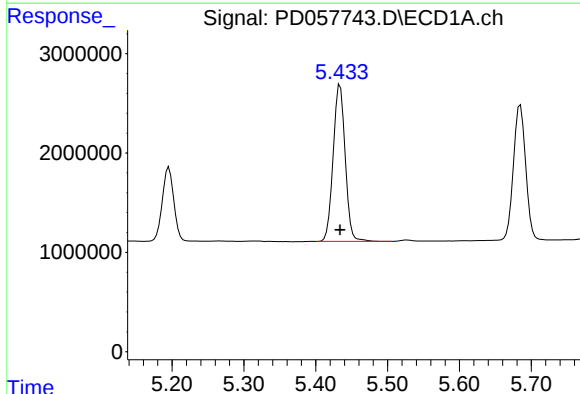


#13 Dieldrin

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 18344588
Conc: 20.12 ng/ml

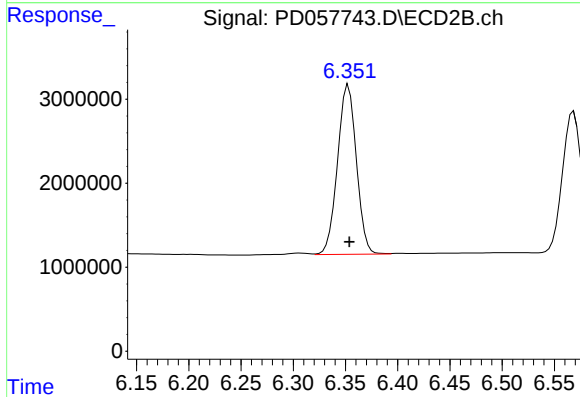

#13 Dieldrin


R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 25356909
Conc: 20.01 ng/ml

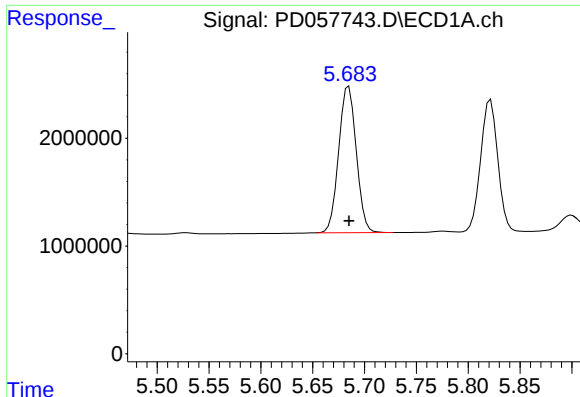

#14 Endrin


R.T.: 5.685 min
Delta R.T.: 0.000 min
Response: 16066936
Conc: 20.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

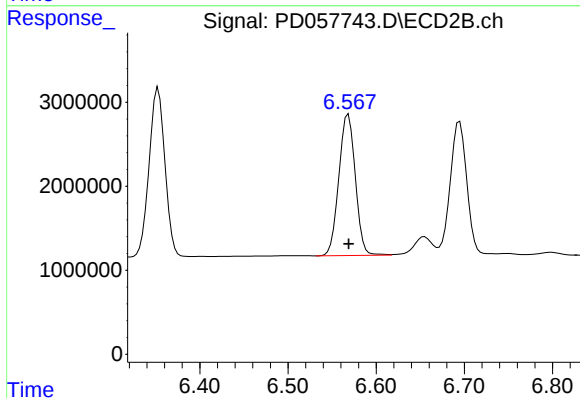


#14 Endrin

R.T.: 6.568 min
Delta R.T.: 0.000 min
Response: 21840744
Conc: 20.24 ng/ml

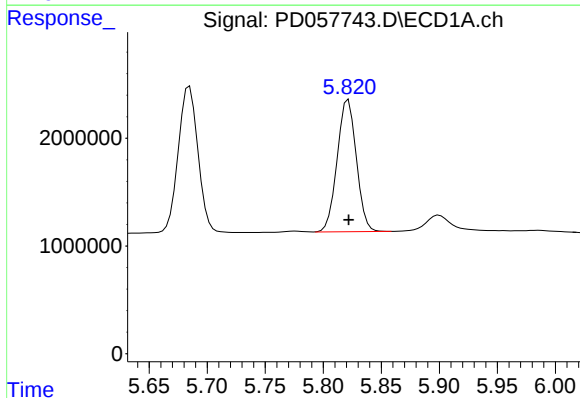


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 14130153
Conc: 20.19 ng/ml

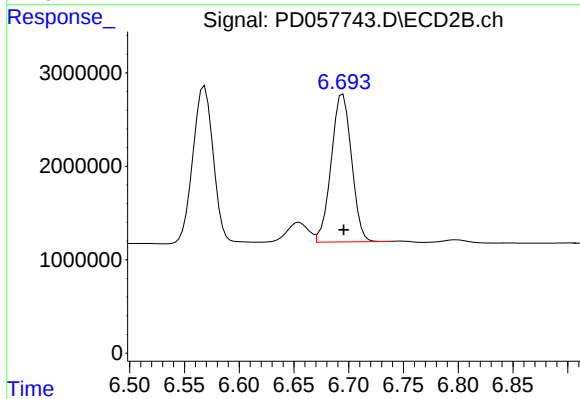

#16 4,4'-DDD


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 20462570
Conc: 20.17 ng/ml

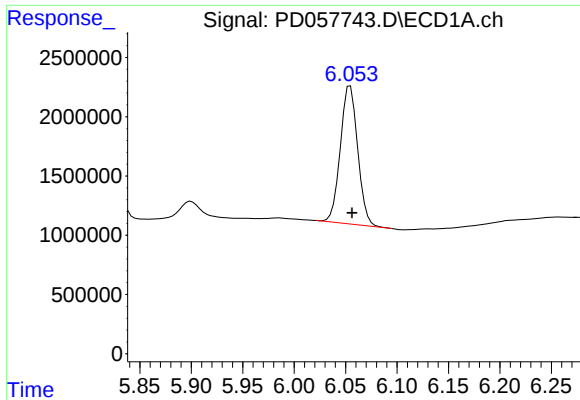

#17 4,4'-DDT


R.T.: 6.054 min
Delta R.T.: -0.002 min
Response: 13628580
Conc: 19.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

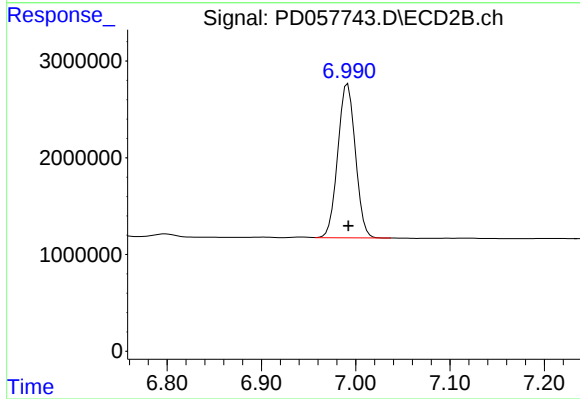


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 20650478
Conc: 19.91 ng/ml

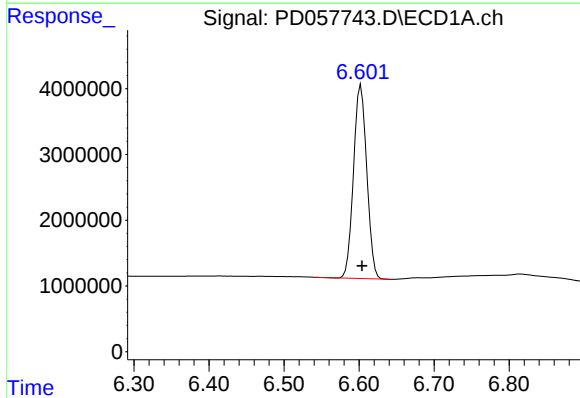


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: -0.002 min
Response: 36190849
Conc: 100.10 ng/ml

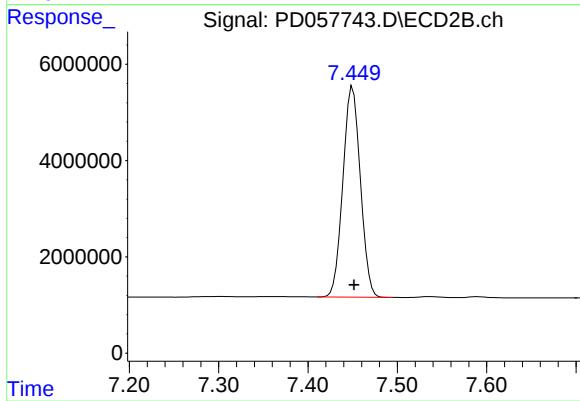

#20 Methoxychlor


R.T.: 7.450 min
Delta R.T.: -0.002 min
Response: 59421336
Conc: 104.67 ng/ml

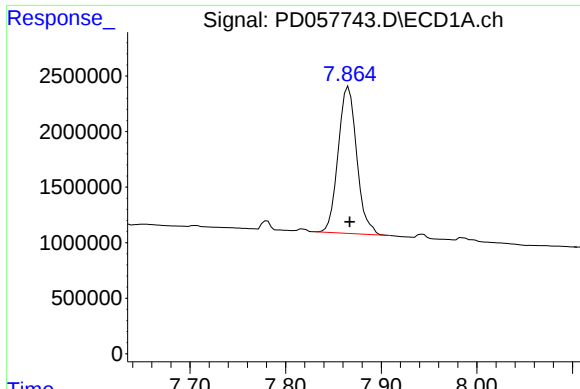

#27 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: -0.001 min
Response: 17824169
Conc: 21.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

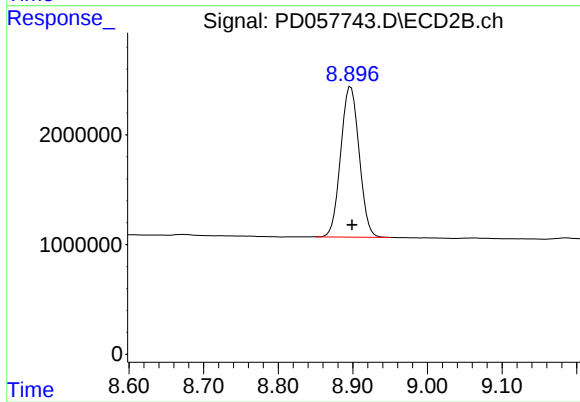

#27 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: -0.002 min
Response: 23540178
Conc: 21.55 ng/ml