

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
 Data File : PD057747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 14:20
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 07:25:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 08 07:20:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	28867619	38678578	40.317	40.001
27)	SA Decachlor...	7.867	8.898	64856492	82139038	78.119	75.192
Target Compounds							
2)	A alpha-BHC	3.649	4.280	43927794	56850584	42.567	41.778
3)	MA gamma-BHC...	3.921	4.560	41364768	53963173	41.460	41.389
4)	MA Heptachlor	4.201	5.061	35778023	53526228	41.344	40.747
9)	A Endosulfan I	5.196	6.098	33480623	46547863	40.907	40.244
13)	MA Dieldrin	5.435	6.354	76258992	103.4E6	83.650	81.620
14)	MA Endrin	5.686	6.569	64178604	87654742	81.990	81.242
16)	A 4,4'-DDD	5.823	6.695	58258142	82374466	83.255	81.200
17)	MA 4,4'-DDT	6.056	6.992	59490686	84902548	85.467	81.864
20)	A Methoxychlor	6.604	7.452	138.0E6	220.1E6	381.614	387.751


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 14:20
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:25:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:20:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

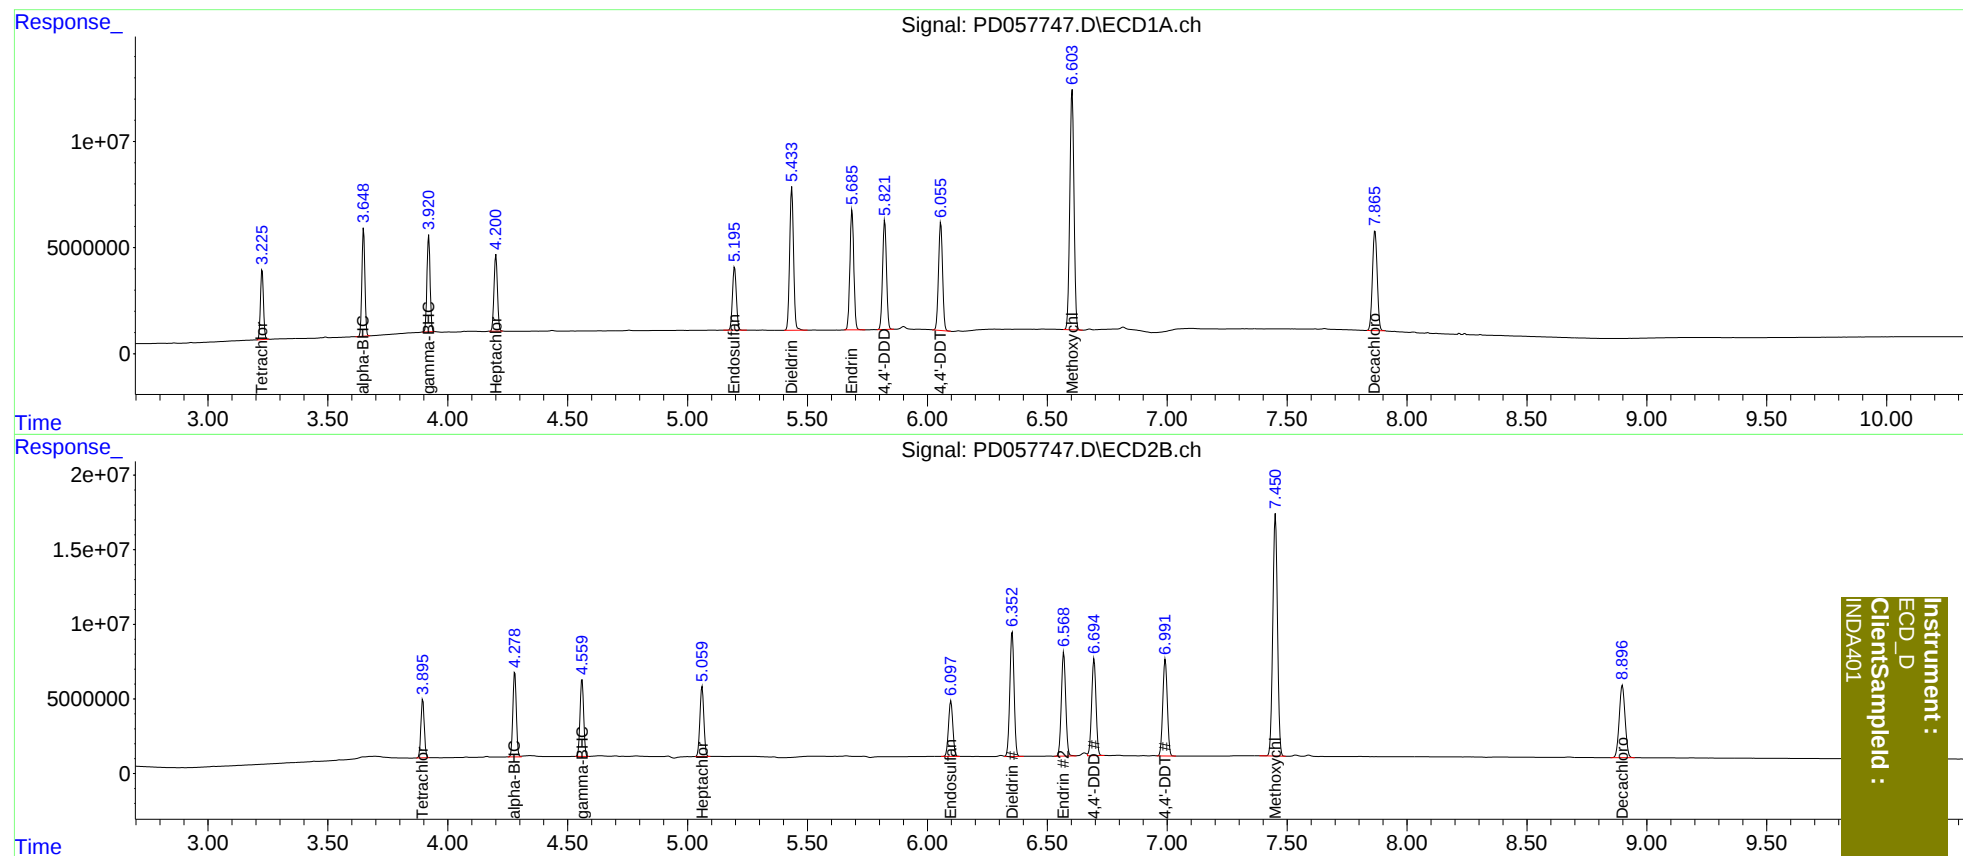


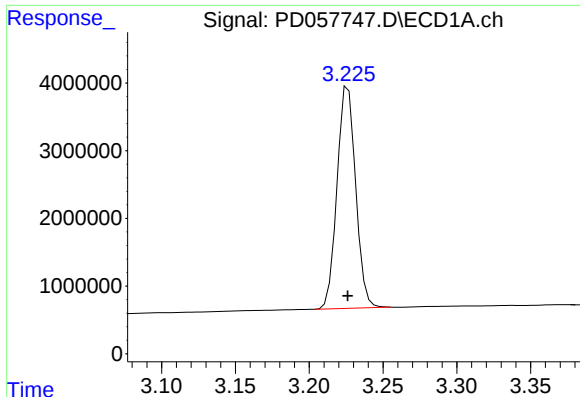

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 28867619
Conc: 40.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

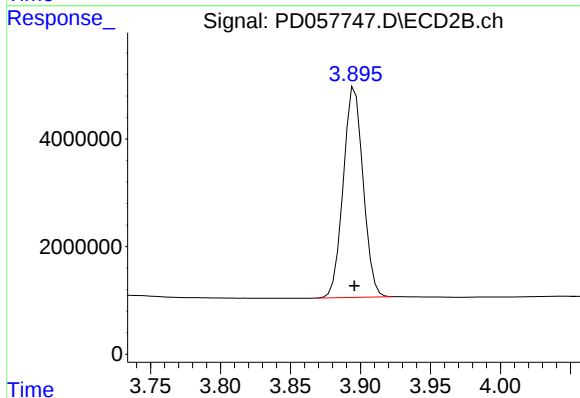


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 38678578
Conc: 40.00 ng/ml

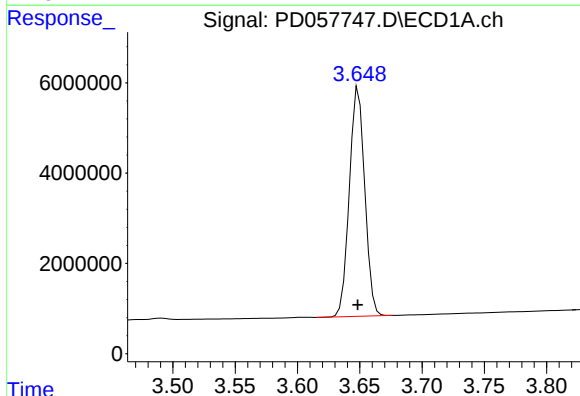


#2 alpha-BHC

R.T.: 3.649 min
Delta R.T.: 0.000 min
Response: 43927794
Conc: 42.57 ng/ml

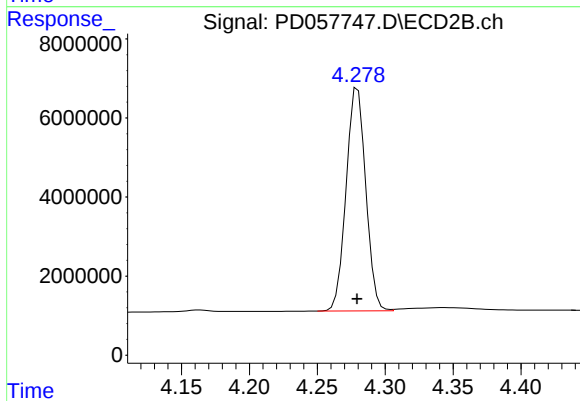

#2 alpha-BHC


R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 56850584
Conc: 41.78 ng/ml

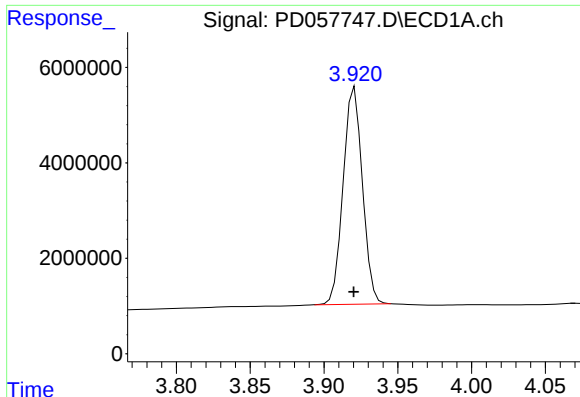

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 41364768
Conc: 41.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

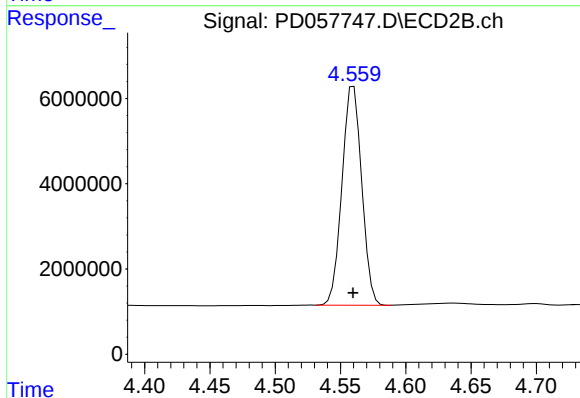


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 53963173
Conc: 41.39 ng/ml

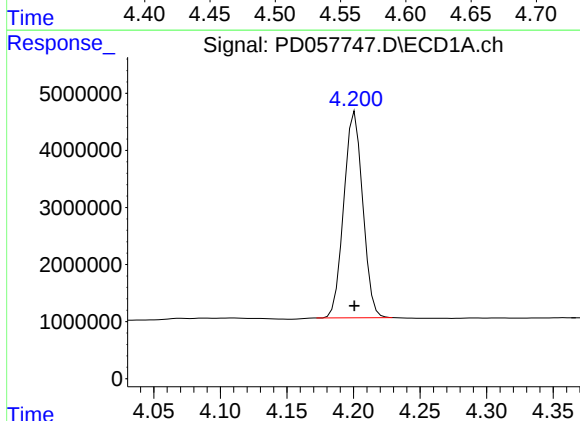


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 35778023
Conc: 41.34 ng/ml

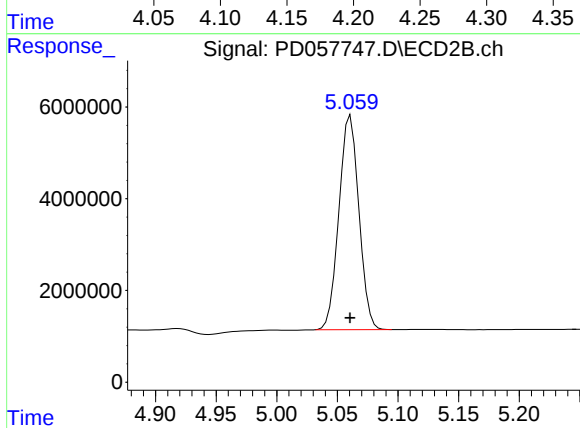

#4 Heptachlor


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 53526228
Conc: 40.75 ng/ml

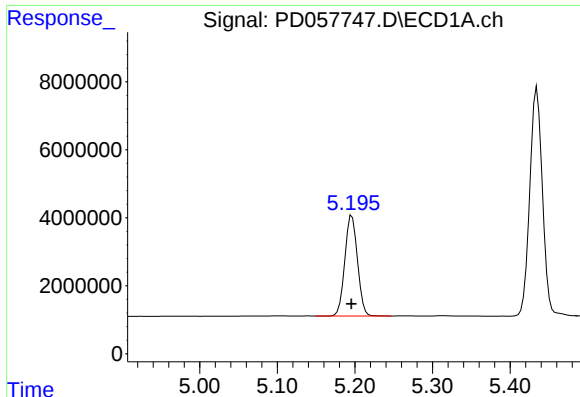

#9 Endosulfan I


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 33480623
Conc: 40.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

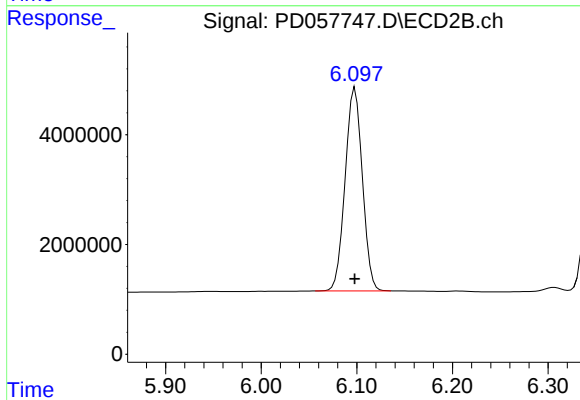


#9 Endosulfan I

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 46547863
Conc: 40.24 ng/ml

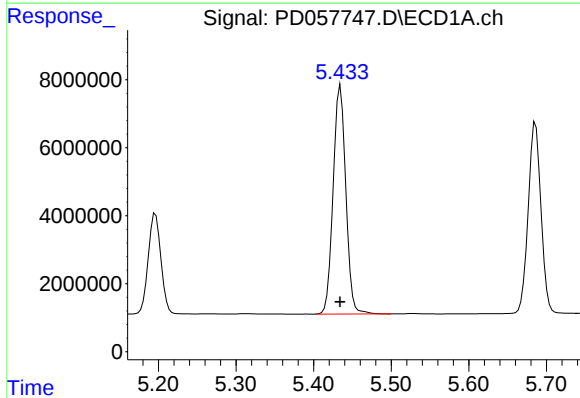


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 76258992
Conc: 83.65 ng/ml

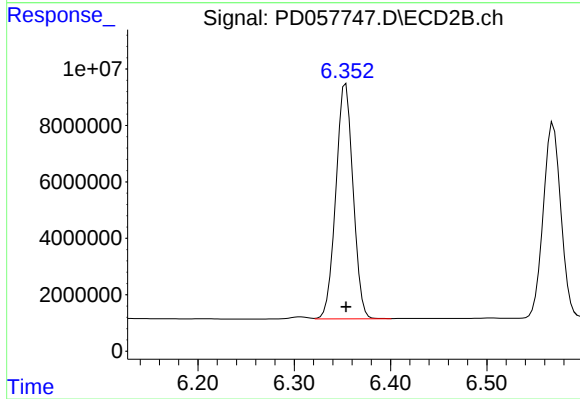

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 103409985
Conc: 81.62 ng/ml

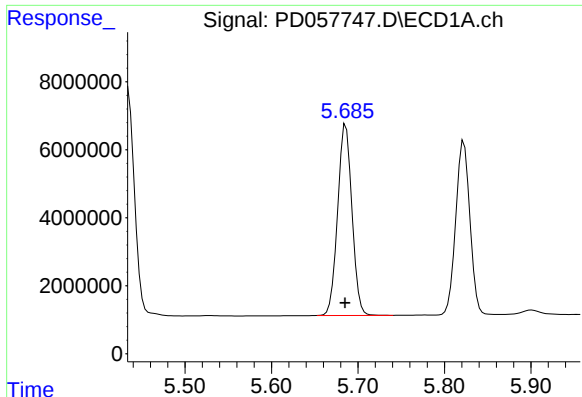

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.001 min
Response: 64178604
Conc: 81.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

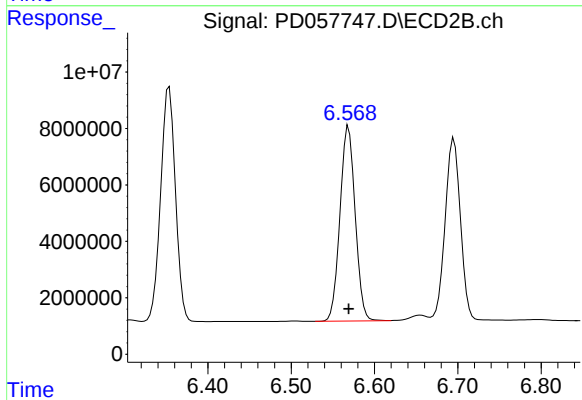


#14 Endrin

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 87654742
Conc: 81.24 ng/ml

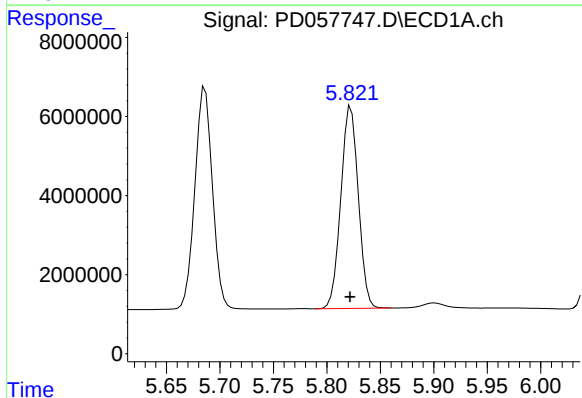


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 58258142
Conc: 83.25 ng/ml

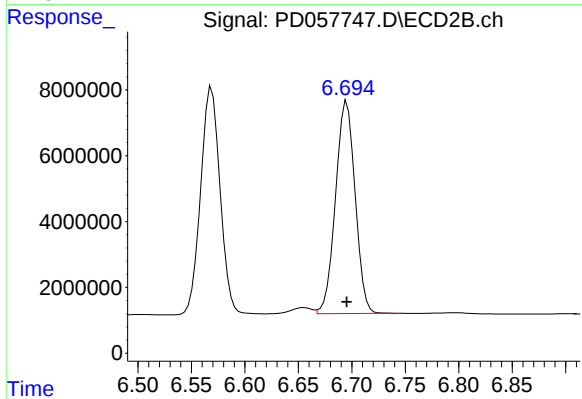

#16 4,4'-DDD


R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 82374466
Conc: 81.20 ng/ml

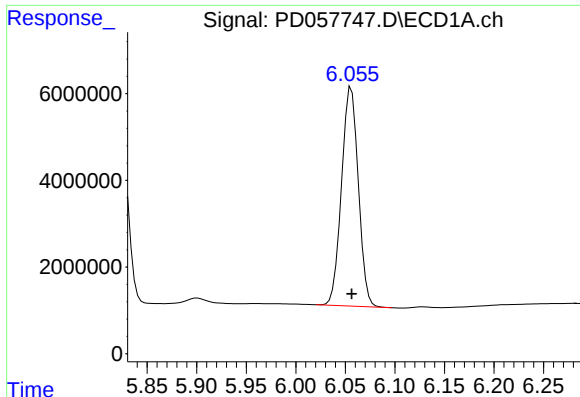

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 59490686
Conc: 85.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

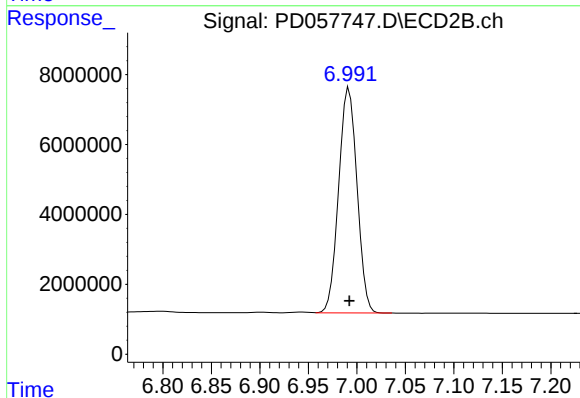


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 84902548
Conc: 81.86 ng/ml

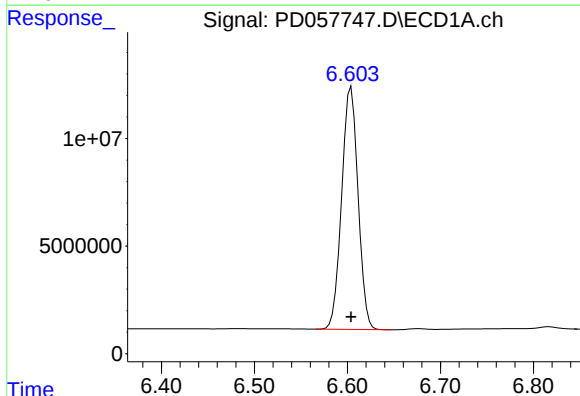


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 137973720
Conc: 381.61 ng/ml

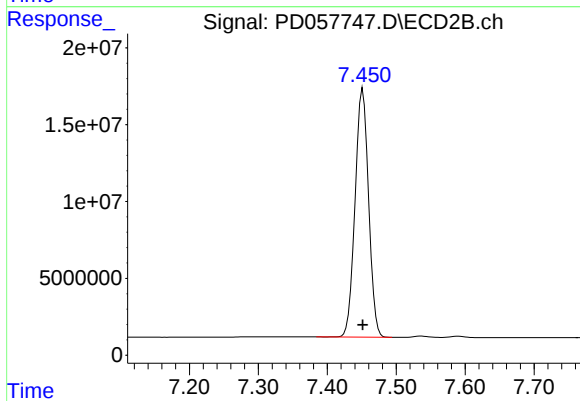

#20 Methoxychlor


R.T.: 7.452 min
Delta R.T.: 0.000 min
Response: 220128825
Conc: 387.75 ng/ml

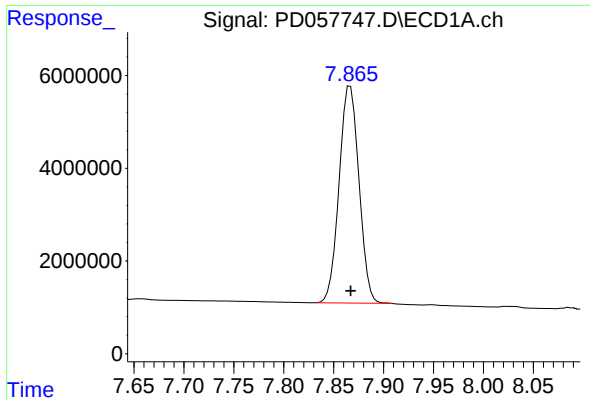

#27 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 64856492
Conc: 78.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

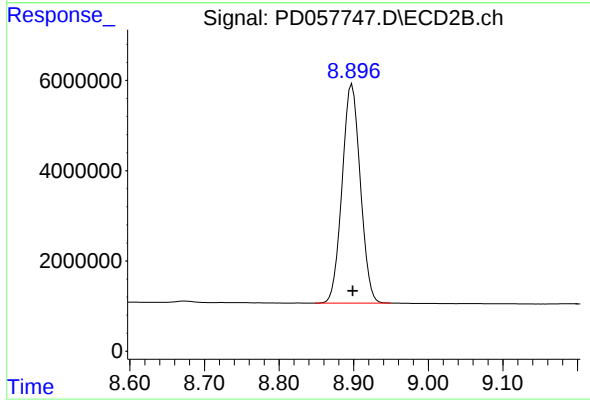

#27 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: -0.001 min
Response: 82139038
Conc: 75.19 ng/ml