

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
 Data File : PD057749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 14:48
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 07:35:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 08 07:20:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	58123816	77538136	81.177	80.190
27)	SA Decachlor...	7.866	8.899	129.0E6	156.1E6	155.328	142.915
Target Compounds							
2)	A alpha-BHC	3.649	4.280	92537306	118.8E6	89.671	87.305
3)	MA gamma-BHC...	3.920	4.560	85893628	111.3E6	86.092	85.387
4)	MA Heptachlor	4.201	5.061	74505062	109.7E6	86.096	83.477
9)	A Endosulfan I	5.196	6.099	68956183	93991785	84.251	81.263
13)	MA Dieldrin	5.434	6.354	158.8E6	211.4E6	174.182	166.863
14)	MA Endrin	5.686	6.569	130.6E6	178.1E6	166.859	165.038
16)	A 4,4'-DDD	5.822	6.696	121.7E6	168.5E6	173.882	166.136
17)	MA 4,4'-DDT	6.056	6.993	126.1E6	174.6E6	181.112	168.386
20)	A Methoxychlor	6.603	7.452	268.9E6	426.2E6	743.624	750.782


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 14:48
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:35:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:20:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

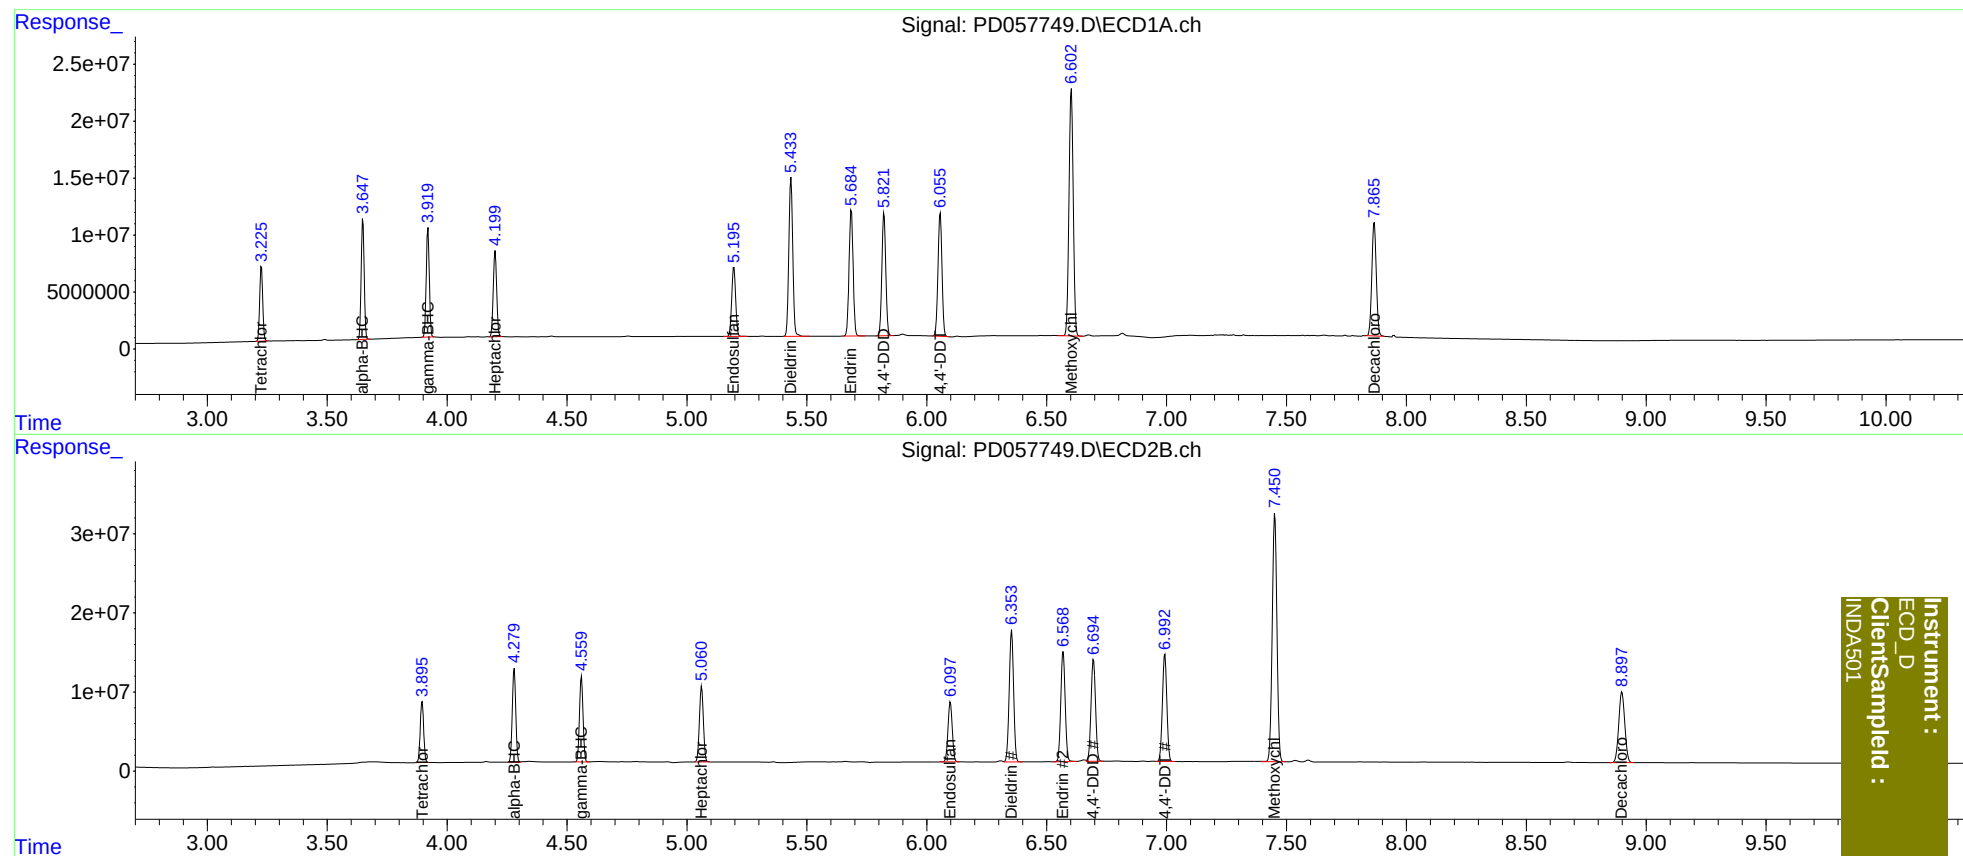


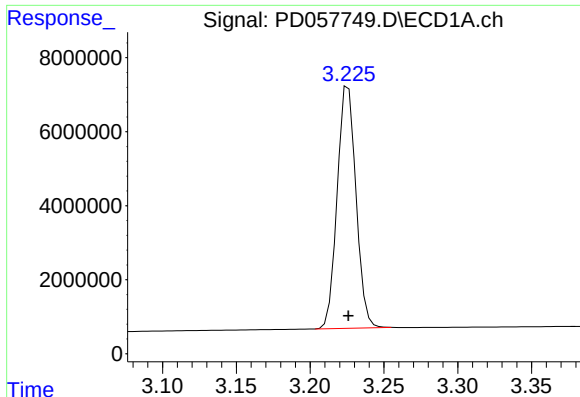

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 58123816
Conc: 81.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

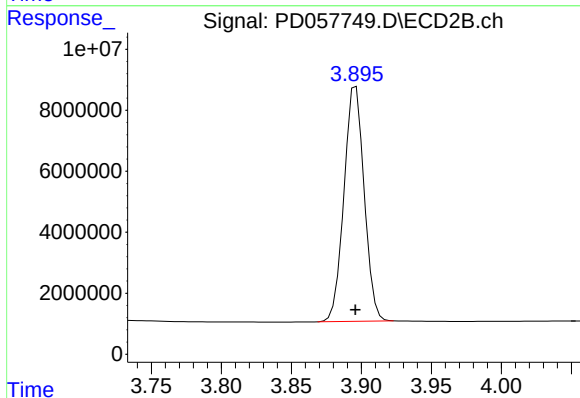


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 77538136
Conc: 80.19 ng/ml

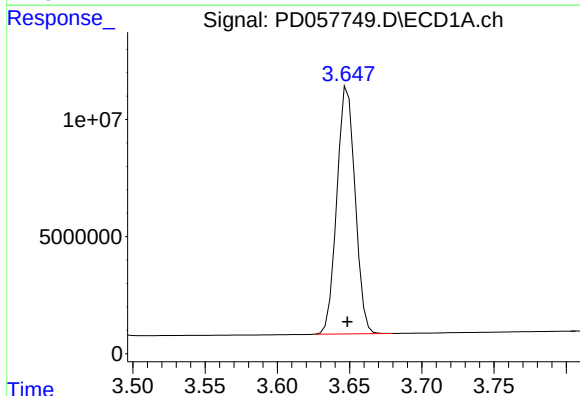


#2 alpha-BHC

R.T.: 3.649 min
Delta R.T.: 0.000 min
Response: 92537306
Conc: 89.67 ng/ml

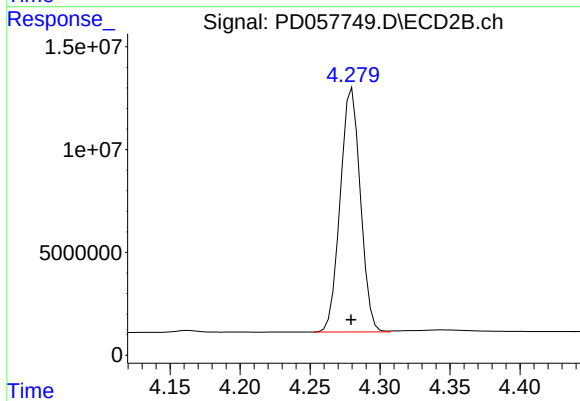

#2 alpha-BHC


R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 118803128
Conc: 87.31 ng/ml

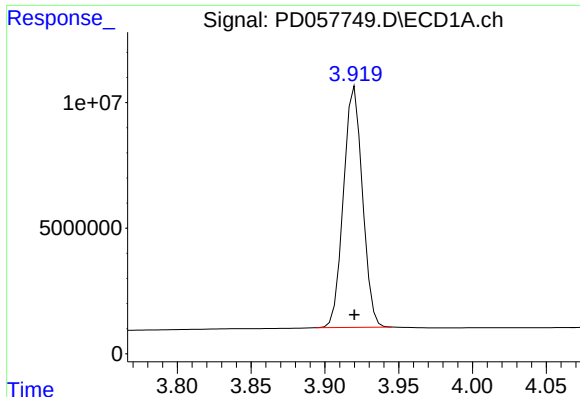

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 85893628
Conc: 86.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

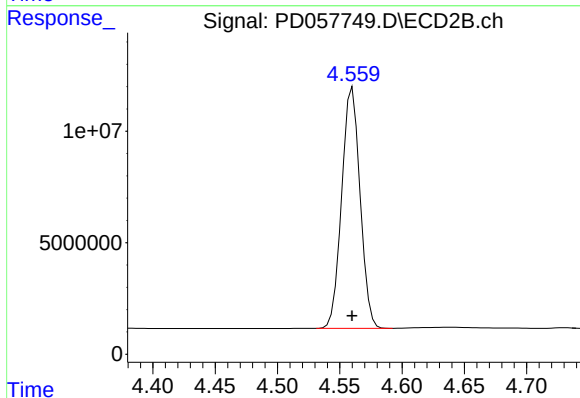


#3 gamma-BHC (Lindane)

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 111329528
Conc: 85.39 ng/ml

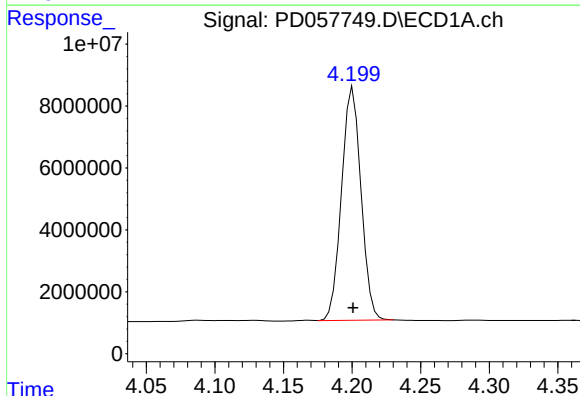


#4 Heptachlor

R.T.: 4.201 min
Delta R.T.: 0.000 min
Response: 74505062
Conc: 86.10 ng/ml

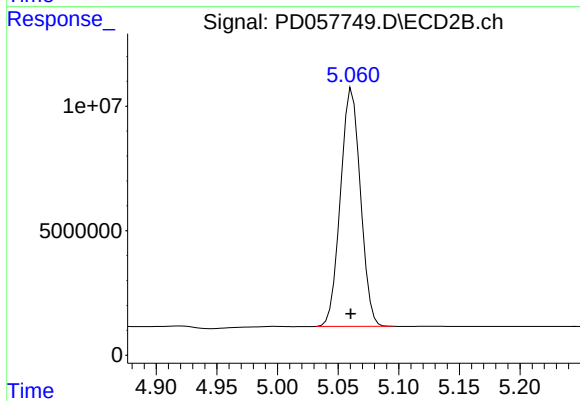

#4 Heptachlor


R.T.: 5.061 min
Delta R.T.: 0.001 min
Response: 109658639
Conc: 83.48 ng/ml

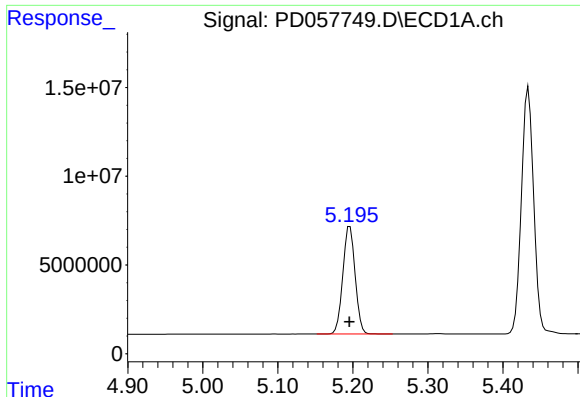

#9 Endosulfan I


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 68956183
Conc: 84.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

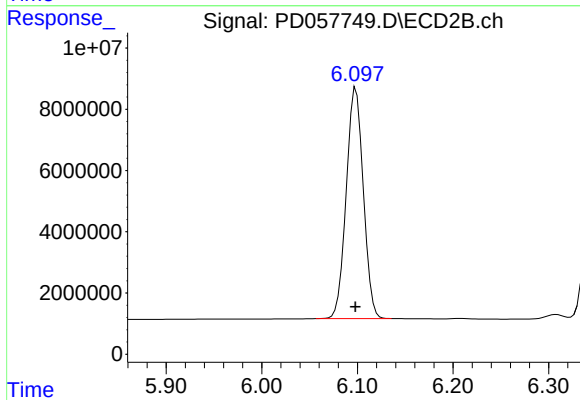


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 93991785
Conc: 81.26 ng/ml

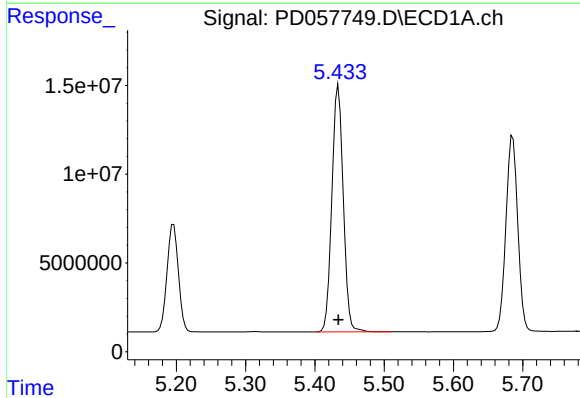


#13 Dieldrin

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 158791417
Conc: 174.18 ng/ml

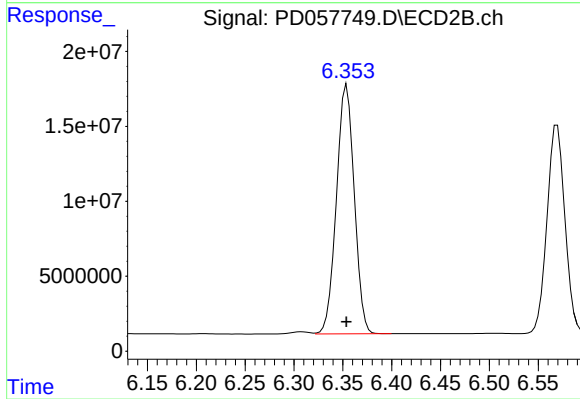

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 211409811
Conc: 166.86 ng/ml

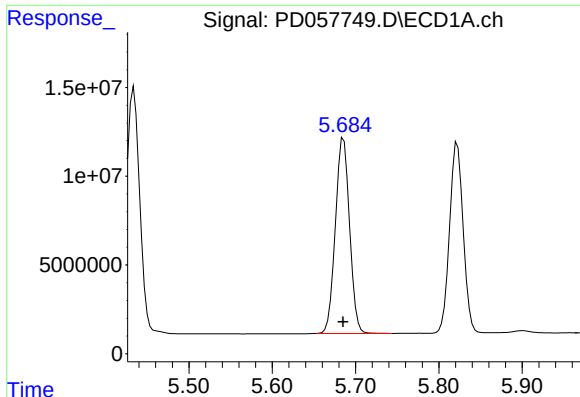

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 130611630
Conc: 166.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

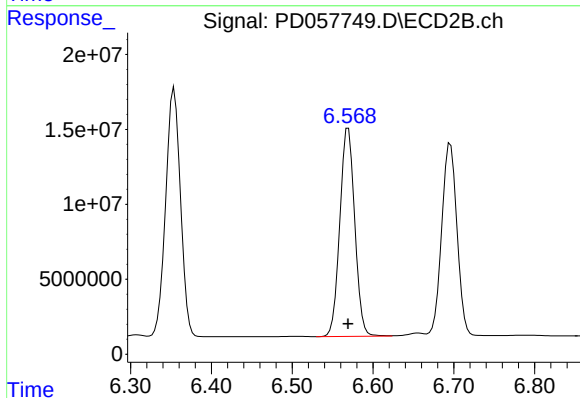


#14 Endrin

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 178065639
Conc: 165.04 ng/ml

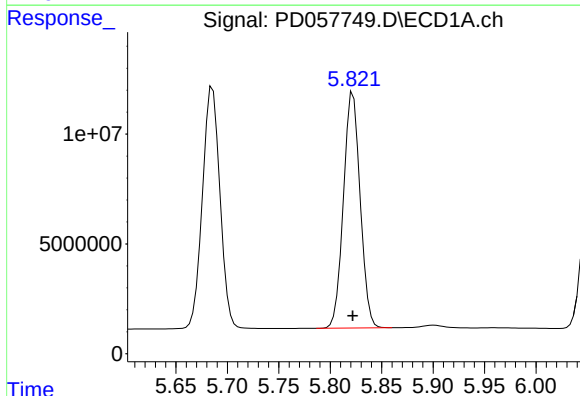


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 121674866
Conc: 173.88 ng/ml

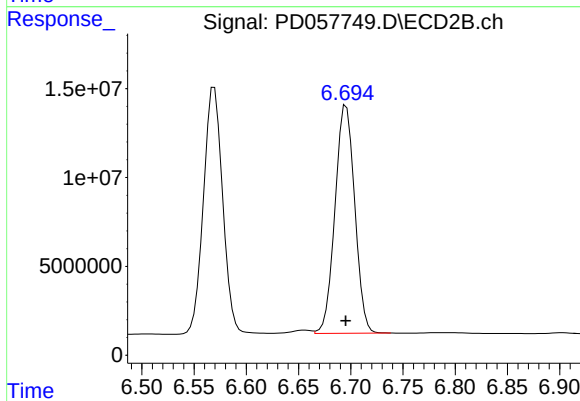

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 168537809
Conc: 166.14 ng/ml

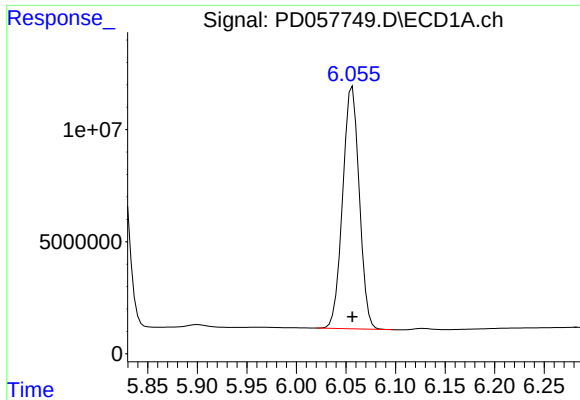

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 126065762
Conc: 181.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

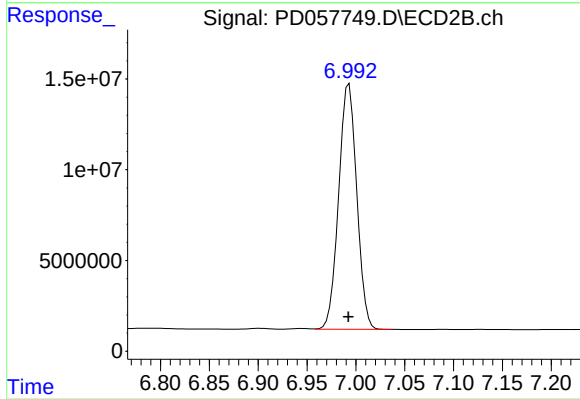


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 174636296
Conc: 168.39 ng/ml

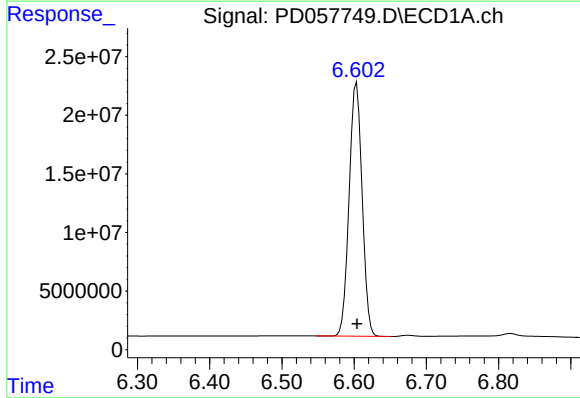


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 268859650
Conc: 743.62 ng/ml

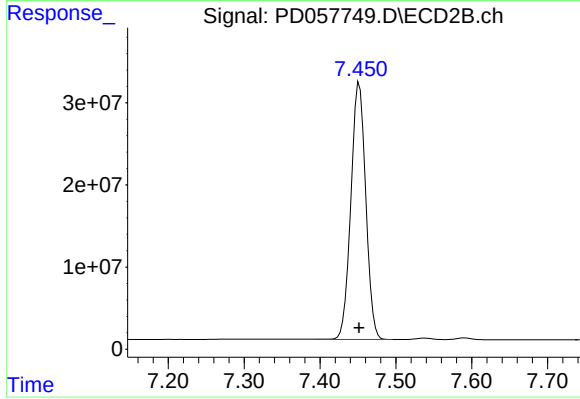

#20 Methoxychlor


R.T.: 7.452 min
Delta R.T.: 0.000 min
Response: 426223616
Conc: 750.78 ng/ml

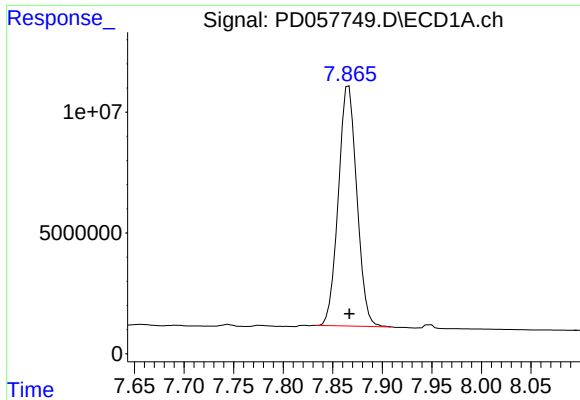

#27 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 128957750
Conc: 155.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

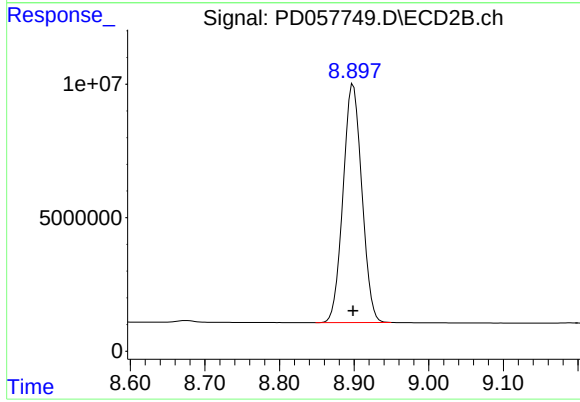

#27 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 156119528
Conc: 142.92 ng/ml