

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
 Data File : PD057734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 11:18
 Operator : AJ\MA
 Sample : RESC01
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 07:54:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 08 07:44:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	13961237	18590713	19.182	19.190
2)	SA Decachlor...	7.866	8.898	31600432	41353392	37.428	37.762
Target Compounds							
2)	A alpha-BHC	3.649	4.280	9339440	12237409	8.900	8.934
3)	MA gamma-BHC...	3.920	4.560	9605352	11761613	9.357	8.976
4)	MA Heptachlor	4.200	5.061	8195478	11968148	9.188	9.009
5)	MB Aldrin	4.436	5.362	8893224	12579736	9.394	9.506
6)	B beta-BHC	4.169	4.730	4399443	6135408	9.452	9.541
7)	B delta-BHC	4.360	4.943	9266310	8089611	8.778	6.846
8)	B Heptachlo...	4.869	5.744	8233975	11216267	9.482	9.267
9)	A Endosulfan I	5.195	6.098	7927135	10879325	9.541	9.311
10)	B trans-Chl...	5.089	5.977	8999867	11864867	10.017	9.476
11)	B cis-Chlor...	5.145	6.050	8913871	12191899	9.923	9.628
12)	B 4,4'-DDE	5.314	6.208	16649983	22194102	18.687	18.484
13)	MA Dieldrin	5.433	6.354	16591588	22356193	17.841	17.566
14)	MA Endrin	5.685	6.569	14734402	19851972	18.512	18.302
15)	B Endosulfa...	5.958	6.778	15074762	19795098	19.135	18.246
16)	A 4,4'-DDD	5.822	6.694	12739221	18590612	17.884	18.213
17)	MA 4,4'-DDT	6.055	6.992	12573964	19407746	17.793	18.651
18)	B Endrin al...	6.126	6.901	12837997	17624417	19.064	18.750
19)	B Endosulfa...	6.335	7.124	14969764	20596302	18.384	18.758
20)	A Methoxychlor	6.604	7.451	32842409	54266538	93.404	95.538
21)	B Endrin ke...	6.817	7.591	17859976	21929778	19.046	18.996

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:54:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:44:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

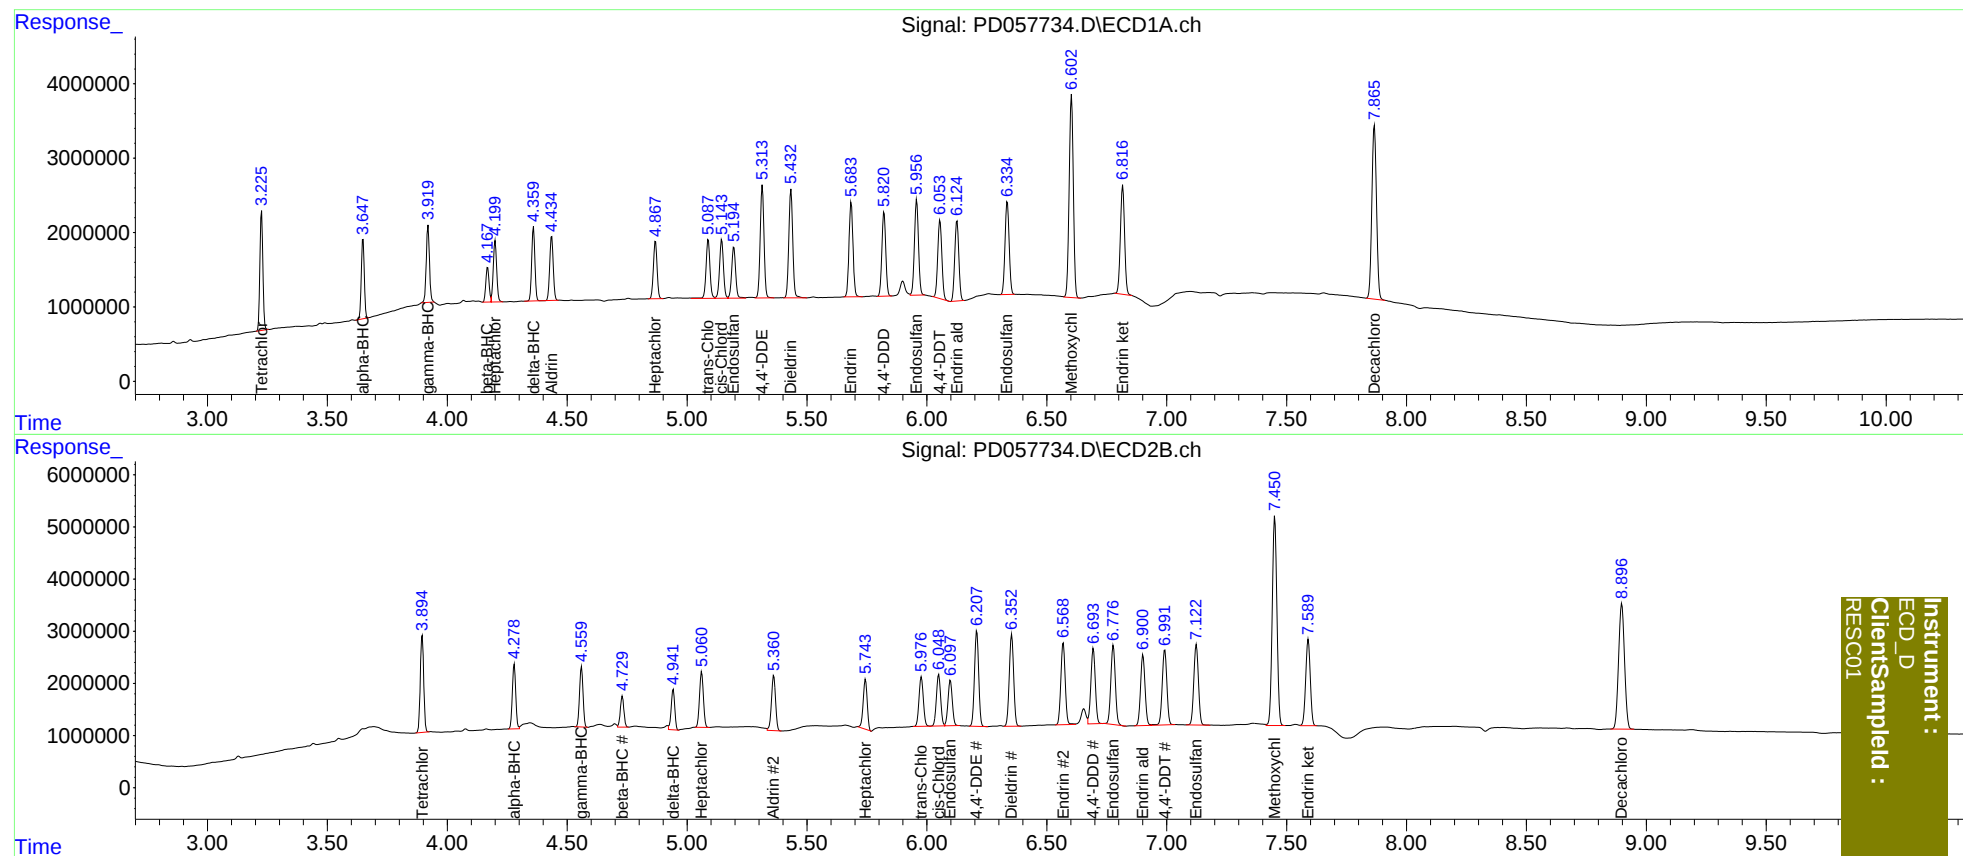

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Title : GC Extractables
Last Update : Wed Apr 08 07:44:07 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.226	3.649	100.00%
3.649	3.920	100.00%
3.920	4.169	100.00%
4.169	4.200	86.77%
4.200	4.360	100.00%
4.360	4.436	100.00%
4.436	4.869	100.00%
4.869	5.089	100.00%
5.089	5.145	99.56%
5.145	5.195	98.17%
5.195	5.314	100.00%
5.314	5.433	100.00%
5.433	5.685	100.00%
5.685	5.822	100.00%
5.822	5.958	100.00%
5.958	6.055	100.00%
6.055	6.126	100.00%
6.126	6.335	100.00%
6.335	6.604	100.00%
6.604	6.817	100.00%
6.817	7.866	100.00%

Signal #2


3.896	4.280	100.00%
4.280	4.560	100.00%
4.560	4.730	100.00%
4.730	4.943	100.00%
4.943	5.061	100.00%
5.061	5.362	100.00%
5.362	5.744	100.00%
5.744	5.977	100.00%
5.977	6.050	100.00%
6.050	6.098	97.98%
6.098	6.208	100.00%
6.208	6.354	100.00%
6.354	6.569	100.00%
6.569	6.694	100.00%
6.694	6.778	100.00%
6.778	6.901	100.00%
6.901	6.992	99.90%
6.992	7.124	100.00%
7.124	7.451	100.00%
7.451	7.591	100.00%
7.591	8.898	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:54:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:44:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

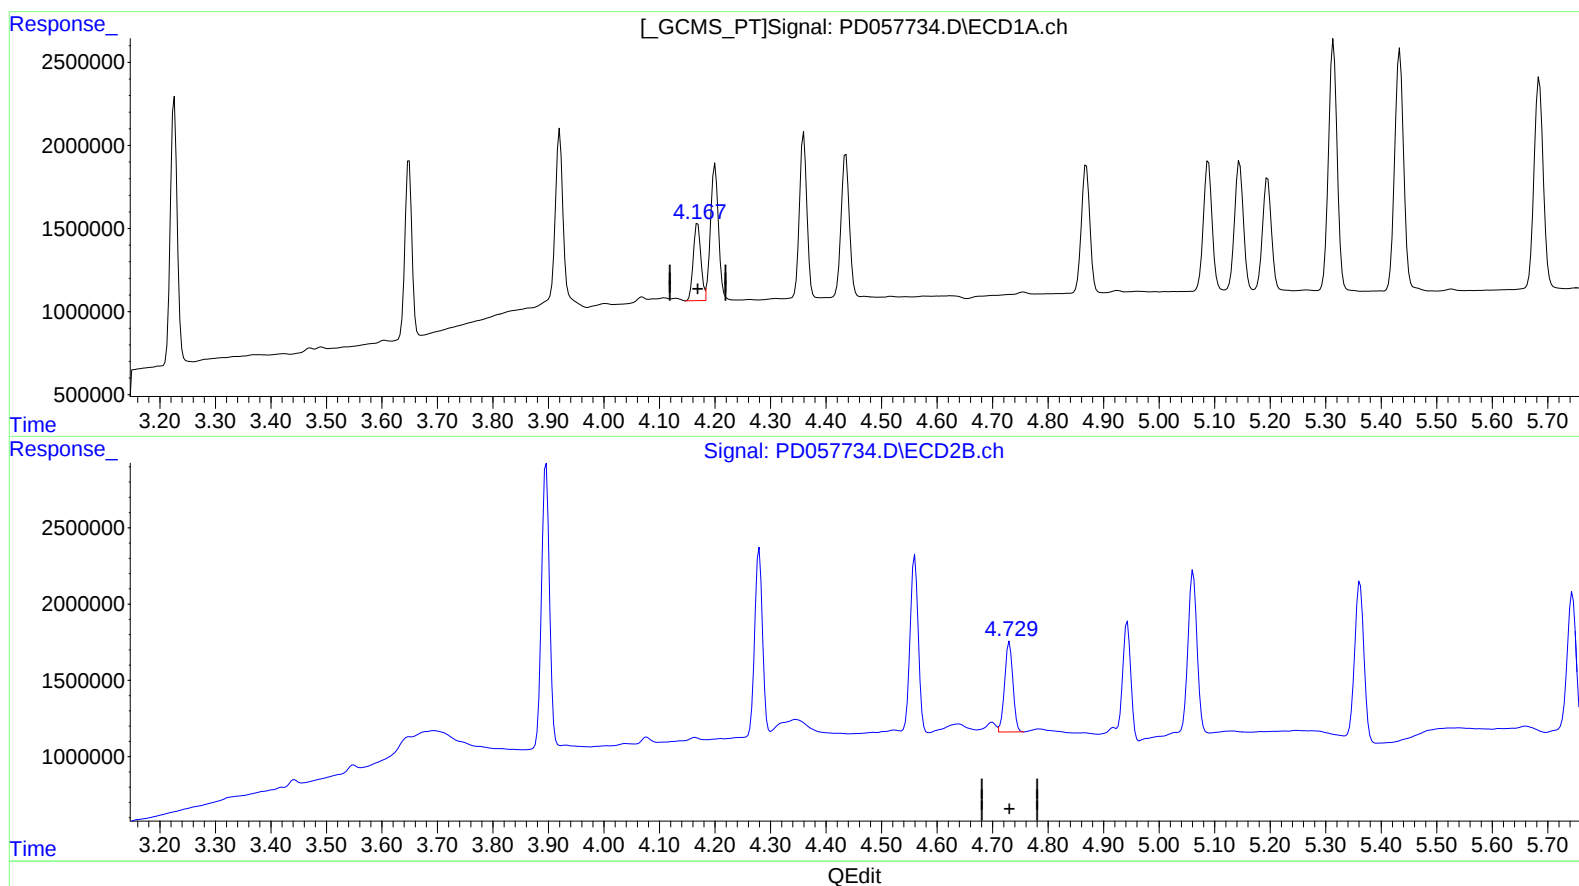

(6) beta-BHC (B)
4.169min 9.452 ng/ml
response 4399443


(6) beta-BHC #2 (B)
4.730min 9.541 ng/ml
response 6135408

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:54:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:44:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

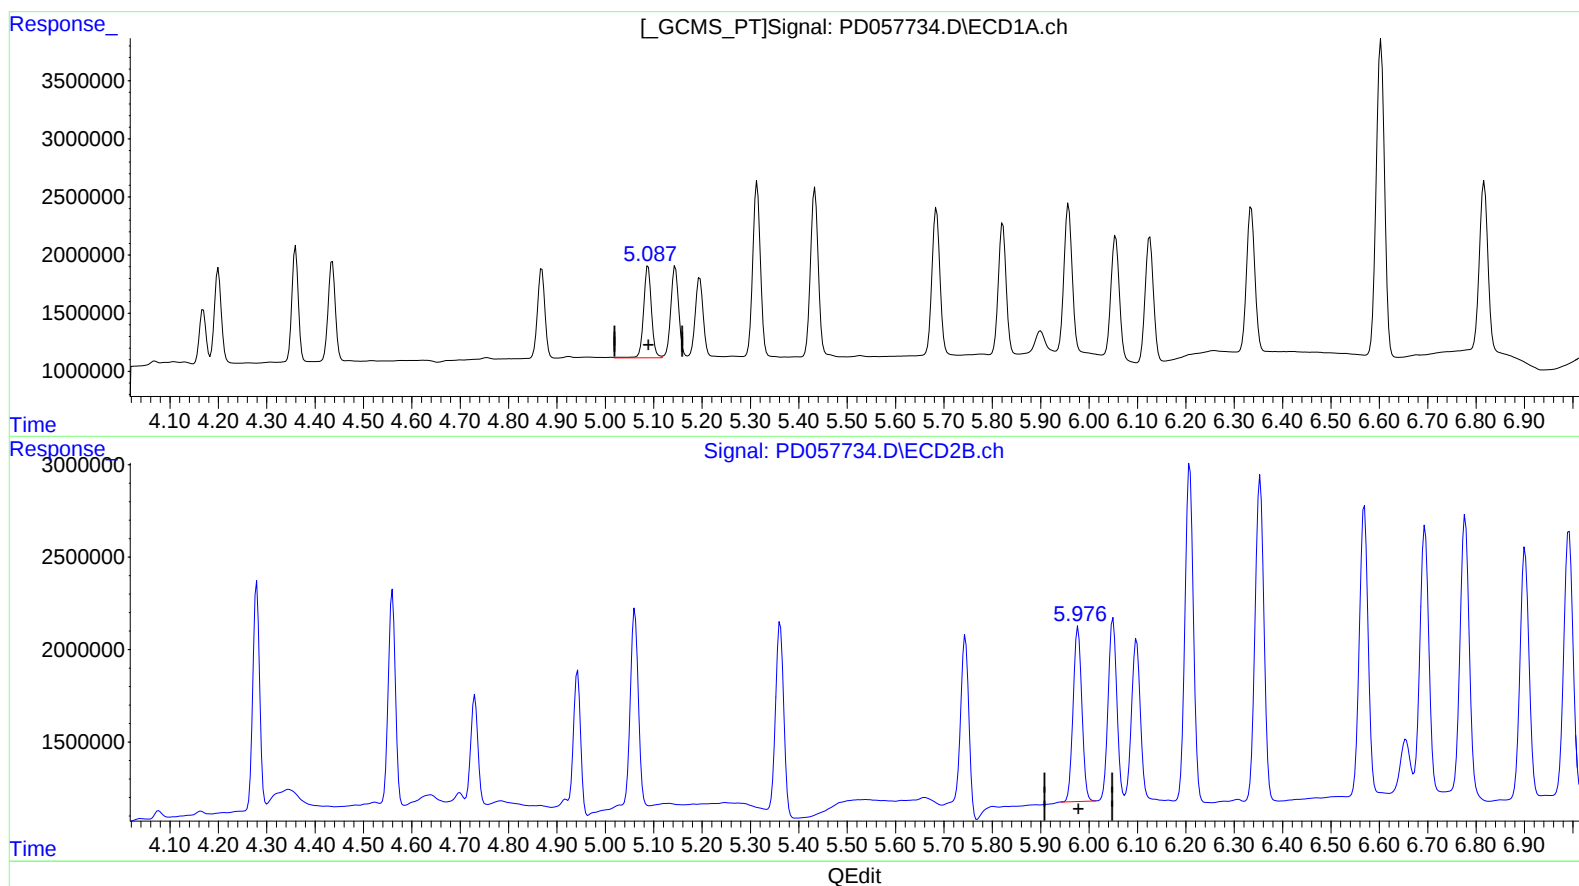

(10) trans-Chlordane (B)

5.089min 10.017 ng/ml

response 8999867

(10) trans-Chlordane #2 (B)

5.977min 9.476 ng/ml


response 11864867

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:54:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:44:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

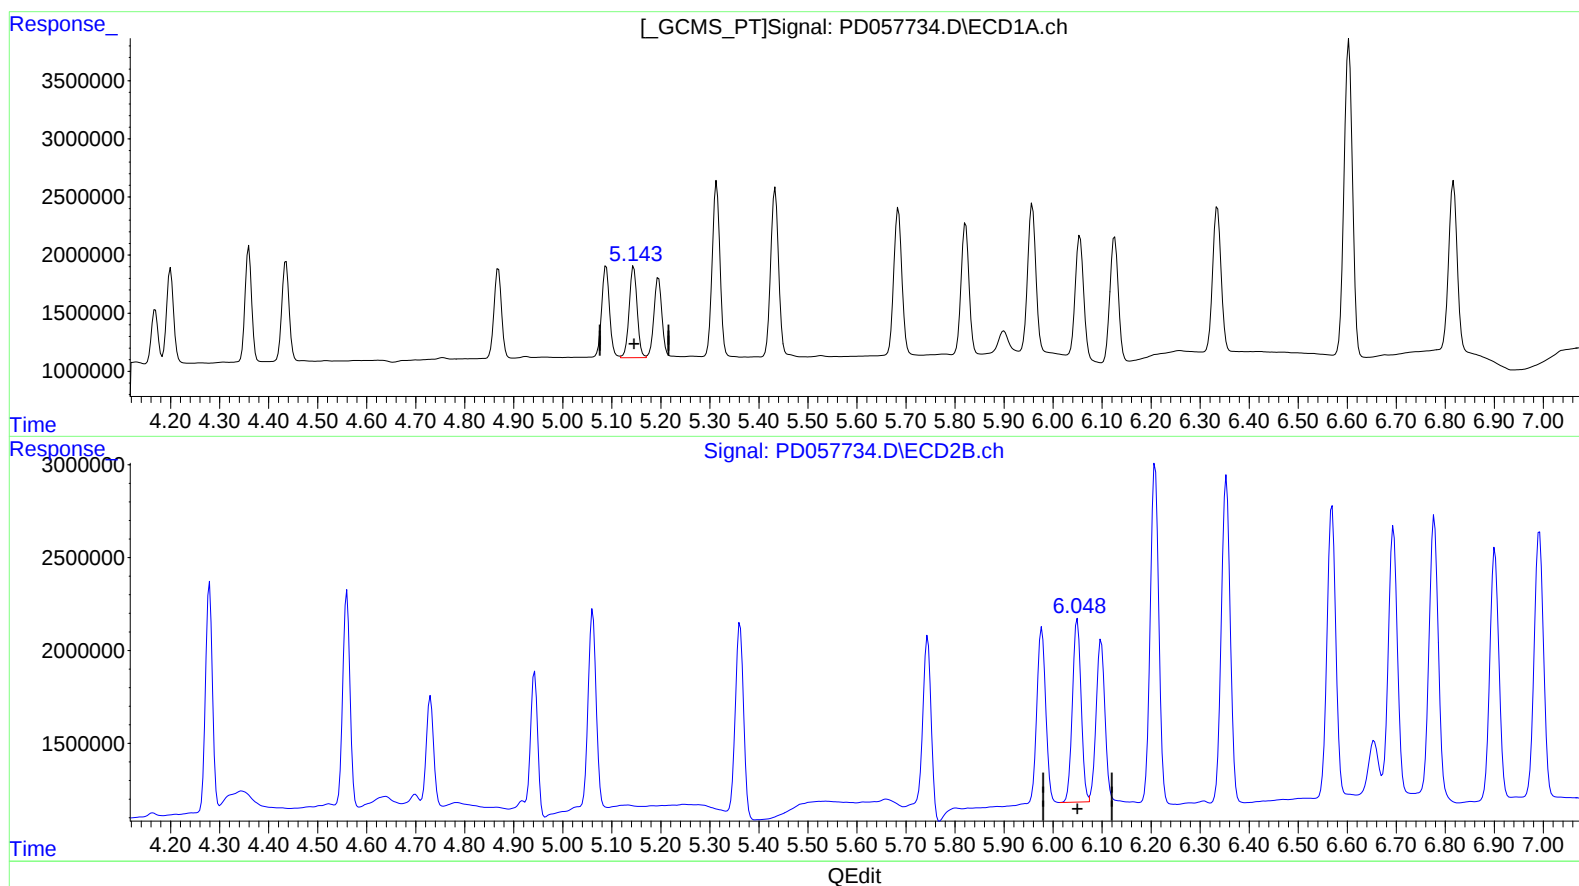

(11) cis-Chlordane (B)

5.145min 9.923 ng/ml

response 8913871

(11) cis-Chlordane #2 (B)

6.050min 9.628 ng/ml


response 12191899

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040720\
Data File : PD057734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 11:18
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 07:54:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040720CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 08 07:44:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

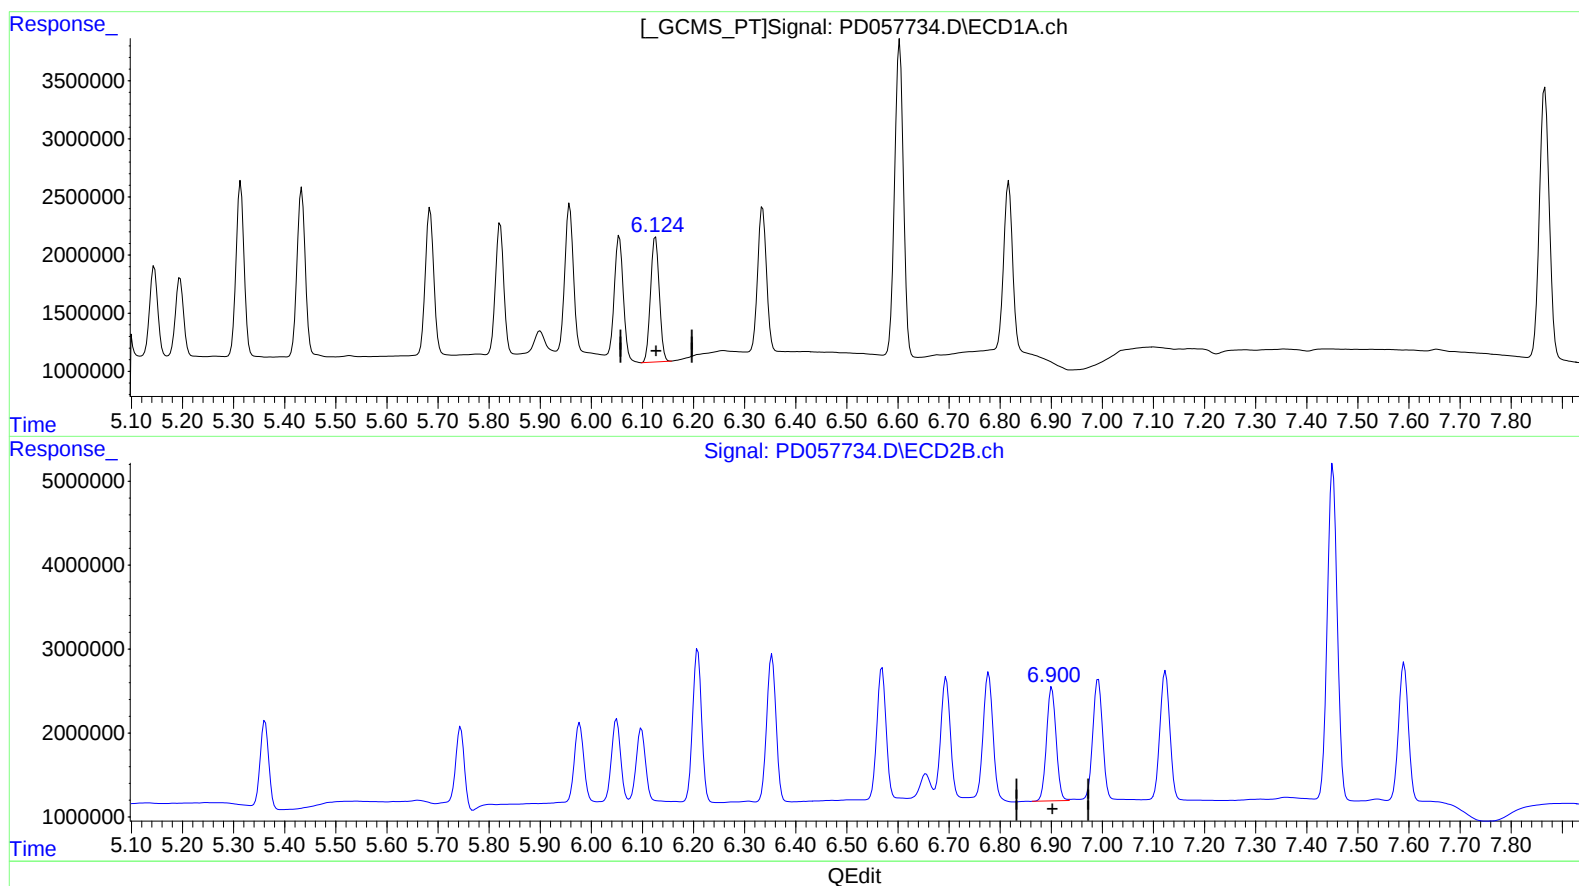

(18) Endrin aldehyde (B)

6.126min 19.064 ng/ml

response 12837997

(18) Endrin aldehyde #2 (B)

6.901min 18.750 ng/ml

response 17624417