

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD061999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 11:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:34:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) MB	Aldrin	0.000	5.482	0	2756483	N.D. 0.222 #
7) B	delta-BHC	0.000	5.036	0	7810538	N.D. 0.590 #
8) B	Heptachlo...	0.000	5.865	0	4149222	N.D. 0.350 #
9) A	Endosulfan I	0.000	6.211	0	1342827	N.D. 0.124 #
10) B	gamma-Chl...	0.000	6.078	0	1165212	N.D. 0.098 #
14) MA	Endrin	0.000	6.667f	0	264756	N.D. 0.027 #
17) MA	4,4'-DDT	0.000	7.106	0	386224	N.D. 0.040 #
19) B	Endosulfa...	0.000	7.252	0	906537	N.D. 0.090 #
25)	Chlordane-3	0.000	6.078	0	1165212	N.D. 0.703 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD061999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 11:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:34:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

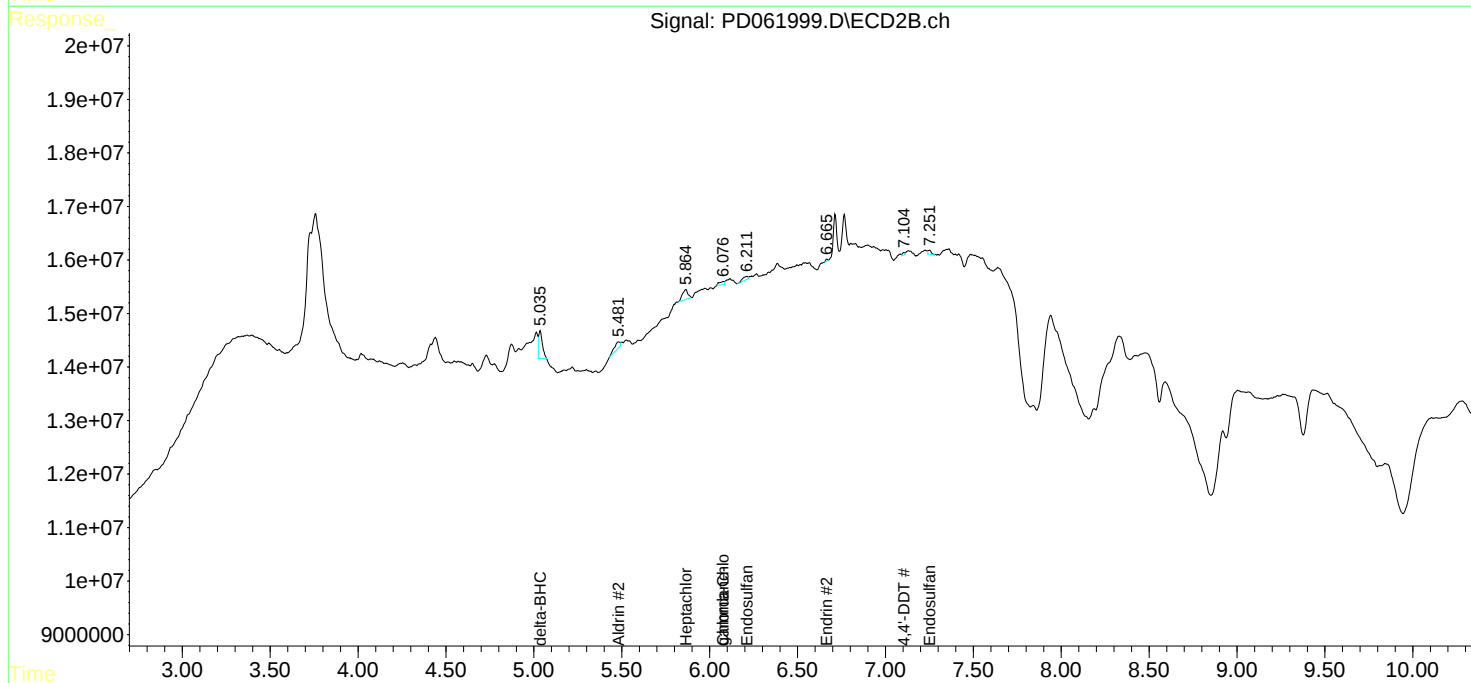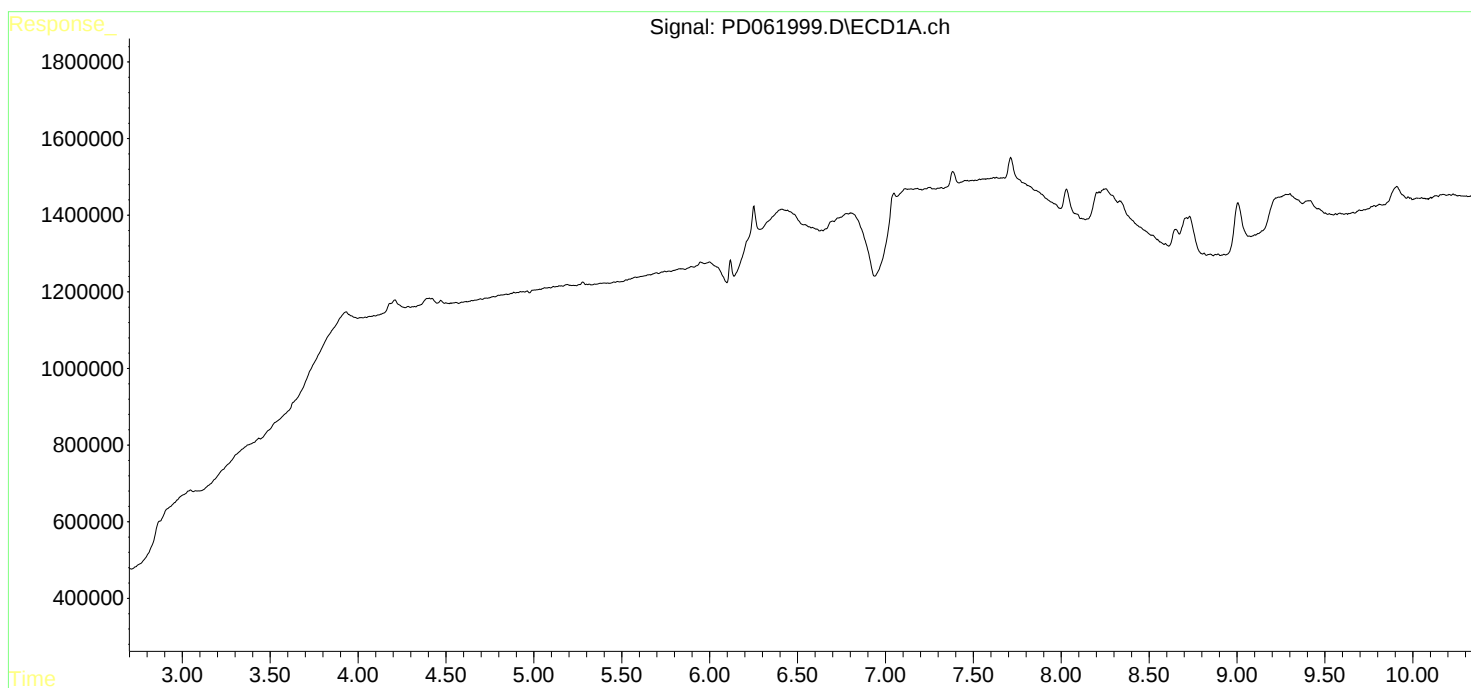


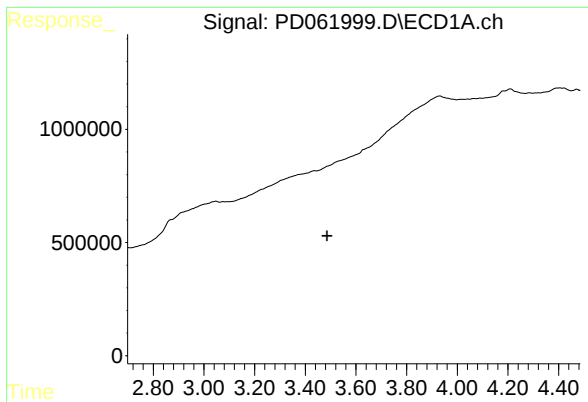

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

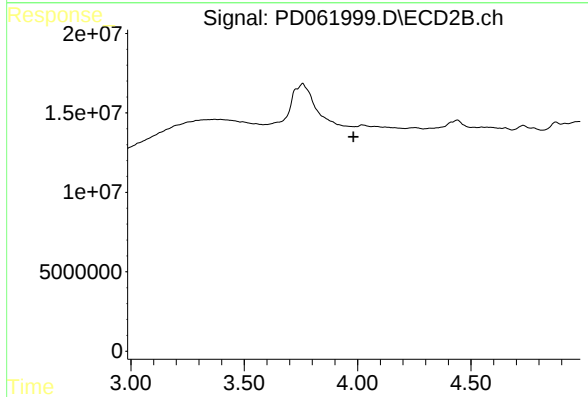


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.982 min
Response: 0
Conc: N.D.

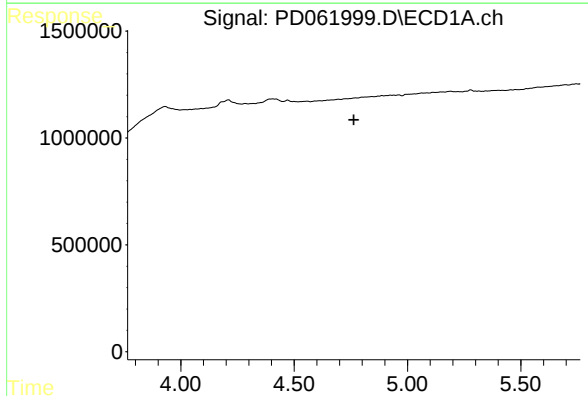


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

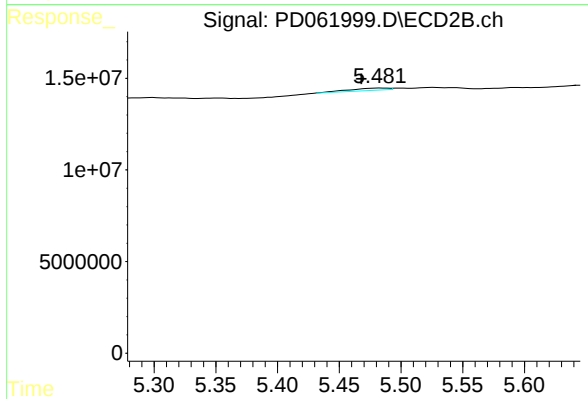

#5 Aldrin


R.T.: 5.482 min
Delta R.T.: 0.014 min
Response: 2756483
Conc: 0.22 ng/ml

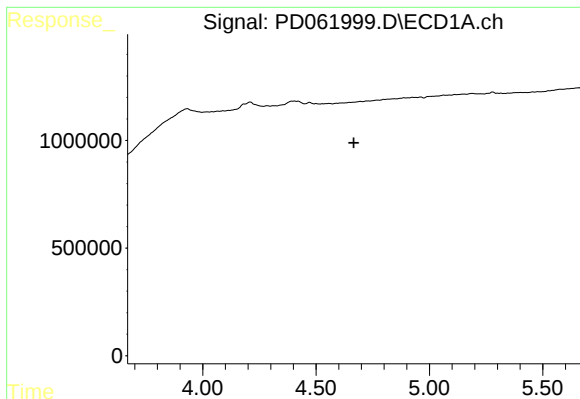

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

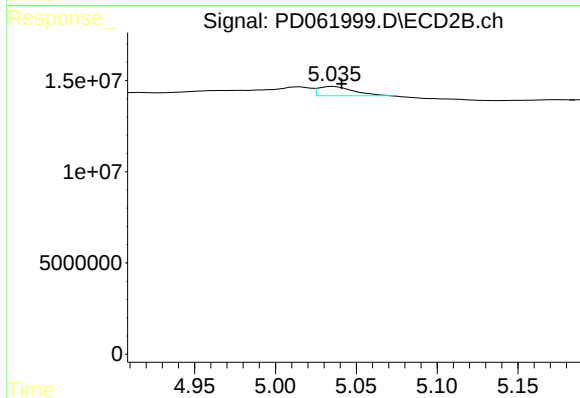


#7 delta-BHC

R.T.: 5.036 min
Delta R.T.: -0.005 min
Response: 7810538
Conc: 0.59 ng/ml

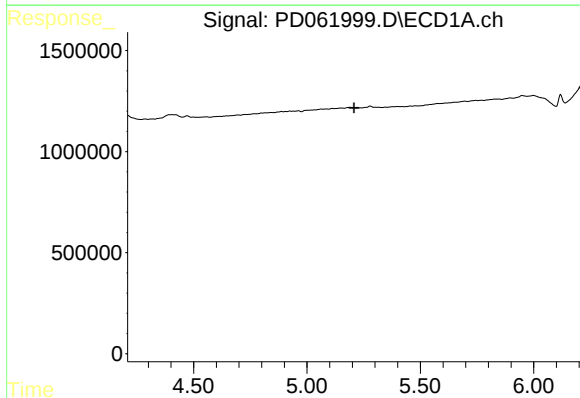


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

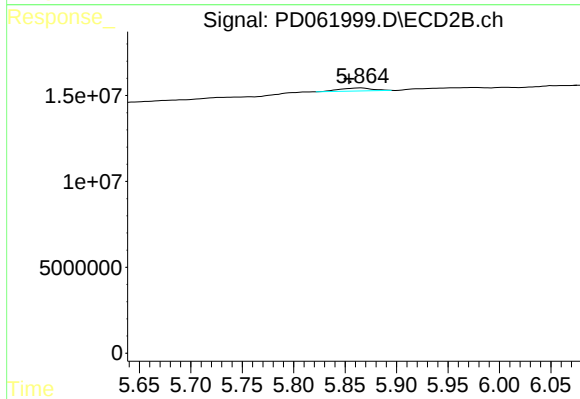

#8 Heptachlor epoxide


R.T.: 5.865 min
Delta R.T.: 0.012 min
Response: 4149222
Conc: 0.35 ng/ml

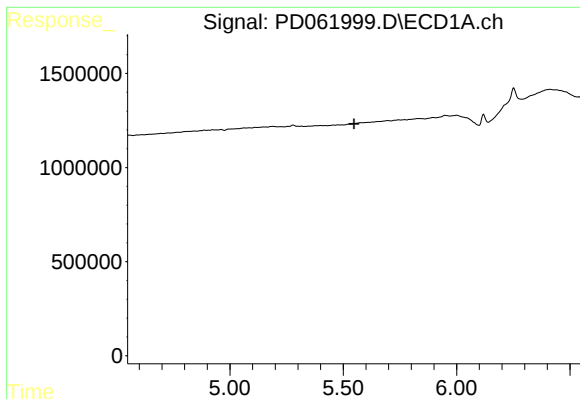

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

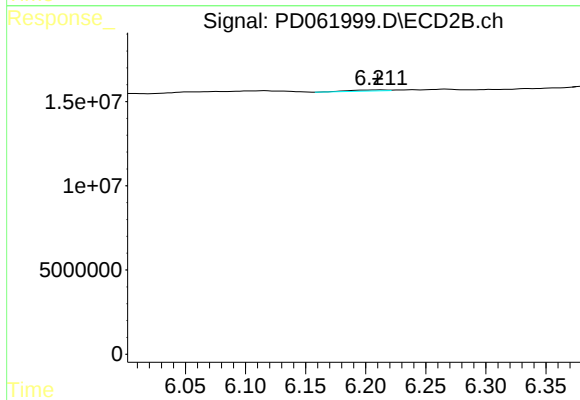


#9 Endosulfan I

R.T.: 6.211 min
Delta R.T.: 0.001 min
Response: 1342827
Conc: 0.12 ng/ml

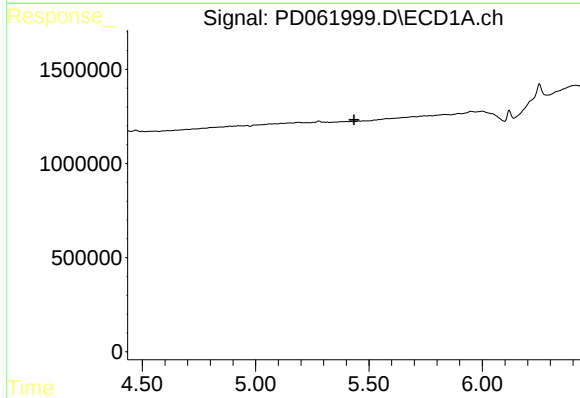


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

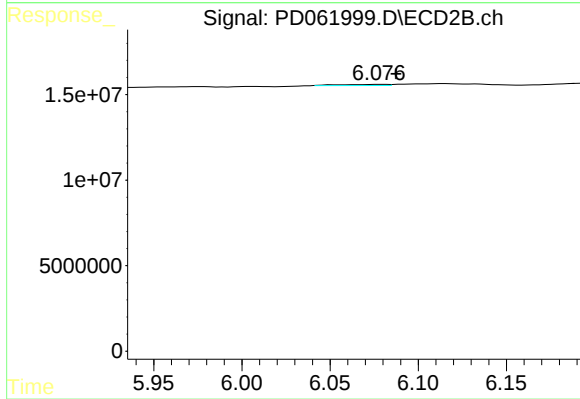

#10 gamma-Chlordane


R.T.: 6.078 min
Delta R.T.: -0.009 min
Response: 1165212
Conc: 0.10 ng/ml

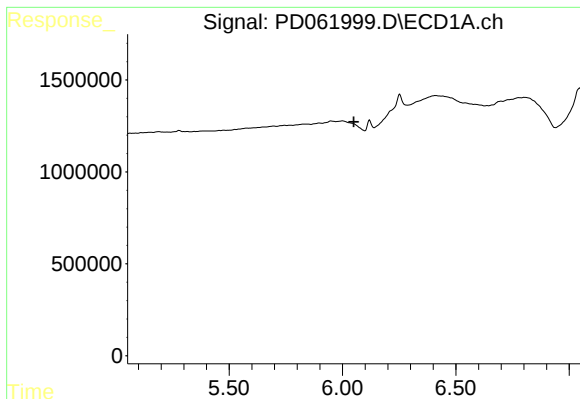

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

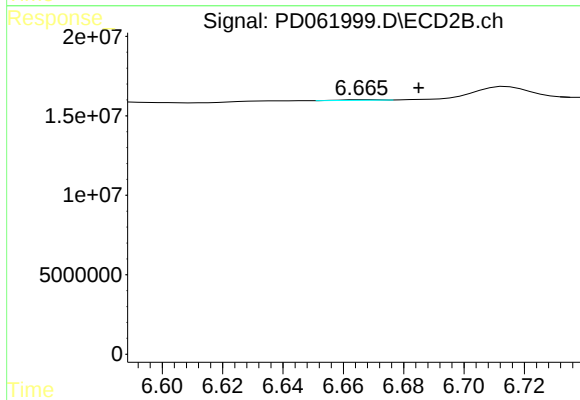


#14 Endrin

R.T.: 6.667 min
Delta R.T.: -0.018 min
Response: 264756
Conc: 0.03 ng/ml

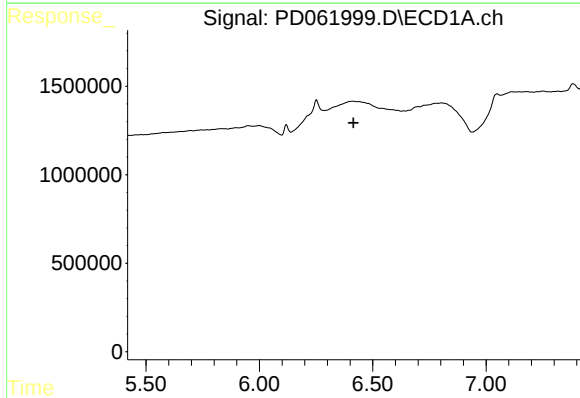


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

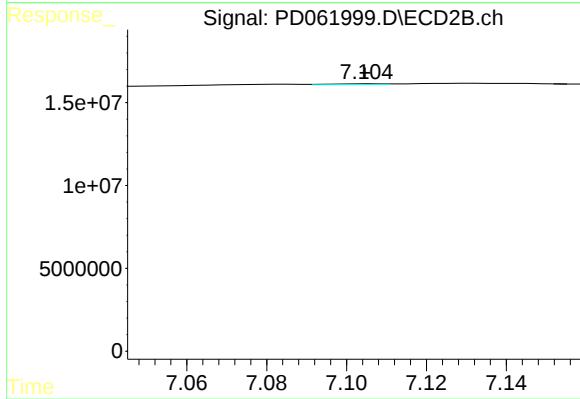

#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.001 min
Response: 386224
Conc: 0.04 ng/ml

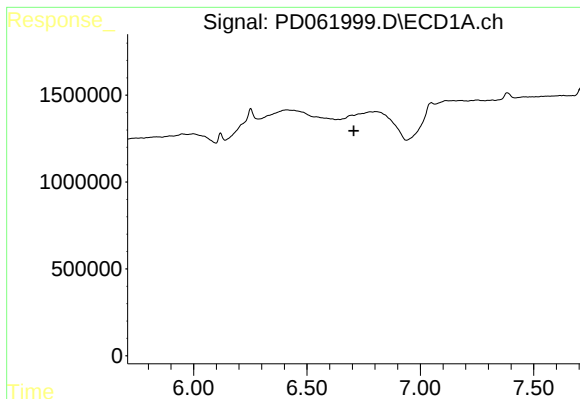

#19 Endosulfan Sulfate


R.T.: 0.000 min

Exp R.T. : 6.706 min

Response: 0

Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

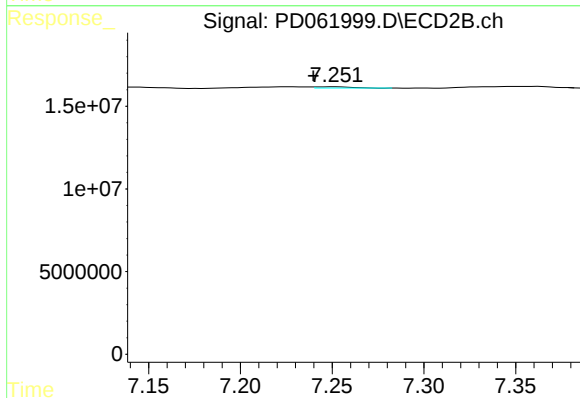


#19 Endosulfan Sulfate

R.T.: 7.252 min

Delta R.T.: 0.012 min

Response: 906537

Conc: 0.09 ng/ml

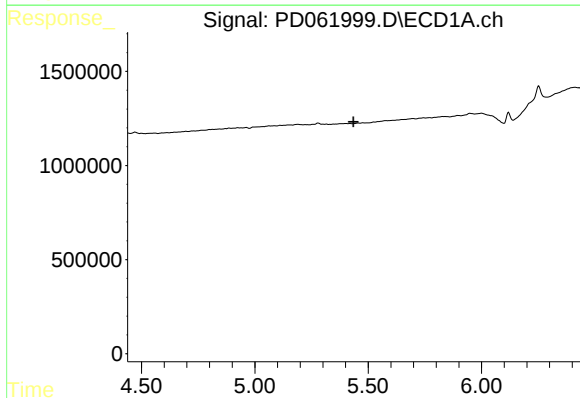


#25 Chlordane-3

R.T.: 0.000 min

Exp R.T. : 5.435 min

Response: 0

Conc: N.D.

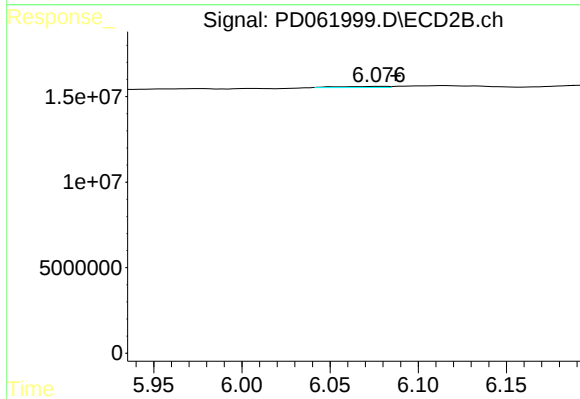


#25 Chlordane-3

R.T.: 6.078 min

Delta R.T.: -0.009 min

Response: 1165212


Conc: 0.70 ng/ml

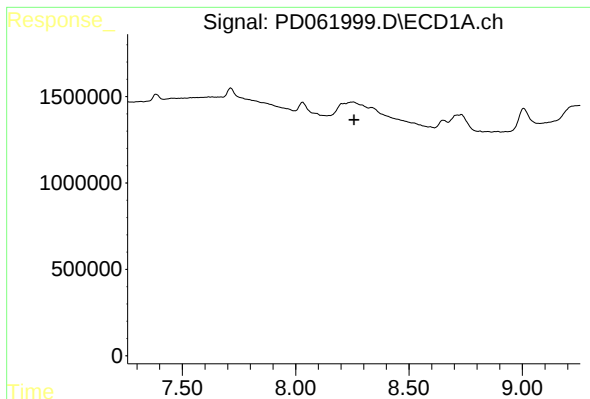

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

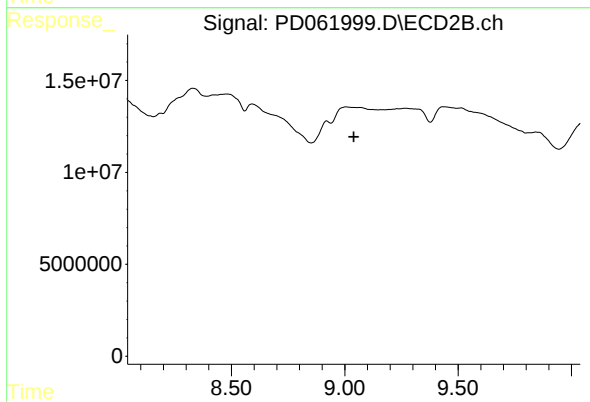

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.040 min
Response: 0
Conc: N.D.