

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 11:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:35:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	18902678	204.7E6	22.576	23.554
28)	SA Decachlor...	8.258	9.039	25920595	183.6E6	21.066	19.452
Target Compounds							
7)	B delta-BHC	0.000	5.036	0	4332192	N.D.	0.328 #
8)	B Heptachlo...	0.000	5.865	0	3577620	N.D.	0.302 #
9)	A Endosulfan I	0.000	6.236f	0	2592596	N.D.	0.239 #
12)	B 4,4'-DDE	0.000	6.309	0	258911	N.D.	0.022 #
13)	MA Dieldrin	0.000	6.460	0	345598	N.D.	0.030 #
14)	MA Endrin	0.000	6.706f	0	31728	N.D.	0.003 #
15)	B Endosulfa...	0.000	6.900	0	917298	N.D.	0.097 #
17)	MA 4,4'-DDT	0.000	7.103	0	3525609	N.D.	0.369 #
18)	B Endrin al...	0.000	7.003	0	4710080	N.D.	0.599 #
23)	Chlordane-1	0.000	4.973	0	960158	N.D.	2.475 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 11:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:35:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

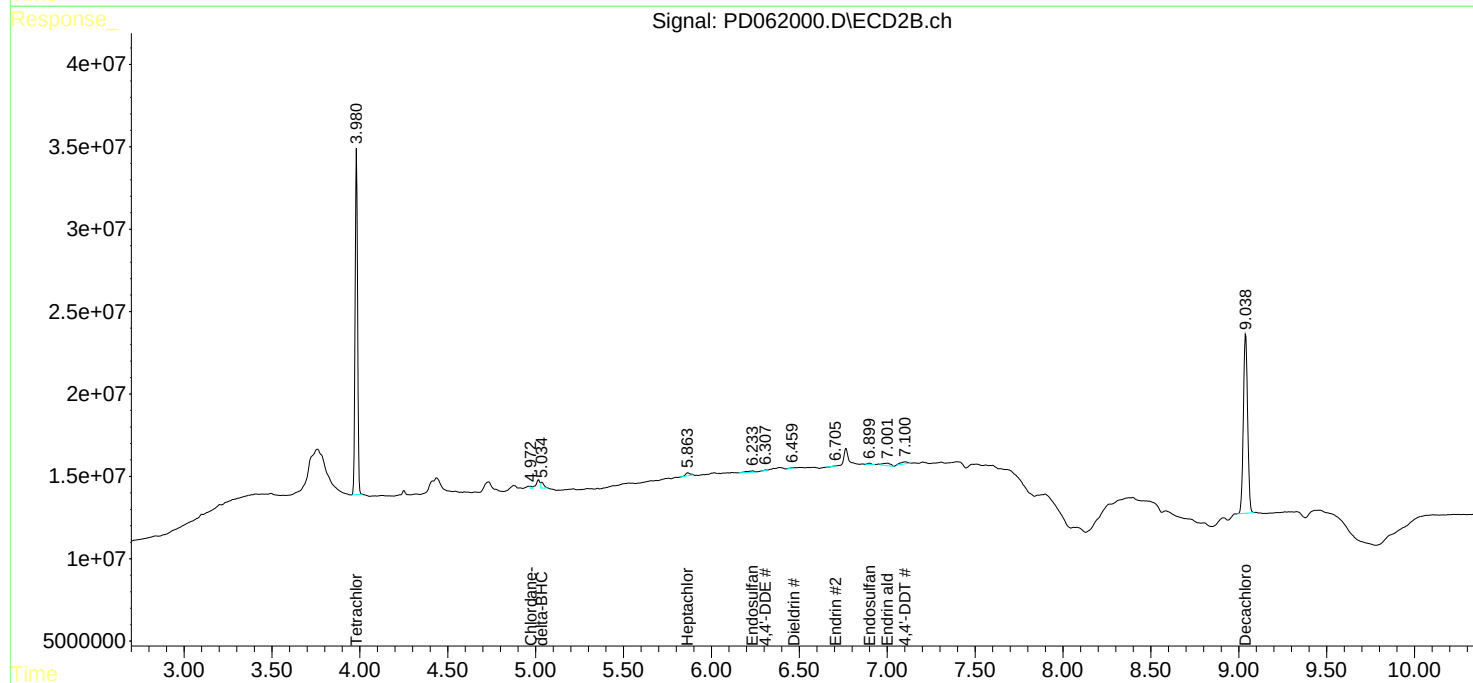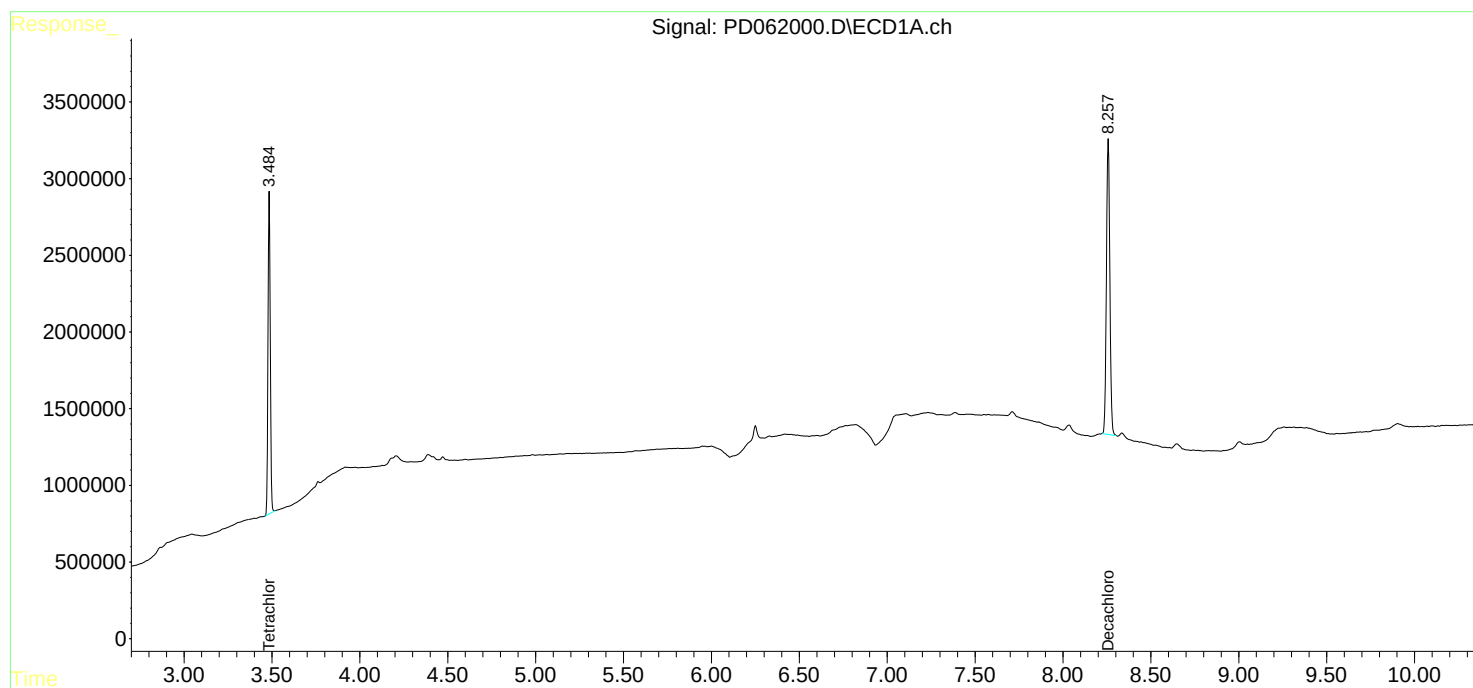


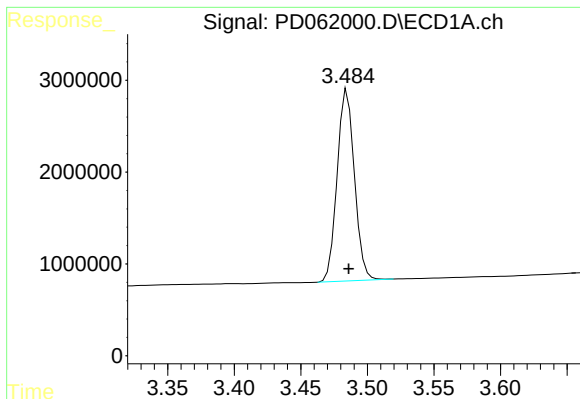

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 18902678
Conc: 22.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

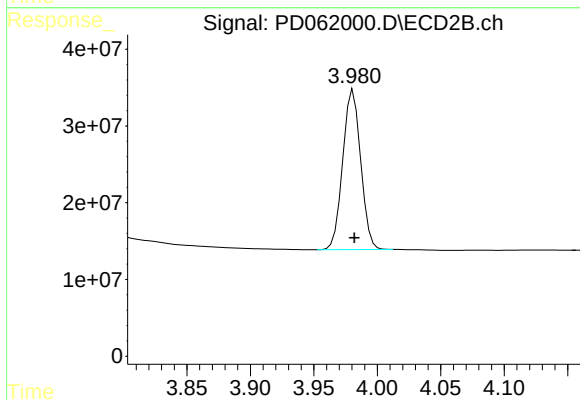


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 204660097
Conc: 23.55 ng/ml

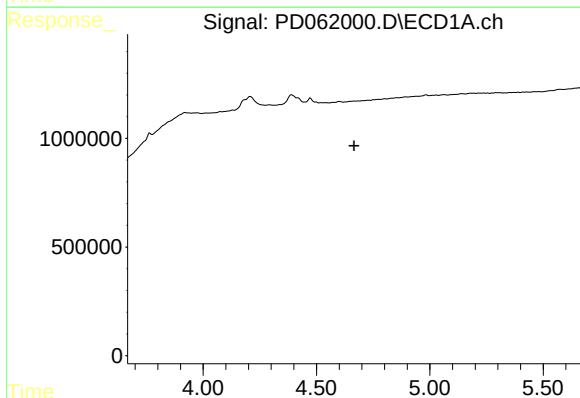


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

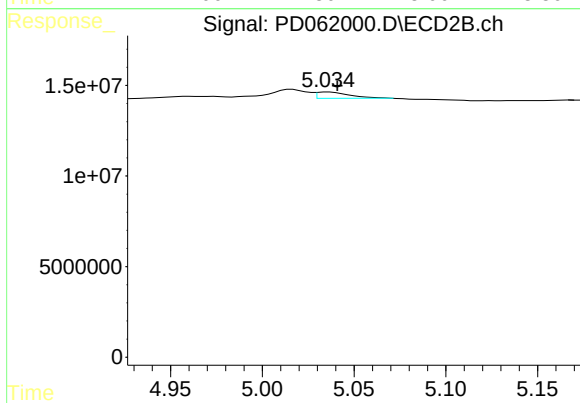

#7 delta-BHC


R.T.: 5.036 min
Delta R.T.: -0.005 min
Response: 4332192
Conc: 0.33 ng/ml

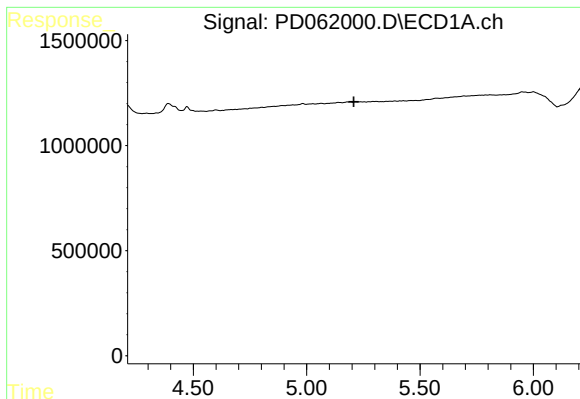

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

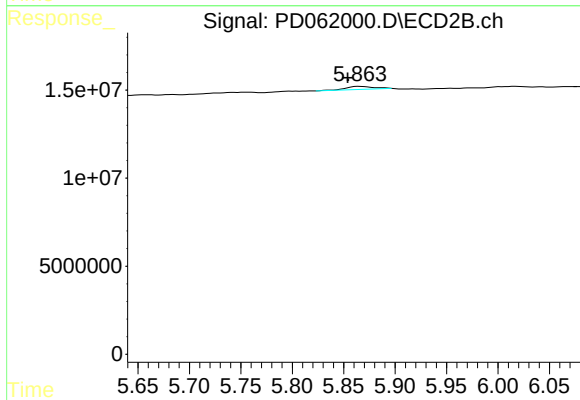


#8 Heptachlor epoxide

R.T.: 5.865 min
Delta R.T.: 0.011 min
Response: 3577620
Conc: 0.30 ng/ml

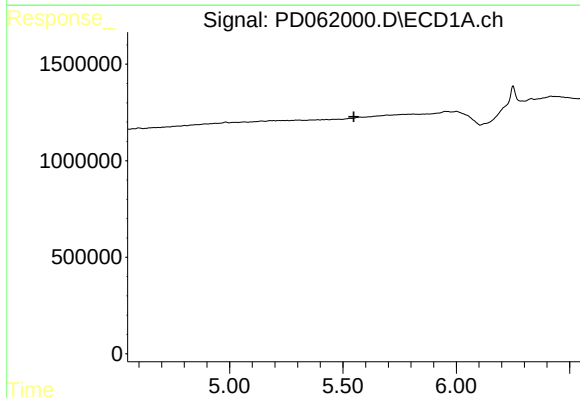


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

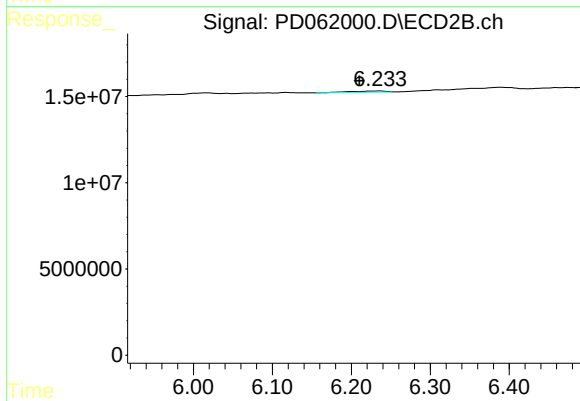

#9 Endosulfan I


R.T.: 6.236 min
Delta R.T.: 0.026 min
Response: 2592596
Conc: 0.24 ng/ml

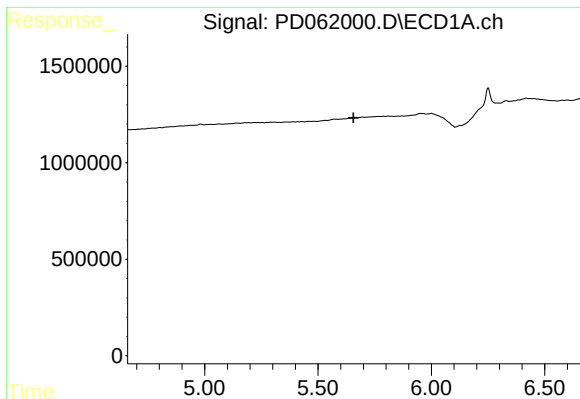

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

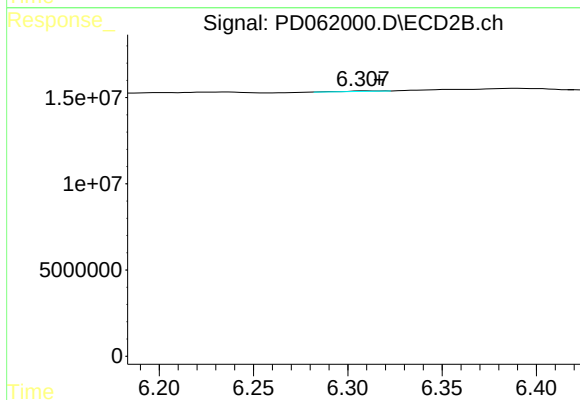


#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.008 min
Response: 258911
Conc: 0.02 ng/ml

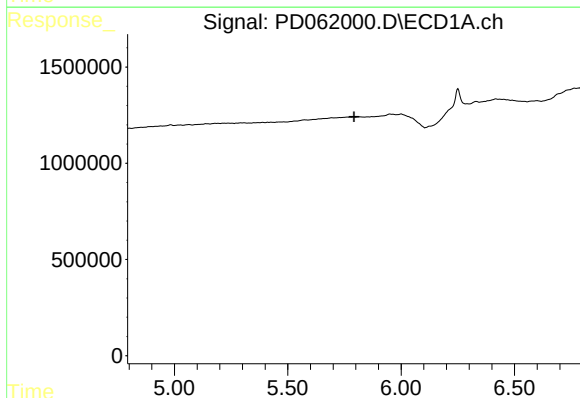


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

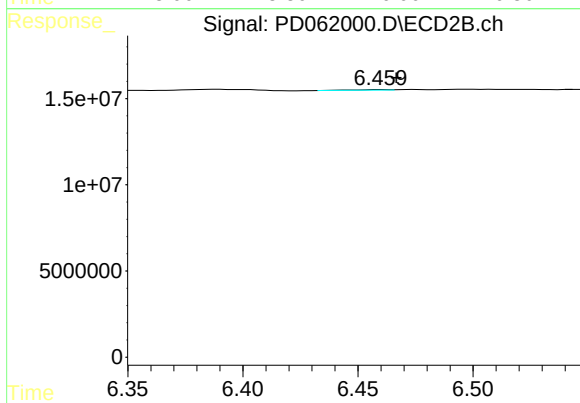

#13 Dieldrin


R.T.: 6.460 min
Delta R.T.: -0.007 min
Response: 345598
Conc: 0.03 ng/ml

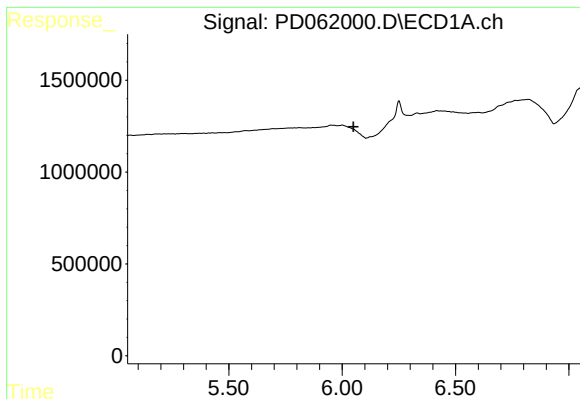

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

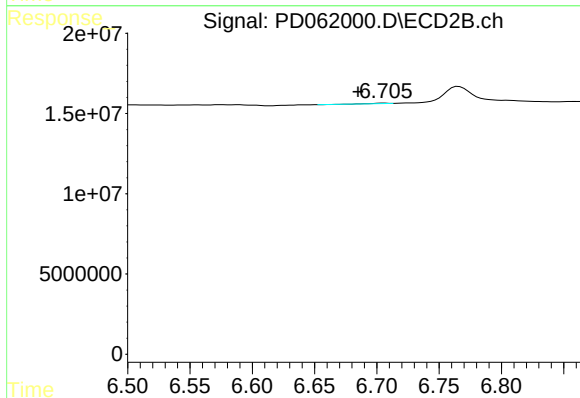


#14 Endrin

R.T.: 6.706 min
Delta R.T.: 0.021 min
Response: 31728
Conc: 0.00 ng/ml

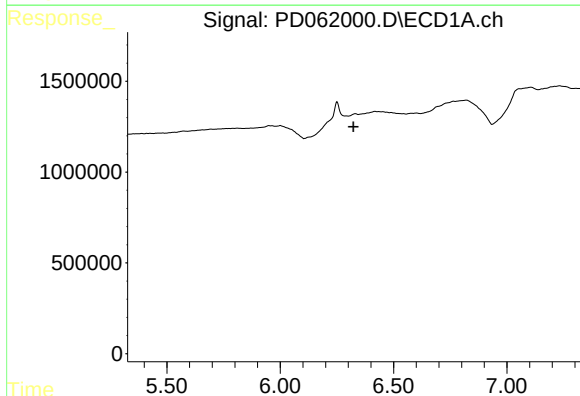


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

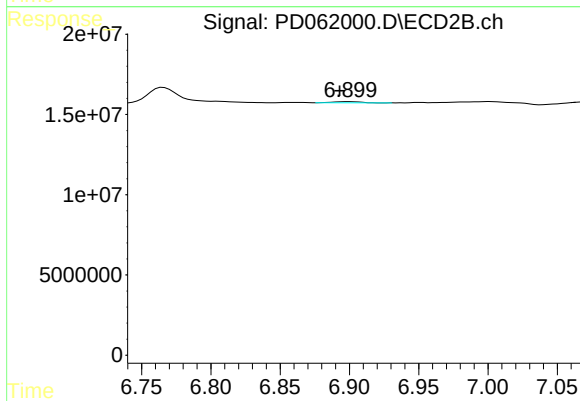

#15 Endosulfan II


R.T.: 6.900 min
Delta R.T.: 0.007 min
Response: 917298
Conc: 0.10 ng/ml

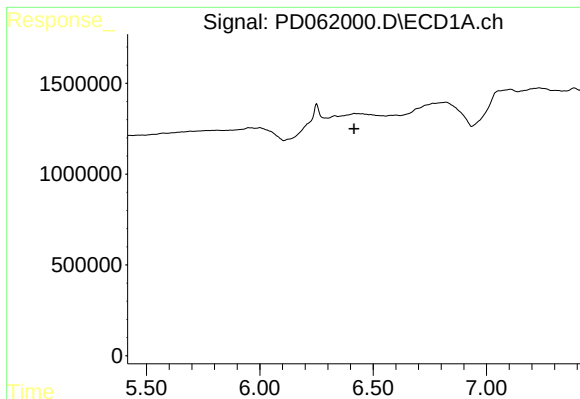

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

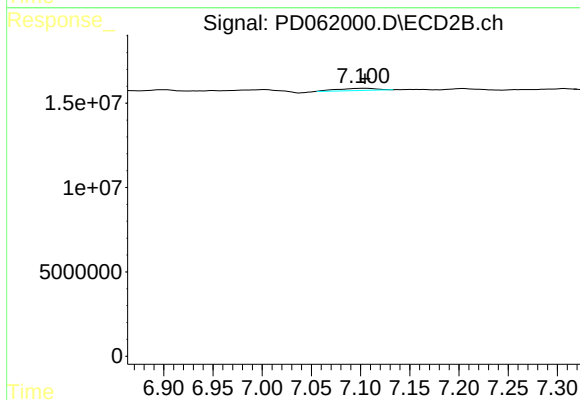


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: -0.001 min
Response: 3525609
Conc: 0.37 ng/ml

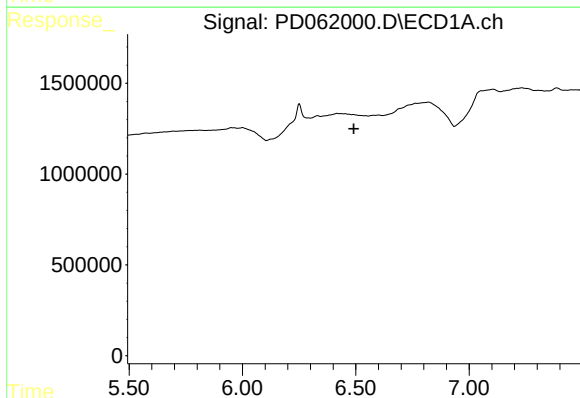


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

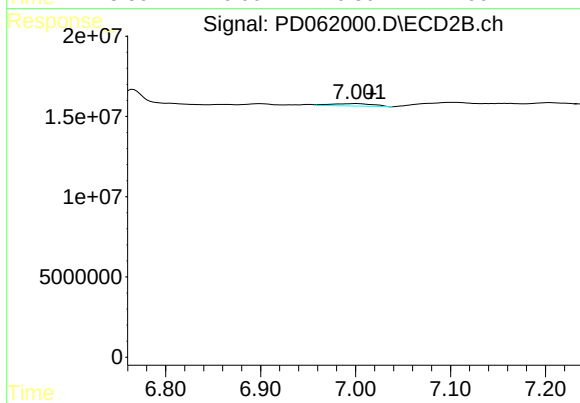

#18 Endrin aldehyde


R.T.: 7.003 min
Delta R.T.: -0.014 min
Response: 4710080
Conc: 0.60 ng/ml

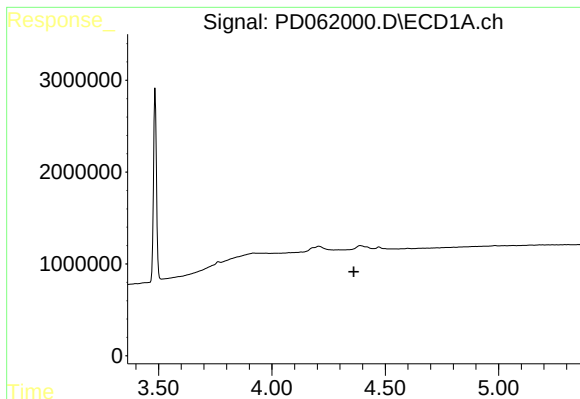

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

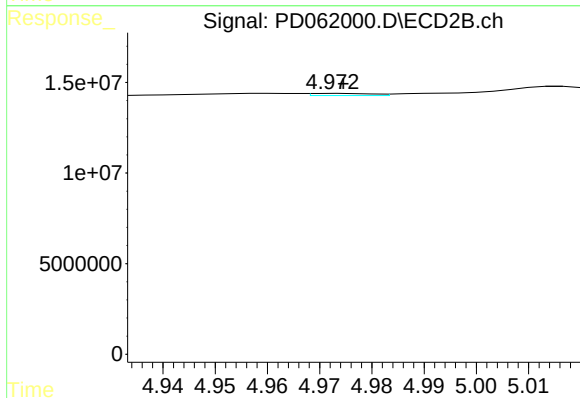


#23 Chlordane-1

R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 960158
Conc: 2.47 ng/ml

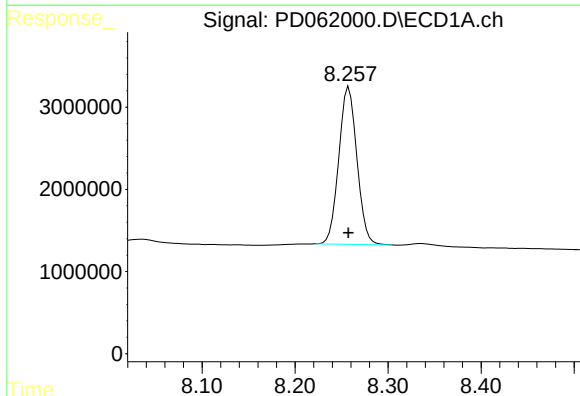

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 25920595
Conc: 21.07 ng/ml

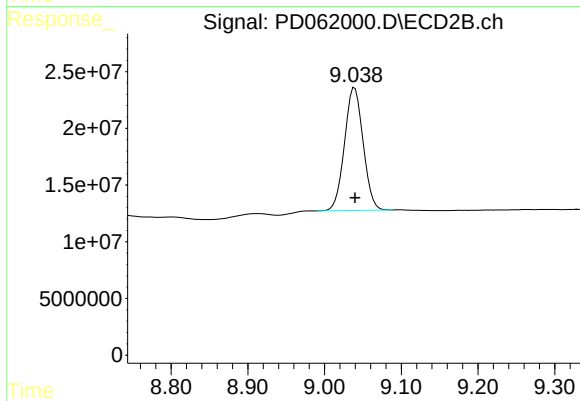

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 183641439
Conc: 19.45 ng/ml