

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 11:28
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:35:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	19304245	206.6E6	23.055	23.781
28)	SA Decachlor...	8.258	9.039	27055329	189.7E6	21.989	20.091
Target Compounds							
2)	A alpha-BHC	3.924	4.370	13827437	154.9E6	10.948	11.513
3)	MA gamma-BHC...	4.209	4.654	13666326	150.6E6	11.511	12.073
6)	B beta-BHC	4.459	4.823	6897942	64852156	12.649	12.556
7)	B delta-BHC	0.000	5.035	0	4755456	N.D.	0.360 #
8)	B Heptachlo...	0.000	5.861	0	4695769	N.D.	0.397 #
9)	A Endosulfan I	0.000	6.204	0	1085716	N.D.	0.100 #
10)	B gamma-Chl...	0.000	6.095	0	825394	N.D.	0.070 #
11)	B alpha-Chl...	0.000	6.174	0	1362070	N.D.	0.119 #
12)	B 4,4'-DDE	0.000	6.316	0	3984802	N.D.	0.346 #
13)	MA Dieldrin	0.000	6.469	0	8272222	N.D.	0.717 #
14)	MA Endrin	6.050	6.683	53347824	490.4E6	51.920	49.555
15)	B Endosulfa...	0.000	6.902	0	4206523	N.D.	0.443 #
16)	A 4,4'-DDD	6.174	6.805	1601444	5961812	1.721	0.630 #
17)	MA 4,4'-DDT	6.416	7.104	105.9E6	948.5E6	117.597	99.299
18)	B Endrin al...	6.491	7.016	1949721	12016774	2.282	1.528 #
20)	A Methoxychlor	6.962	7.562	132.4E6	1082.4E6	280.244	240.102
21)	B Endrin ke...	7.198	7.709	4793757	26013884	3.756	2.565 #
25)	Chlordane-3	0.000	6.095	0	825394	N.D.	0.498 #
26)	Chlordane-4	0.000	6.174	0	1362070	N.D.	0.710 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 11:28
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:35:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

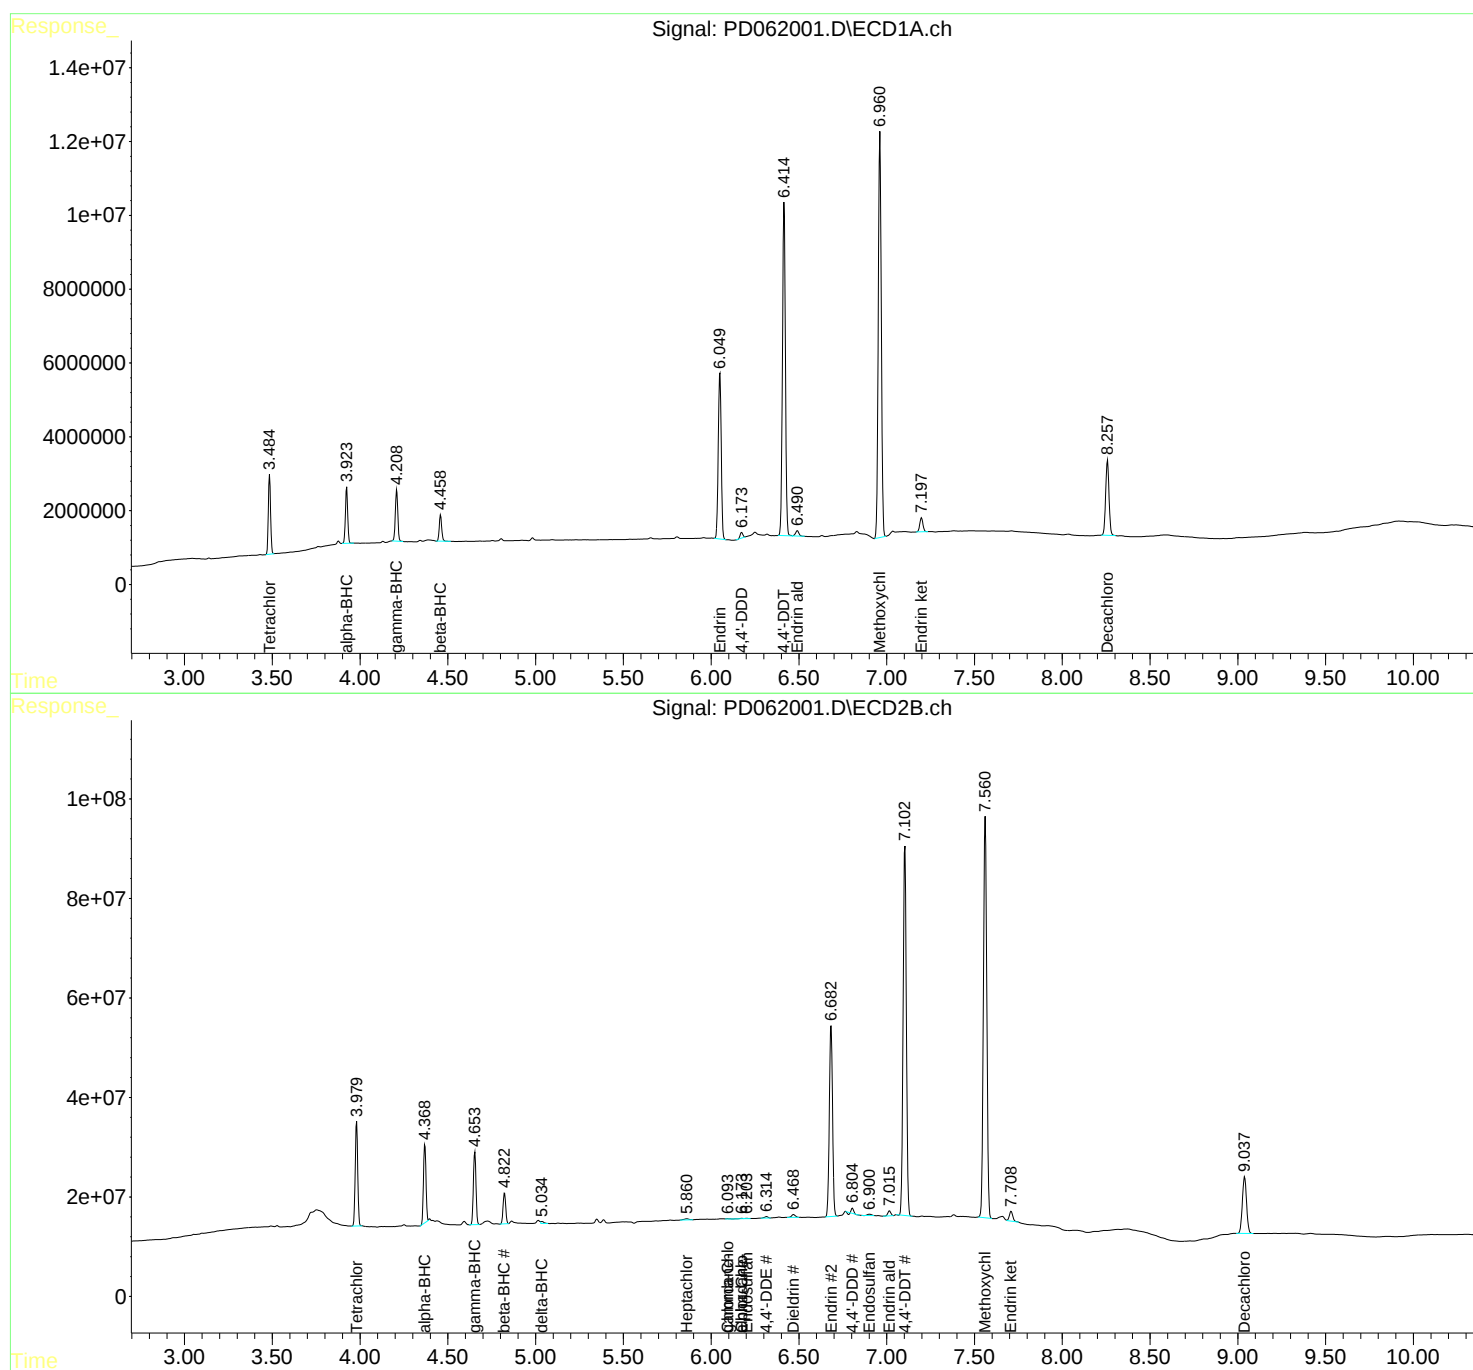


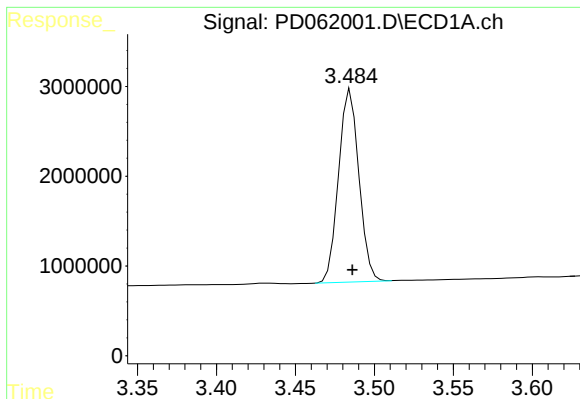

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 19304245
Conc: 23.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

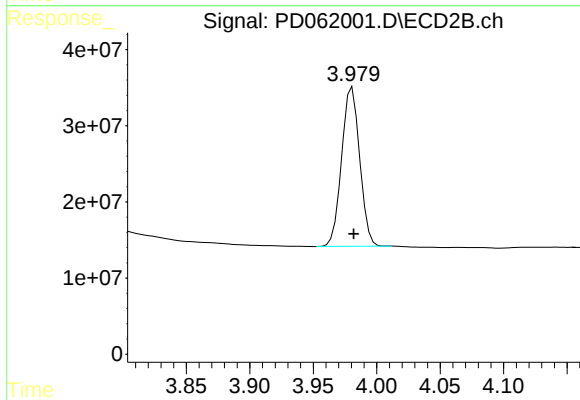


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 206631054
Conc: 23.78 ng/ml

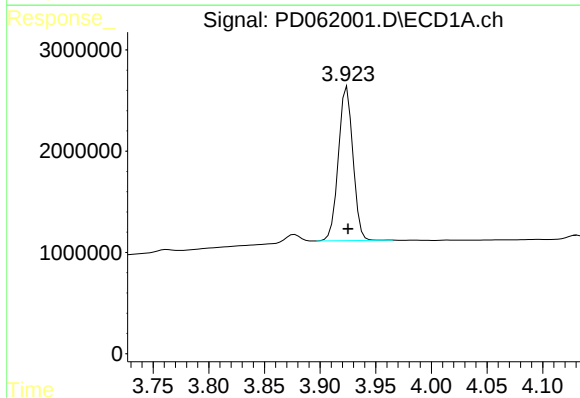


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 13827437
Conc: 10.95 ng/ml

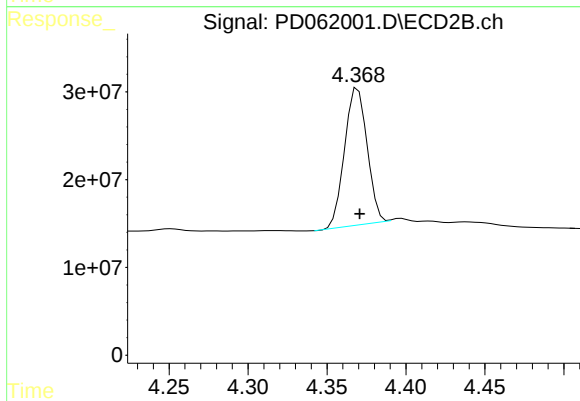

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: -0.001 min
Response: 154855857
Conc: 11.51 ng/ml

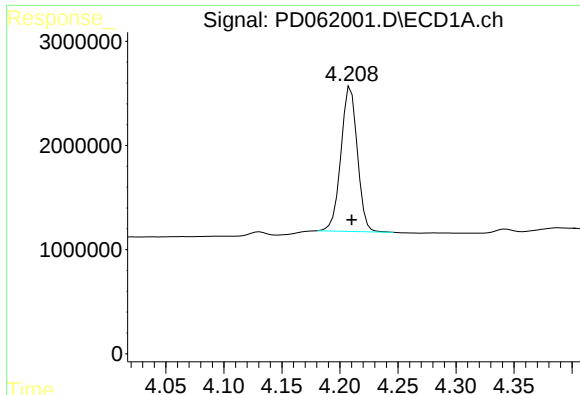

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 13666326
Conc: 11.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

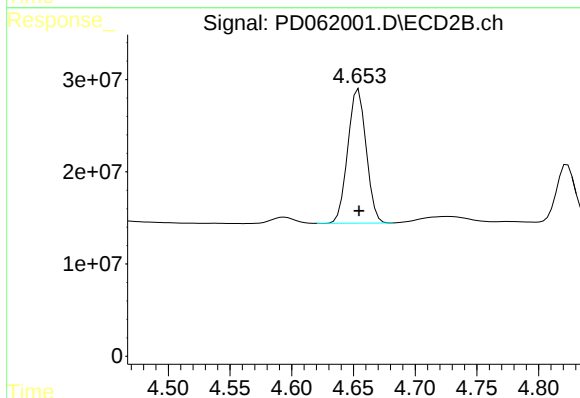


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 150590782
Conc: 12.07 ng/ml

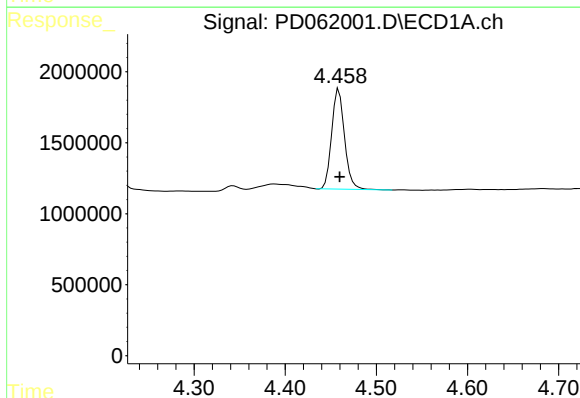


#6 beta-BHC

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 6897942
Conc: 12.65 ng/ml

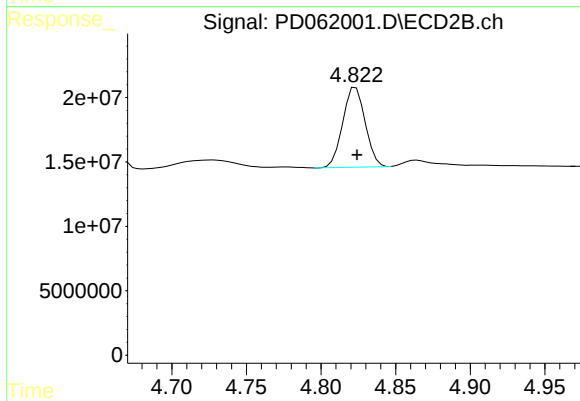

#6 beta-BHC


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 64852156
Conc: 12.56 ng/ml

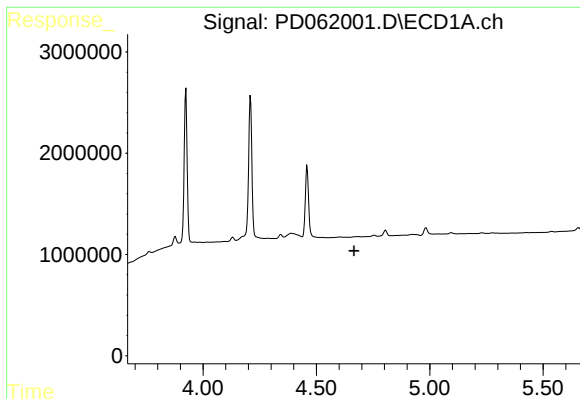

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

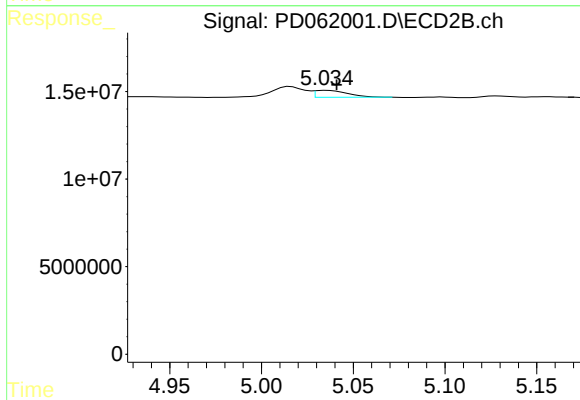


#7 delta-BHC

R.T.: 5.035 min
Delta R.T.: -0.006 min
Response: 4755456
Conc: 0.36 ng/ml

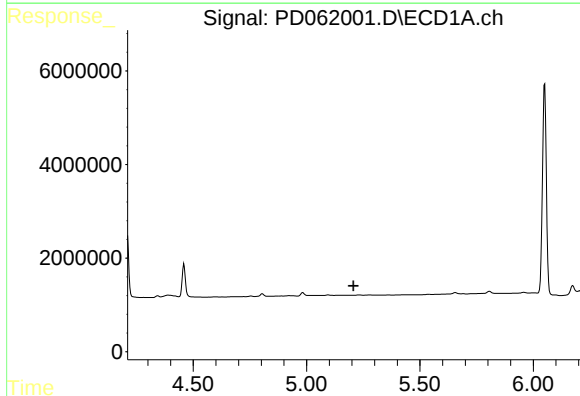


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

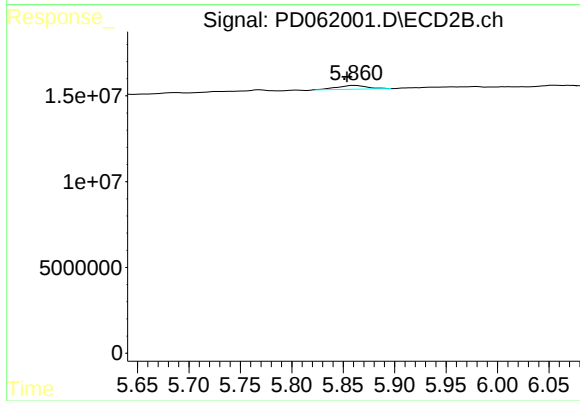

#8 Heptachlor epoxide


R.T.: 5.861 min
Delta R.T.: 0.008 min
Response: 4695769
Conc: 0.40 ng/ml

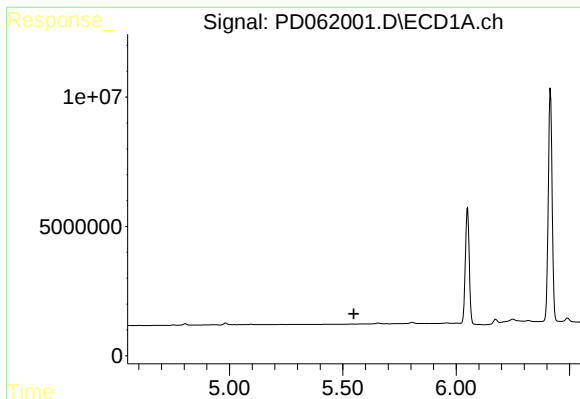

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

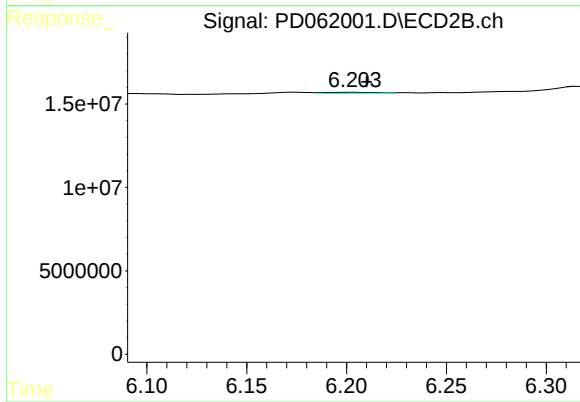


#9 Endosulfan I

R.T.: 6.204 min
Delta R.T.: -0.006 min
Response: 1085716
Conc: 0.10 ng/ml

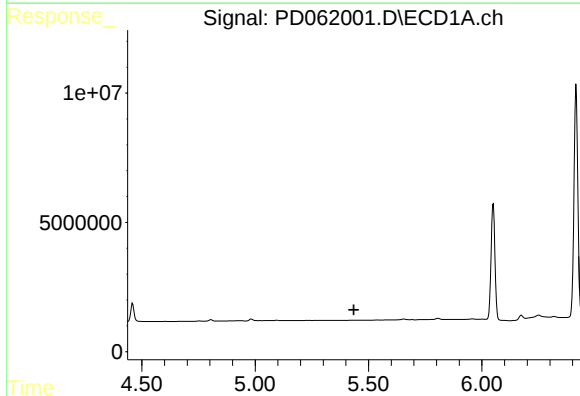


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

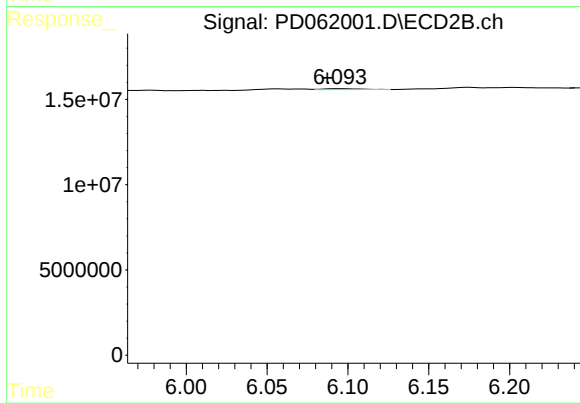

#10 gamma-Chlordane


R.T.: 6.095 min
Delta R.T.: 0.008 min
Response: 825394
Conc: 0.07 ng/ml

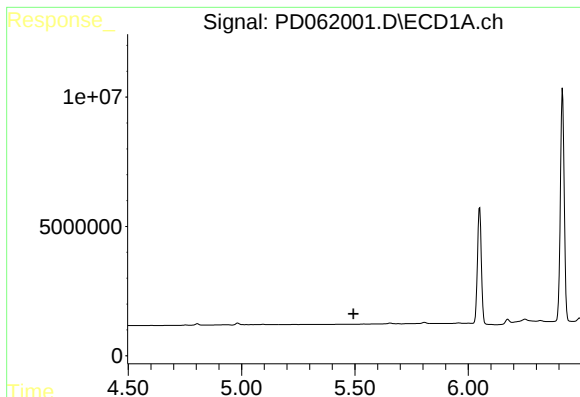

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

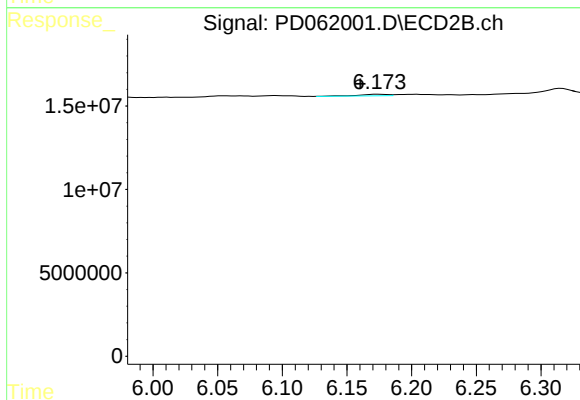


#11 alpha-Chlordane

R.T.: 6.174 min
Delta R.T.: 0.014 min
Response: 1362070
Conc: 0.12 ng/ml

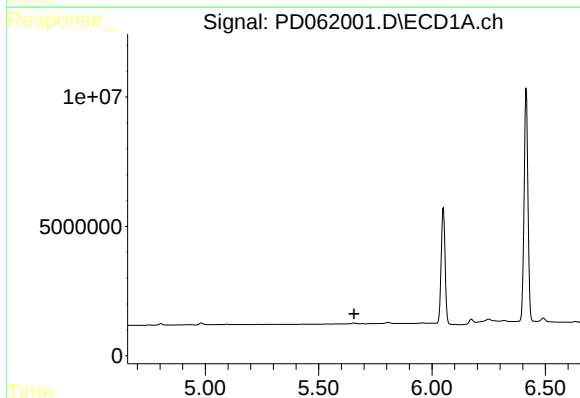


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

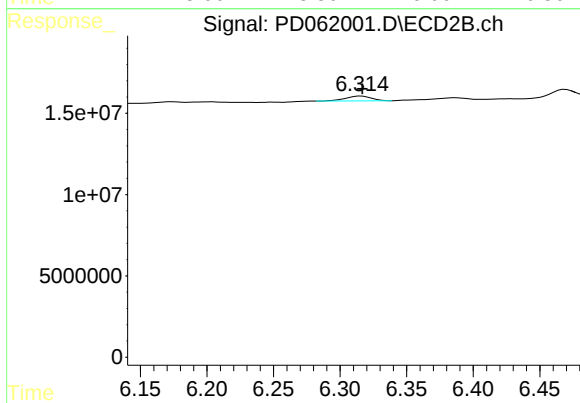

#12 4,4'-DDE


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 3984802
Conc: 0.35 ng/ml

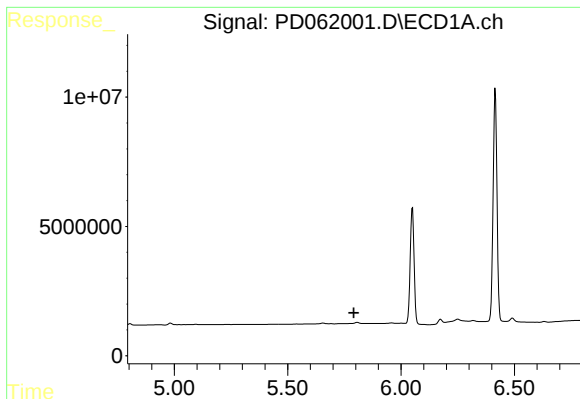

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

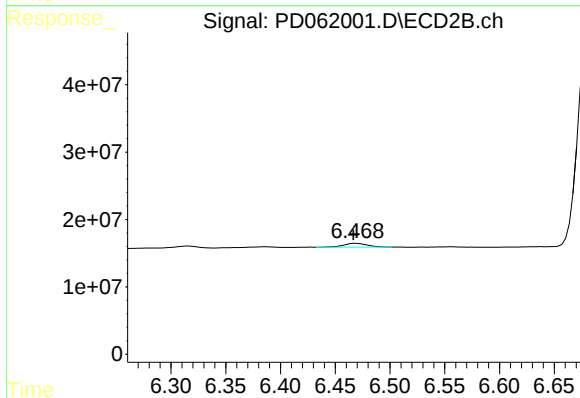


#13 Dieldrin

R.T.: 6.469 min
Delta R.T.: 0.002 min
Response: 8272222
Conc: 0.72 ng/ml

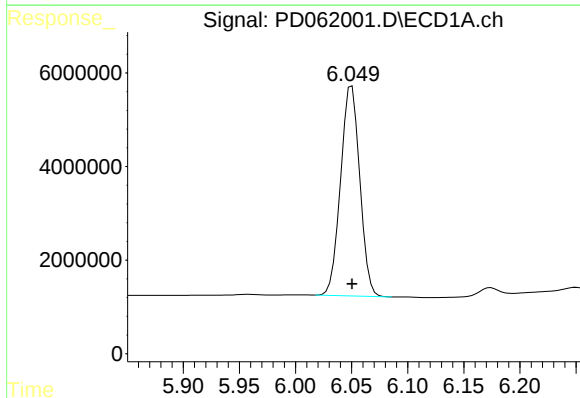


#14 Endrin

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 53347824
Conc: 51.92 ng/ml

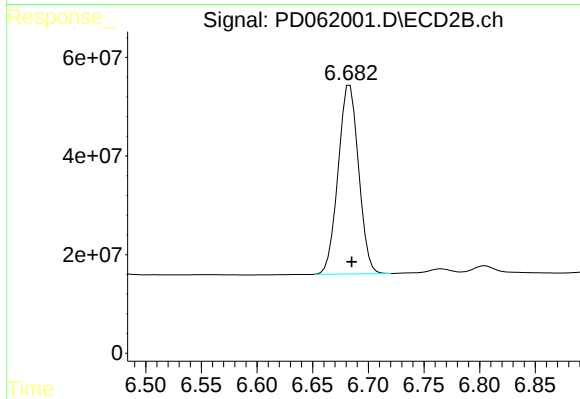

#14 Endrin


R.T.: 6.683 min
Delta R.T.: -0.002 min
Response: 490412324
Conc: 49.56 ng/ml

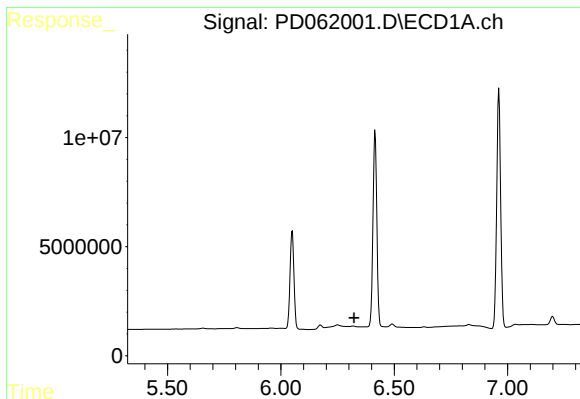

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

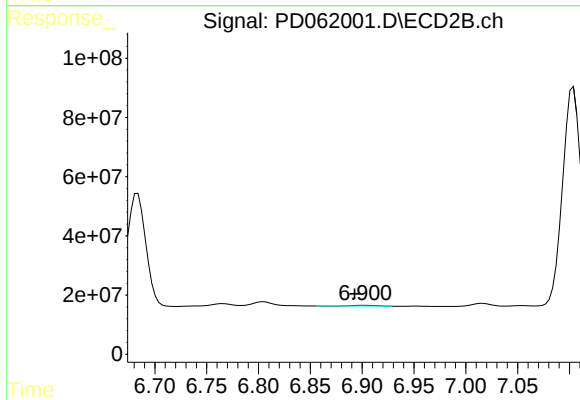


#15 Endosulfan II

R.T.: 6.902 min
Delta R.T.: 0.009 min
Response: 4206523
Conc: 0.44 ng/ml

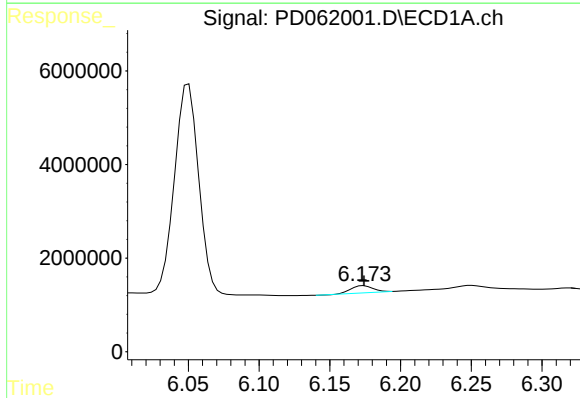


#16 4,4'-DDD

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 1601444
Conc: 1.72 ng/ml

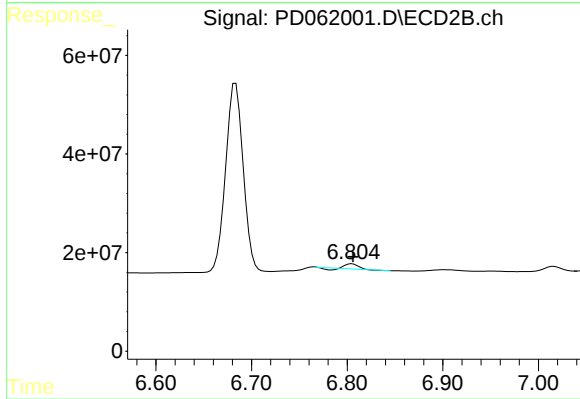

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: -0.001 min
Response: 5961812
Conc: 0.63 ng/ml

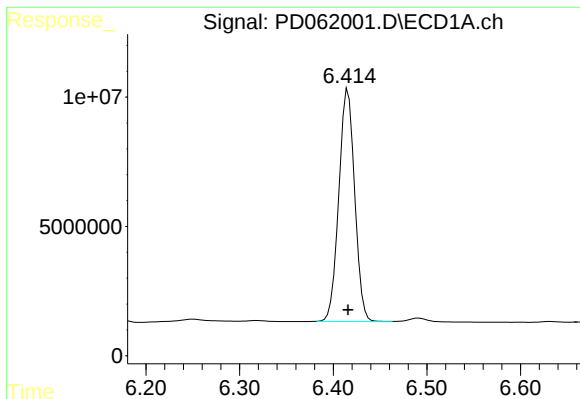

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 105922552
Conc: 117.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

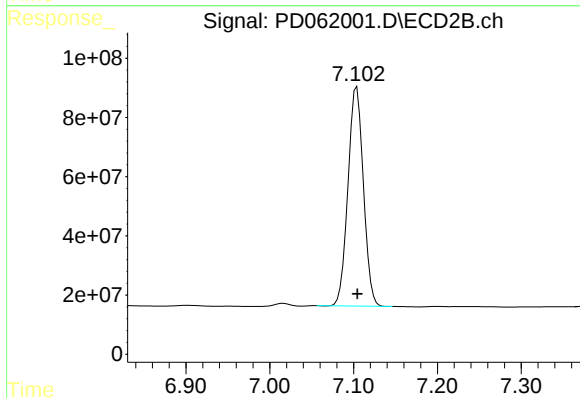


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 948463284
Conc: 99.30 ng/ml

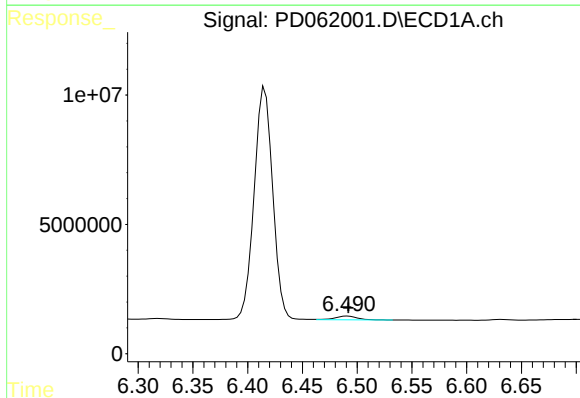


#18 Endrin aldehyde

R.T.: 6.491 min
Delta R.T.: 0.000 min
Response: 1949721
Conc: 2.28 ng/ml

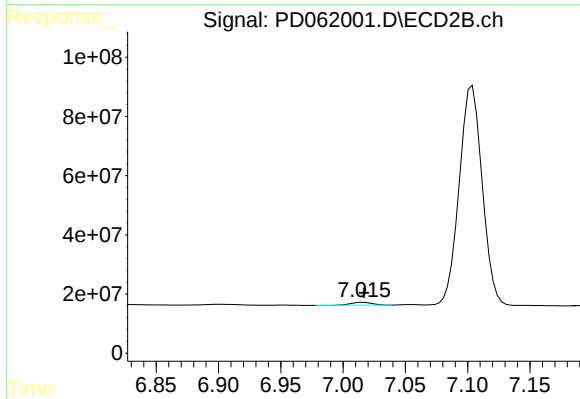

#18 Endrin aldehyde


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 12016774
Conc: 1.53 ng/ml

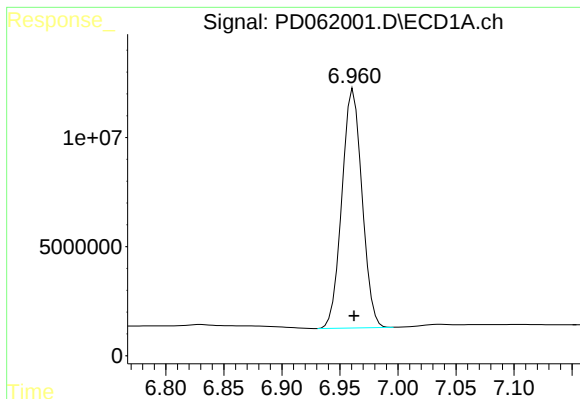

#20 Methoxychlor


R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 132415636
Conc: 280.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

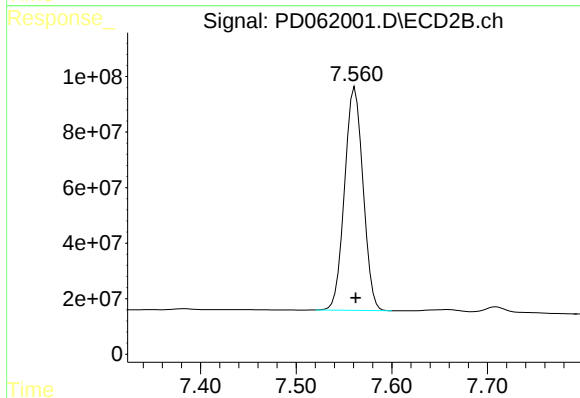


#20 Methoxychlor

R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 1082358770
Conc: 240.10 ng/ml

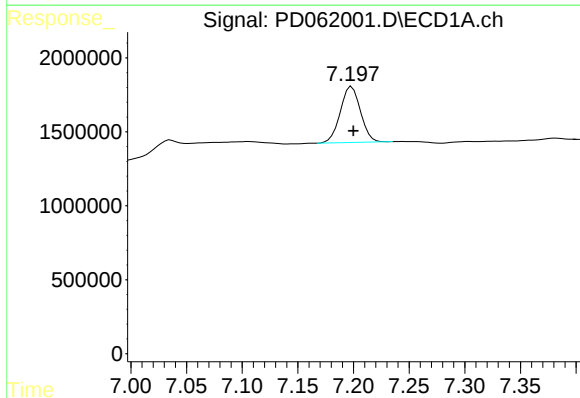


#21 Endrin ketone

R.T.: 7.198 min
Delta R.T.: -0.001 min
Response: 4793757
Conc: 3.76 ng/ml

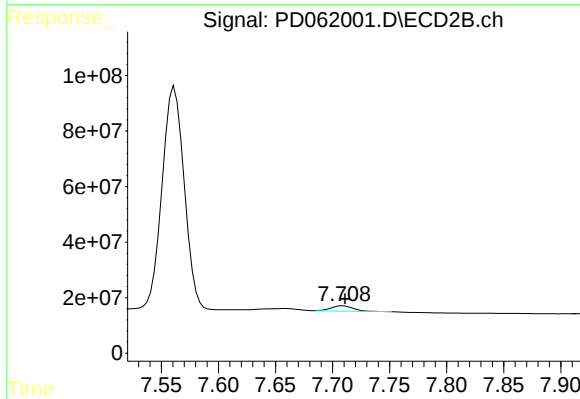

#21 Endrin ketone


R.T.: 7.709 min
Delta R.T.: -0.002 min
Response: 26013884
Conc: 2.56 ng/ml

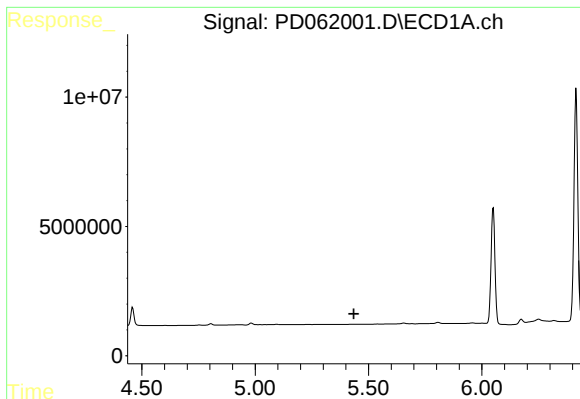

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

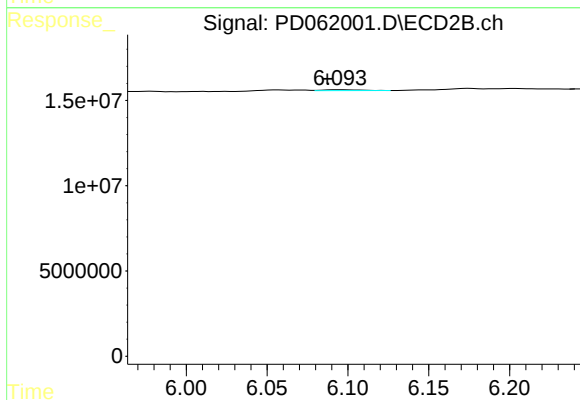


#25 Chlordane-3

R.T.: 6.095 min
Delta R.T.: 0.008 min
Response: 825394
Conc: 0.50 ng/ml

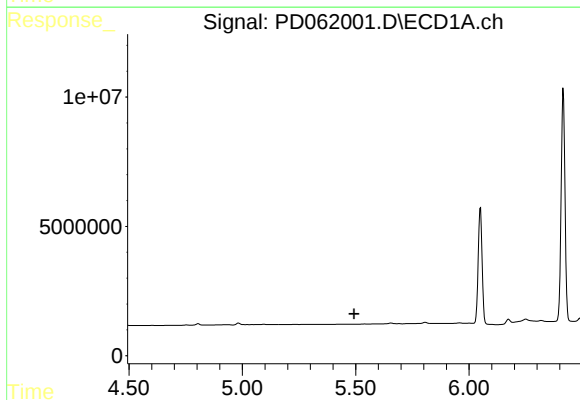


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

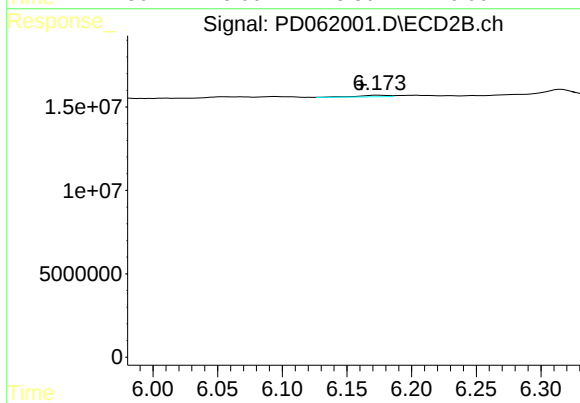

#26 Chlordane-4


R.T.: 6.174 min
Delta R.T.: 0.013 min
Response: 1362070
Conc: 0.71 ng/ml

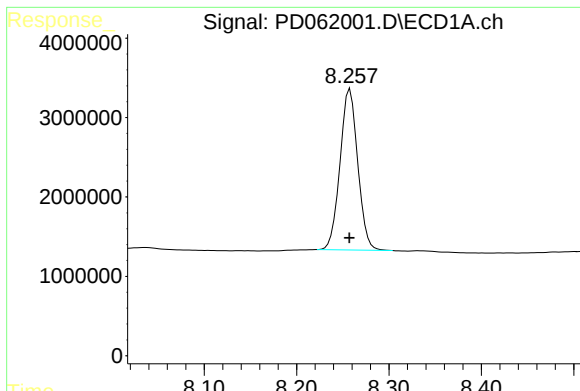

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 27055329
Conc: 21.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

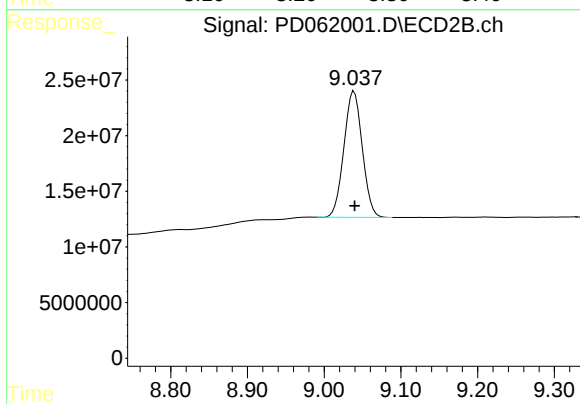

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 189666417
Conc: 20.09 ng/ml