

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 13:55
 Operator : AR\AJ
 Sample : M1949-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:36:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	21369702	229.1E6	25.522	26.372
28)	SA Decachlor...	8.258	9.041	27071972	193.3E6	22.002	20.475
Target Compounds							
7)	B delta-BHC	0.000	5.034	0 10395517	N.D.	0.786	#
8)	B Heptachlo...	0.000	5.862	0 8763657	N.D.	0.740	#
9)	A Endosulfan I	0.000	6.239f	0 781359	N.D.	0.072	#
10)	B gamma-Chl...	0.000	6.101	0 1343049	N.D.	0.113	#
15)	B Endosulfa...	0.000	6.871f	0 8205708	N.D.	0.864	#
17)	MA 4,4'-DDT	0.000	7.121f	0 4639132	N.D.	0.486	#
19)	B Endosulfa...	0.000	7.228	0 3292892	N.D.	0.329	#
21)	B Endrin ke...	0.000	7.708	0 1934119	N.D.	0.191	#
25)	Chlordane-3	0.000	6.101	0 1343049	N.D.	0.810	#
27)	Chlordane-5	0.000	6.949f	0 4981228	N.D.	13.821	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 13:55
Operator : AR\AJ
Sample : M1949-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:36:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

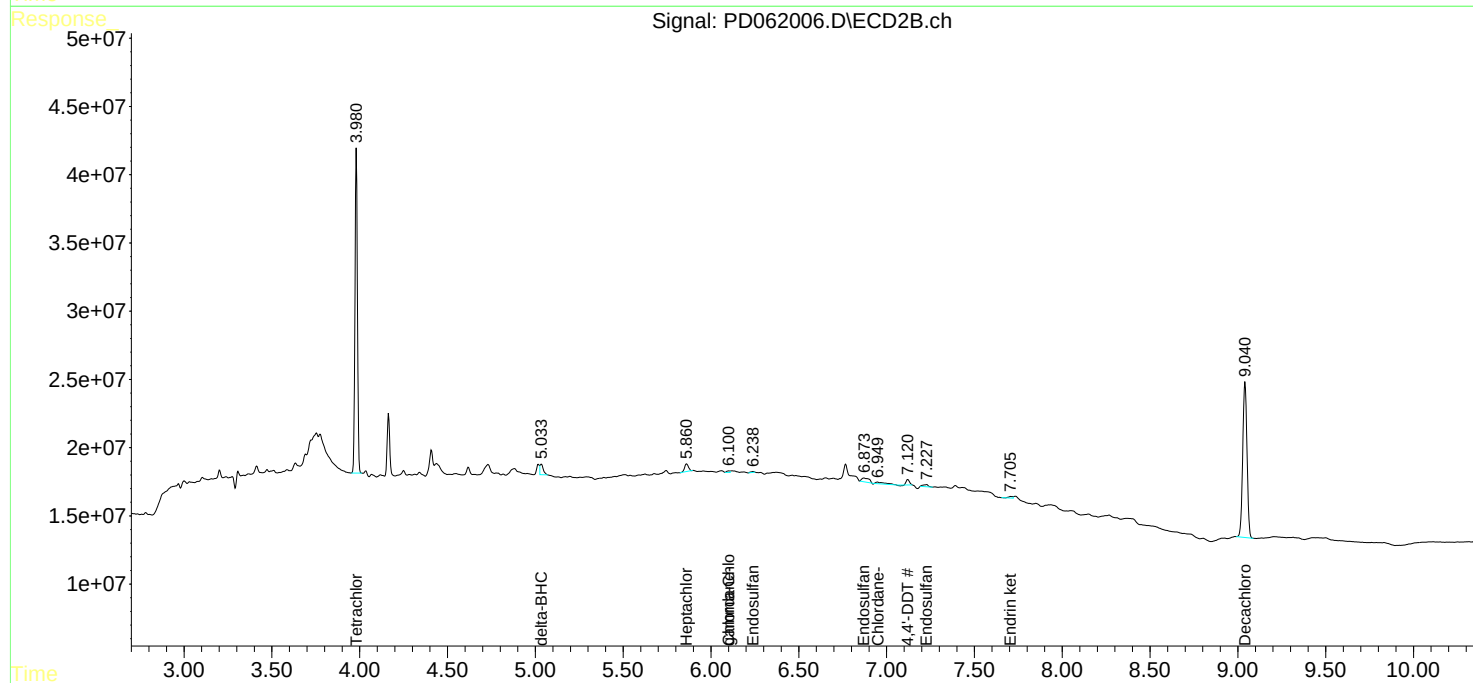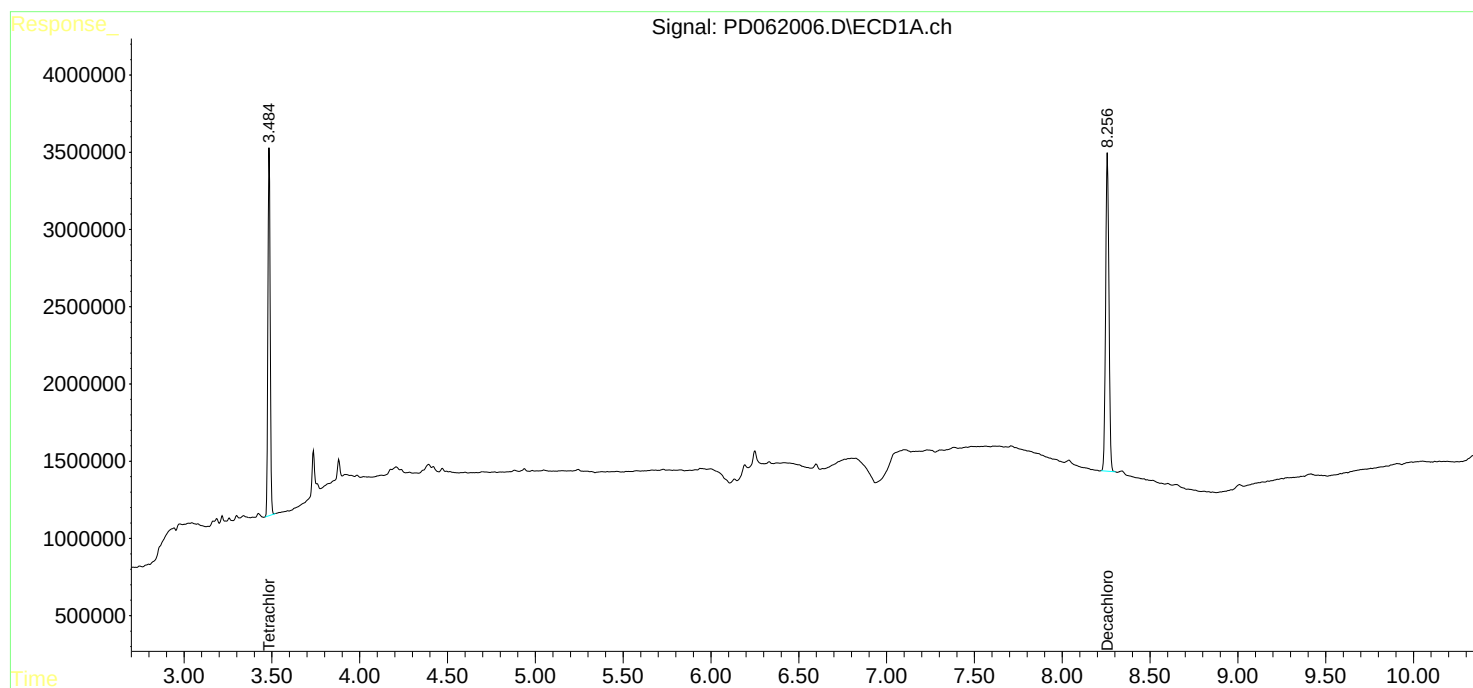


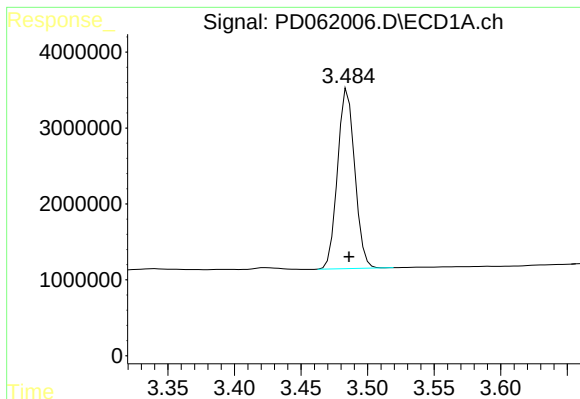

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 21369702
Conc: 25.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

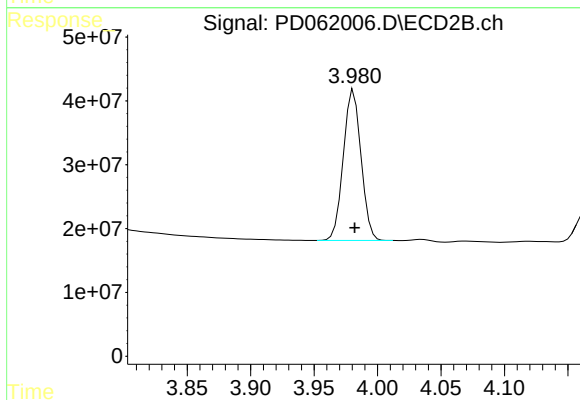


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 229147276
Conc: 26.37 ng/ml

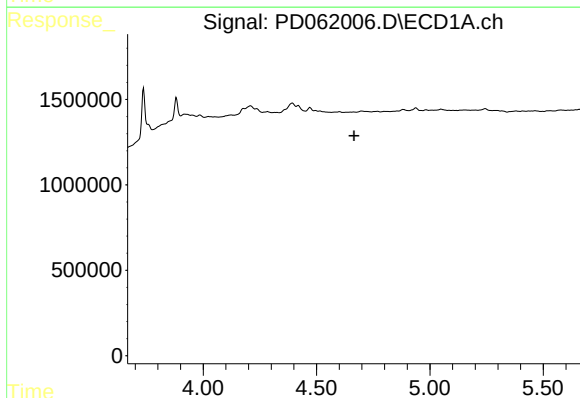


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

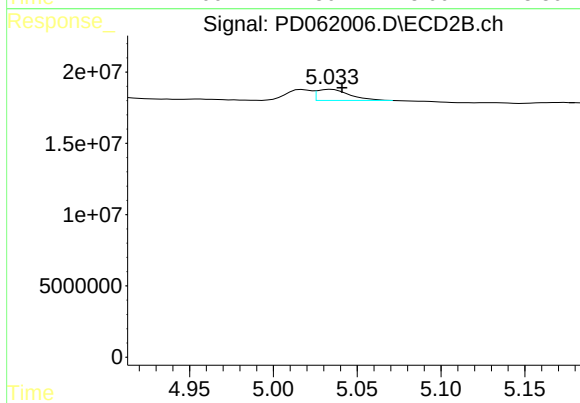

#7 delta-BHC


R.T.: 5.034 min
Delta R.T.: -0.007 min
Response: 10395517
Conc: 0.79 ng/ml

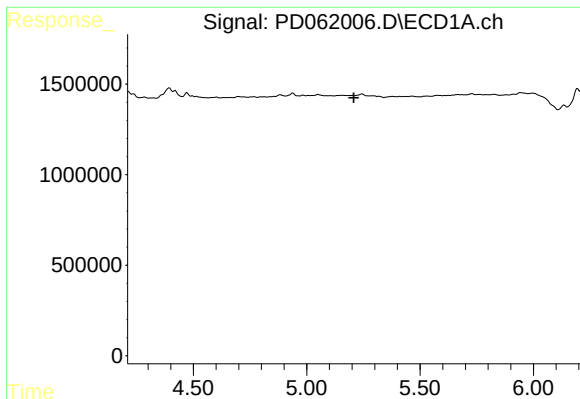

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

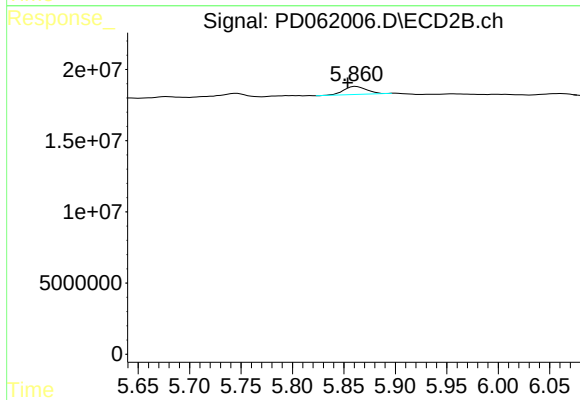


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.008 min
Response: 8763657
Conc: 0.74 ng/ml

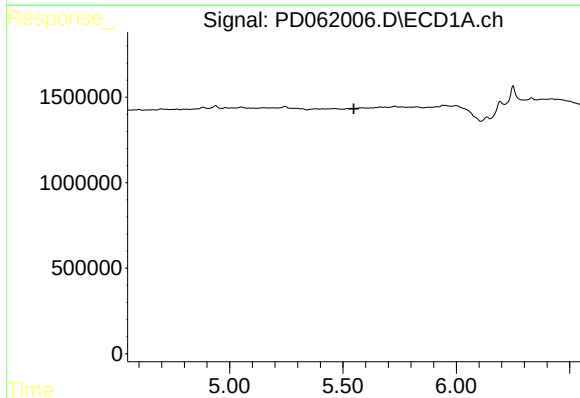


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

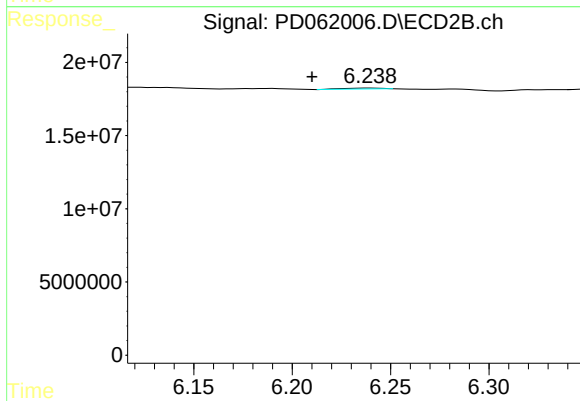

#9 Endosulfan I


R.T.: 6.239 min
Delta R.T.: 0.029 min
Response: 781359
Conc: 0.07 ng/ml

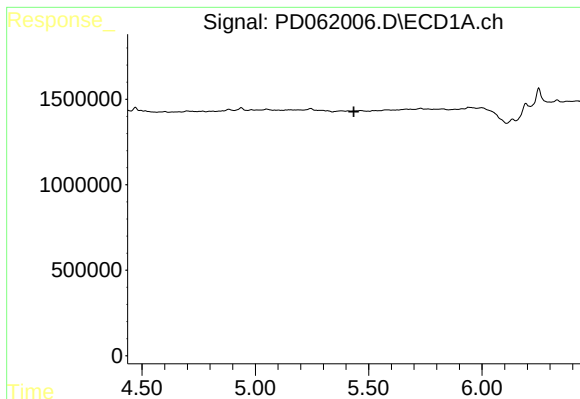

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

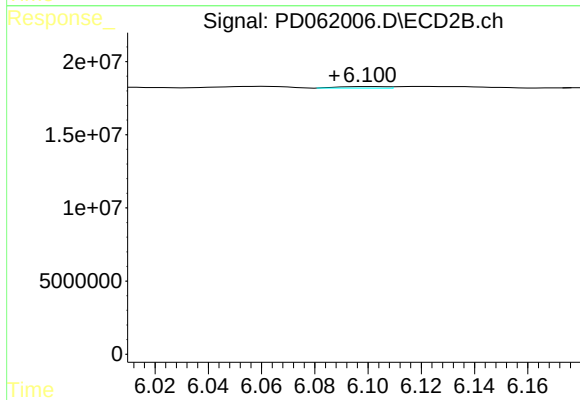


#10 gamma-Chlordane

R.T.: 6.101 min
Delta R.T.: 0.014 min
Response: 1343049
Conc: 0.11 ng/ml

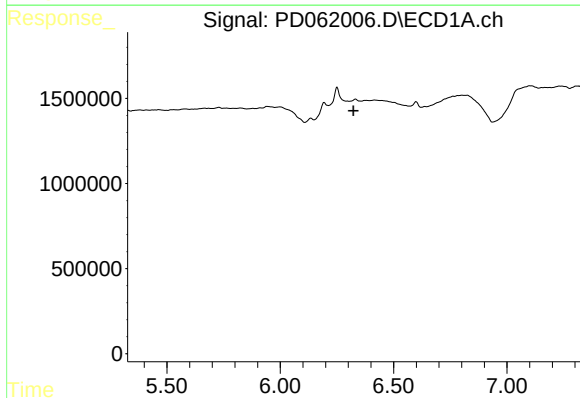


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

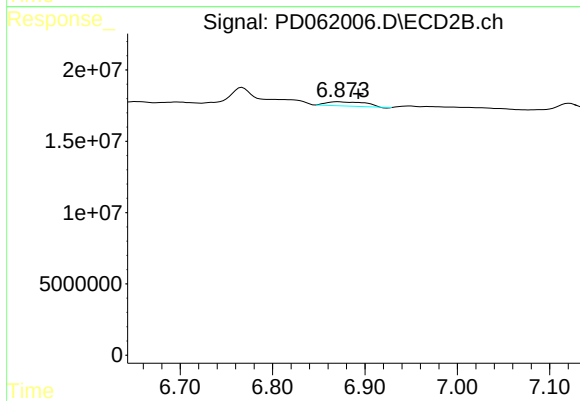

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: -0.022 min
Response: 8205708
Conc: 0.86 ng/ml

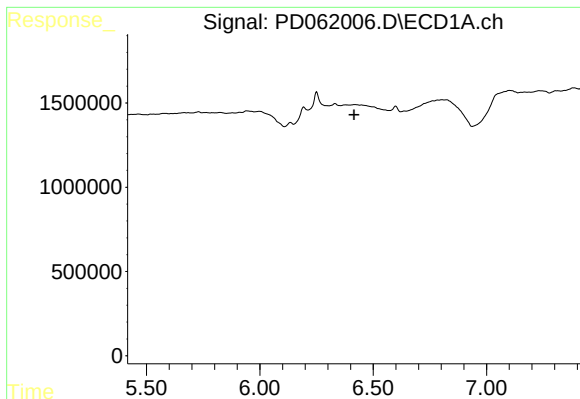

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

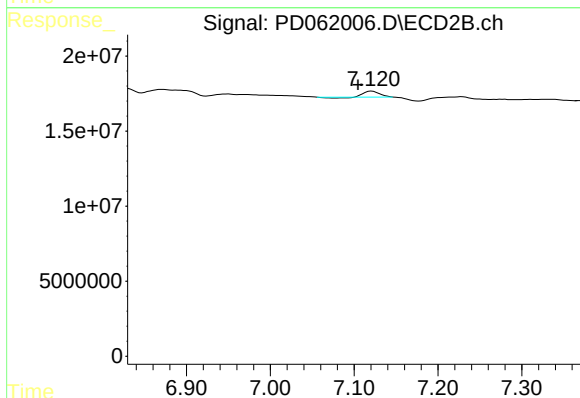


#17 4,4'-DDT

R.T.: 7.121 min
Delta R.T.: 0.016 min
Response: 4639132
Conc: 0.49 ng/ml

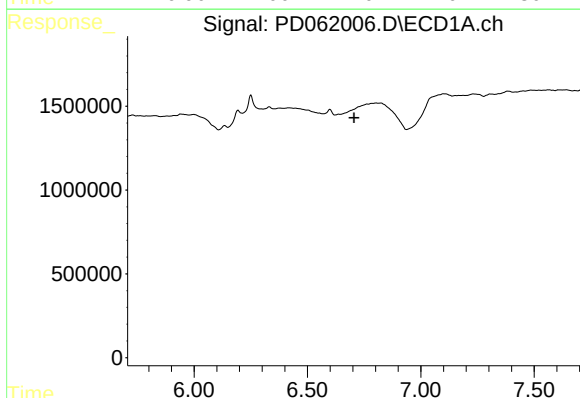


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

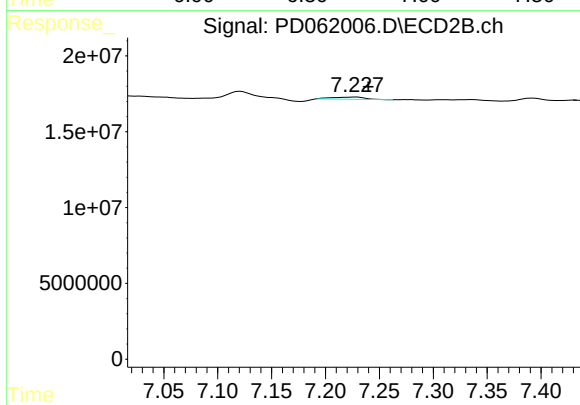

#19 Endosulfan Sulfate


R.T.: 7.228 min
Delta R.T.: -0.012 min
Response: 3292892
Conc: 0.33 ng/ml

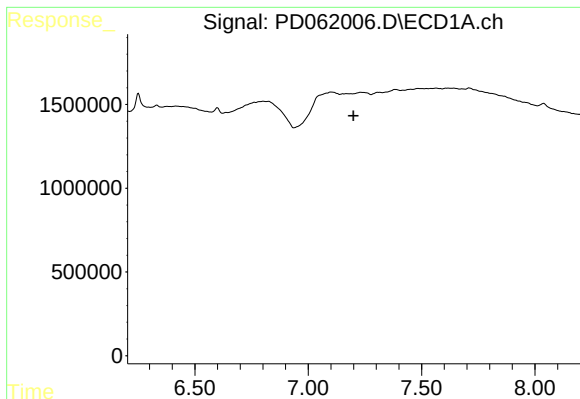

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

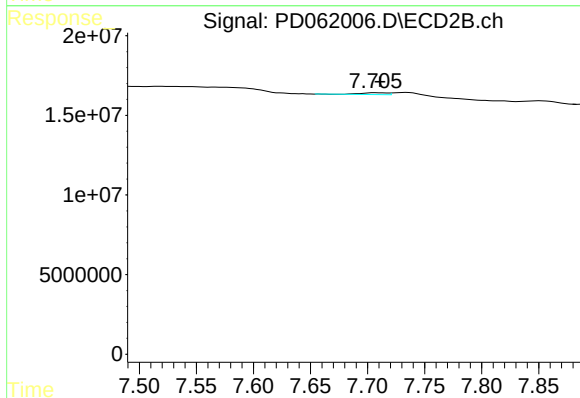


#21 Endrin ketone

R.T.: 7.708 min
Delta R.T.: -0.003 min
Response: 1934119
Conc: 0.19 ng/ml

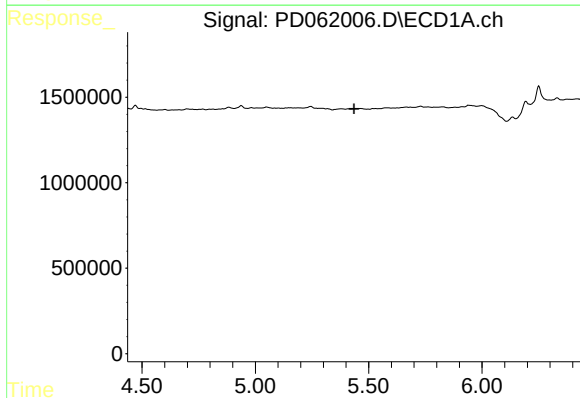


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

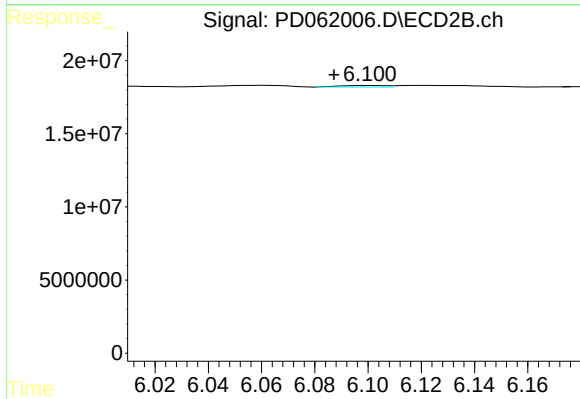

#25 Chlordane-3


R.T.: 6.101 min
Delta R.T.: 0.014 min
Response: 1343049
Conc: 0.81 ng/ml

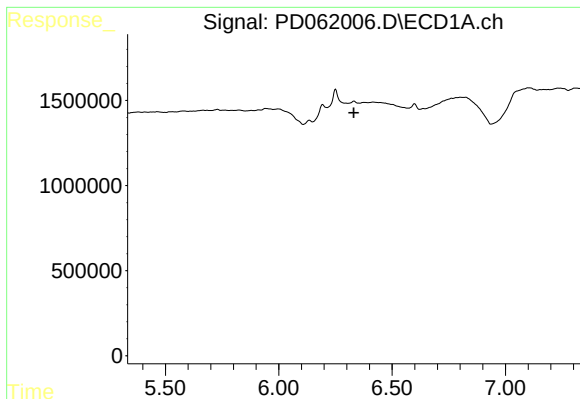

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

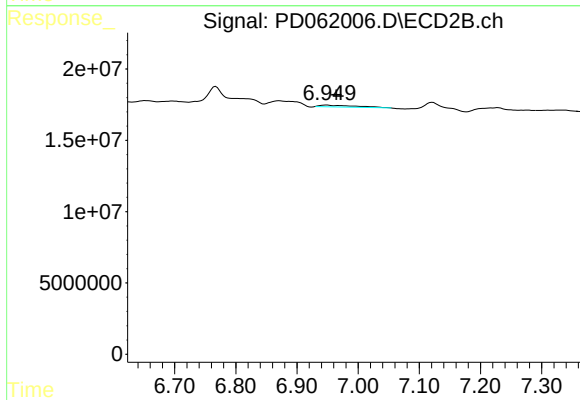


#27 Chlordane-5

R.T.: 6.949 min
Delta R.T.: -0.015 min
Response: 4981228
Conc: 13.82 ng/ml

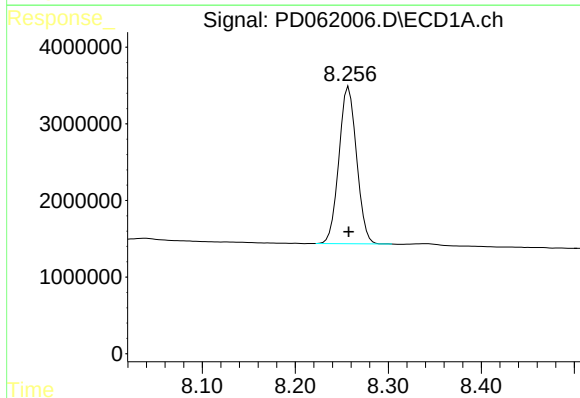

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 27071972
Conc: 22.00 ng/ml

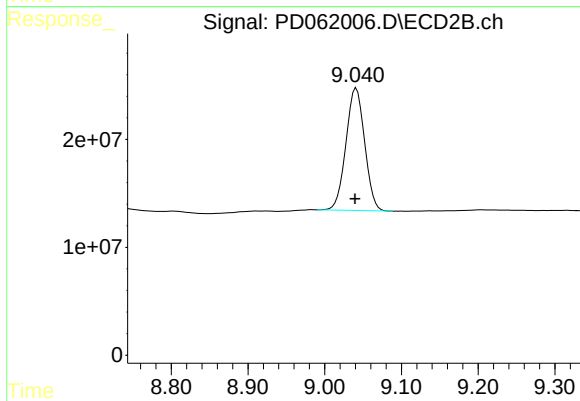

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 193295662
Conc: 20.48 ng/ml