

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 20:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:44:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	19245368	207.3E6	22.985	23.853
28)	SA Decachlor...	8.257	9.040	26016793	181.0E6	21.144	19.174
Target Compounds							
5)	MB Aldrin	0.000	5.463	0	912593	N.D.	0.073 #
7)	B delta-BHC	0.000	5.037	0	10354675	N.D.	0.783 #
8)	B Heptachlo...	0.000	5.862	0	8360921	N.D.	0.706 #
9)	A Endosulfan I	0.000	6.192f	0	482968	N.D.	0.045 #
17)	MA 4,4'-DDT	0.000	7.108	0	695962	N.D.	0.073 #
19)	B Endosulfa...	0.000	7.267f	0	669350	N.D.	0.067 #
22)	Mirex	0.000	8.190f	0	5077	N.D.	0.001 #
24)	Chlordane-2	0.000	5.463f	0	912593	N.D.	2.378 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 20:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:44:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

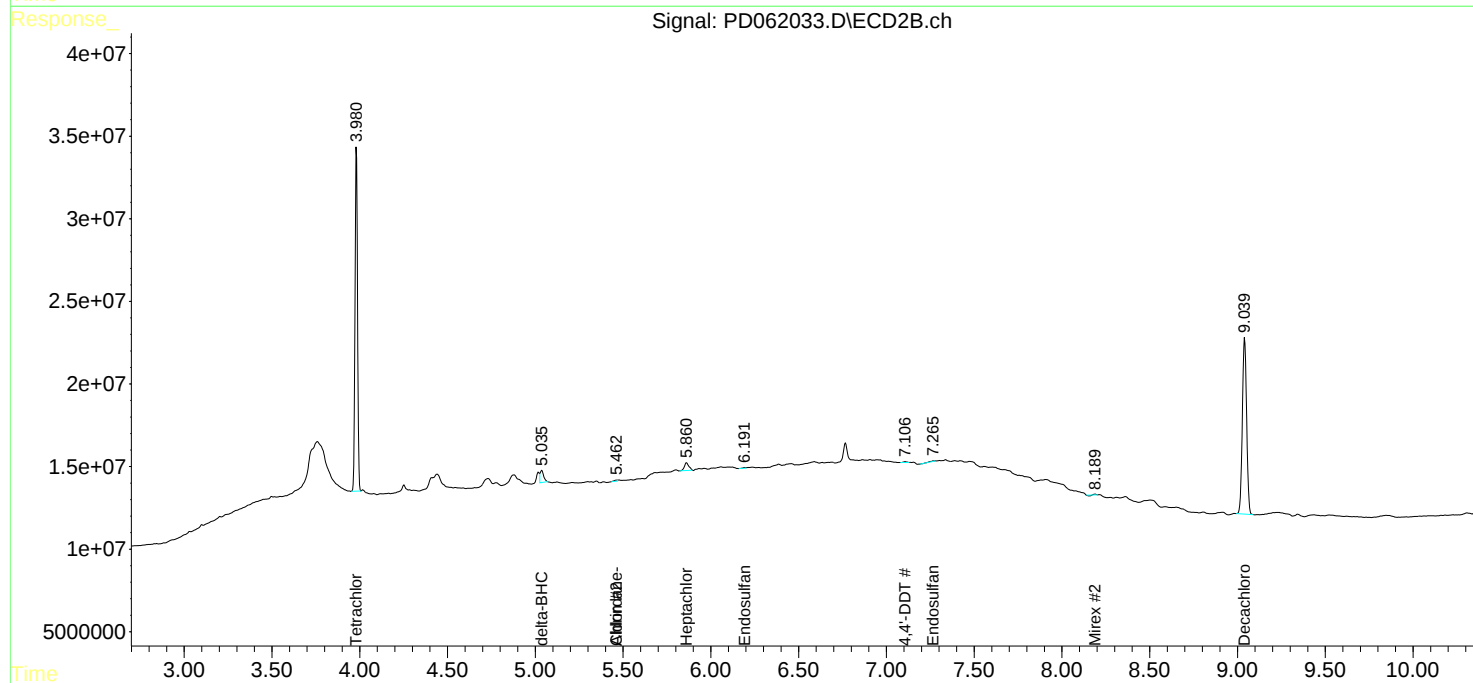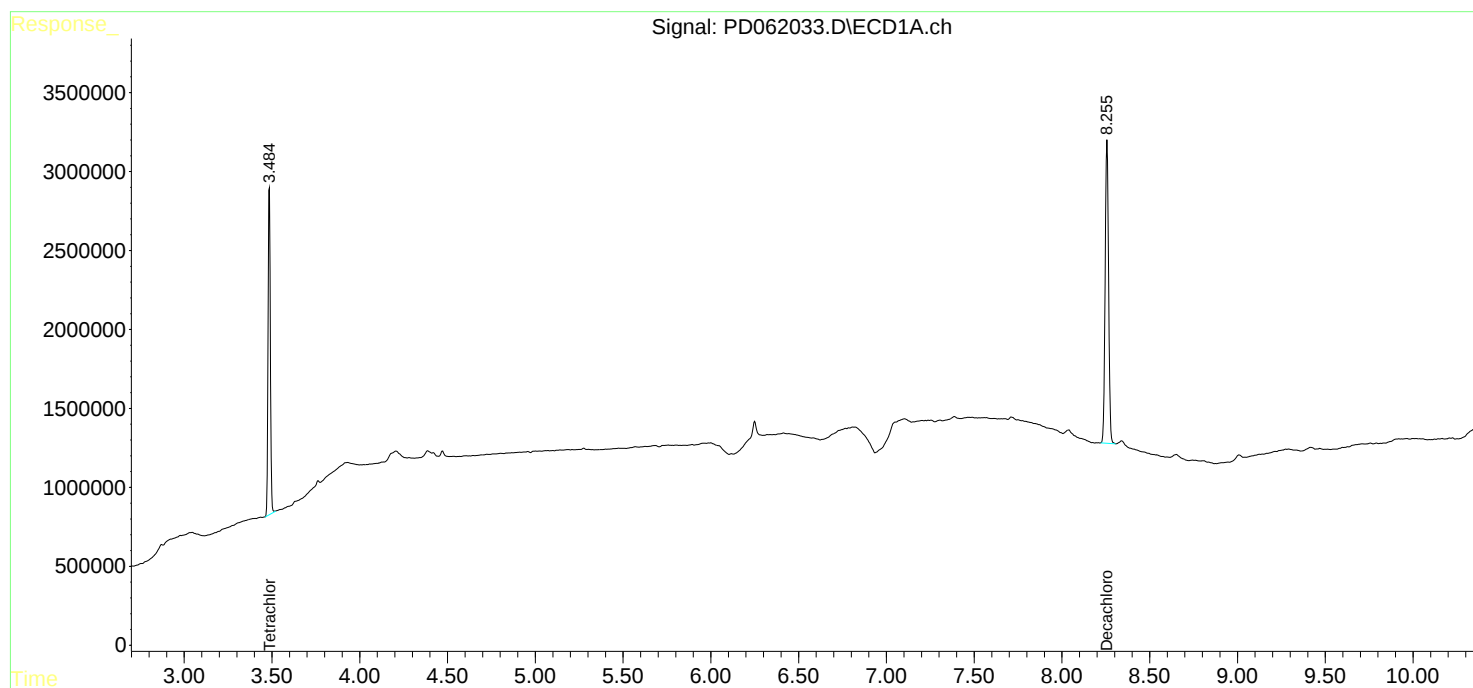


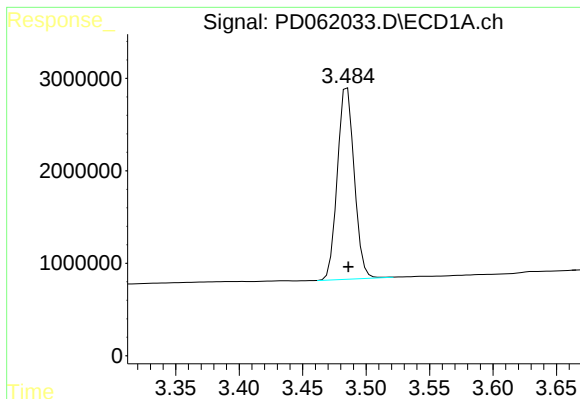

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 19245368
Conc: 22.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

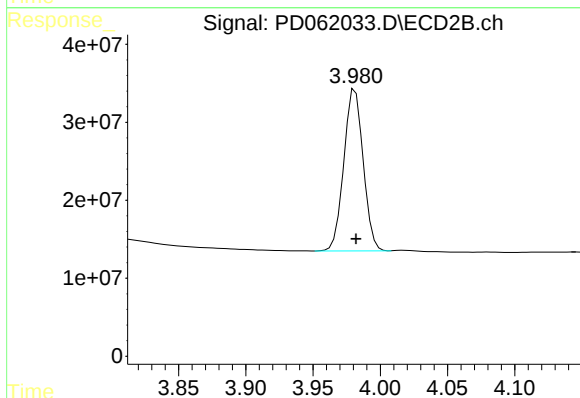


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 207254357
Conc: 23.85 ng/ml

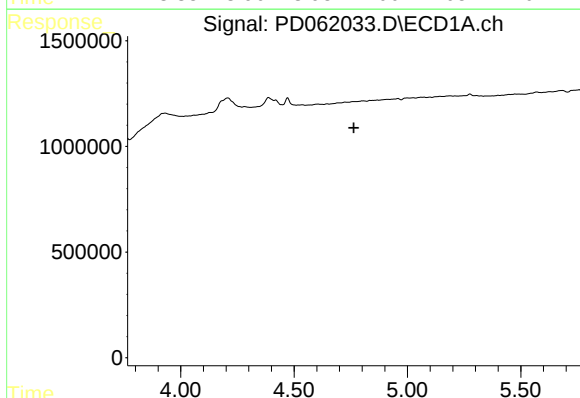


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

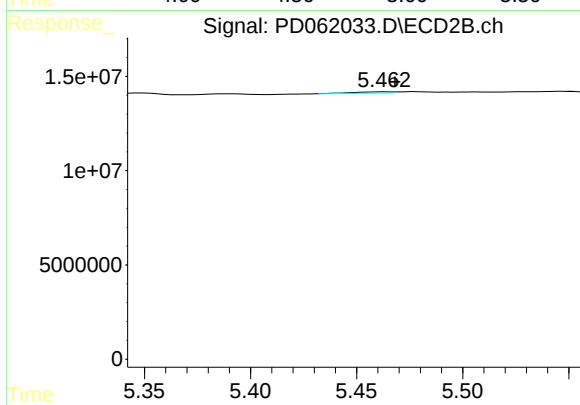

#5 Aldrin


R.T.: 5.463 min
Delta R.T.: -0.005 min
Response: 912593
Conc: 0.07 ng/ml

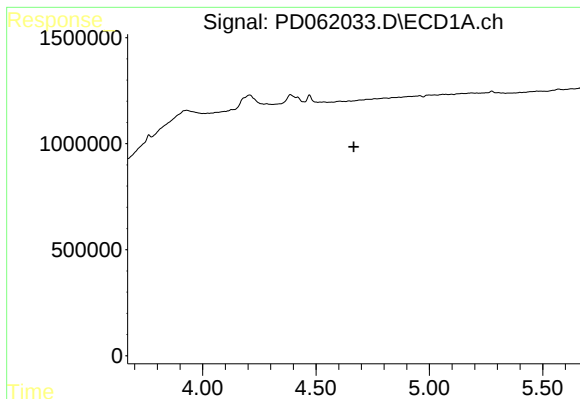

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

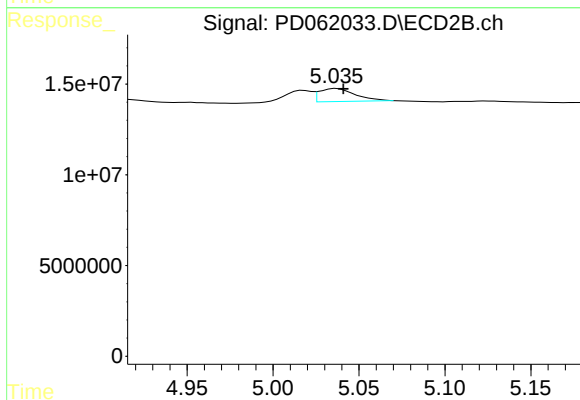


#7 delta-BHC

R.T.: 5.037 min
Delta R.T.: -0.004 min
Response: 10354675
Conc: 0.78 ng/ml

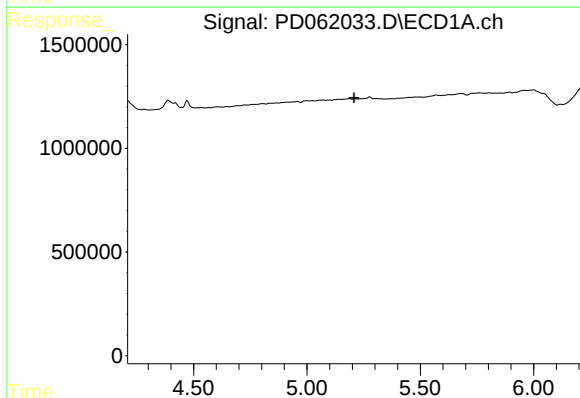


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

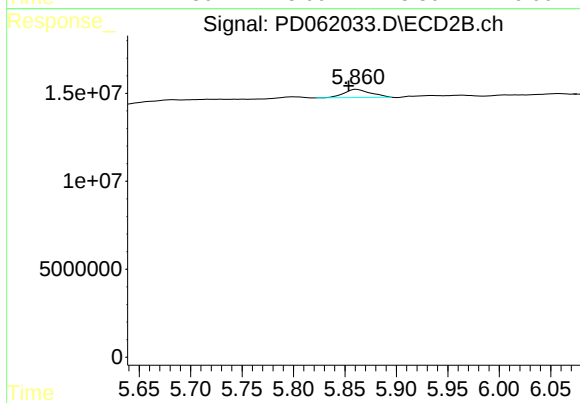

#8 Heptachlor epoxide


R.T.: 5.862 min
Delta R.T.: 0.008 min
Response: 8360921
Conc: 0.71 ng/ml

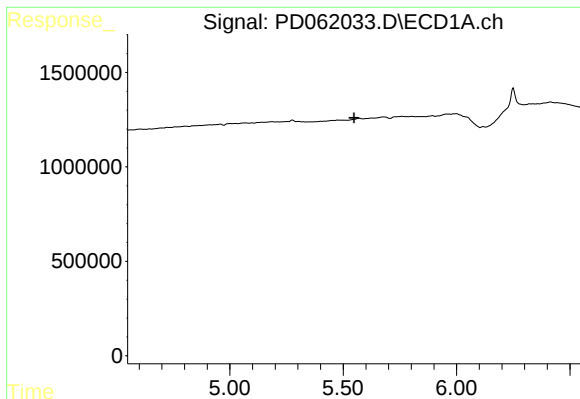

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

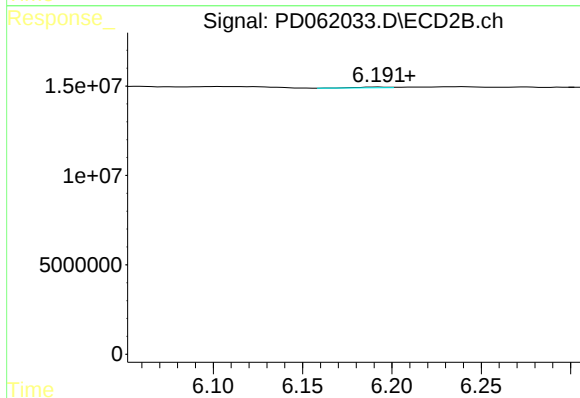


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: -0.018 min
Response: 482968
Conc: 0.04 ng/ml

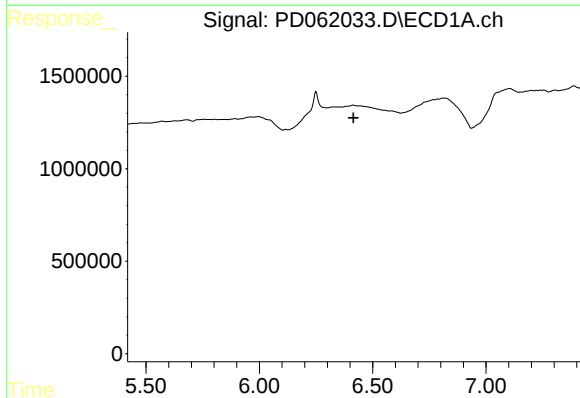


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

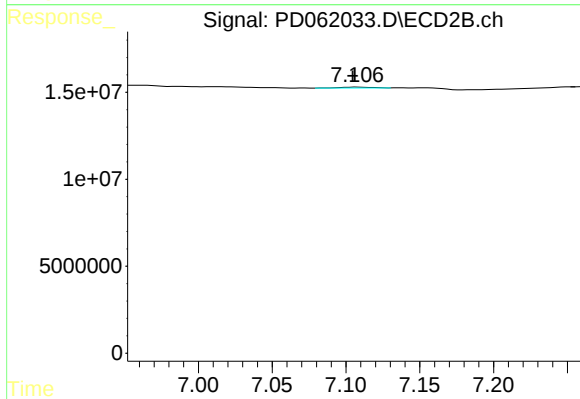

#17 4,4'-DDT


R.T.: 7.108 min
Delta R.T.: 0.003 min
Response: 695962
Conc: 0.07 ng/ml

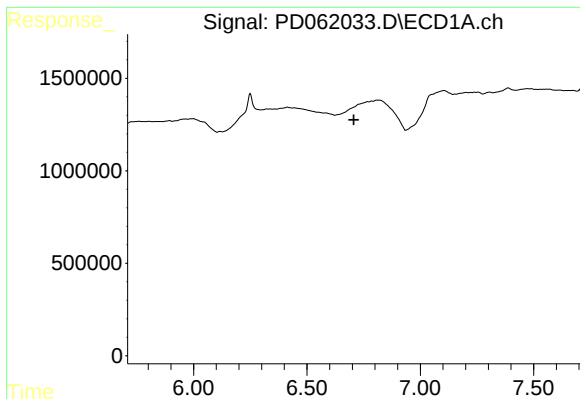

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

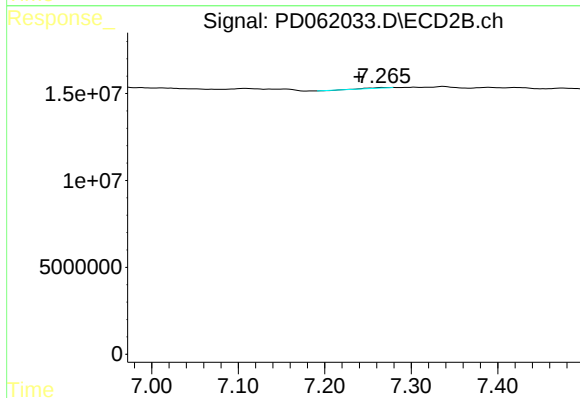


#19 Endosulfan Sulfate

R.T.: 7.267 min
Delta R.T.: 0.027 min
Response: 669350
Conc: 0.07 ng/ml

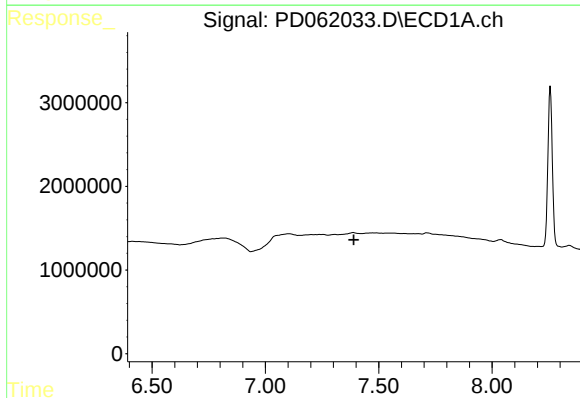


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

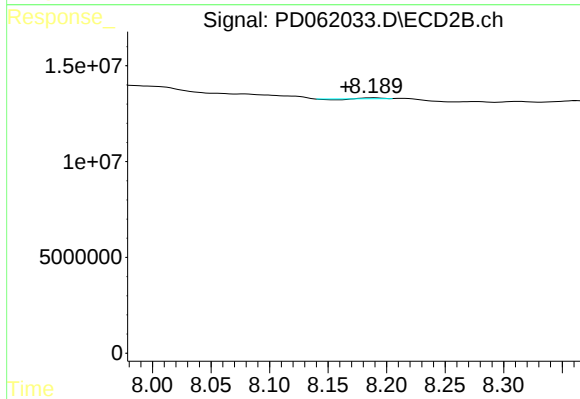

#22 Mirex


R.T.: 8.190 min
Delta R.T.: 0.025 min
Response: 5077
Conc: 0.00 ng/ml

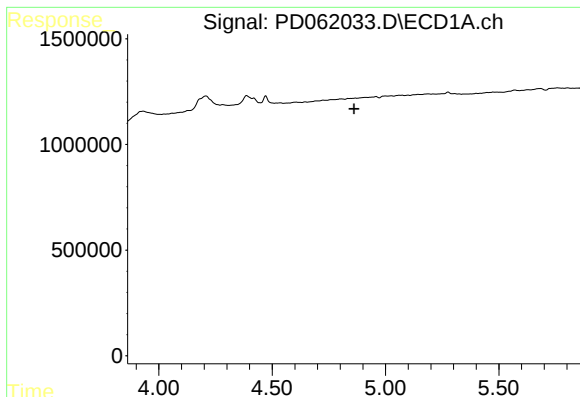

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

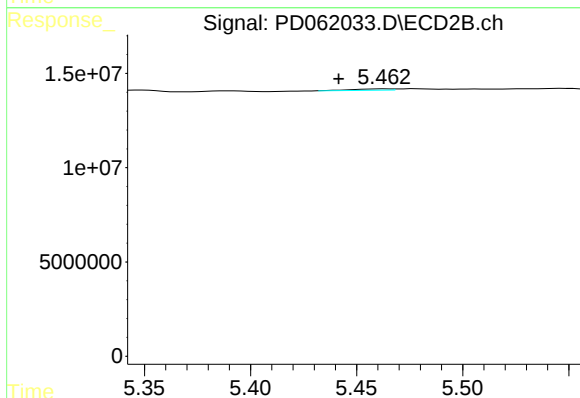


#24 Chlordane-2

R.T.: 5.463 min
Delta R.T.: 0.021 min
Response: 912593
Conc: 2.38 ng/ml

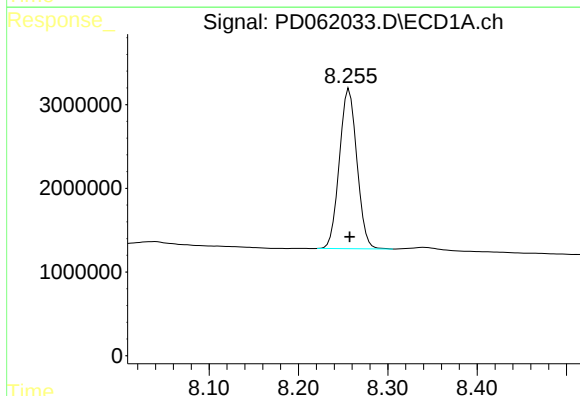

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 26016793
Conc: 21.14 ng/ml

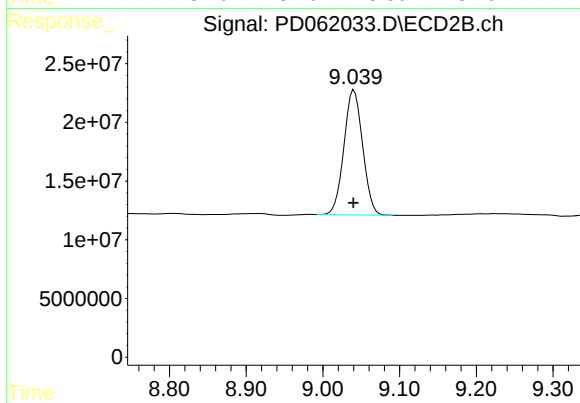

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 181017432
Conc: 19.17 ng/ml