

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 23:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:47:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	19371301	210.7E6	23.136	24.251
28)	SA Decachlor...	8.257	9.040	26060225	181.8E6	21.180	19.258
Target Compounds							
7)	B delta-BHC	0.000	5.036	0	4182720	N.D.	0.316 #
8)	B Heptachlo...	0.000	5.860	0	8726095	N.D.	0.737 #
9)	A Endosulfan I	0.000	6.191f	0	56328	N.D.	0.005 #
10)	B gamma-Chl...	0.000	6.098	0	748090	N.D.	0.063 #
13)	MA Dieldrin	0.000	6.484f	0	369817	N.D.	0.032 #
17)	MA 4,4'-DDT	0.000	7.112	0	2595224	N.D.	0.272 #
20)	A Methoxychlor	0.000	7.562	0	2356919	N.D.	0.523 #
25)	Chlordane-3	0.000	6.098	0	748090	N.D.	0.451 #
26)	Chlordane-4	0.000	6.191f	0	56328	N.D.	0.029 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 23:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:47:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

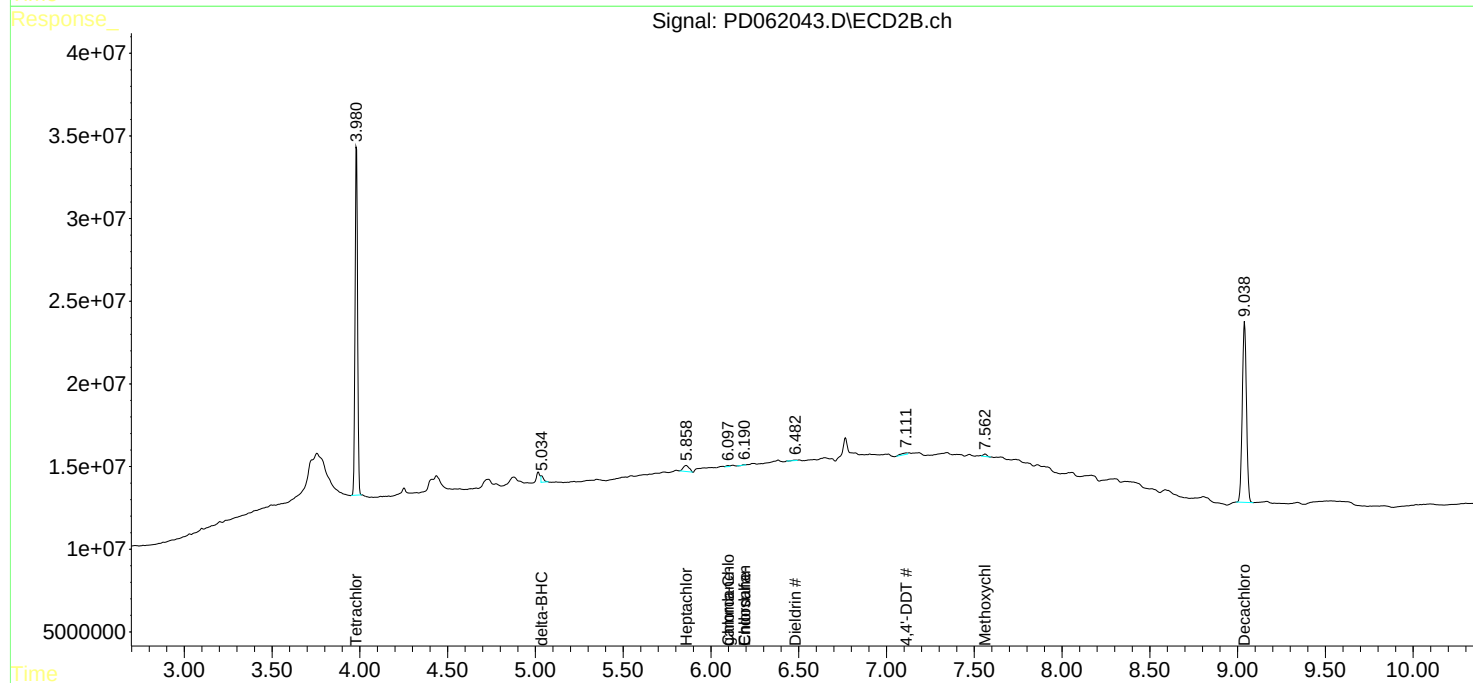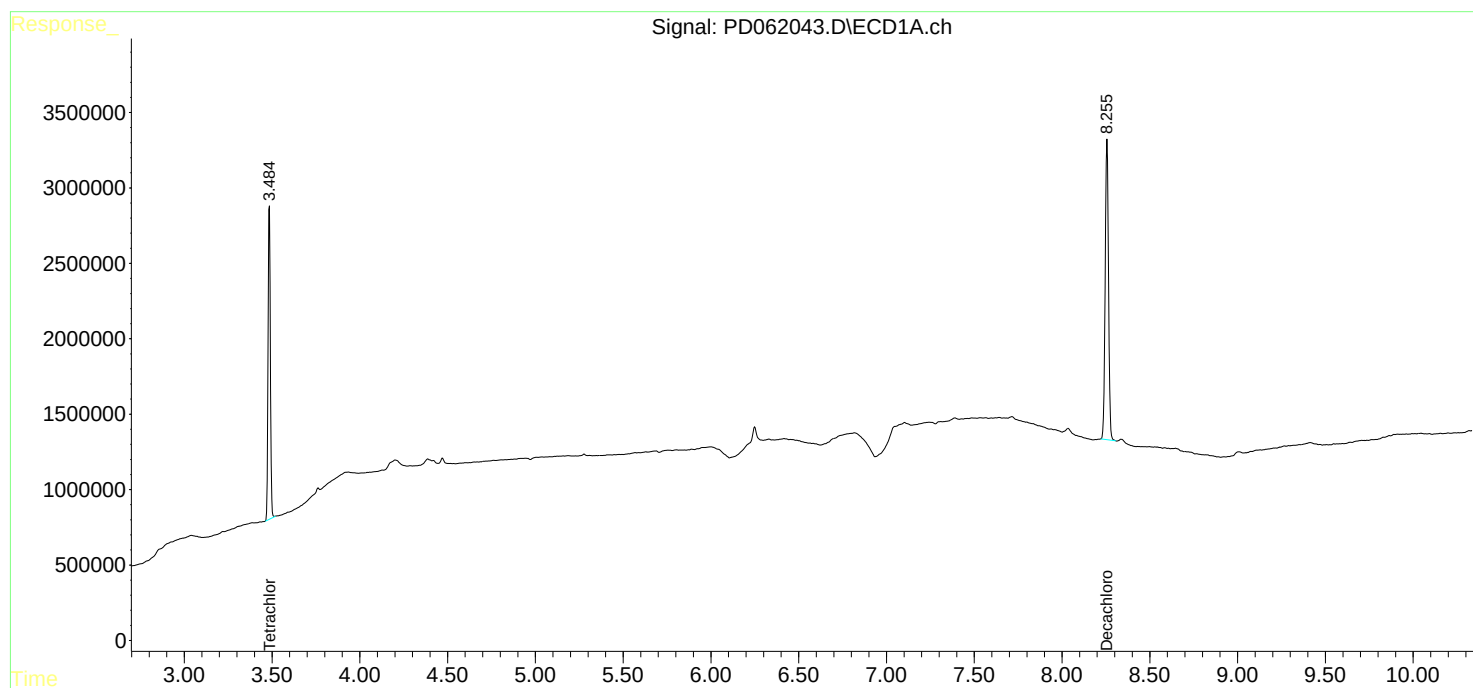


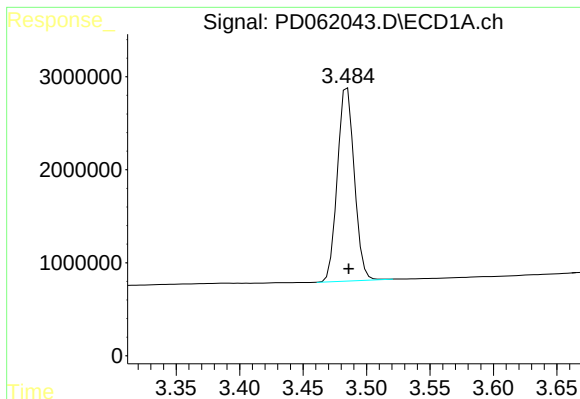

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 19371301
Conc: 23.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

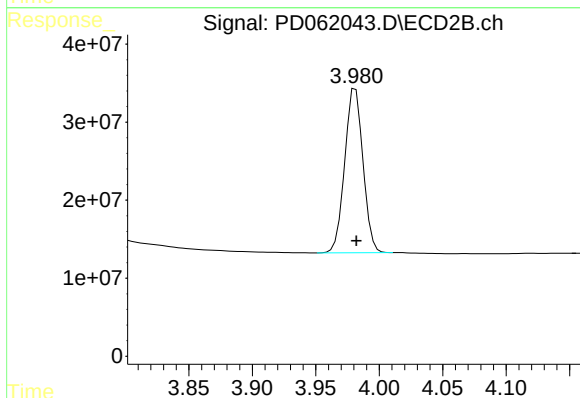


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 210709983
Conc: 24.25 ng/ml

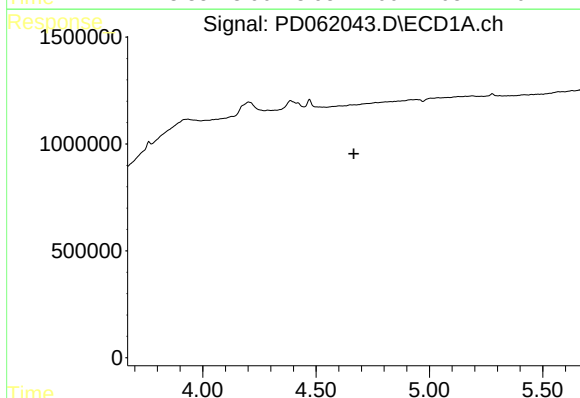


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

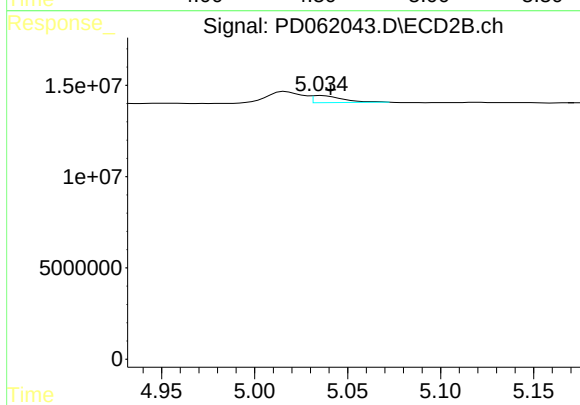

#7 delta-BHC


R.T.: 5.036 min
Delta R.T.: -0.005 min
Response: 4182720
Conc: 0.32 ng/ml

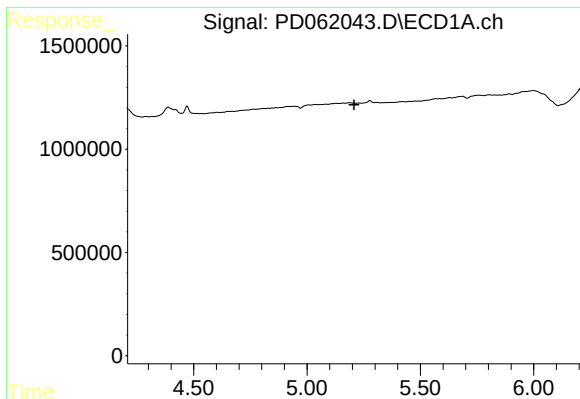

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

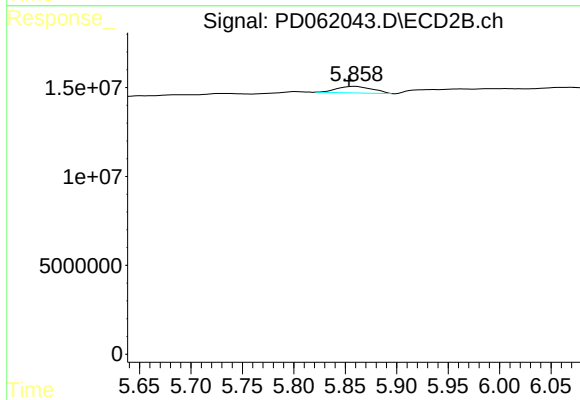


#8 Heptachlor epoxide

R.T.: 5.860 min
Delta R.T.: 0.006 min
Response: 8726095
Conc: 0.74 ng/ml

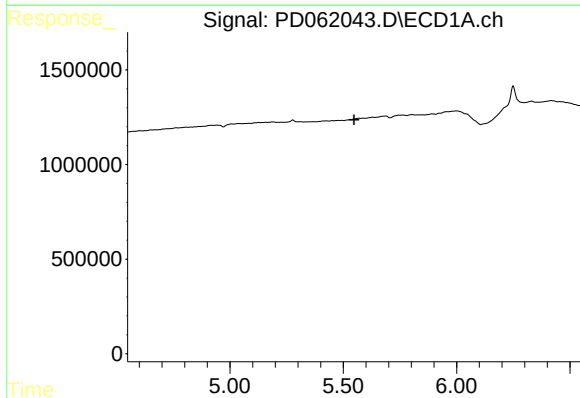


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

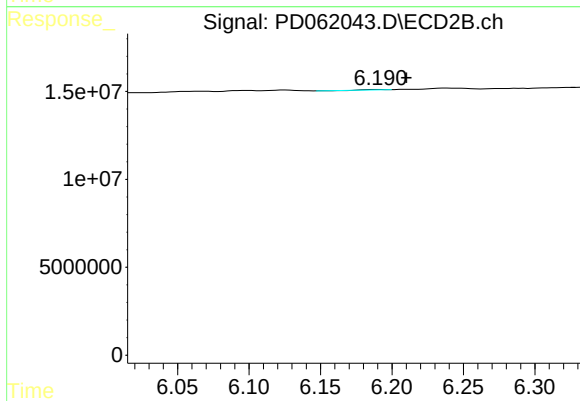

#9 Endosulfan I


R.T.: 6.191 min
Delta R.T.: -0.019 min
Response: 56328
Conc: 0.01 ng/ml

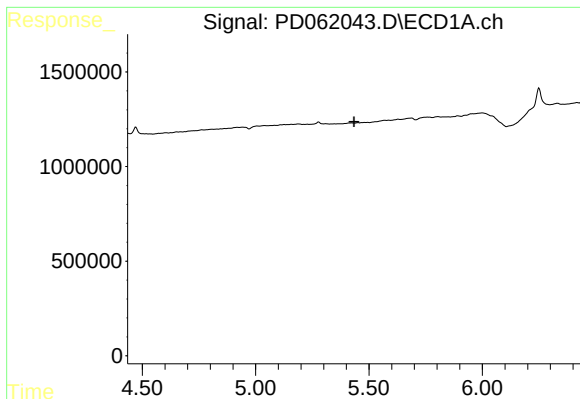

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

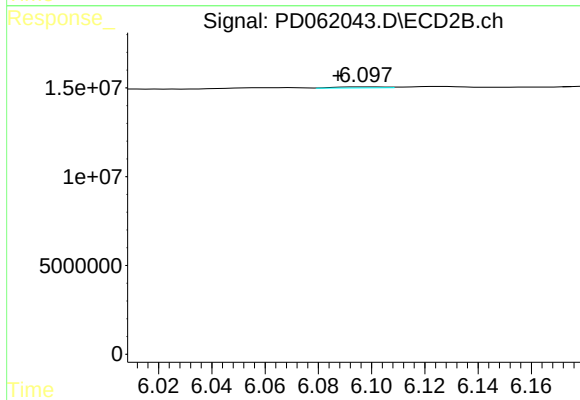


#10 gamma-Chlordane

R.T.: 6.098 min
Delta R.T.: 0.011 min
Response: 748090
Conc: 0.06 ng/ml

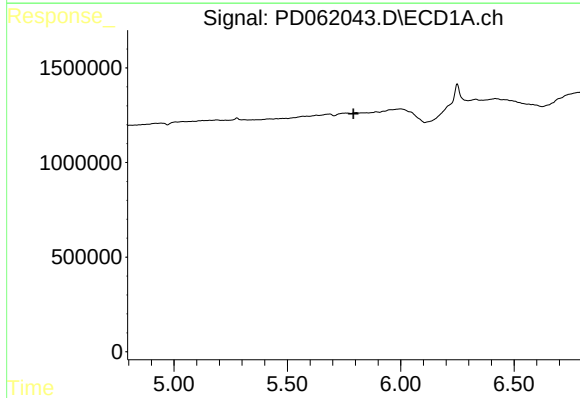


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

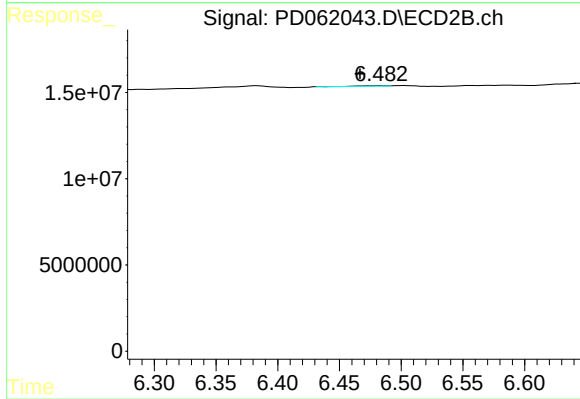

#13 Dieldrin


R.T.: 6.484 min
Delta R.T.: 0.017 min
Response: 369817
Conc: 0.03 ng/ml

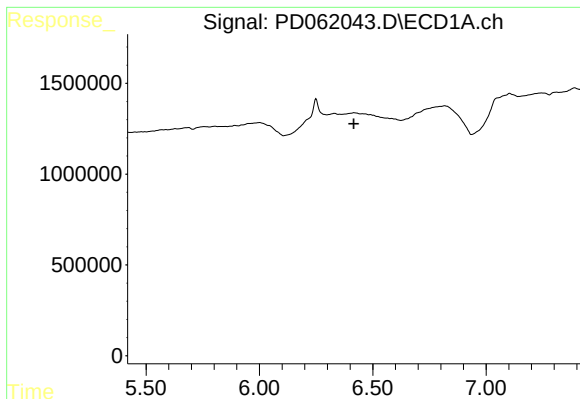

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

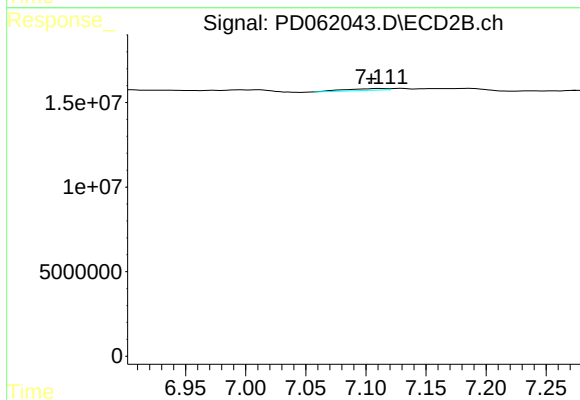


#17 4,4'-DDT

R.T.: 7.112 min
Delta R.T.: 0.007 min
Response: 2595224
Conc: 0.27 ng/ml

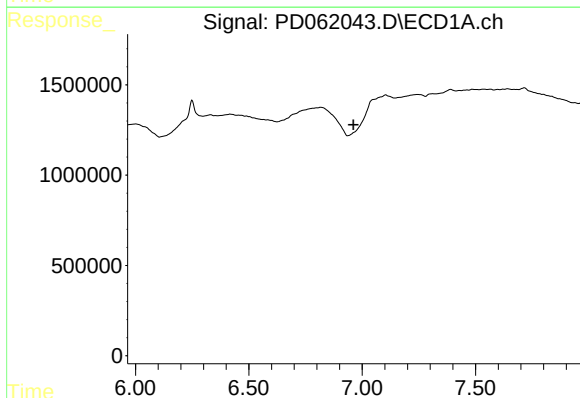


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

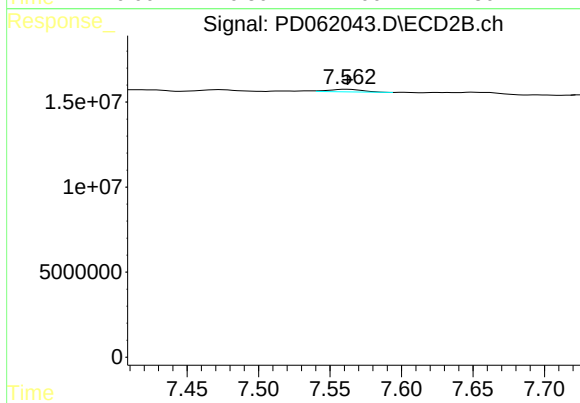

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 2356919
Conc: 0.52 ng/ml

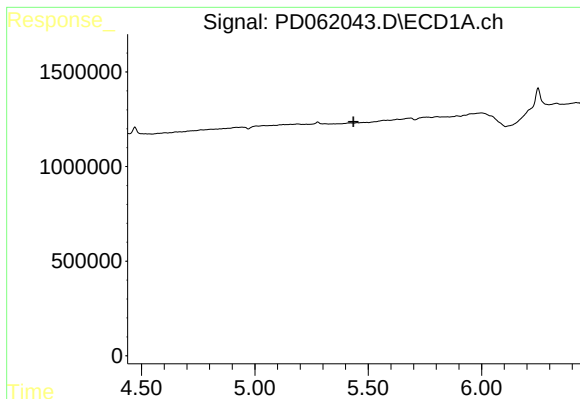

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

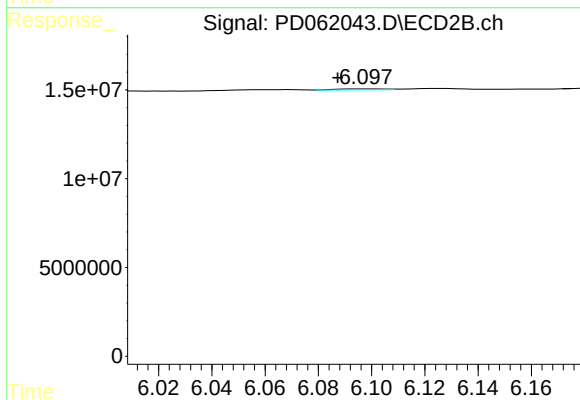


#25 Chlordane-3

R.T.: 6.098 min
Delta R.T.: 0.011 min
Response: 748090
Conc: 0.45 ng/ml

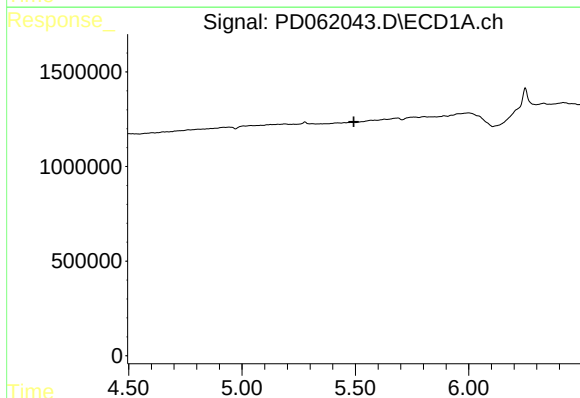


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

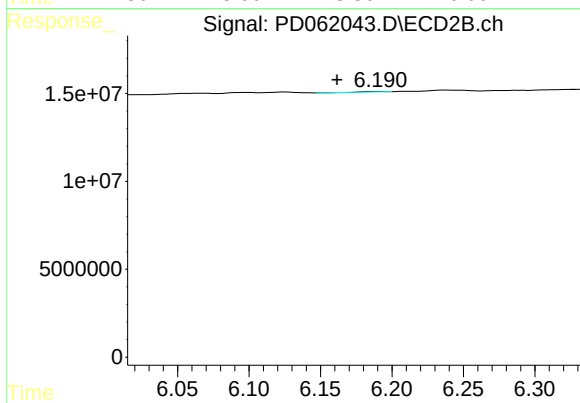

#26 Chlordane-4


R.T.: 6.191 min
Delta R.T.: 0.030 min
Response: 56328
Conc: 0.03 ng/ml

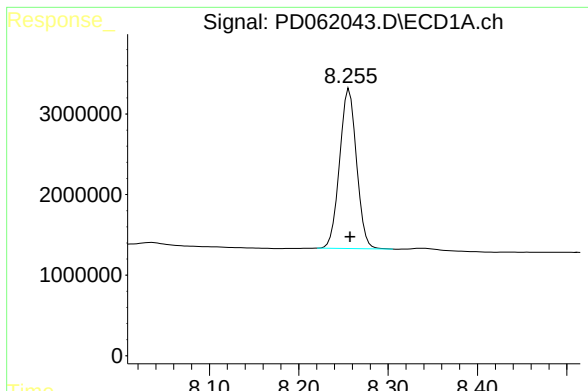

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 26060225
Conc: 21.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

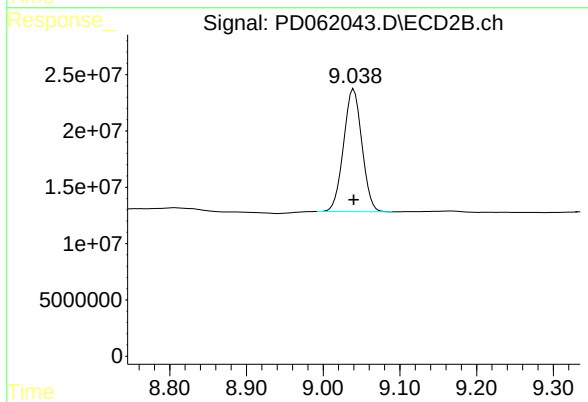

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 181802549
Conc: 19.26 ng/ml