

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 16:39
 Operator : AR\AJ
 Sample : M1933-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BENNETT_BH_01_0-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:39:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	11379924	127.4E6	13.591	14.662
28)	SA Decachlor...	8.258	9.042	14762400	100.7E6	11.998	10.668
Target Compounds							
11)	B alpha-Chl...	5.494	6.162	1658864	42563665	1.428	3.734 #
12)	B 4,4'-DDE	5.657	6.317	18854234	206.5E6	16.779	17.920
17)	MA 4,4'-DDT	6.417	7.105	5584268	62194846	6.200	6.511



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 16:39
Operator : AR\AJ
Sample : M1933-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_01_0-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:39:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

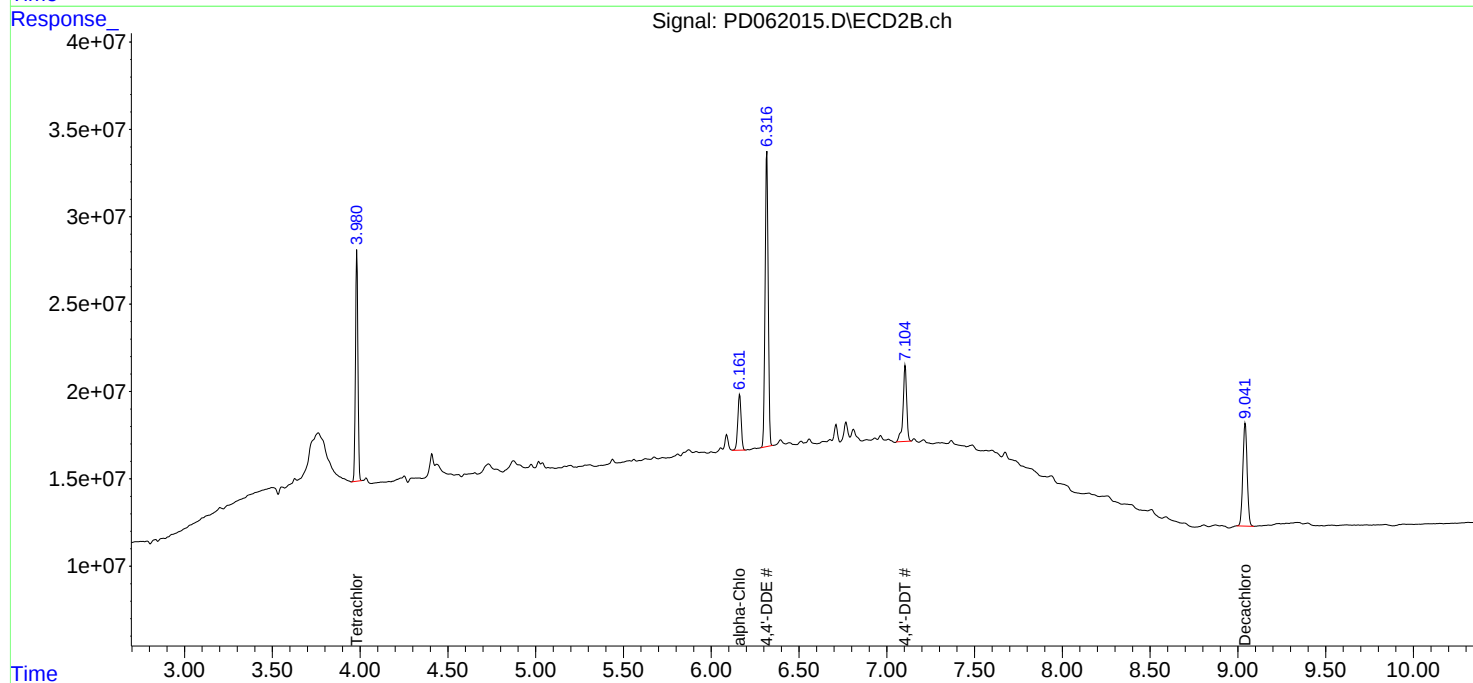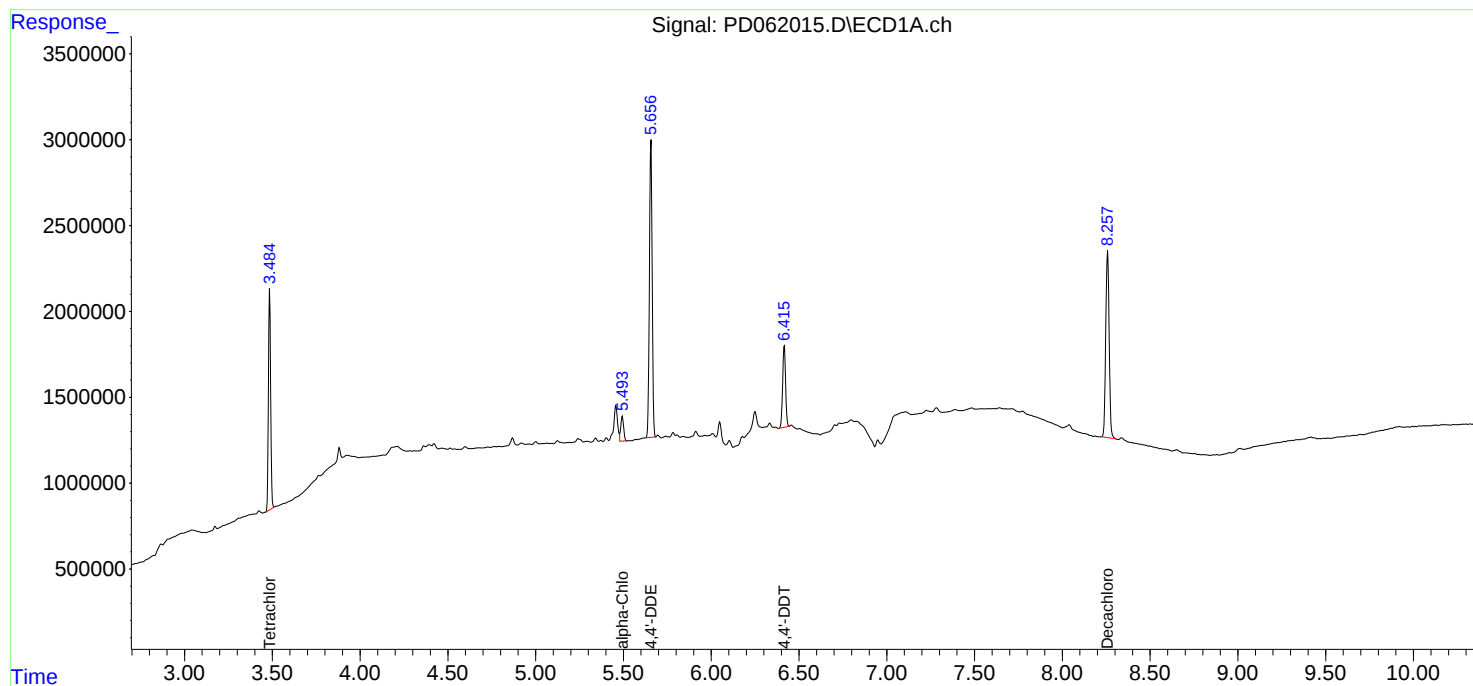


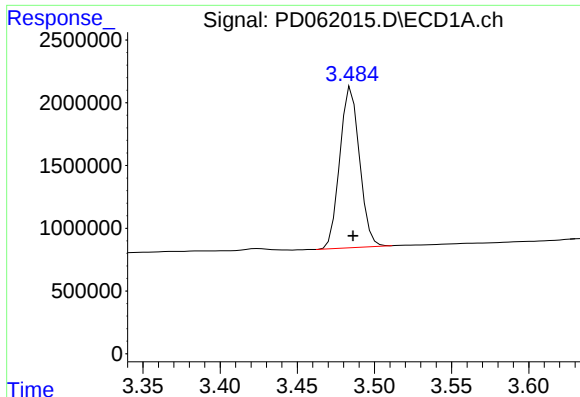

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 11379924
Conc: 13.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_01_0-1

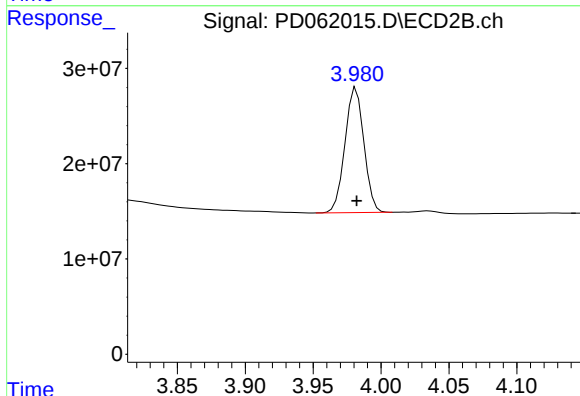


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 127393083
Conc: 14.66 ng/ml

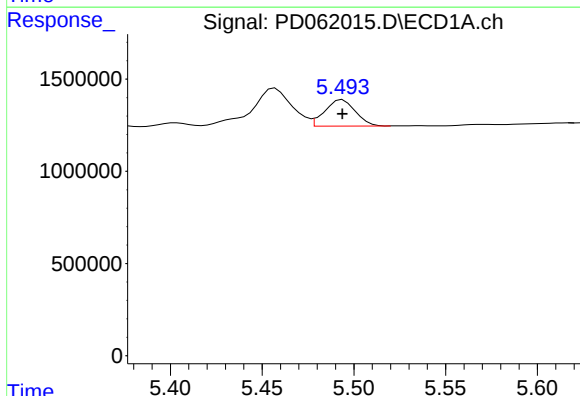


#11 alpha-Chlordane

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 1658864
Conc: 1.43 ng/ml

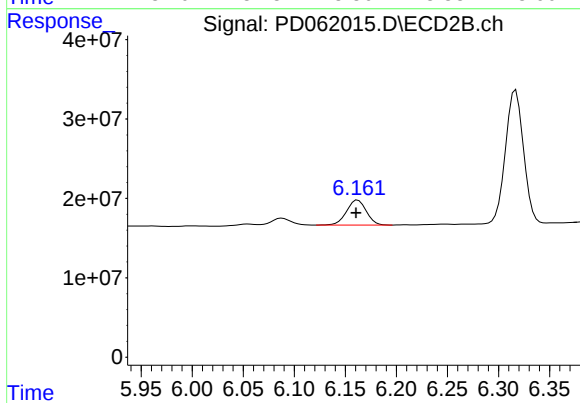

#11 alpha-Chlordane


R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 42563665
Conc: 3.73 ng/ml

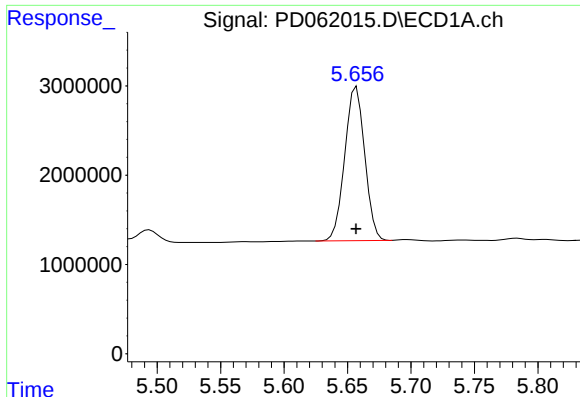

#12 4,4'-DDE


R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 18854234
Conc: 16.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_01_0-1

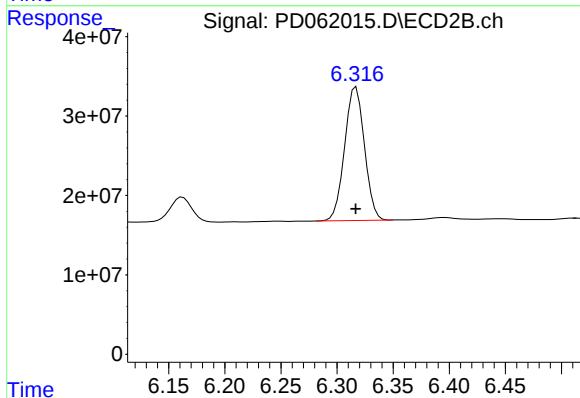


#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 206507933
Conc: 17.92 ng/ml

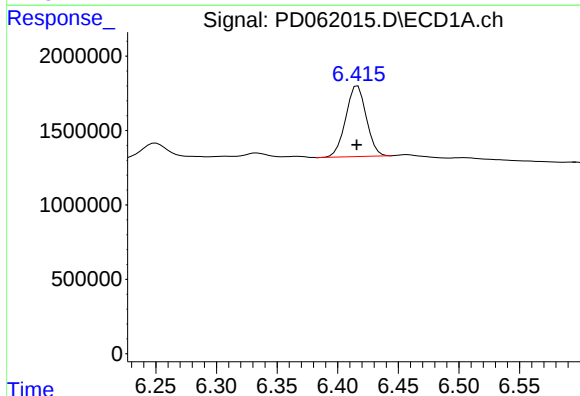


#17 4,4'-DDT

R.T.: 6.417 min
Delta R.T.: 0.000 min
Response: 5584268
Conc: 6.20 ng/ml

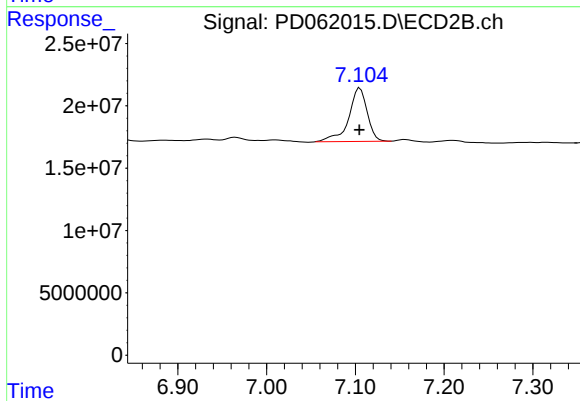

#17 4,4'-DDT


R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 62194846
Conc: 6.51 ng/ml

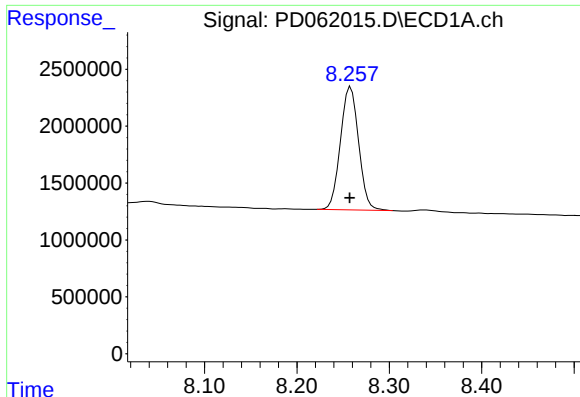

#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 14762400
Conc: 12.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_01_0-1

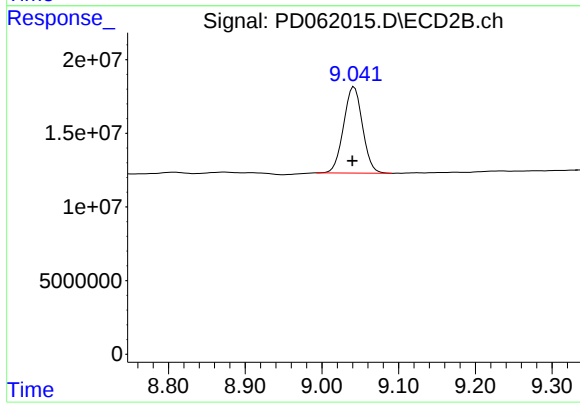

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 100713947
Conc: 10.67 ng/ml