

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 16:53
 Operator : AR\AJ
 Sample : M1933-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BENNETT_BH_04_0-1

Manual Integrations
 APPROVED

Ankita
 4/8/2021 3:08:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:39:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	11081171	123.0E6	13.234	14.153
28)	SA Decachlor...	8.258	9.042	18635684	130.6E6	15.146	13.839
Target Compounds							
11)	B alpha-Chl...	5.492	6.163	709625	29348982	0.611m	2.574 #
12)	B 4,4'-DDE	5.657	6.317	27431534	294.8E6	24.412	25.585
17)	MA 4,4'-DDT	6.416	7.104	7378606	60742452	8.192	6.359m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 16:53
Operator : AR\AJ
Sample : M1933-08
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_04_0-1


Manual Integrations
APPROVED

Ankita
4/8/2021 3:08:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:39:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

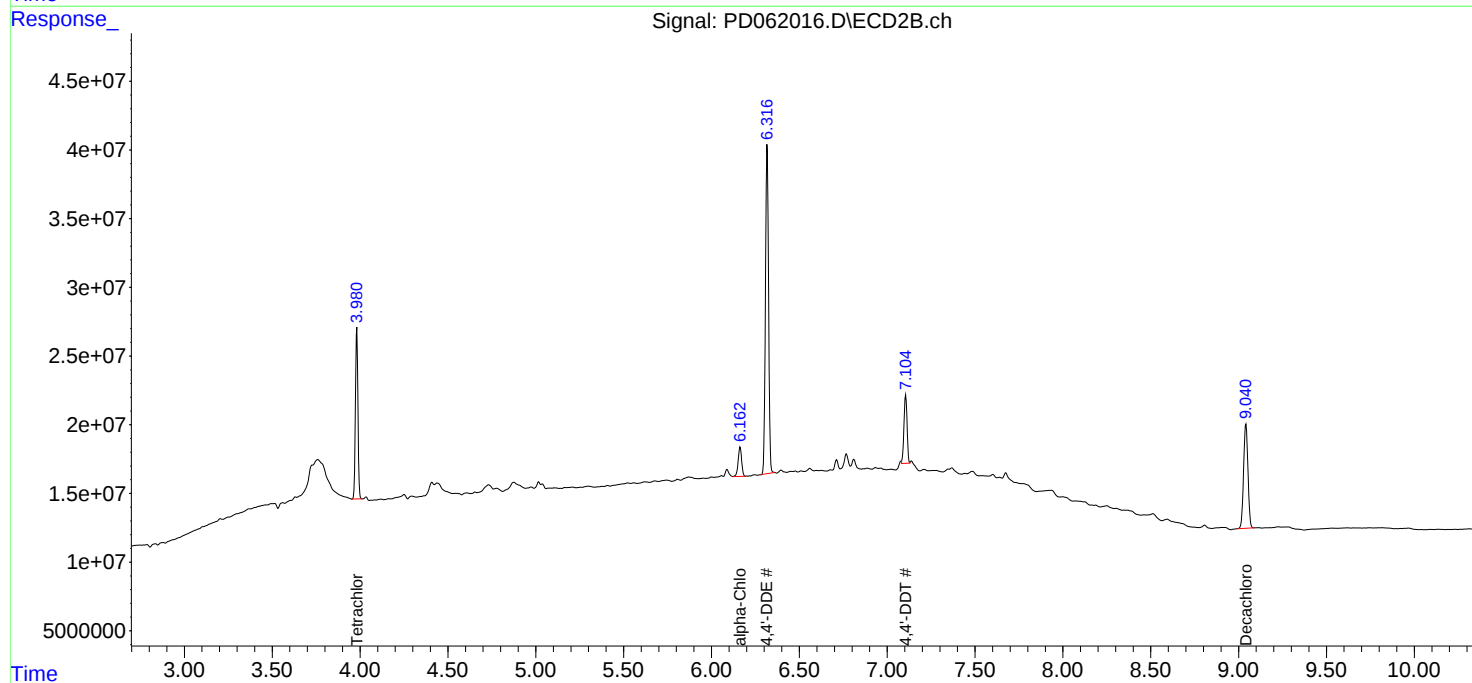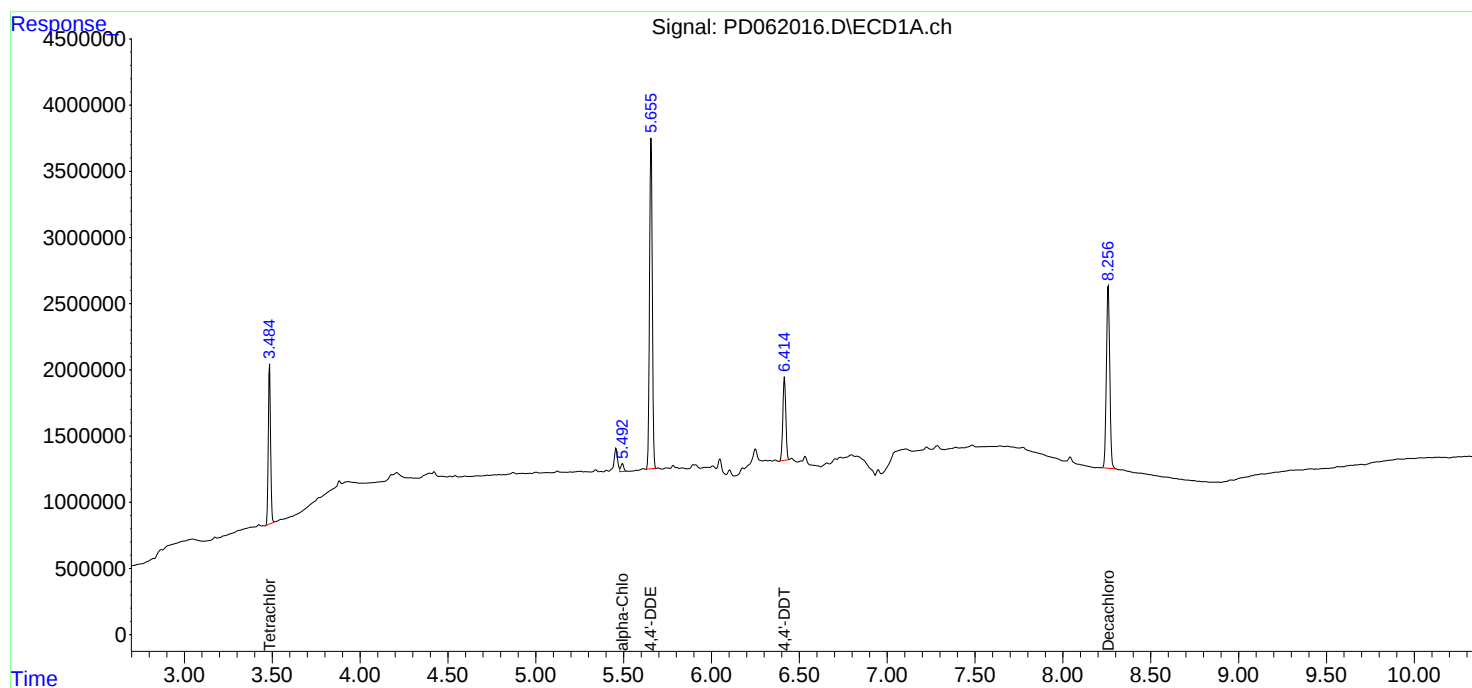

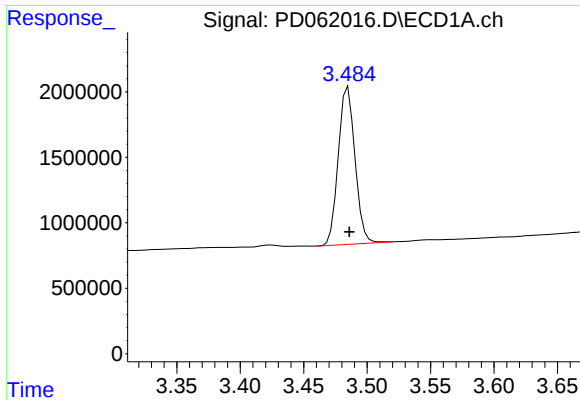


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 11081171
Conc: 13.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_04_0-1


Manual Integrations
APPROVED

Ankita
4/8/2021 3:08:56 PM

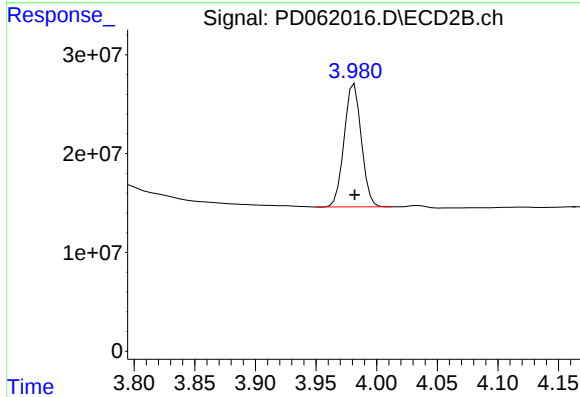


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 122974252
Conc: 14.15 ng/ml

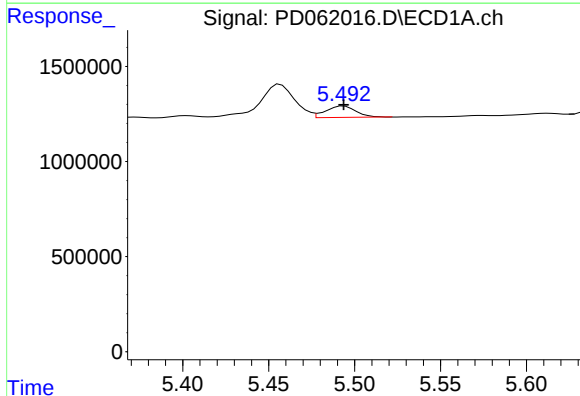


#11 alpha-Chlordane

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 709625
Conc: 0.61 ng/ml m

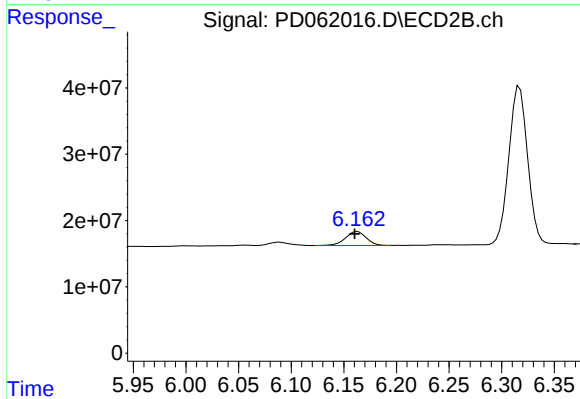

#11 alpha-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.003 min
Response: 29348982
Conc: 2.57 ng/ml

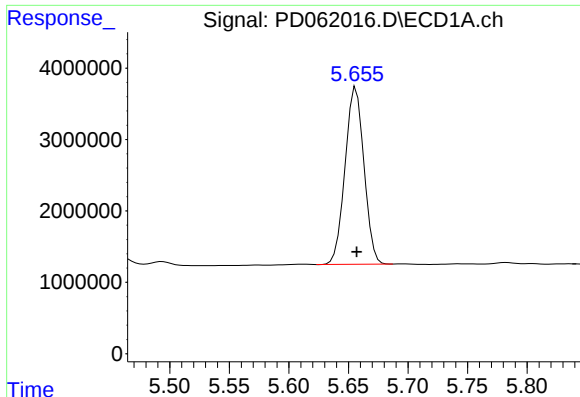


#12 4,4'-DDE

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 27431534
Conc: 24.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_04_0-1


Manual Integrations
APPROVED

Ankita
4/8/2021 3:08:56 PM

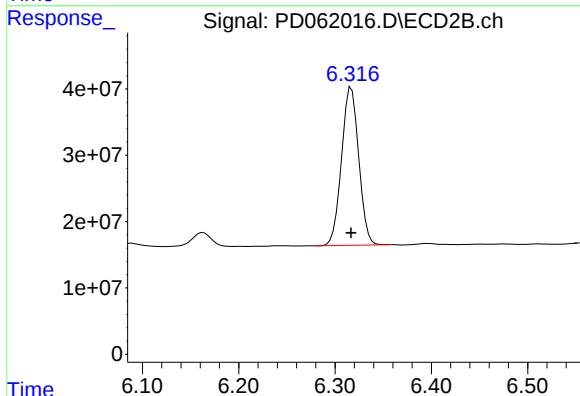


#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 294839160
Conc: 25.58 ng/ml

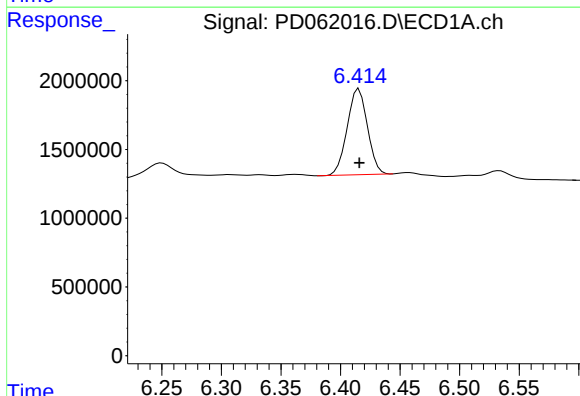


#17 4,4'-DDT

R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 7378606
Conc: 8.19 ng/ml

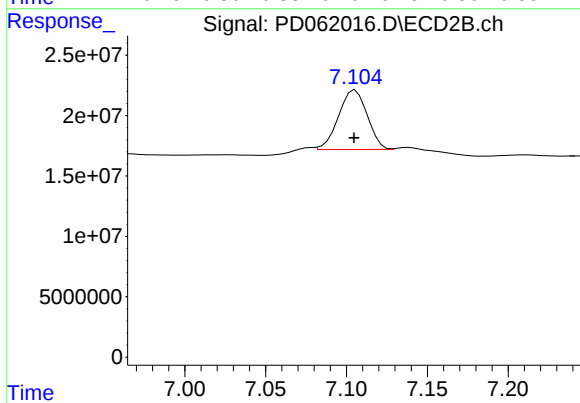

#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 60742452
Conc: 6.36 ng/ml m

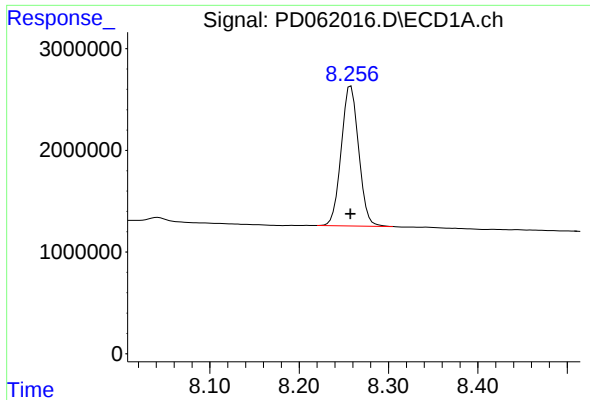


#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 18635684
Conc: 15.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
BENNETT_BH_04_0-1

Manual Integrations
APPROVED

Ankita
4/8/2021 3:08:56 PM

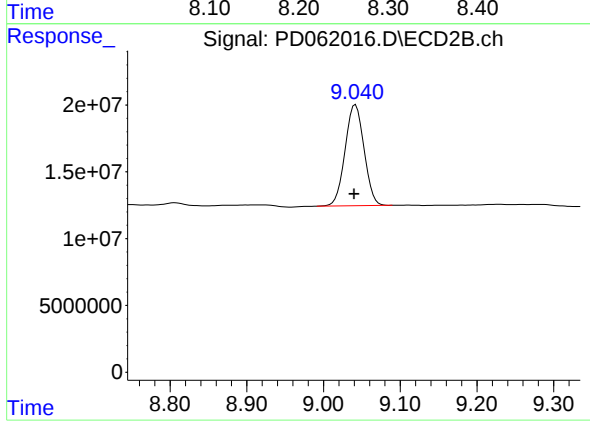

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 130645254
Conc: 13.84 ng/ml