

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
 Data File : PD062025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 18:59
 Operator : AR\AJ
 Sample : M1961-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TR2-A-D-COMP

Manual Integrations
 APPROVED

Ankita
 4/8/2021 3:10:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:42:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	11772282	130.3E6	14.060	14.997
28)	SA Decachlor...	8.257	9.041	15837545	105.4E6	12.872	11.168
Target Compounds							
11)	B alpha-Chl...	5.492	6.162	496039	9812302	0.427m	0.861 #
12)	B 4,4'-DDE	5.656	6.317	1299466	17316571	1.156	1.503 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040721\
Data File : PD062025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 18:59
Operator : AR\AJ
Sample : M1961-12
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
4/8/2021 3:10:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:42:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

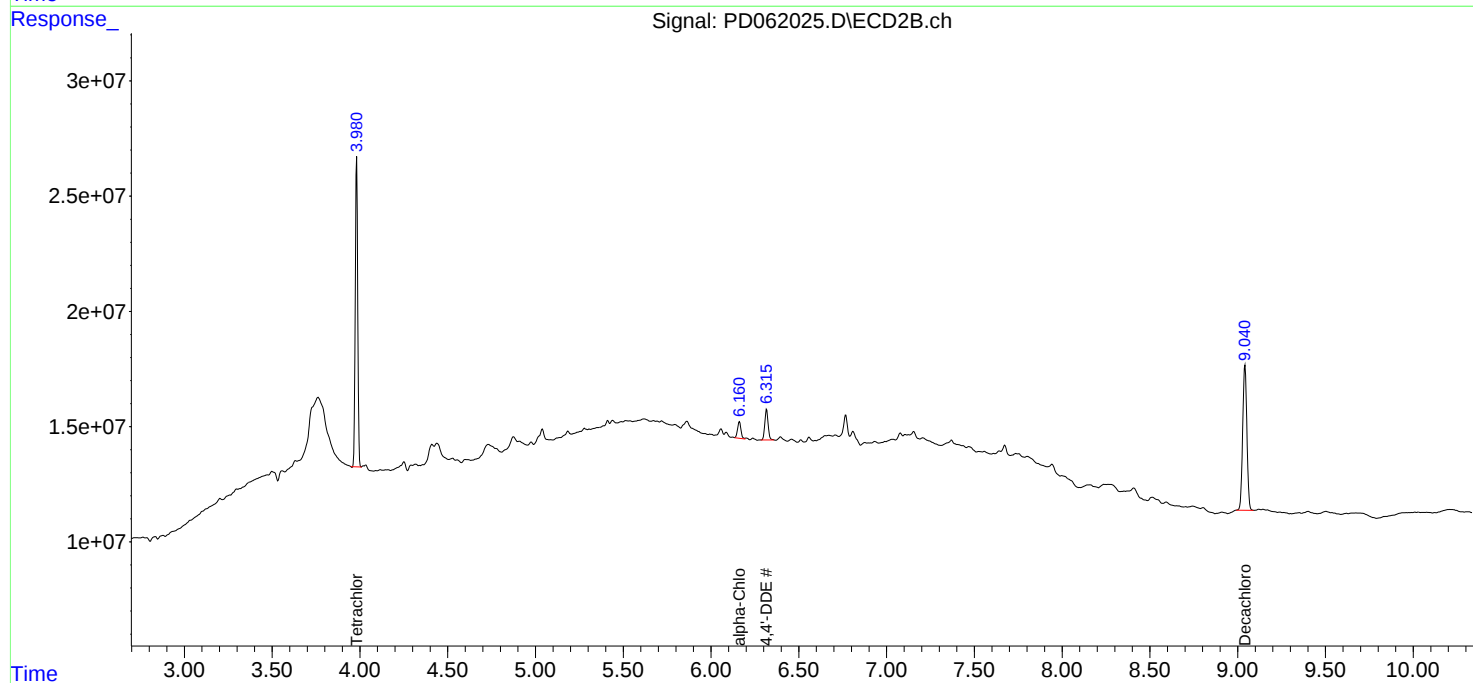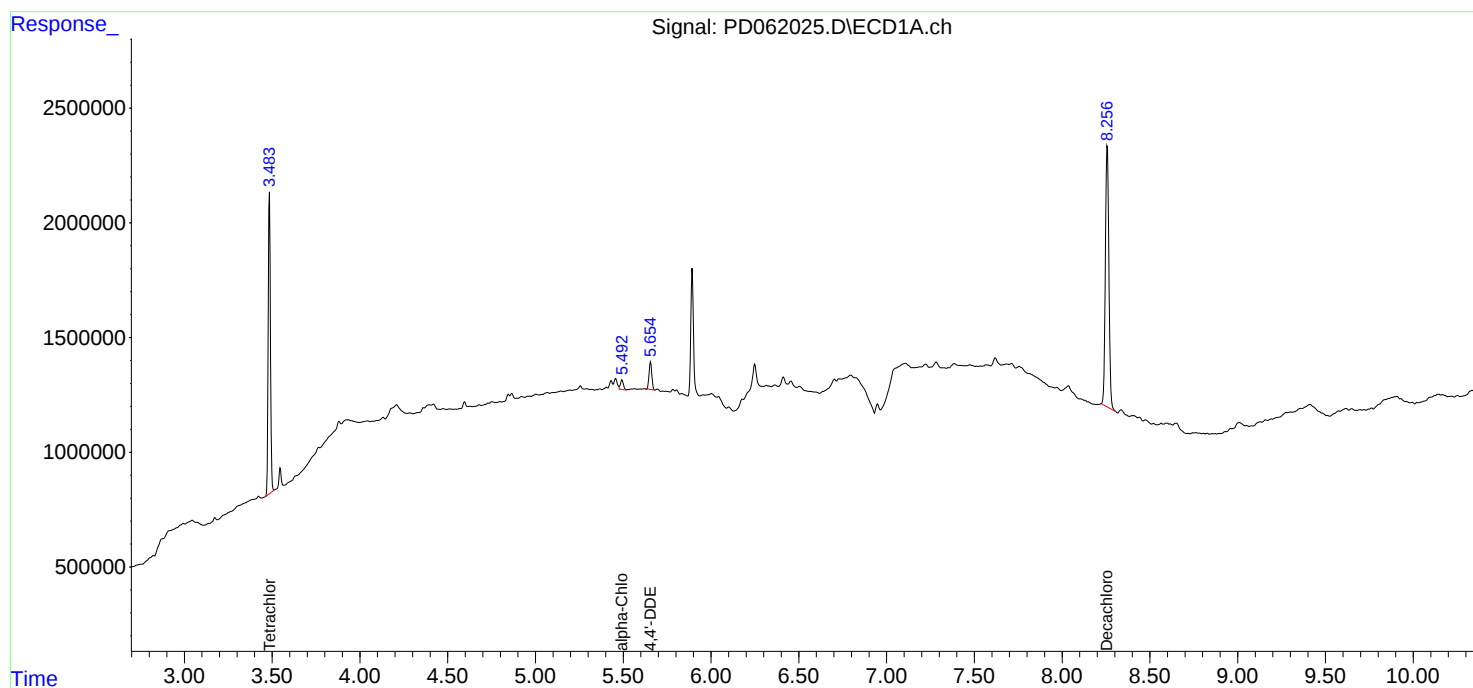

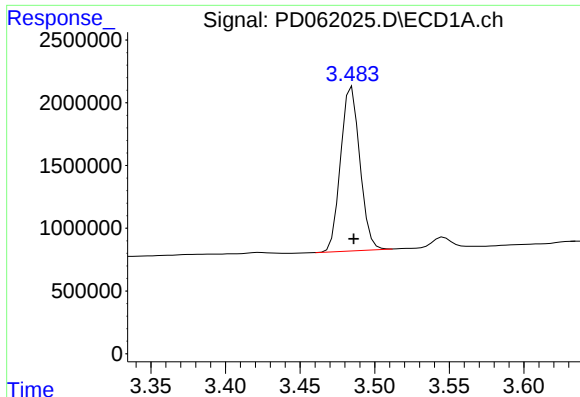


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 11772282
Conc: 14.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
4/8/2021 3:10:29 PM

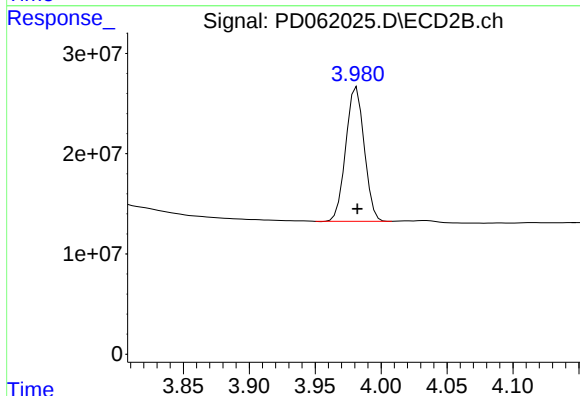


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 130311072
Conc: 15.00 ng/ml

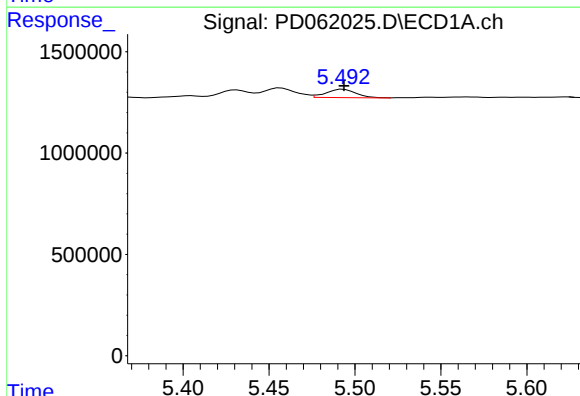


#11 alpha-Chlordane

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 496039
Conc: 0.43 ng/ml m

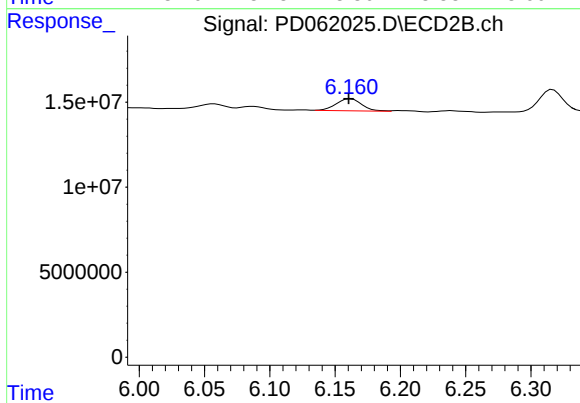

#11 alpha-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.001 min
Response: 9812302
Conc: 0.86 ng/ml

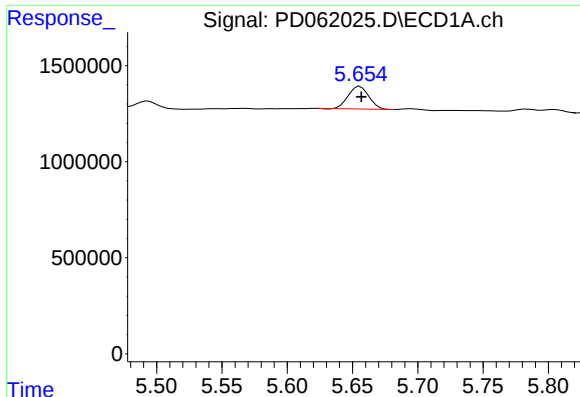


#12 4,4'-DDE

R.T.: 5.656 min
Delta R.T.: 0.000 min
Response: 1299466
Conc: 1.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
4/8/2021 3:10:29 PM

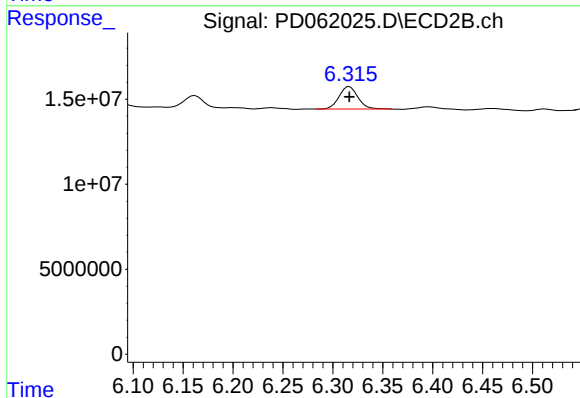


#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 17316571
Conc: 1.50 ng/ml

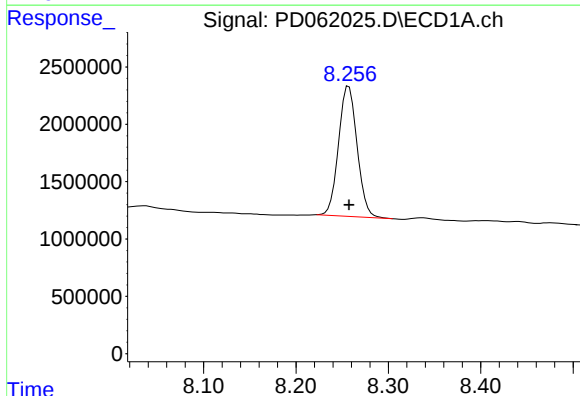

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 15837545
Conc: 12.87 ng/ml

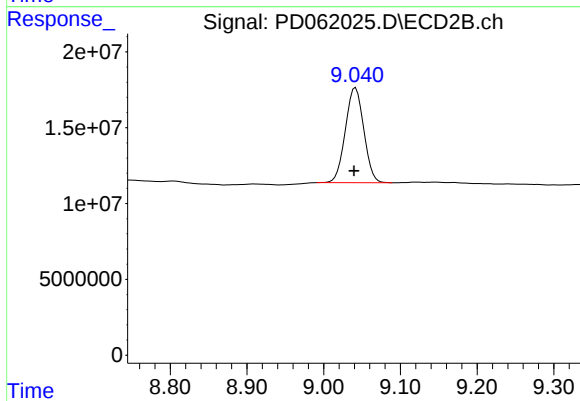

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 105430360
Conc: 11.17 ng/ml