

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040724\
 Data File : PD082318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2024 20:13
 Operator : AR\AJ
 Sample : P2017-09MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5F0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/08/2024
 Supervised By :Ankita Jodhani 04/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:34:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 30 04:18:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.774	25820680	79043317	17.461	23.627m#
27)	SA Decachlor...	9.120	7.909	25646904	29939396	13.803	11.350m
Target Compounds							
2)	A alpha-BHC	4.022	3.277	131.4E6	240.0E6	52.694m	47.406
3)	MA gamma-BHC...	4.357	3.606	102.7E6	237.6E6	42.897	51.430
4)	MA Heptachlor	4.950	3.944	120.5E6	214.0E6	48.611	49.932m
5)	MB Aldrin	5.294	4.224	108.8E6	192.0E6	46.484	45.802m
6)	B beta-BHC	4.551	3.902	42091141	95026783	40.179m	49.079
7)	B delta-BHC	4.801	4.132	59251285	140.0E6	25.438m	31.183
8)	B Heptachlo...	5.721	4.727	111.5E6	189.6E6	50.801	51.121
9)	A Endosulfan I	6.107	5.096	103.9E6	191.2E6	49.702m	56.320
10)	B trans-Chl...	5.976	4.976	103.9E6	213.6E6	49.920m	59.364
11)	B cis-Chlor...	6.057	5.041	94108839	209.0E6	44.408	56.615 #
12)	B 4,4'-DDE	6.227	5.229	201.7E6	367.1E6	99.040m	107.679
13)	MA Dieldrin	6.384	5.359	224.8E6	421.9E6	104.353	114.929m
14)	MA Endrin	6.615	5.634	187.9E6	341.3E6	105.844	110.257m
15)	B Endosulfa...	6.833	5.927	148.0E6	323.1E6	83.666	106.624m#
16)	A 4,4'-DDD	6.746	5.783	148.1E6	280.6E6	98.774	104.170
17)	MA 4,4'-DDT	7.061	6.034	158.4E6	296.3E6	101.850m	107.243
18)	B Endrin al...	6.960	6.109	289.1E6	242.2E6	218.122m	107.345 #
19)	B Endosulfa...	7.199	6.331	149.4E6	267.4E6	91.618	93.812
20)	A Methoxychlor	7.538	6.609	388.9E6	695.9E6	474.495	499.297
21)	B Endrin ke...	7.686	6.836	167.6E6	335.7E6	98.020	104.944

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040724\
Data File : PD082318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2024 20:13
Operator : AR\AJ
Sample : P2017-09MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:34:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 30 04:18:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

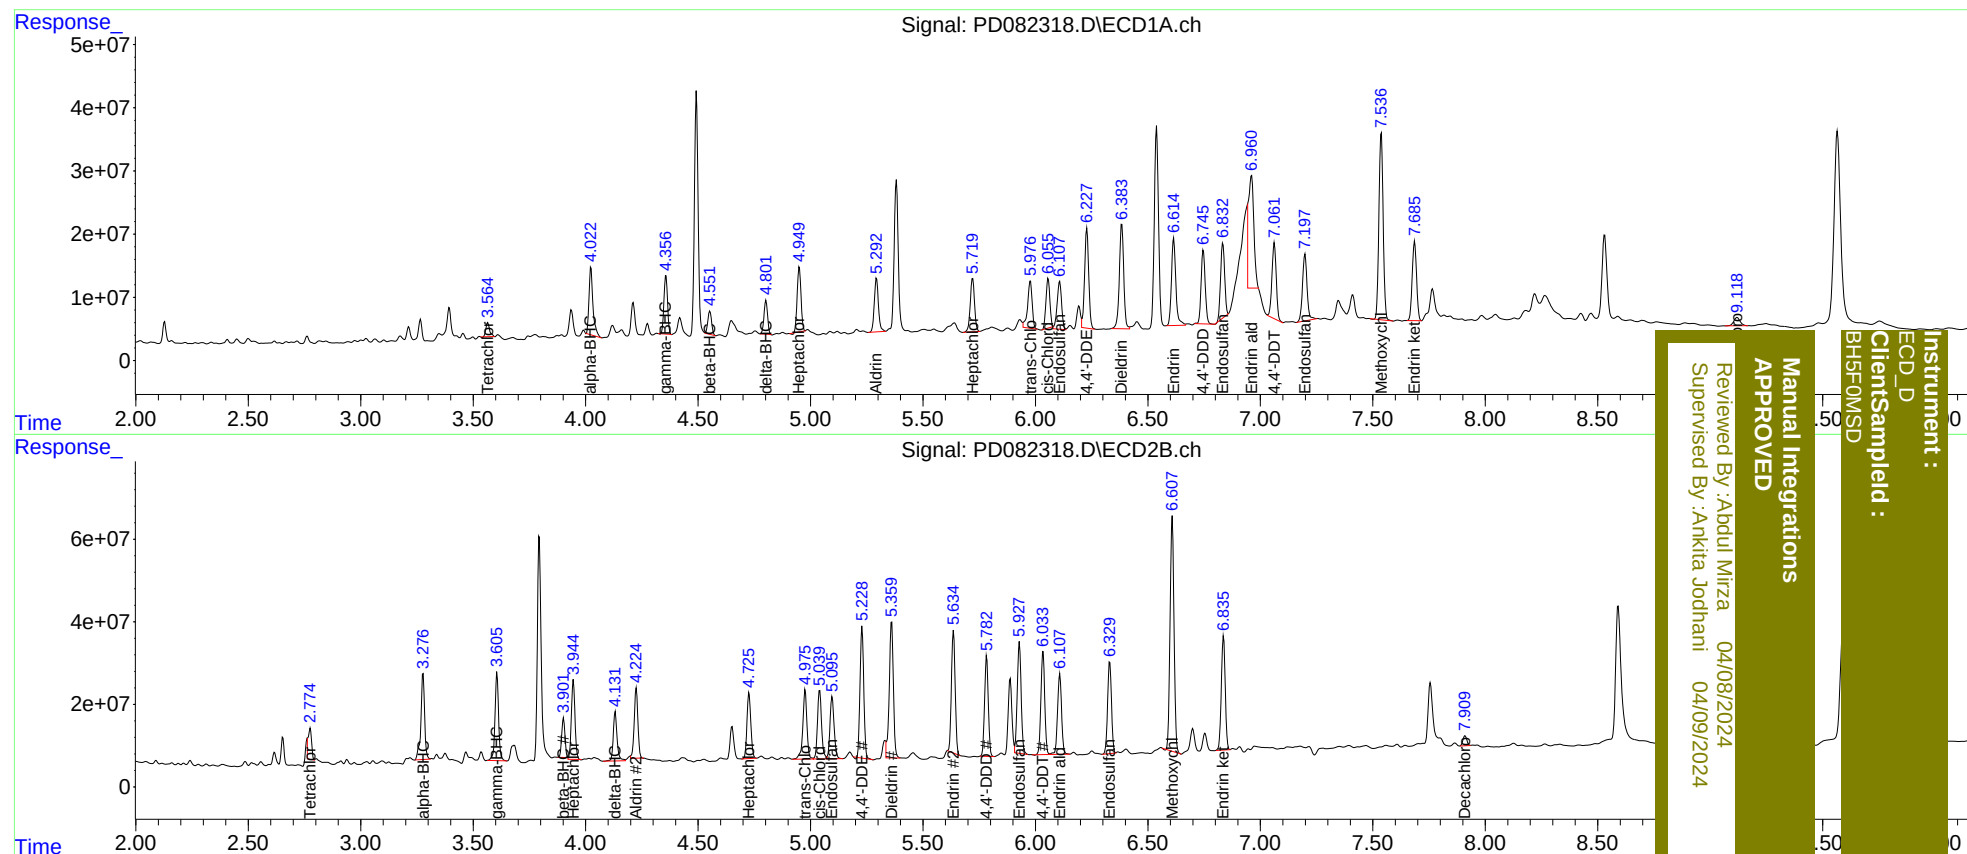

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/08/2024
Supervised By: Ankita Jodhani 04/09/2024

Instrument :
ECD_D
Client Sampled :
BHSFOMSD