Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040724\
Data File : PD082304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2024 16:54
Operator : AR\AJ
Sample : P2018-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BH5F1

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 04/08/2024
Supervised By :Ankita Jodhani 04/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:29:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 30 04:18:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.558	2.775	42718077	71505257	28.887m	21.374m#
27)	SA Decachlor...	9.121	7.908	9812516	8651023	5.281	3.280m#
	Target Compounds						
9)	A Endosulfan I	6.094	5.110	34672406	56496978	16.591m	16.640
12)	B 4,4'-DDE	6.255	5.233	9061763	15084257	4.449m	4.425m
13)	MA Dieldrin	6.390	5.370	6606903	8344909	3.067m	2.273m#
14)	MA Endrin	6.634	5.633	7463661	10455471	4.204m	3.378m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040724\
Data File : PD082304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2024 16:54
Operator : AR\AJ
Sample : P2018-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:29:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 30 04:18:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

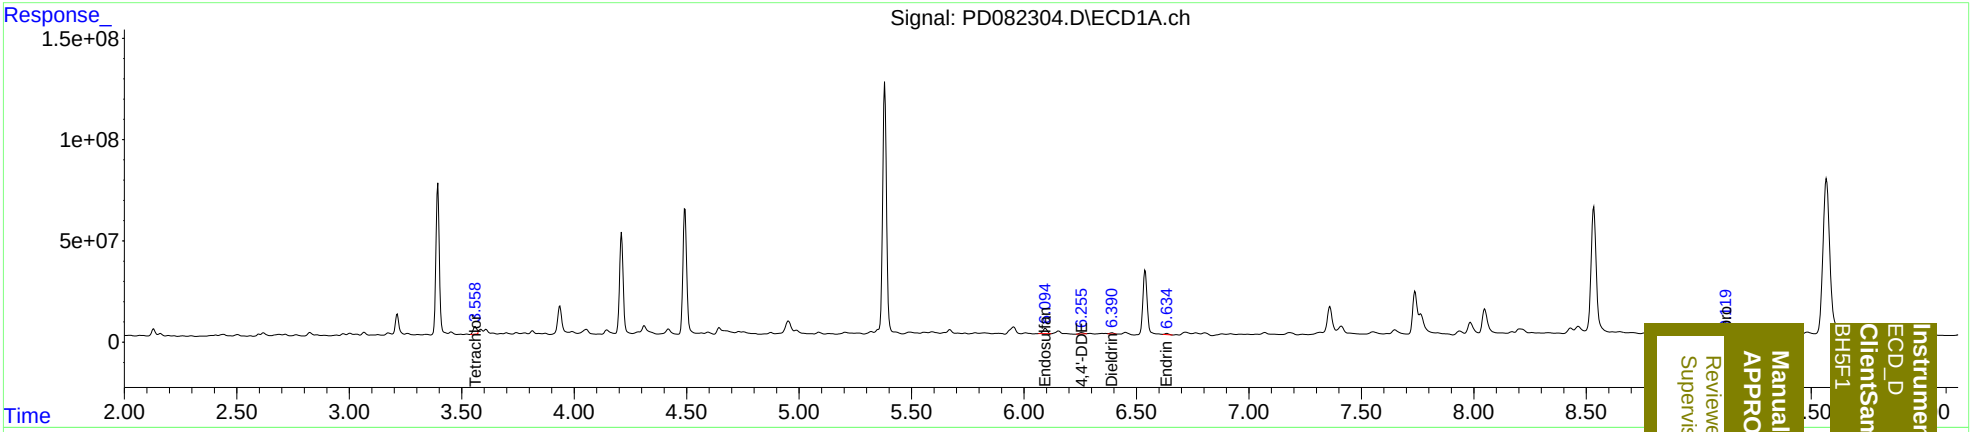

Manual Integrations APPROVED
Reviewed By :Abdul Mirza 04/08/2024
Supervised By :Ankita Jodhani 04/09/2024

Instrument : ECD_D
ClientSampleId : BH5F1