

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040819\
 Data File : PD052767.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 14:46
 Operator : AJ\SJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:56:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 06:55:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.044	124.0E6	2224.5E6	80.566	68.241
27)	SA Decachlor...	7.818	9.163	213.9E6	2093.2E6	151.109	141.189
Target Compounds							
2)	A alpha-BHC	3.640	4.436	211.1E6	3445.7E6	86.753	70.306
3)	MA gamma-BHC...	3.909	4.723	197.3E6	3103.7E6	81.961	70.124
4)	MA Heptachlor	4.185	5.236	205.5E6	3044.7E6	83.871	68.030
9)	A Endosulfan I	5.166	6.291	168.2E6	2286.9E6	81.566	68.039
13)	MA Dieldrin	5.401	6.550	401.1E6	4666.1E6	170.223	139.517
14)	MA Endrin	5.649	6.769	338.2E6	3630.4E6	167.738	139.660
16)	A 4,4'-DDD	5.789	6.889	306.9E6	3650.6E6	168.125	141.704
17)	MA 4,4'-DDT	6.020	7.190	312.3E6	3344.1E6	185.014	161.174
20)	A Methoxychlor	6.565	7.650	818.9E6	6996.2E6	811.545	707.991


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040819\
Data File : PD052767.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 14:46
Operator : AJ\SJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:56:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 06:55:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

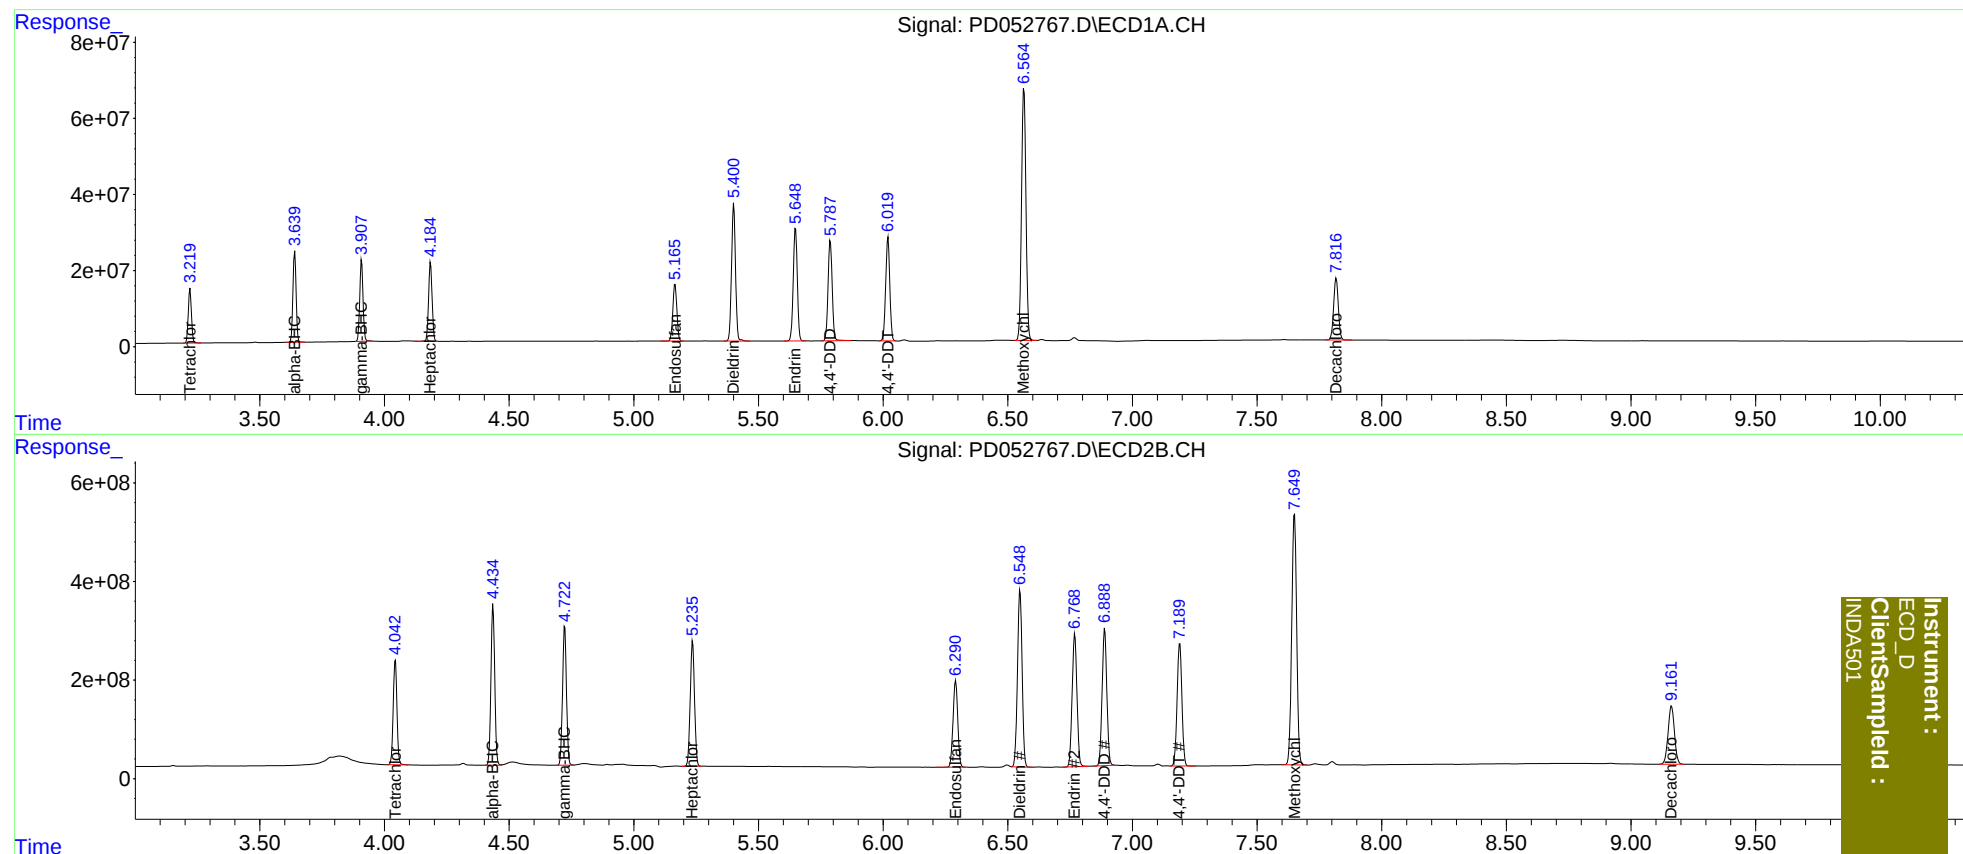


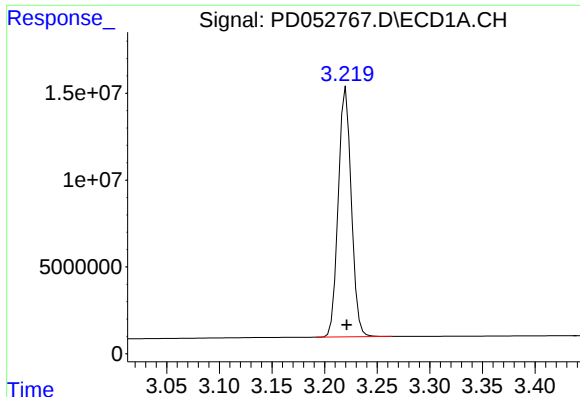

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 124014140
Conc: 80.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

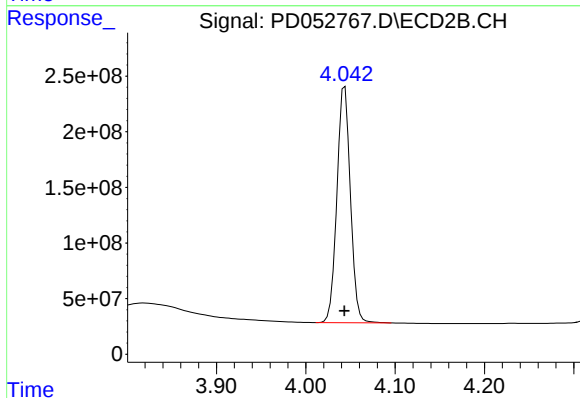


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 2224495656
Conc: 68.24 ng/ml

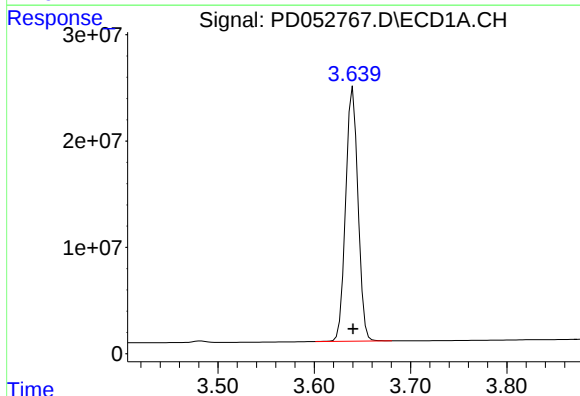


#2 alpha-BHC

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 211075402
Conc: 86.75 ng/ml

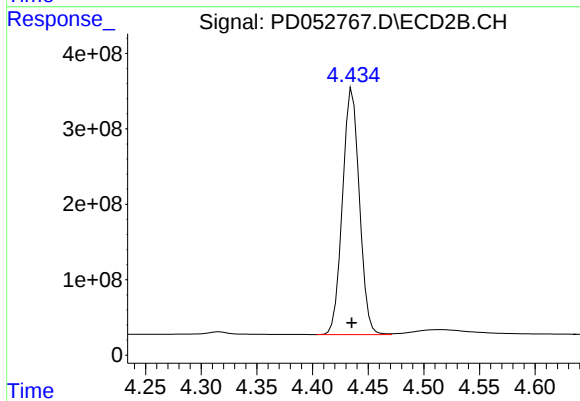

#2 alpha-BHC


R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 3445740722
Conc: 70.31 ng/ml

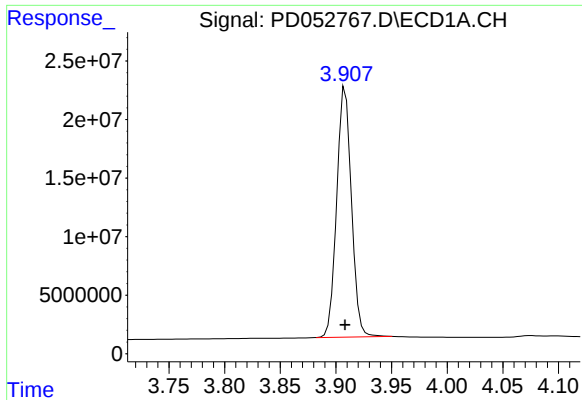

#3 gamma-BHC (Lindane)


R.T.: 3.909 min
Delta R.T.: 0.000 min
Response: 197250563
Conc: 81.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

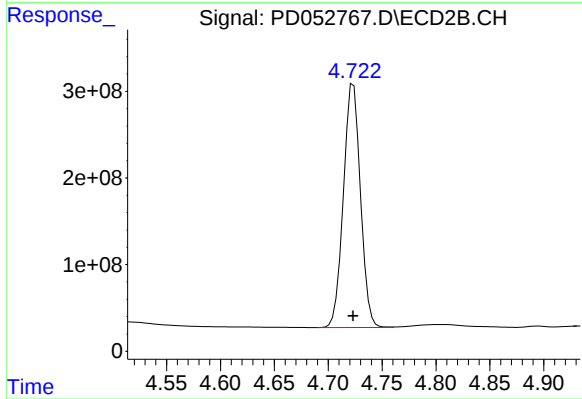


#3 gamma-BHC (Lindane)

R.T.: 4.723 min
Delta R.T.: 0.000 min
Response: 3103680551
Conc: 70.12 ng/ml

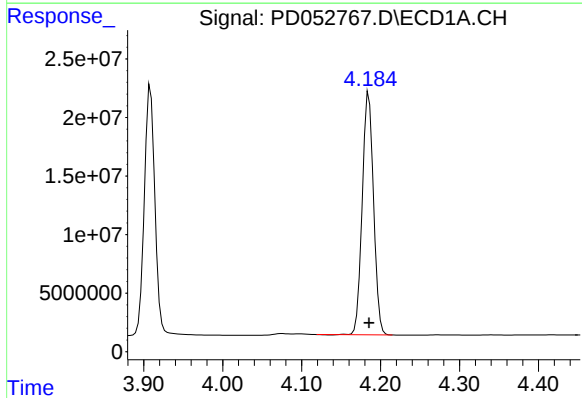


#4 Heptachlor

R.T.: 4.185 min
Delta R.T.: 0.000 min
Response: 205464076
Conc: 83.87 ng/ml

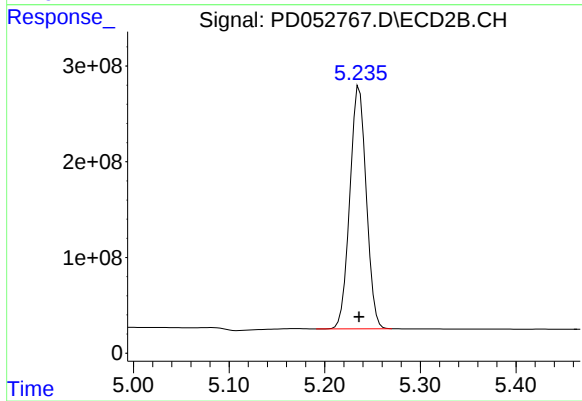

#4 Heptachlor


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 3044664511
Conc: 68.03 ng/ml

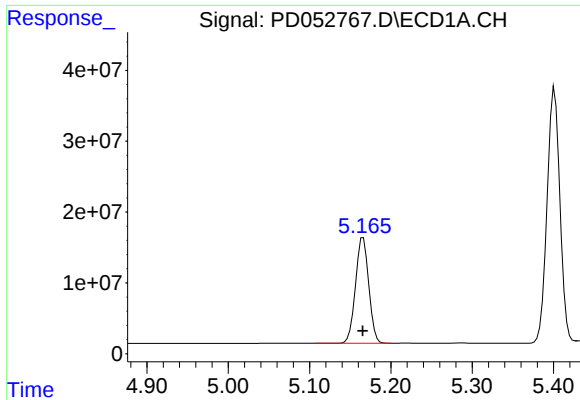

#9 Endosulfan I


R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 168160768
Conc: 81.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

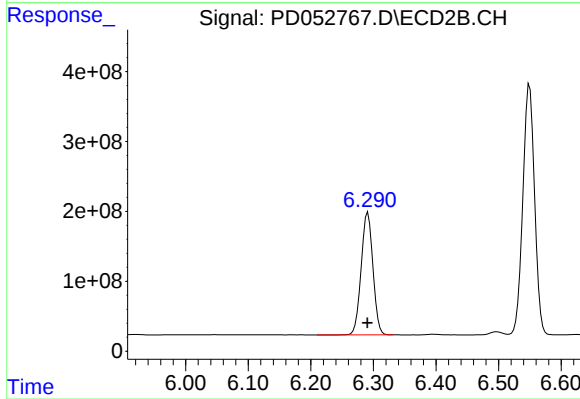


#9 Endosulfan I

R.T.: 6.291 min
Delta R.T.: 0.000 min
Response: 2286912669
Conc: 68.04 ng/ml

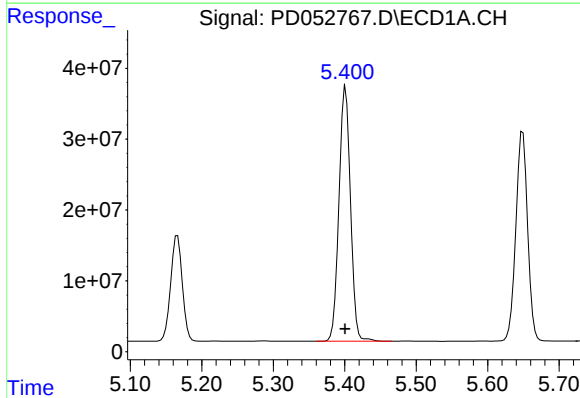


#13 Dieldrin

R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 401100199
Conc: 170.22 ng/ml

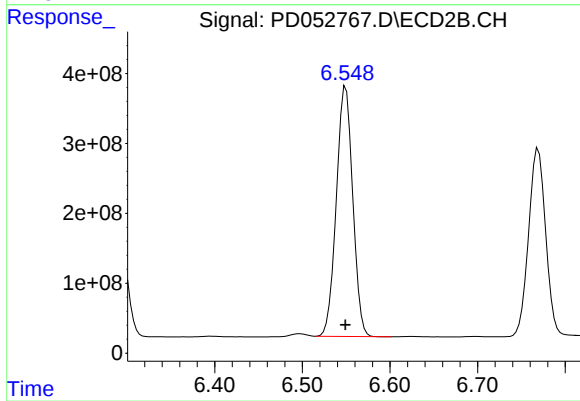

#13 Dieldrin


R.T.: 6.550 min
Delta R.T.: 0.000 min
Response: 4666069498
Conc: 139.52 ng/ml

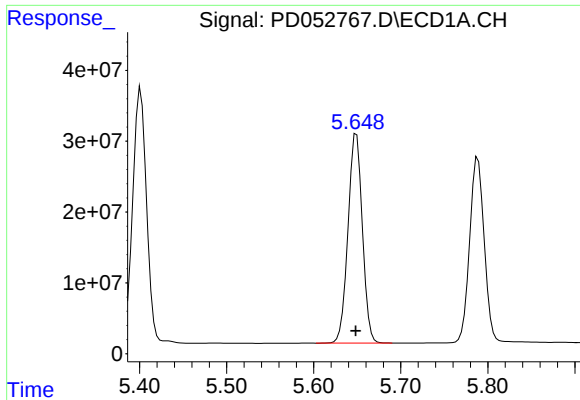

#14 Endrin


R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 338196811
Conc: 167.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

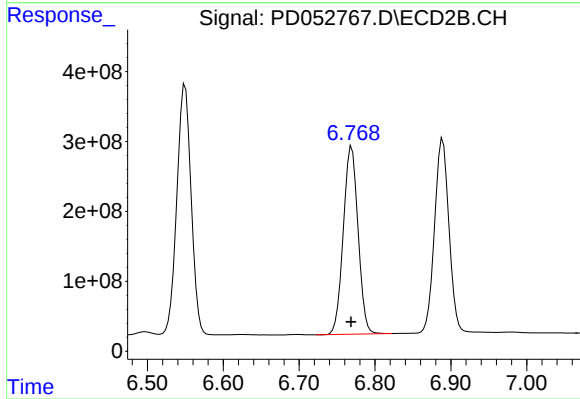


#14 Endrin

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 3630415110
Conc: 139.66 ng/ml

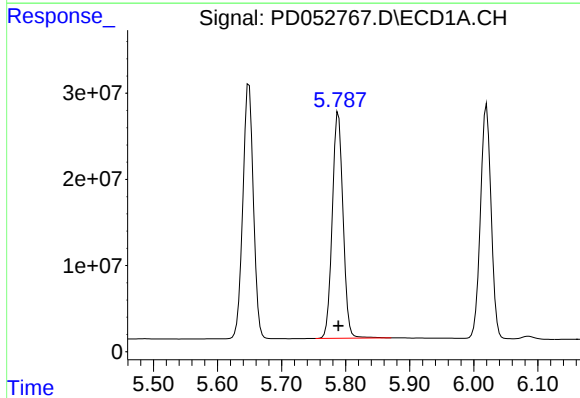


#16 4,4'-DDD

R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 306903054
Conc: 168.13 ng/ml

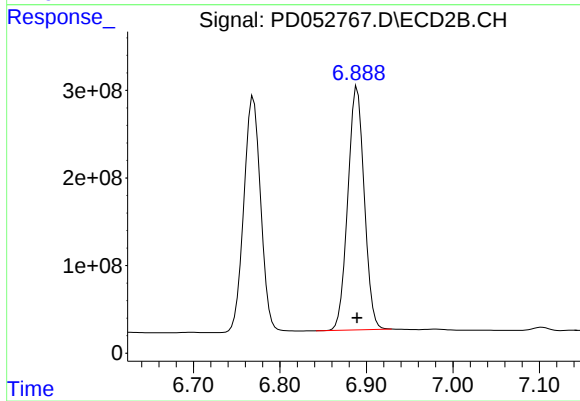

#16 4,4'-DDD


R.T.: 6.889 min
Delta R.T.: 0.000 min
Response: 3650595640
Conc: 141.70 ng/ml

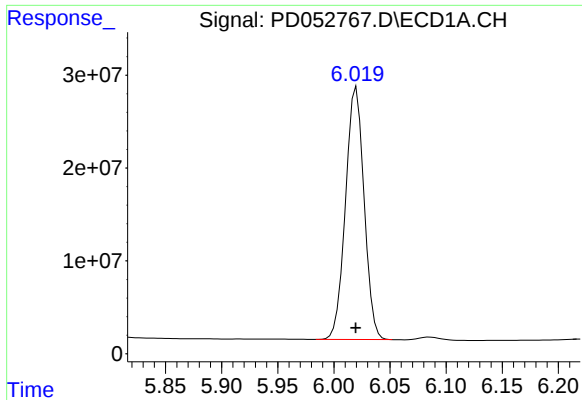

#17 4,4'-DDT


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 312336952
Conc: 185.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

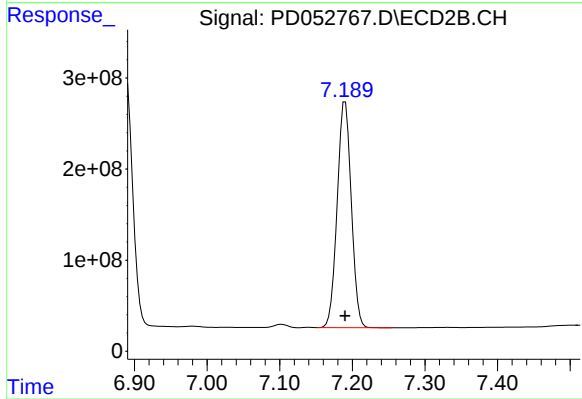


#17 4,4'-DDT

R.T.: 7.190 min
Delta R.T.: 0.000 min
Response: 3344143766
Conc: 161.17 ng/ml

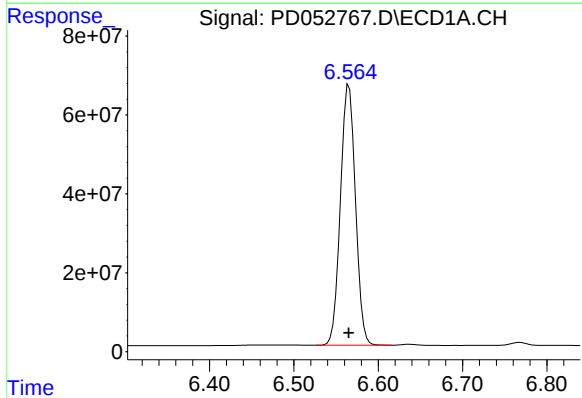


#20 Methoxychlor

R.T.: 6.565 min
Delta R.T.: 0.000 min
Response: 818884816
Conc: 811.54 ng/ml

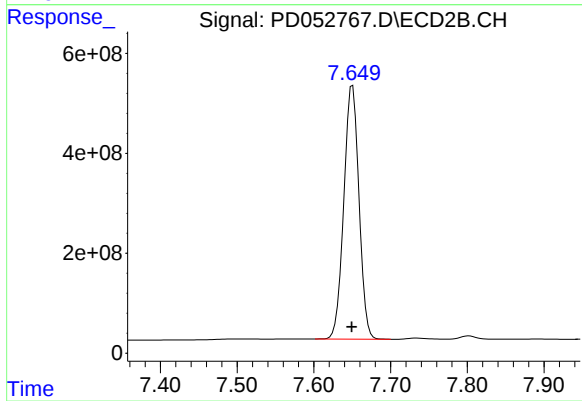

#20 Methoxychlor


R.T.: 7.650 min
Delta R.T.: 0.001 min
Response: 6996195375
Conc: 707.99 ng/ml

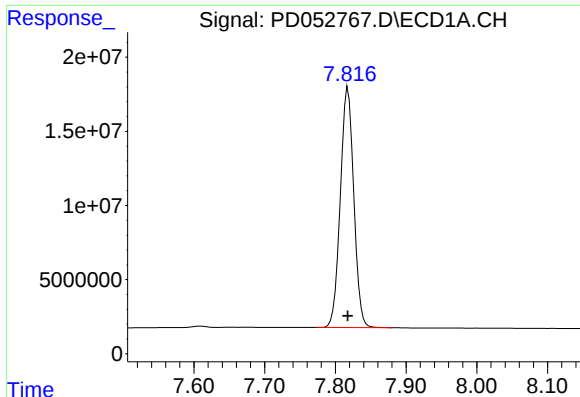

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 213940089
Conc: 151.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

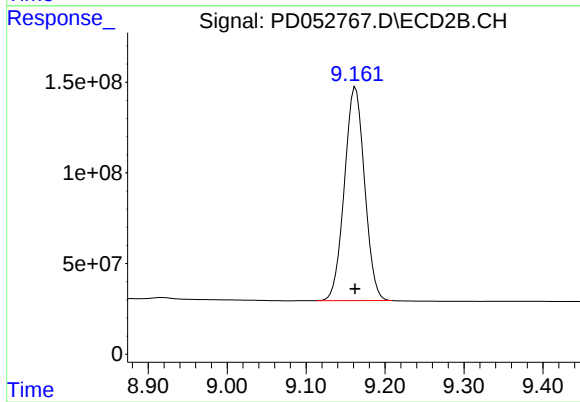

#27 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.000 min
Response: 2093195211
Conc: 141.19 ng/ml