

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040821\
 Data File : PD062050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2021 09:50
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 02:30:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
3) MA gamma-BHC...	0.000	4.652	0	753953	N.D.	0.060 #
4) MA Heptachlor	0.000	5.158	0	2194878	N.D.	0.168 #
7) B delta-BHC	0.000	5.027	0	72101498	N.D.	5.451 #
8) B Heptachlo...	0.000	5.857	0	51962769	N.D.	4.388 #
9) A Endosulfan I	0.000	6.219	0	1036001	N.D.	0.096 #
11) B alpha-Chl...	0.000	6.172	0	1781307	N.D.	0.156 #
15) B Endosulfa...	0.000	6.901	0	2086704	N.D.	0.220 #
17) MA 4,4'-DDT	0.000	7.119	0	1349312	N.D.	0.141 #
19) B Endosulfa...	0.000	7.236	0	2044653	N.D.	0.204 #
21) B Endrin ke...	0.000	7.730f	0	1543450	N.D.	0.152 #
26) Chlordane-4	0.000	6.172	0	1781307	N.D.	0.928 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040821\
Data File : PD062050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2021 09:50
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 02:30:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

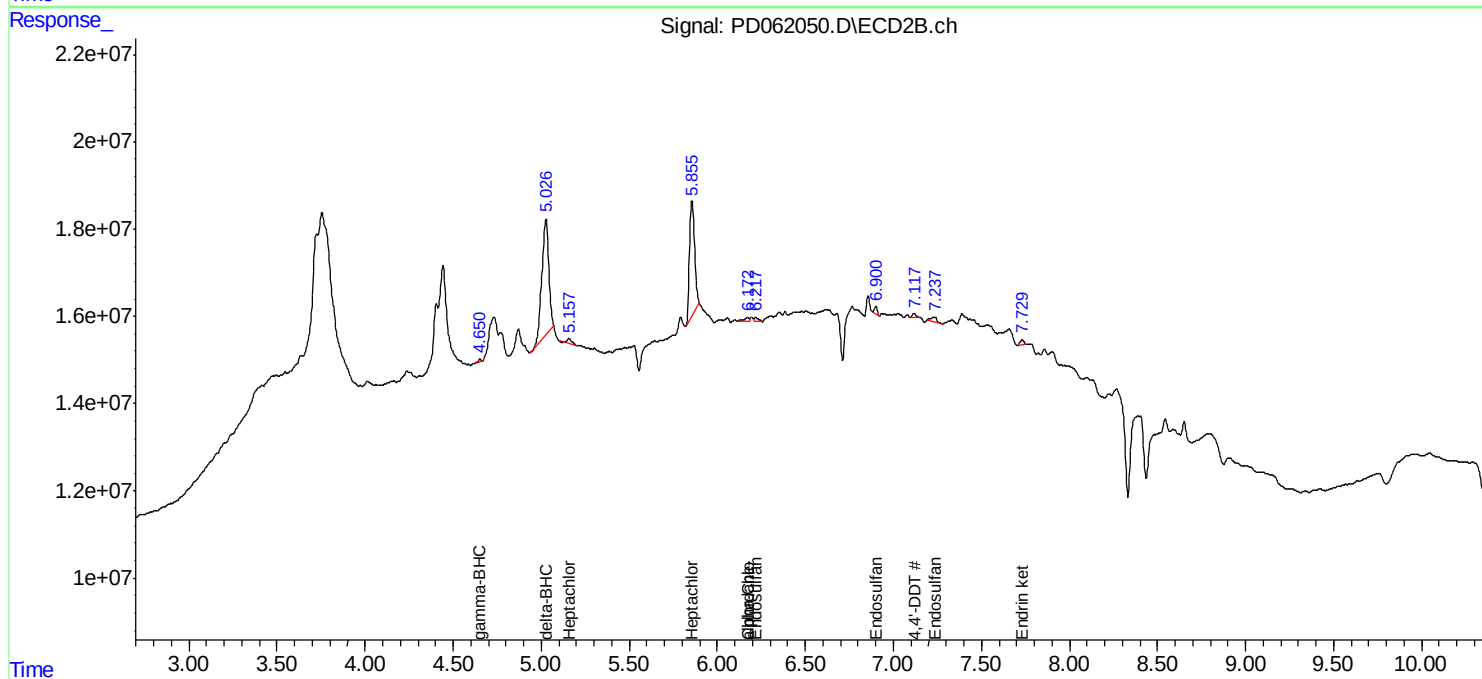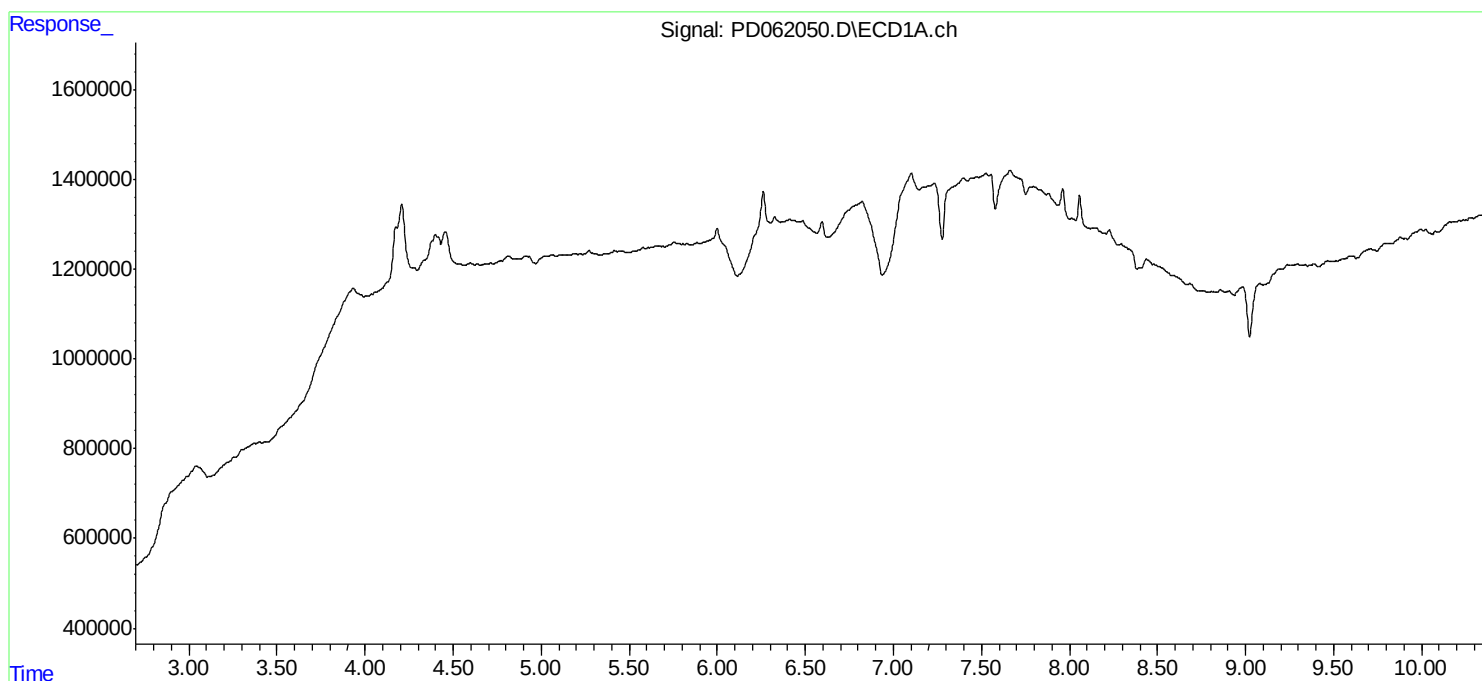


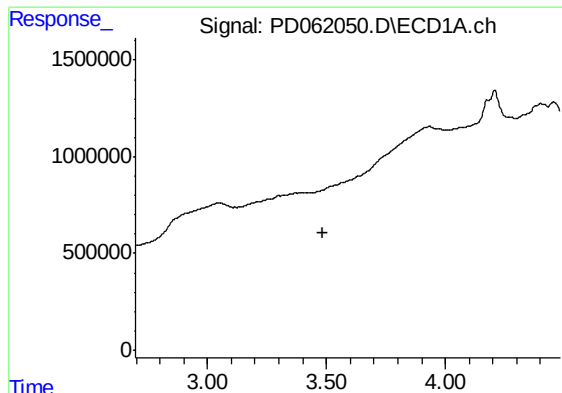

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

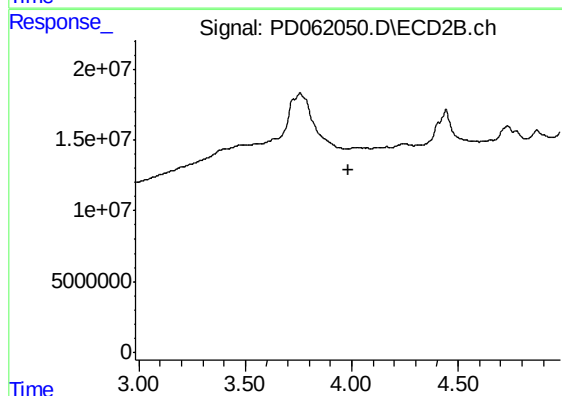


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.982 min
Response: 0
Conc: N.D.

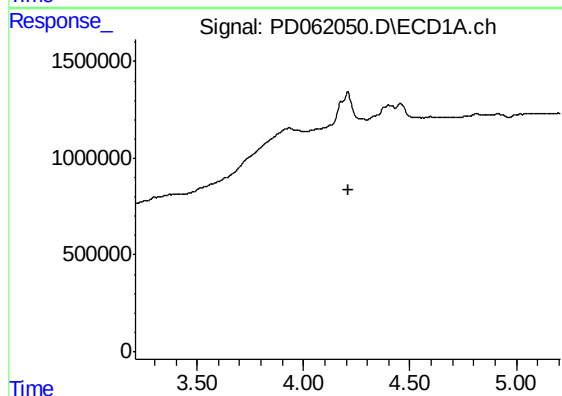


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.210 min
Response: 0
Conc: N.D.

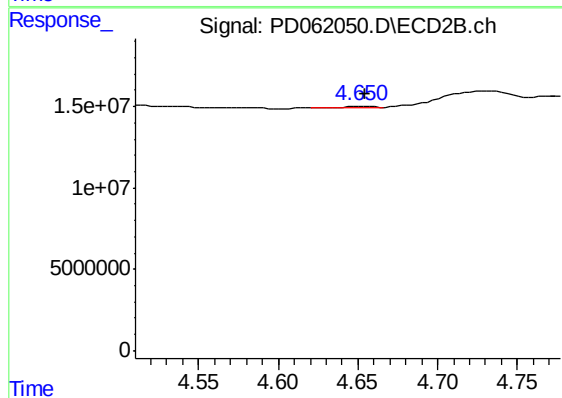

#3 gamma-BHC (Lindane)


R.T.: 4.652 min
Delta R.T.: -0.003 min
Response: 753953
Conc: 0.06 ng/ml

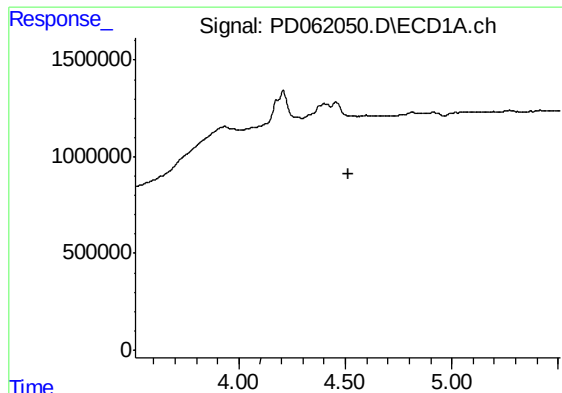

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.513 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

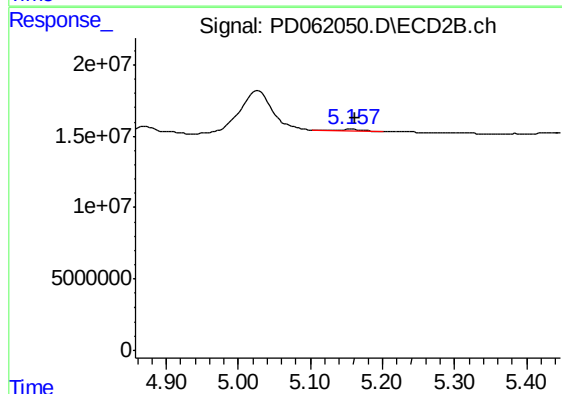


#4 Heptachlor

R.T.: 5.158 min
Delta R.T.: -0.004 min
Response: 2194878
Conc: 0.17 ng/ml

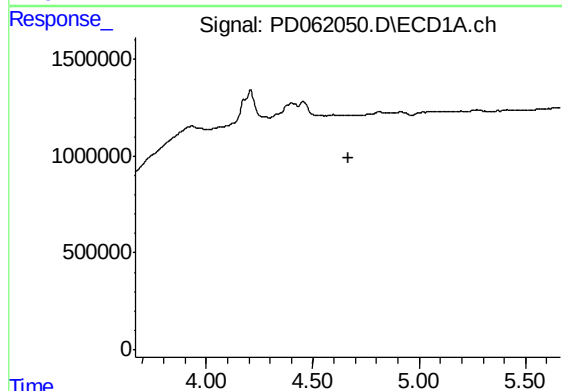


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

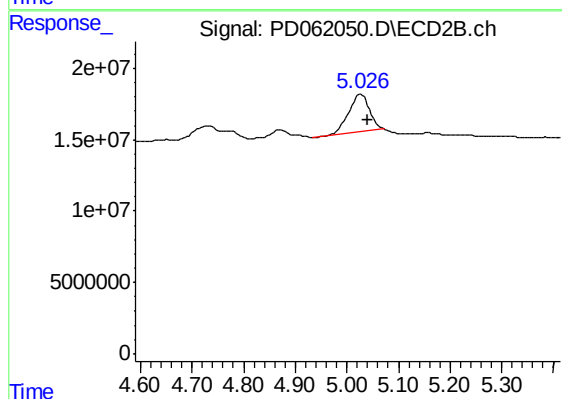

#7 delta-BHC


R.T.: 5.027 min
Delta R.T.: -0.014 min
Response: 72101498
Conc: 5.45 ng/ml

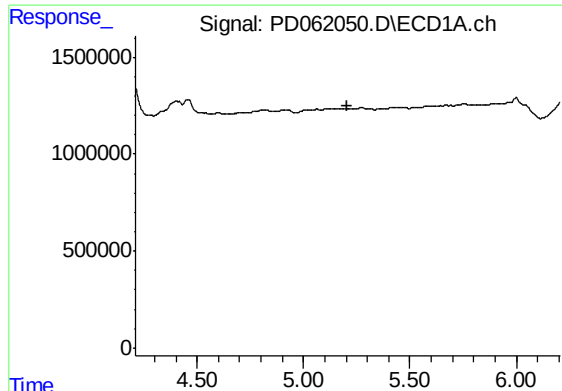

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

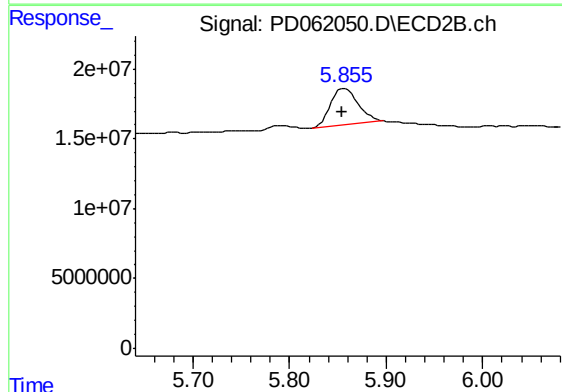


#8 Heptachlor epoxide

R.T.: 5.857 min
Delta R.T.: 0.003 min
Response: 51962769
Conc: 4.39 ng/ml

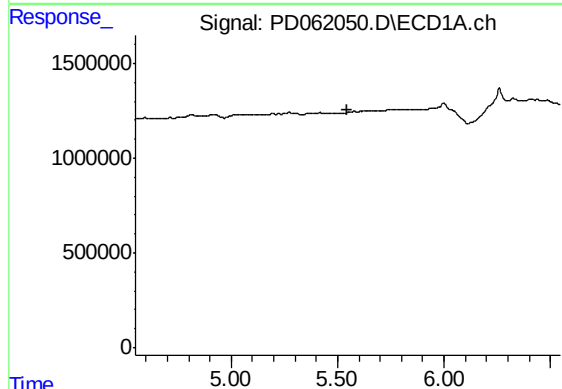


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

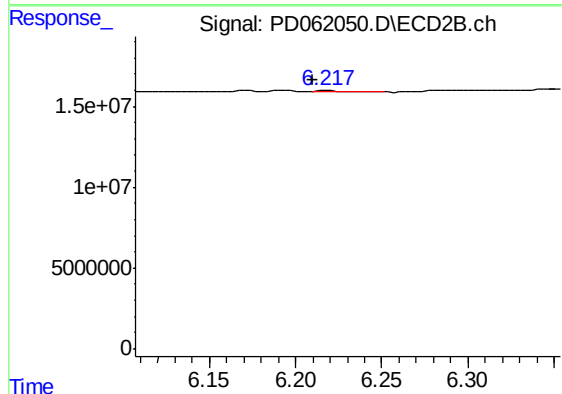

#9 Endosulfan I


R.T.: 6.219 min
Delta R.T.: 0.009 min
Response: 1036001
Conc: 0.10 ng/ml

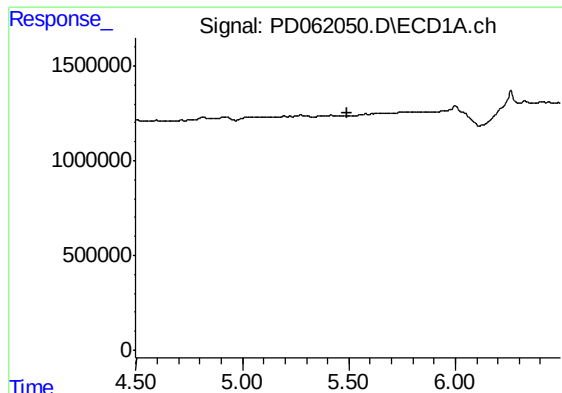

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

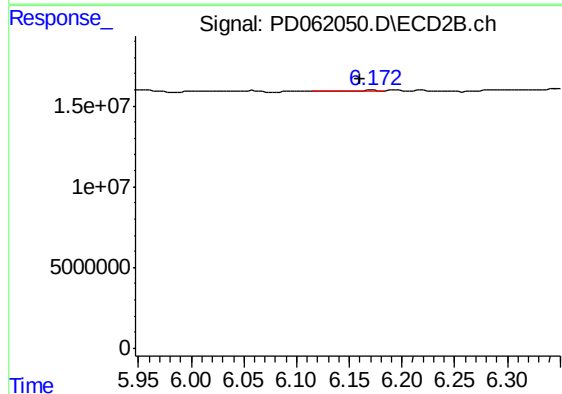


#11 alpha-Chlordane

R.T.: 6.172 min
Delta R.T.: 0.012 min
Response: 1781307
Conc: 0.16 ng/ml

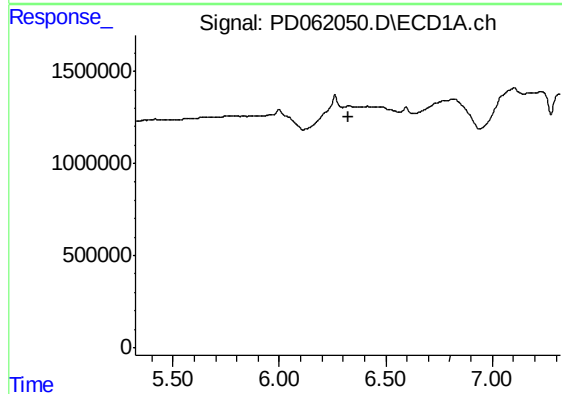


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

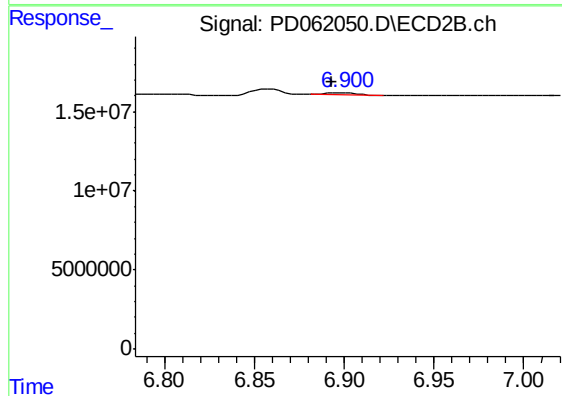

#15 Endosulfan II


R.T.: 6.901 min
Delta R.T.: 0.008 min
Response: 2086704
Conc: 0.22 ng/ml

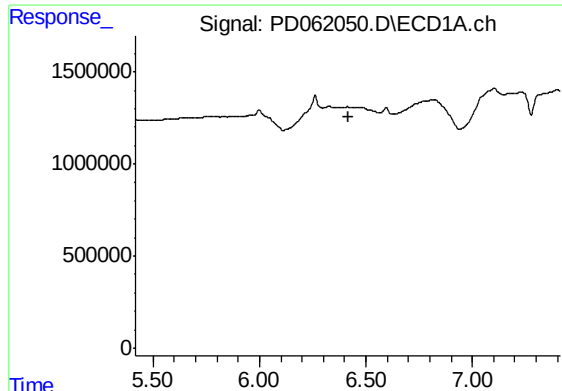

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

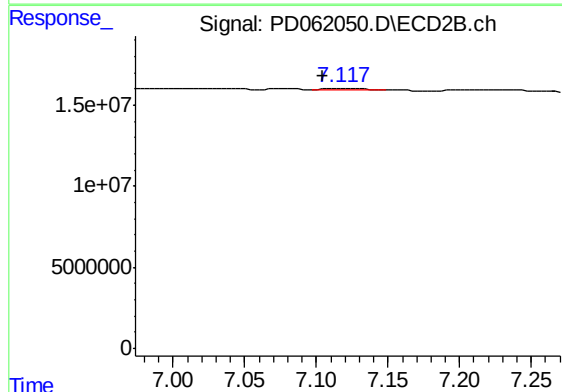


#17 4,4'-DDT

R.T.: 7.119 min
Delta R.T.: 0.014 min
Response: 1349312
Conc: 0.14 ng/ml

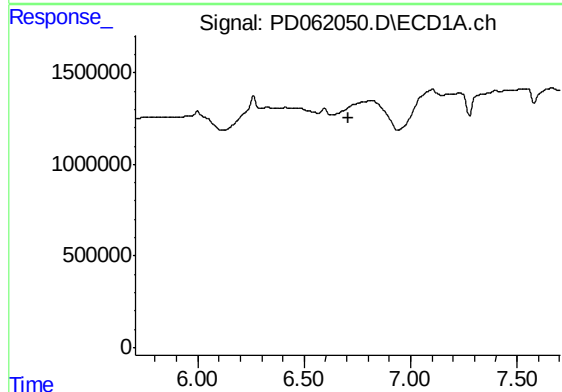


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.706 min
Response: 0
Conc: N.D.

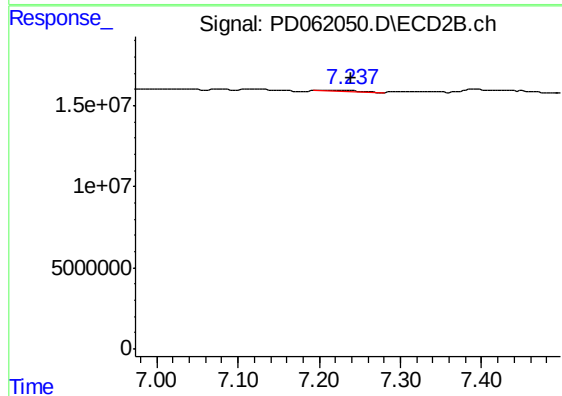

#19 Endosulfan Sulfate


R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 2044653
Conc: 0.20 ng/ml

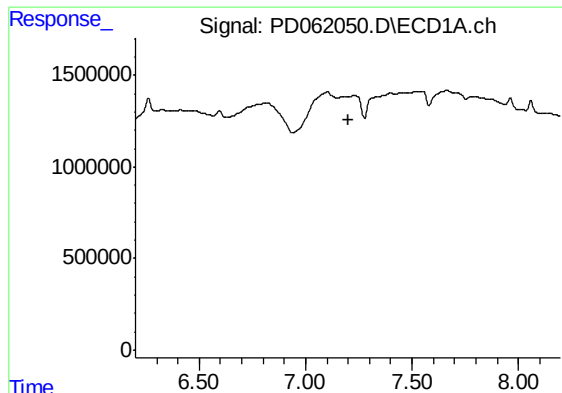

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

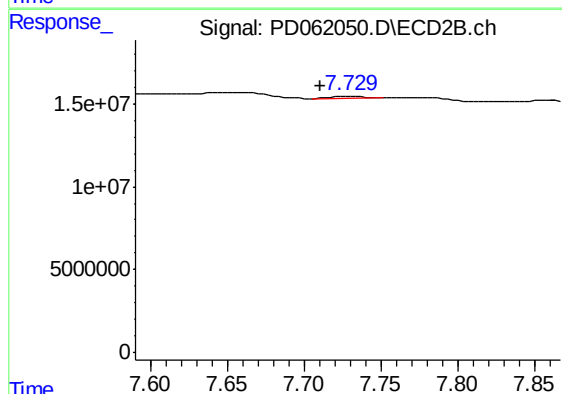


#21 Endrin ketone

R.T.: 7.730 min
Delta R.T.: 0.019 min
Response: 1543450
Conc: 0.15 ng/ml

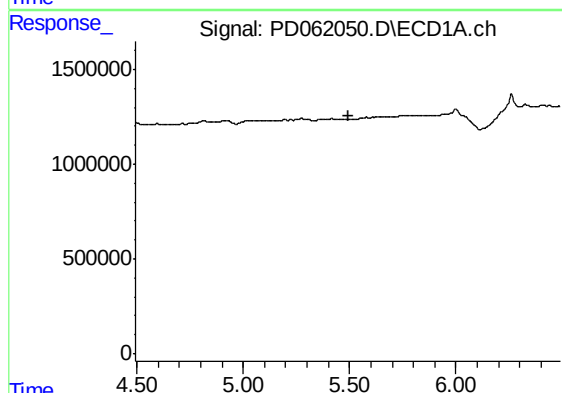


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.493 min
Response: 0
Conc: N.D.

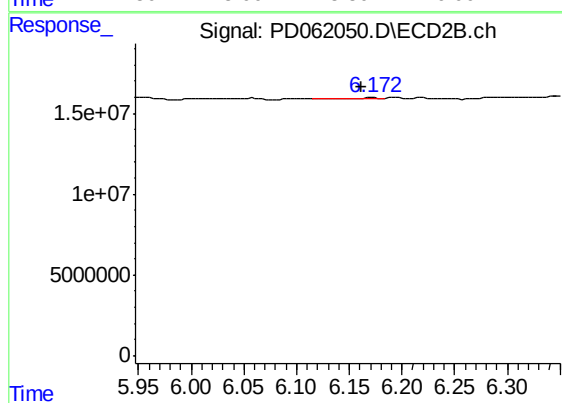

#26 Chlordane-4


R.T.: 6.172 min
Delta R.T.: 0.011 min
Response: 1781307
Conc: 0.93 ng/ml

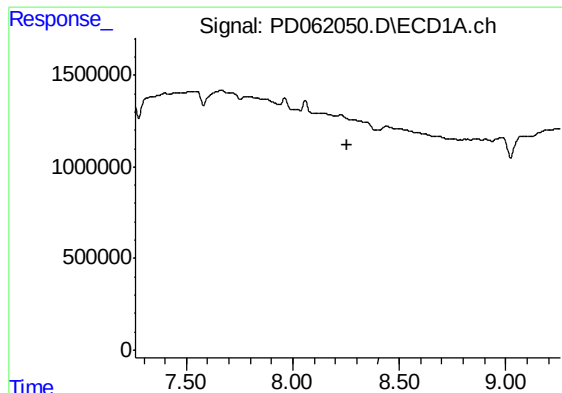

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

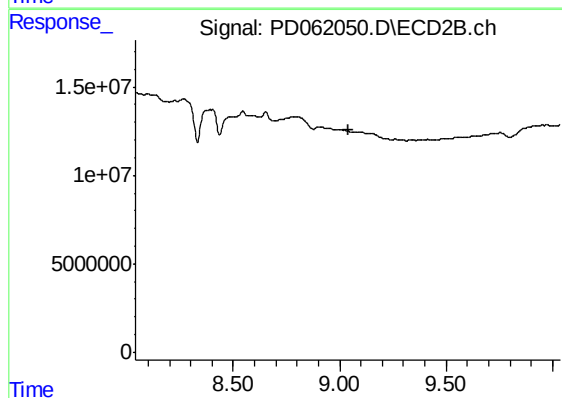

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.040 min
Response: 0
Conc: N.D.