

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040821\
 Data File : PD062074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2021 16:02
 Operator : AR\AJ
 Sample : M1975-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RBR-200032

Manual Integrations
 APPROVED

Ankita
 4/9/2021 8:42:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 02:40:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	12445149	135.0E6	14.864	15.538
28)	SA Decachlor...	8.256	9.038	20007279	131.3E6	16.260	13.905
Target Compounds							
12)	B 4,4'-DDE	5.654	6.315	2747401	29336381	2.445	2.546
17)	MA 4,4'-DDT	6.412	7.102	1059623	9273111	1.176m	0.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040821\
Data File : PD062074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2021 16:02
Operator : AR\AJ
Sample : M1975-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
RBR-200032


Manual Integrations
APPROVED

Ankita
4/9/2021 8:42:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 02:40:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

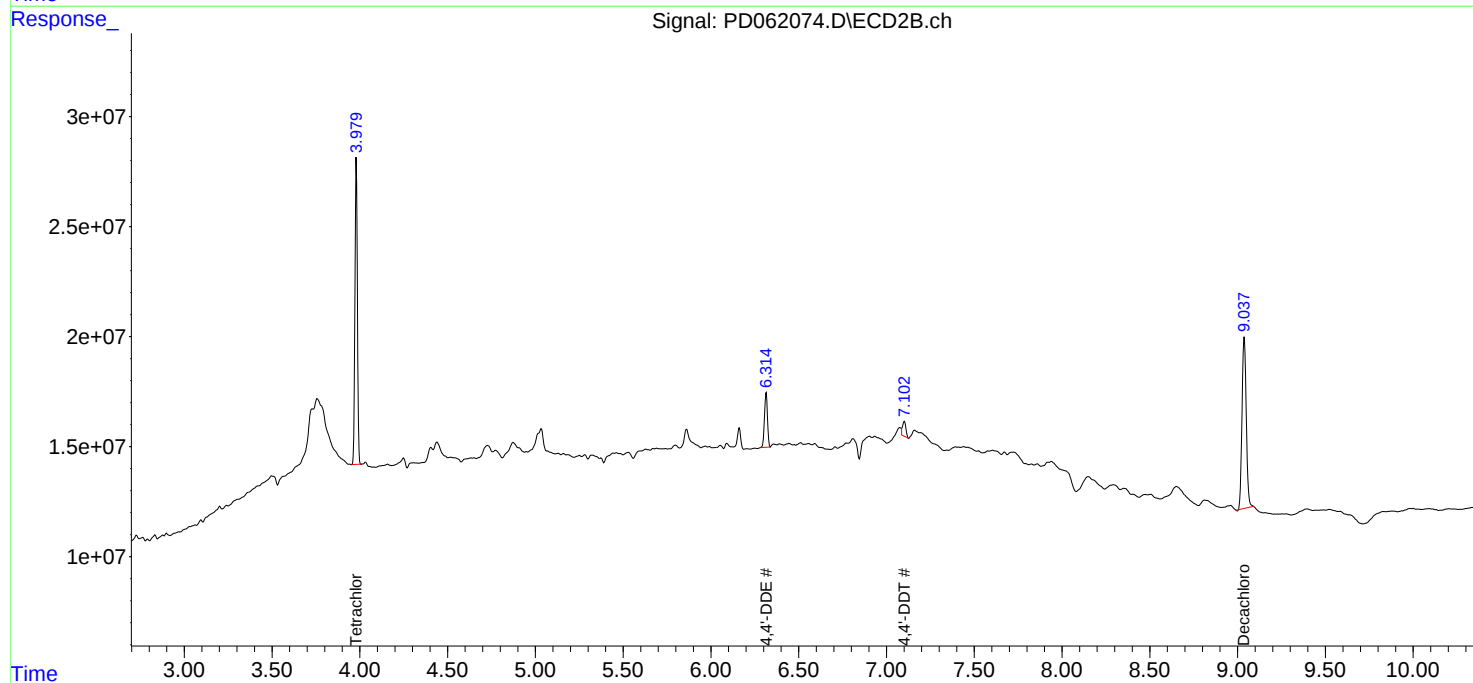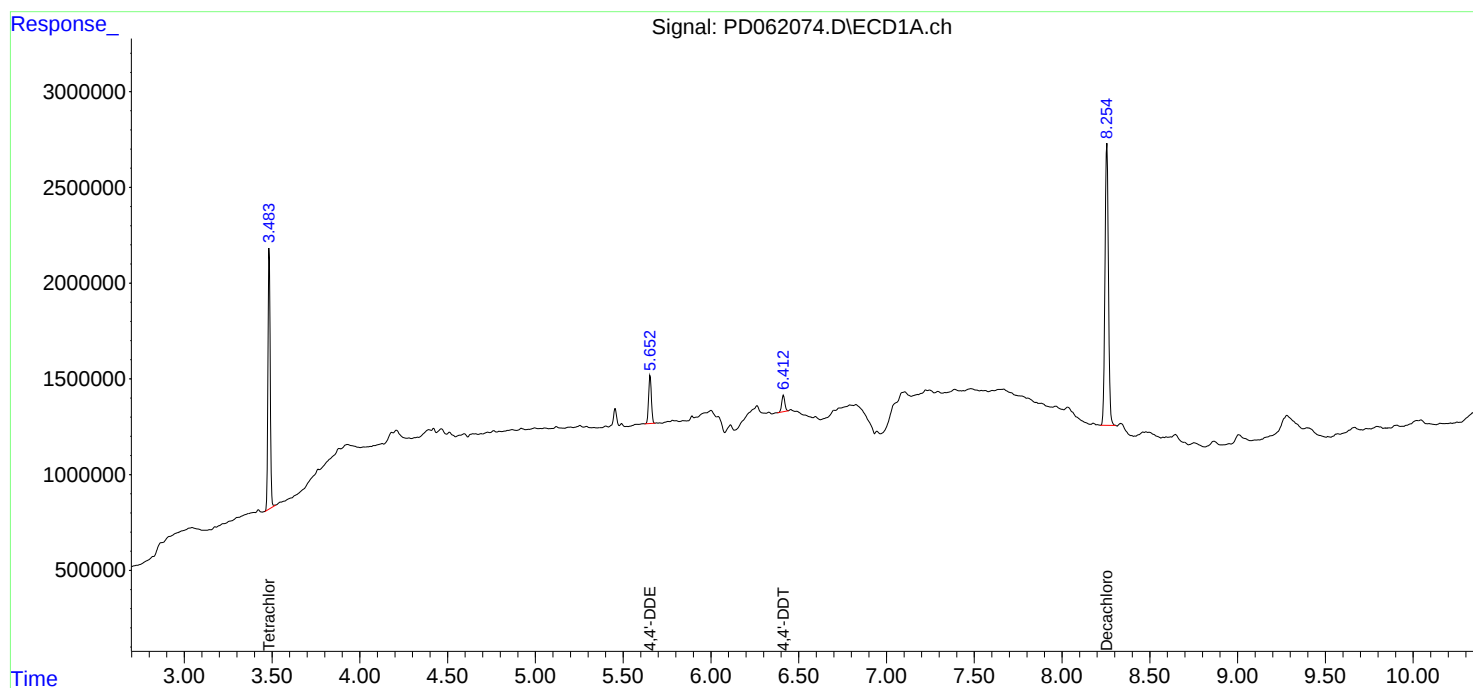

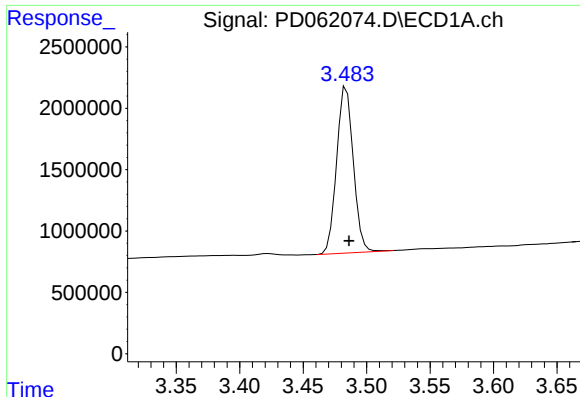


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 12445149
Conc: 14.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
RBR-200032


Manual Integrations
APPROVED

Ankita
4/9/2021 8:42:21 AM

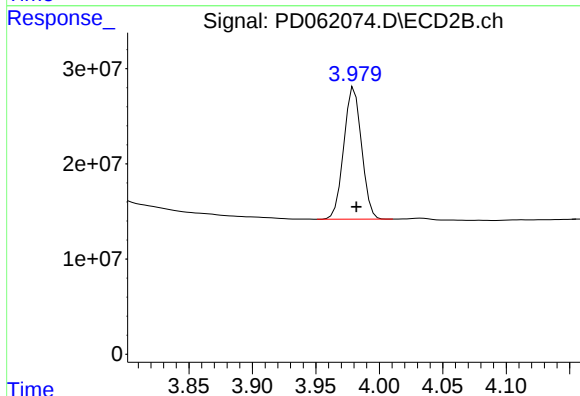


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 135007485
Conc: 15.54 ng/ml

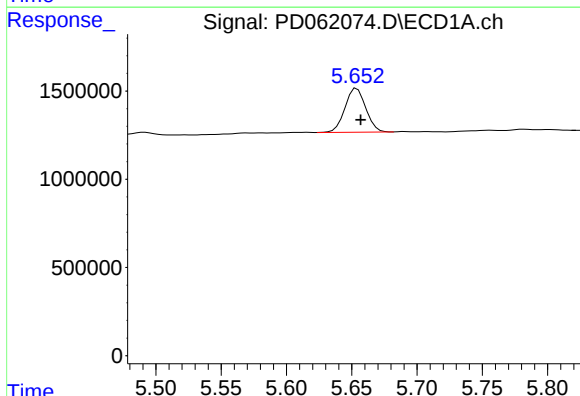


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 2747401
Conc: 2.45 ng/ml

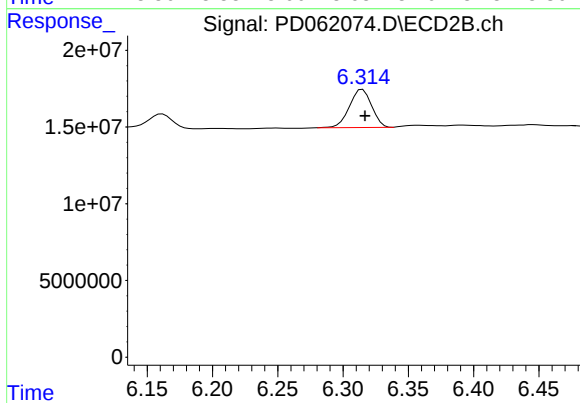

#12 4,4'-DDE

R.T.: 6.315 min
Delta R.T.: -0.002 min
Response: 29336381
Conc: 2.55 ng/ml

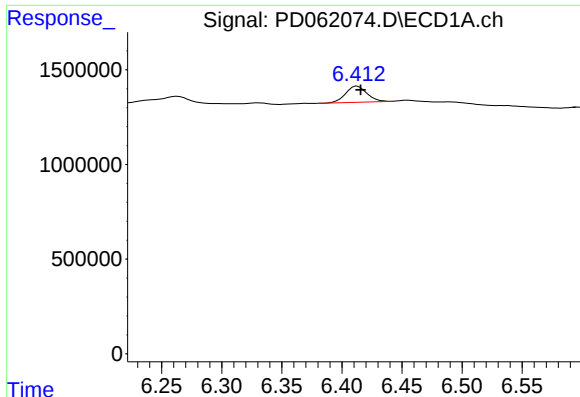


#17 4,4'-DDT

R.T.: 6.412 min
Delta R.T.: -0.004 min
Response: 1059623
Conc: 1.18 ng/ml m

Instrument :
ECD_D
ClientSampleId :
RBR-200032


Manual Integrations
APPROVED

Ankita
4/9/2021 8:42:21 AM

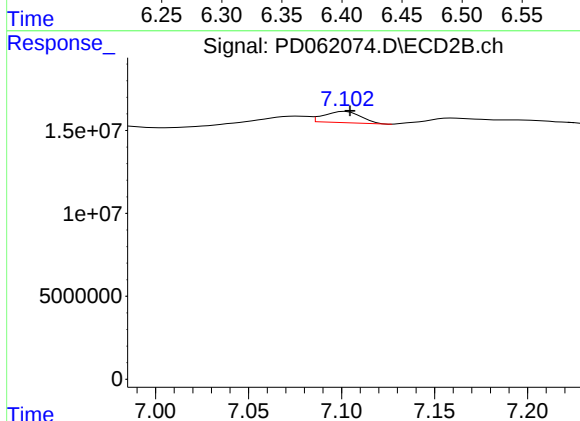


#17 4,4'-DDT

R.T.: 7.102 min
Delta R.T.: -0.003 min
Response: 9273111
Conc: 0.97 ng/ml

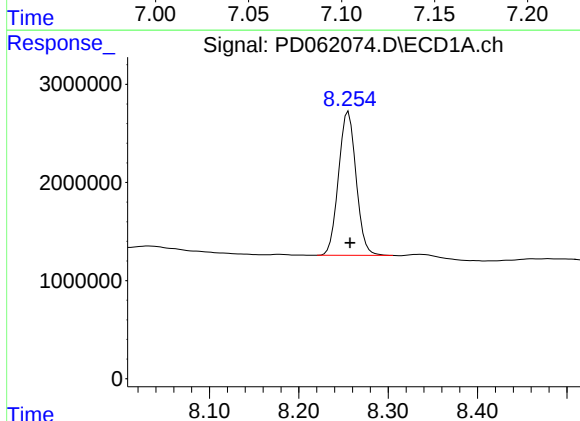

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 20007279
Conc: 16.26 ng/ml

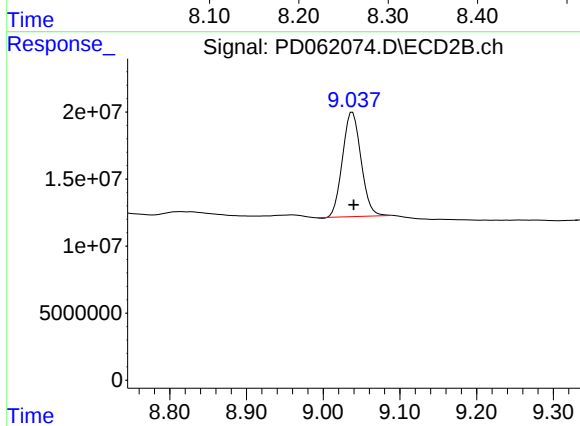

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 131270723
Conc: 13.90 ng/ml