

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040822\
 Data File : PD069006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 18:28
 Operator : AR\AJ
 Sample : N2281-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TR-05-040622

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/08/2022
 Supervised By : mohammad ahmed 04/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:13:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.175	11760300	116.3E6	9.686	12.162 #
2) SA Decachlor...	8.207	9.372	12144400	70415546	9.613	12.426 #
Target Compounds						
11) B alpha-Chl...	5.445	6.402	861170	18798605	0.576	1.888m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040822\
Data File : PD069006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 18:28
Operator : AR\AJ
Sample : N2281-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TR-05-040622


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/08/2022
Supervised By : mohammad ahmed 04/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:13:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

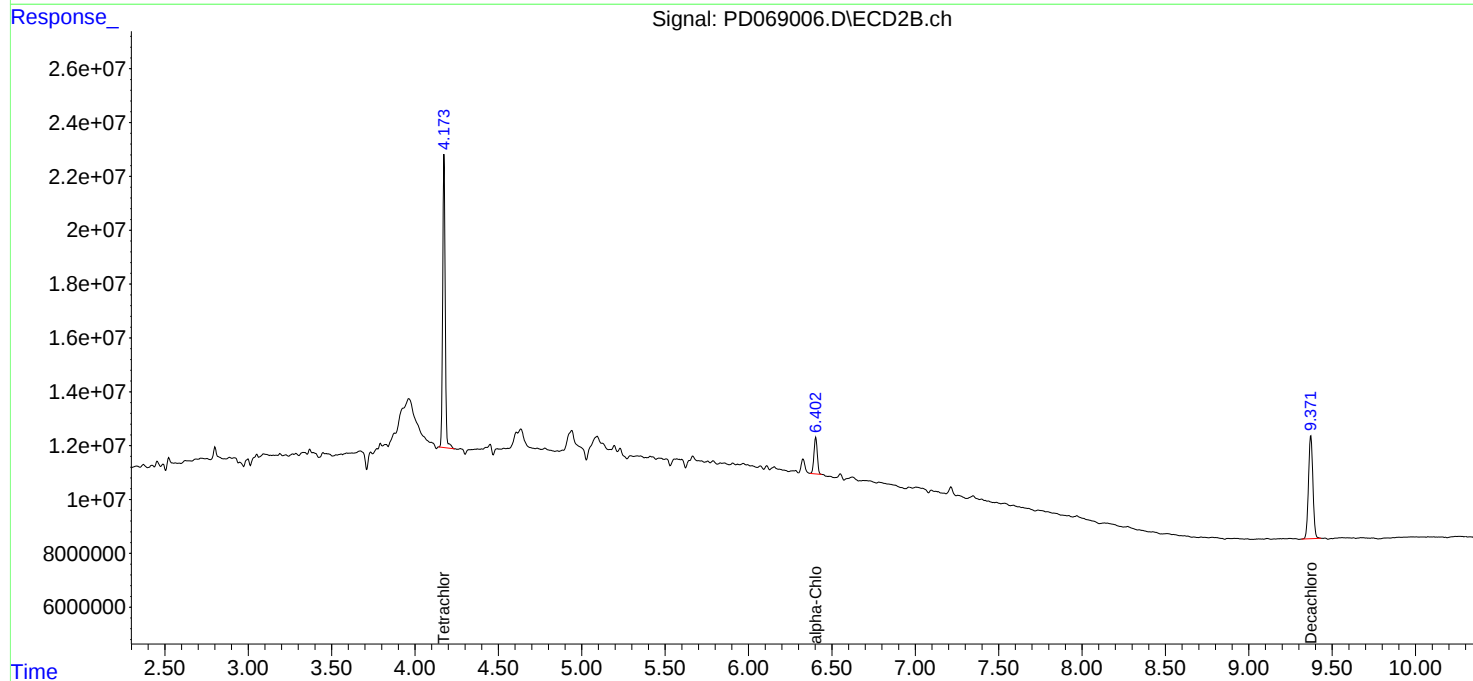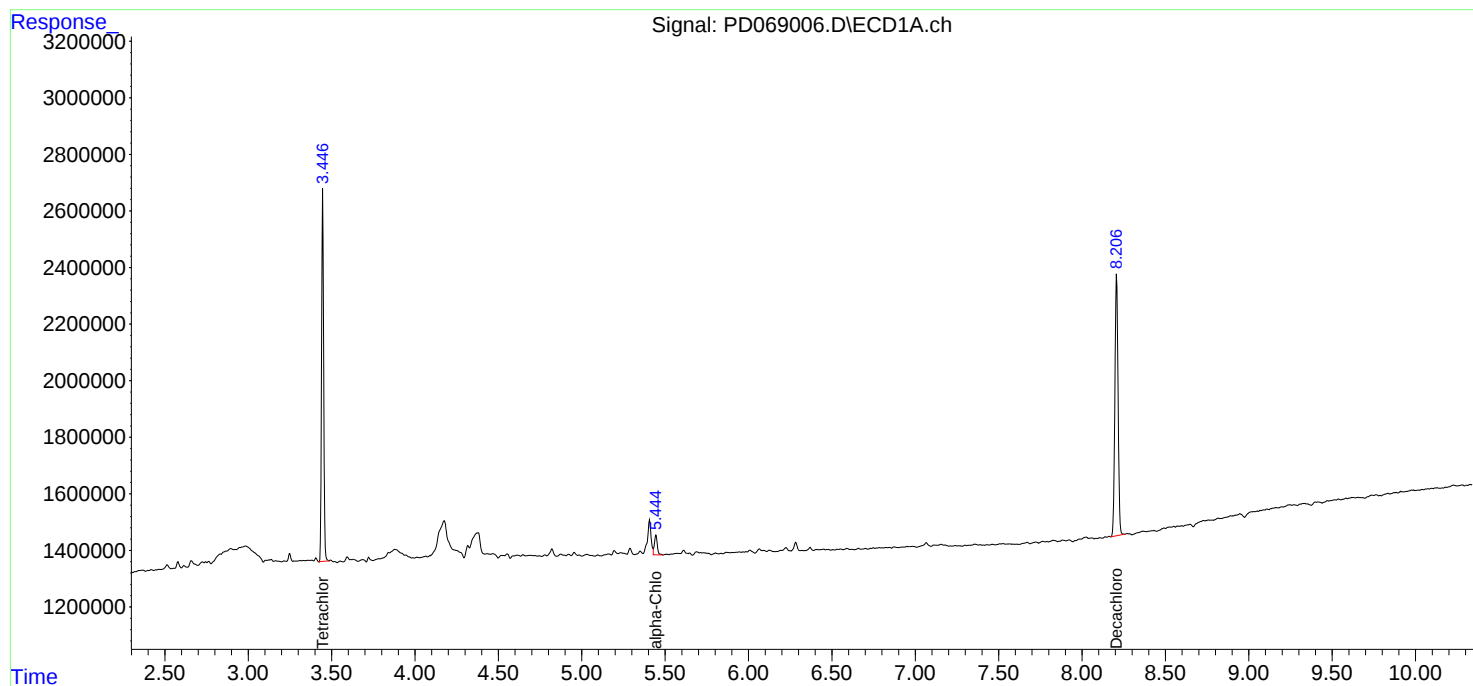

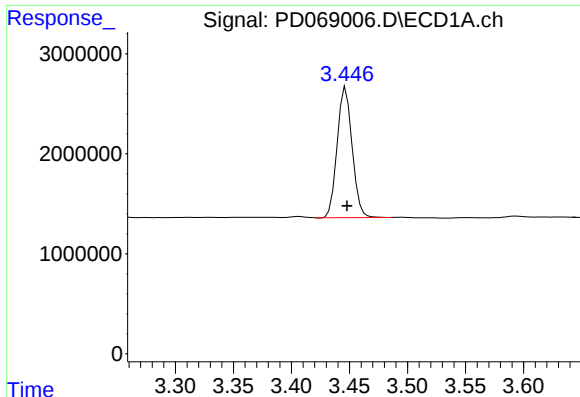


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.001 min
Response: 11760300
Conc: 9.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-05-040622


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/08/2022
Supervised By :mohammad ahmed 04/08/2022

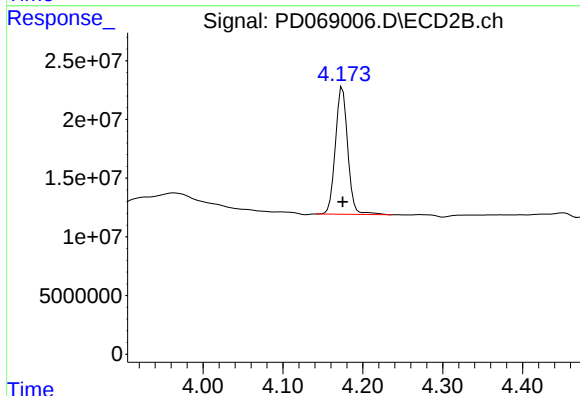


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 116277582
Conc: 12.16 ng/ml

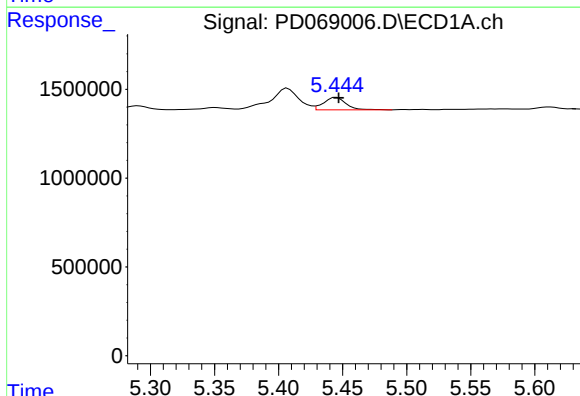


#11 alpha-Chlordane

R.T.: 5.445 min
Delta R.T.: -0.002 min
Response: 861170
Conc: 0.58 ng/ml

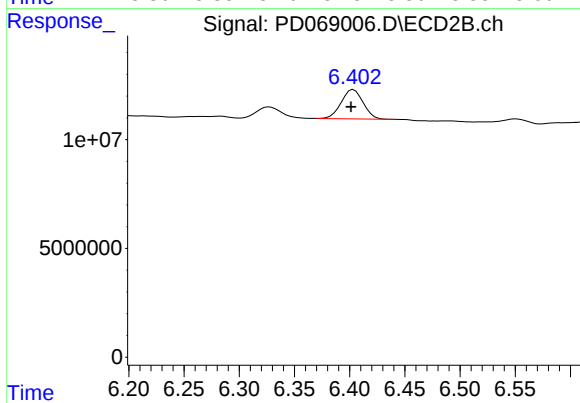

#11 alpha-Chlordane

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 18798605
Conc: 1.89 ng/ml m

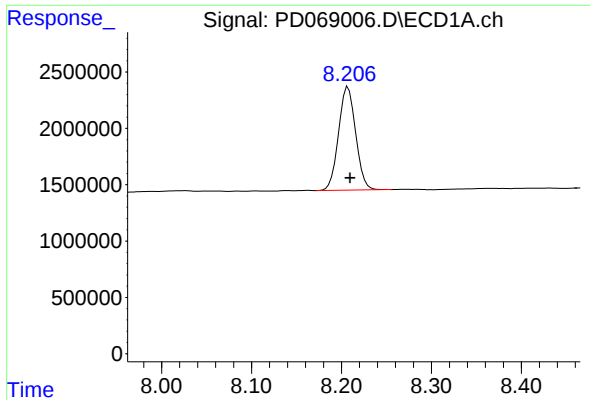


#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.002 min
Response: 12144400
Conc: 9.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-05-040622

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/08/2022
Supervised By :mohammad ahmed 04/08/2022

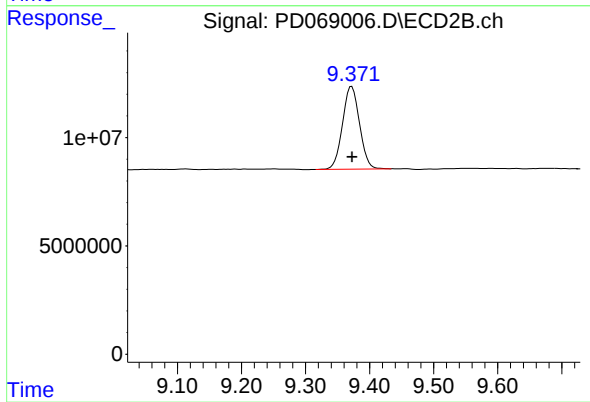

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 70415546
Conc: 12.43 ng/ml