

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040921\
 Data File : PD062100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:11
 Operator : AR\AJ
 Sample : M1966-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB_2021-04-06_GW

Manual Integrations
 APPROVED

Ankita
 4/12/2021 4:15:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:58:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.483	3.980	18938081	186.5E6	22.618m	21.462
28) SA Decachlor...	8.255	9.036	7890704	54022393	6.413	5.722m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040921\
Data File : PD062100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:11
Operator : AR\AJ
Sample : M1966-08
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
EB 2021-04-06_GW


Manual Integrations
APPROVED

Ankita
4/12/2021 4:15:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:58:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

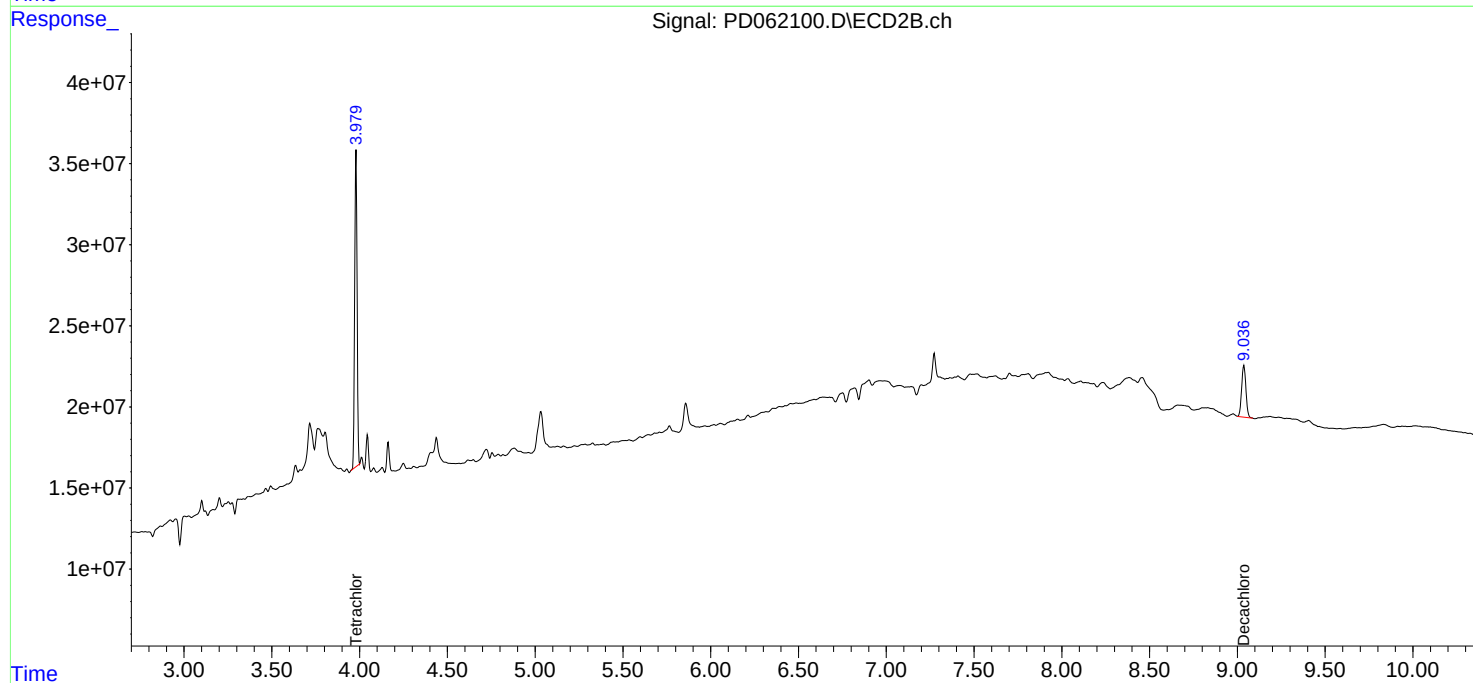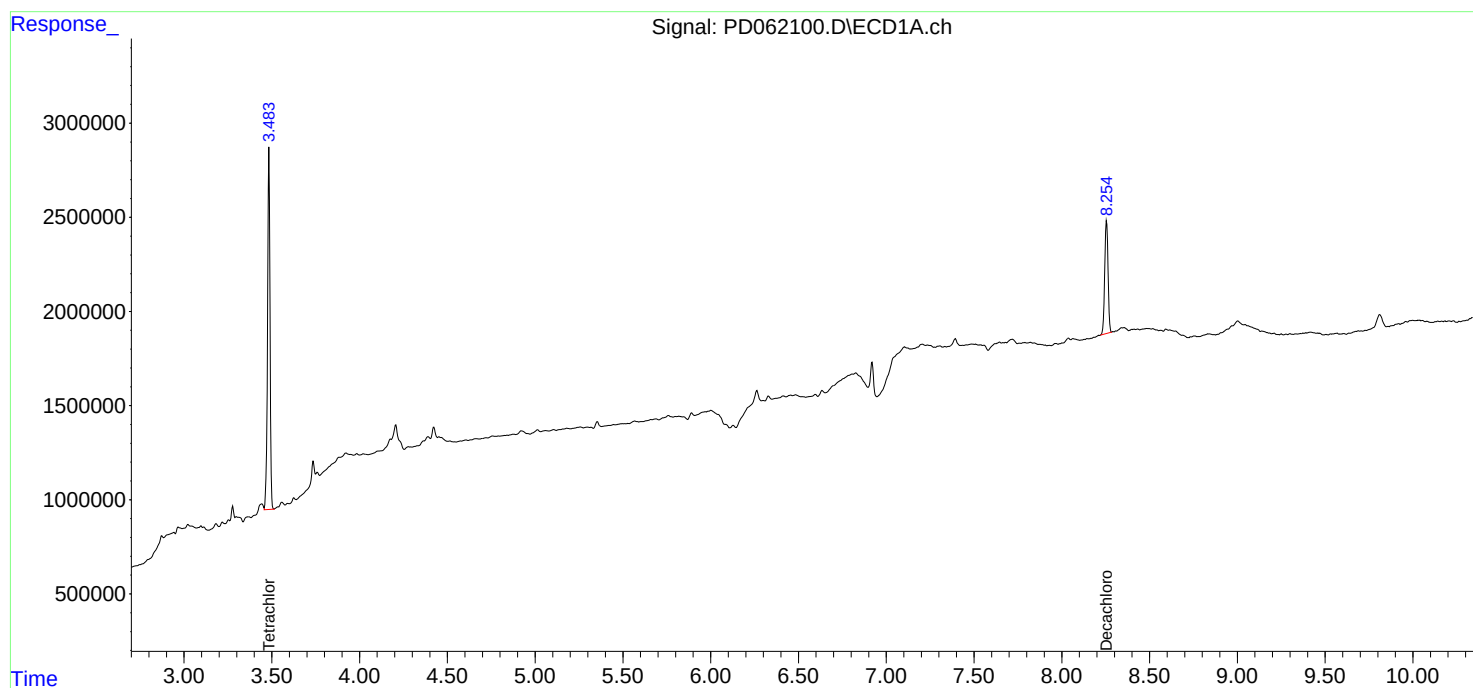

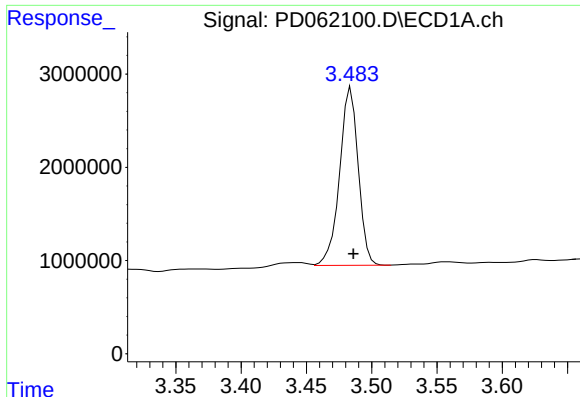

#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: -0.003 min
Response: 18938081
Conc: 22.62 ng/ml m

Instrument :


ECD_D

ClientSampleId :

EB_2021-04-06_GW


Manual Integrations
APPROVED

Ankita
4/12/2021 4:15:57 PM

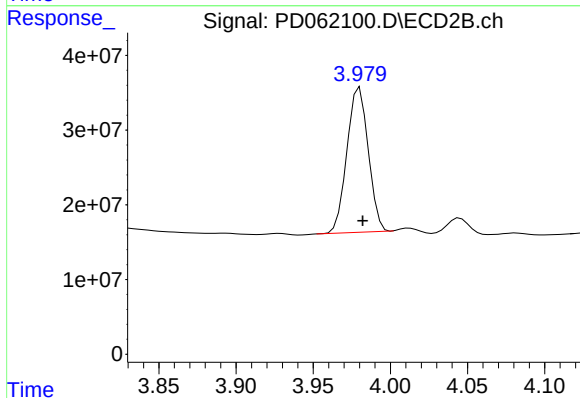


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 186479732
Conc: 21.46 ng/ml

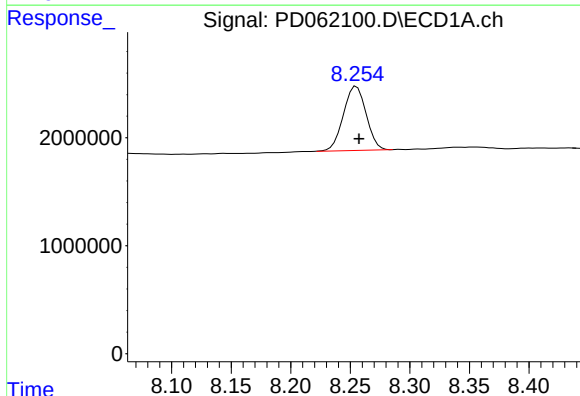

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 7890704
Conc: 6.41 ng/ml

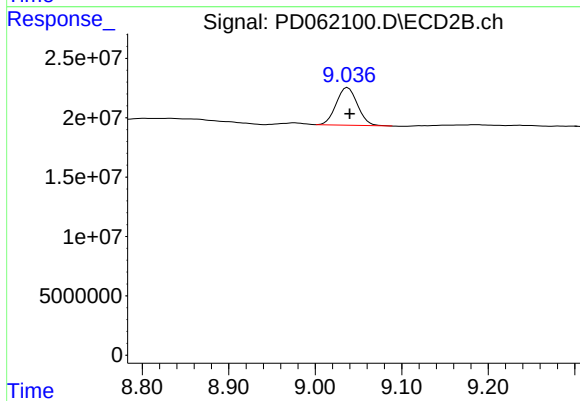

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.004 min
Response: 54022393
Conc: 5.72 ng/ml m