

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
 Data File : PD069016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 13:06
 Operator : AR\AJ
 Sample : PB143970BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 23:17:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.455	4.174	20310023	205.3E6	16.727	21.471 #
28)	SA Decachlor...	8.217	9.375	23653297	135.3E6	18.722	23.884 #
Target Compounds							
2)	A alpha-BHC	3.884	0.000	196578	0	0.109	N.D. #
3)	MA gamma-BHC...	4.184	4.859	612847	16516	0.367	0.001 #
4)	MA Heptachlor	0.000	5.389	0	449741	N.D.	0.038 #
6)	B beta-BHC	0.000	5.040f	0	6728396	N.D.	1.226 #
7)	B delta-BHC	0.000	5.228f	0	1187346	N.D.	0.099 #
8)	B Heptachlo...	0.000	6.075	0	488901	N.D.	0.047 #
11)	B alpha-Chl...	0.000	6.398	0	470369	N.D.	0.047 #
14)	MA Endrin	0.000	6.925	0	107077	N.D.	0.014 #
21)	B Endrin ke...	0.000	7.969	0	2219093	N.D.	0.286 #
26)	Chlordane-4	0.000	6.398	0	470369	N.D.	0.303 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
Data File : PD069016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 13:06
Operator : AR\AJ
Sample : PB143970BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 23:17:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

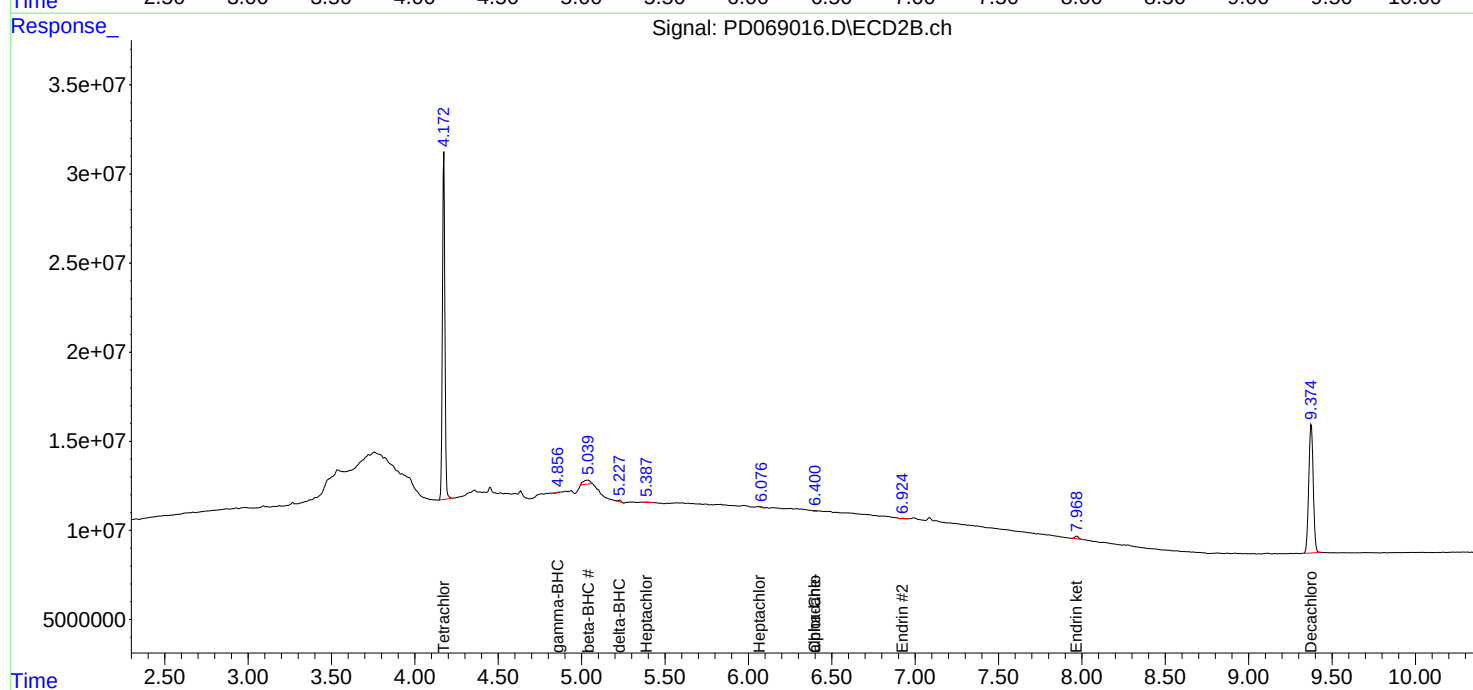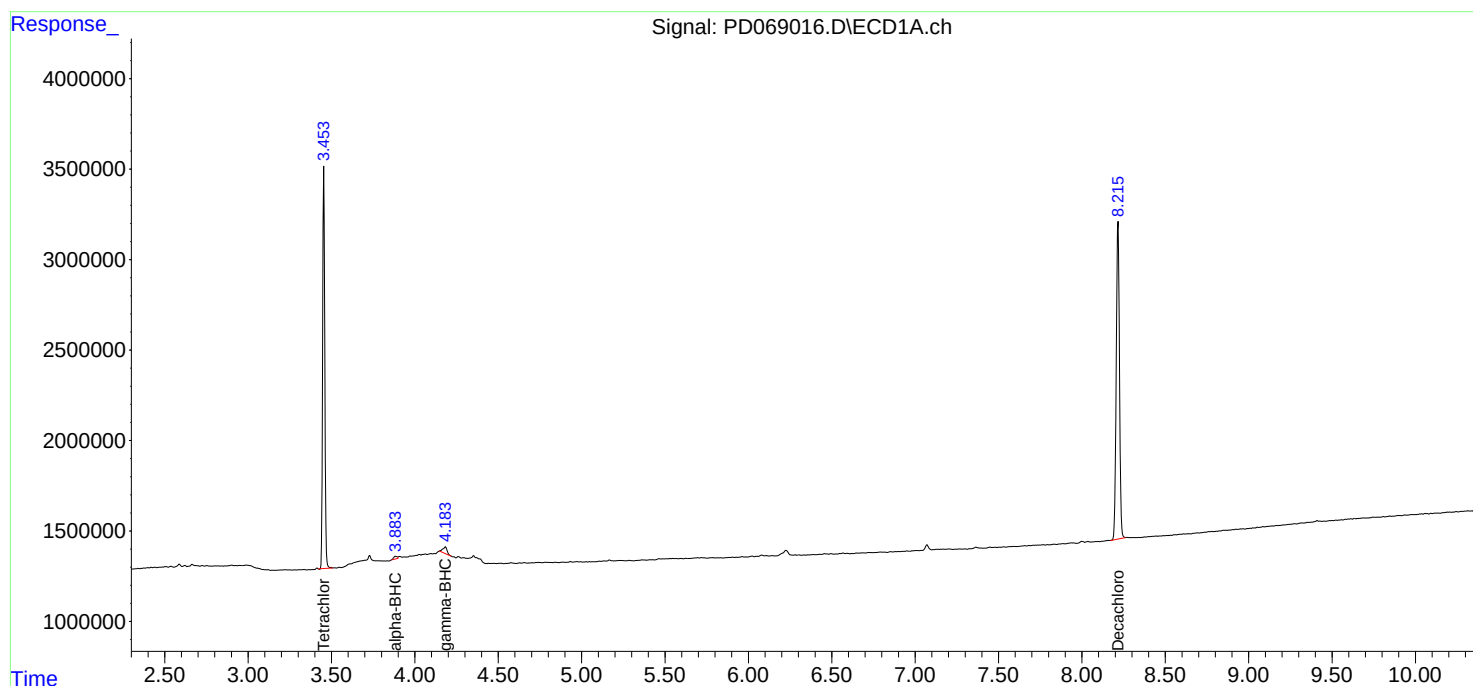


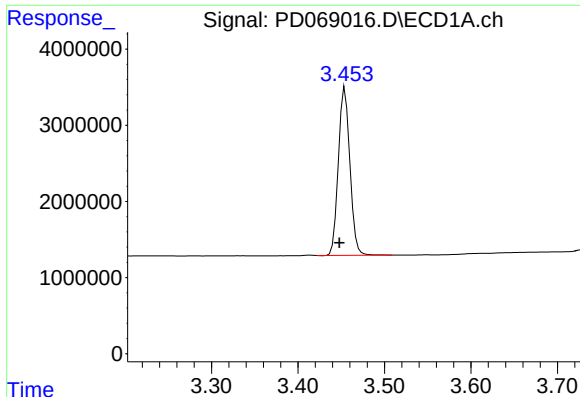

#1 Tetrachloro-m-xylene


R.T.: 3.455 min
Delta R.T.: 0.007 min
Response: 20310023
Conc: 16.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

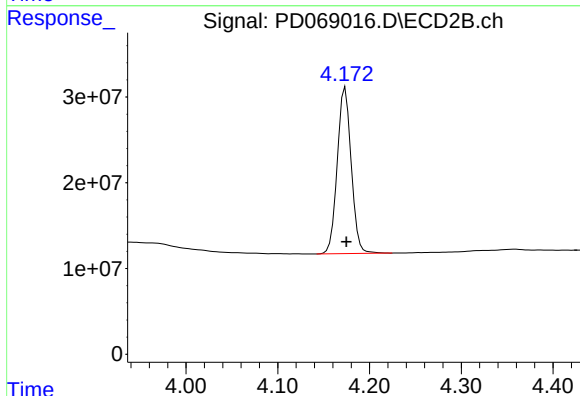


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.001 min
Response: 205278778
Conc: 21.47 ng/ml

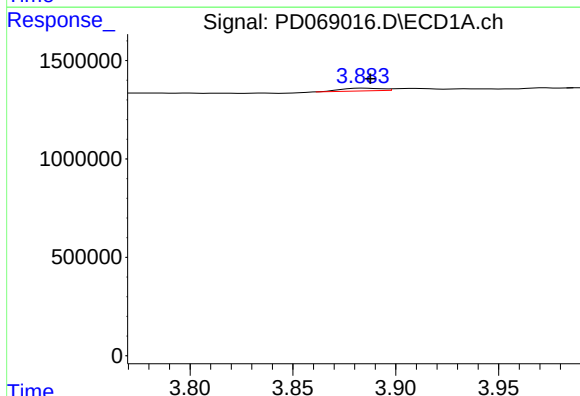


#2 alpha-BHC

R.T.: 3.884 min
Delta R.T.: -0.004 min
Response: 196578
Conc: 0.11 ng/ml

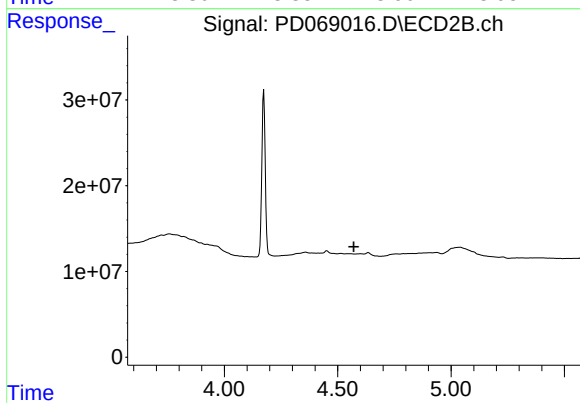

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

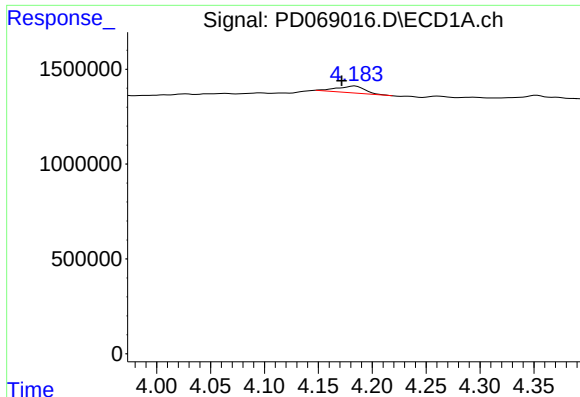

#3 gamma-BHC (Lindane)


R.T.: 4.184 min
Delta R.T.: 0.012 min
Response: 612847
Conc: 0.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

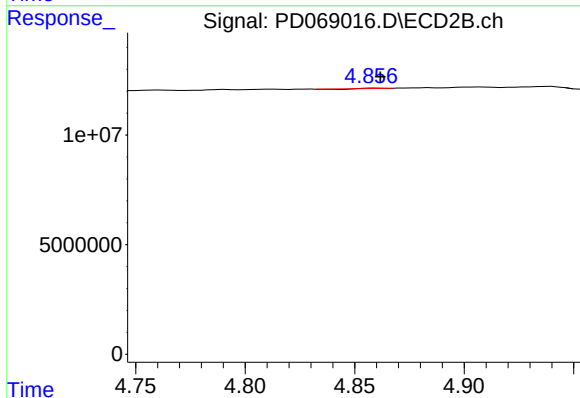


#3 gamma-BHC (Lindane)

R.T.: 4.859 min
Delta R.T.: -0.003 min
Response: 16516
Conc: 0.00 ng/ml

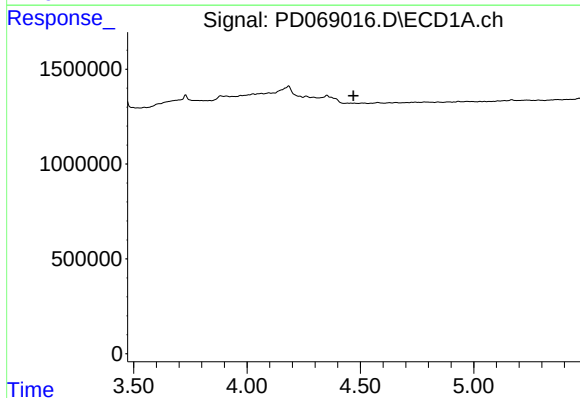


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

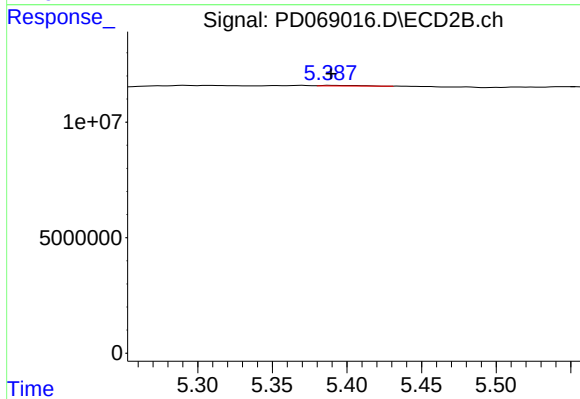

#4 Heptachlor


R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 449741
Conc: 0.04 ng/ml

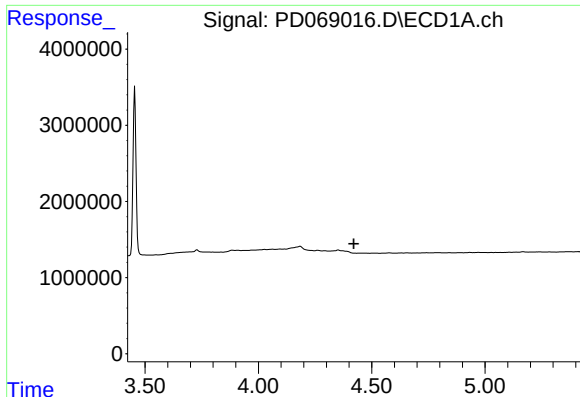

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

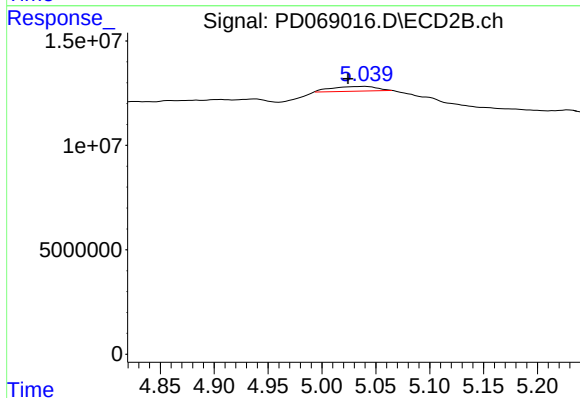


#6 beta-BHC

R.T.: 5.040 min
Delta R.T.: 0.016 min
Response: 6728396
Conc: 1.23 ng/ml

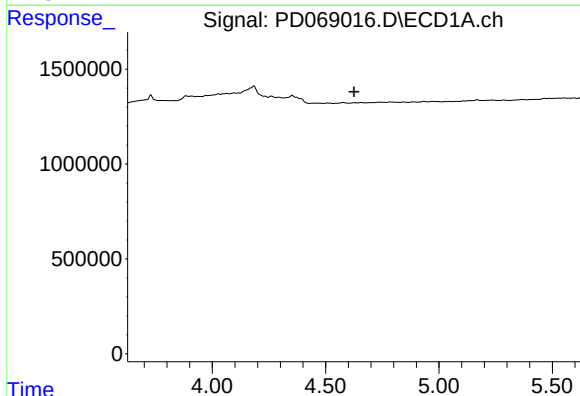


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

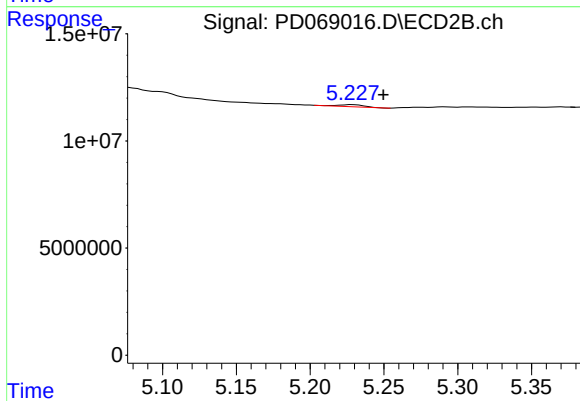

#7 delta-BHC


R.T.: 5.228 min
Delta R.T.: -0.021 min
Response: 1187346
Conc: 0.10 ng/ml

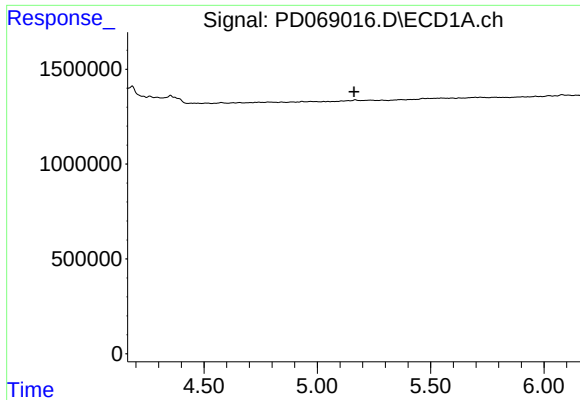

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

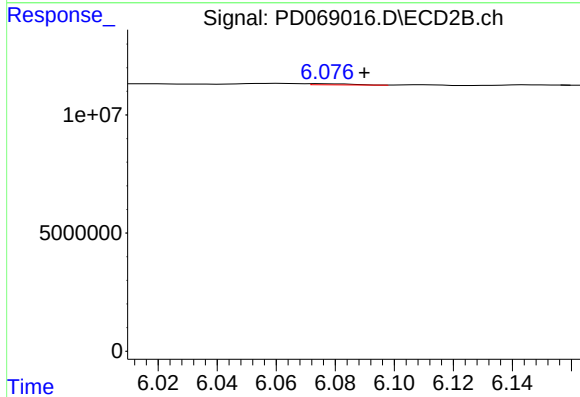


#8 Heptachlor epoxide

R.T.: 6.075 min
Delta R.T.: -0.015 min
Response: 488901
Conc: 0.05 ng/ml

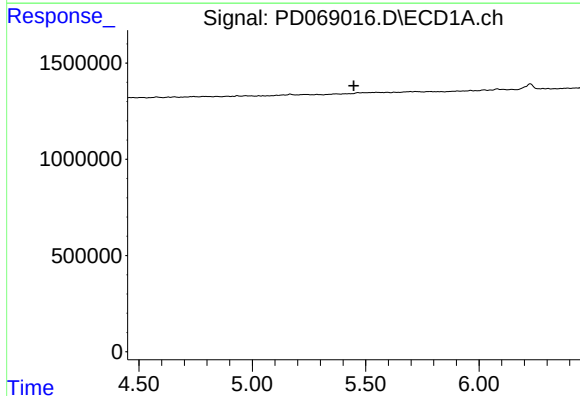


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

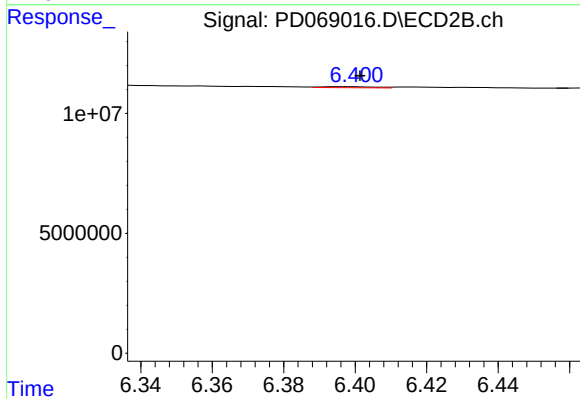

#11 alpha-Chlordane


R.T.: 6.398 min
Delta R.T.: -0.003 min
Response: 470369
Conc: 0.05 ng/ml

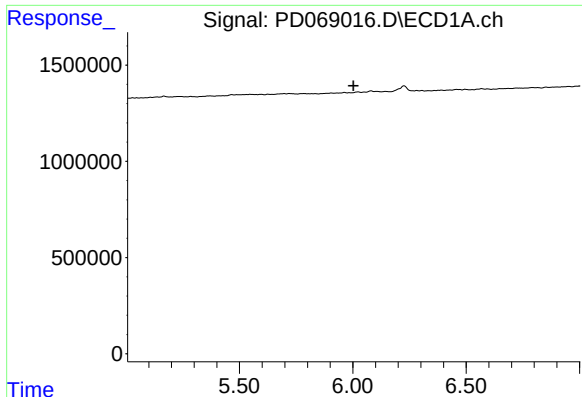

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

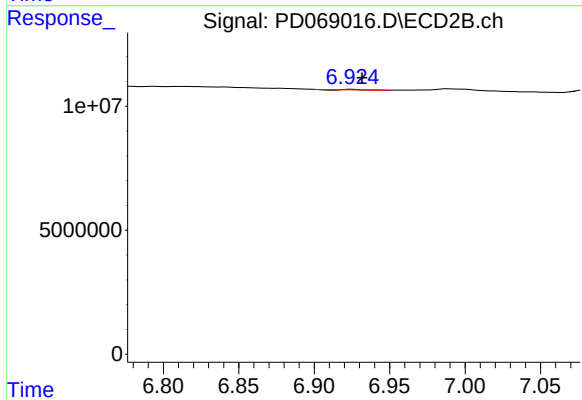


#14 Endrin

R.T.: 6.925 min
Delta R.T.: -0.006 min
Response: 107077
Conc: 0.01 ng/ml

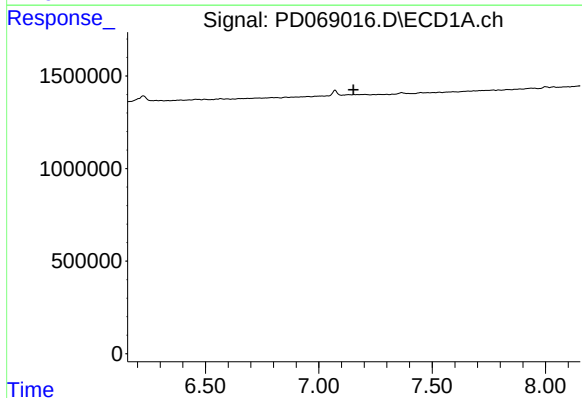


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

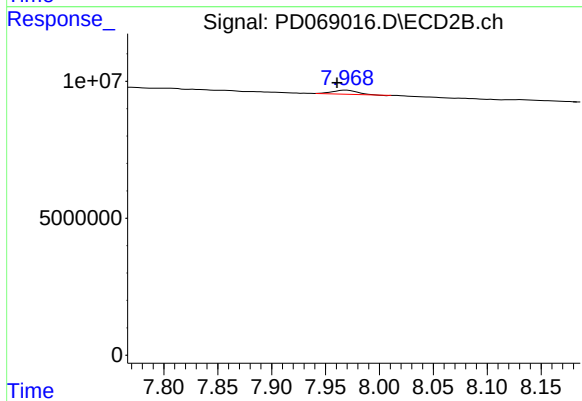

#21 Endrin ketone


R.T.: 7.969 min
Delta R.T.: 0.008 min
Response: 2219093
Conc: 0.29 ng/ml

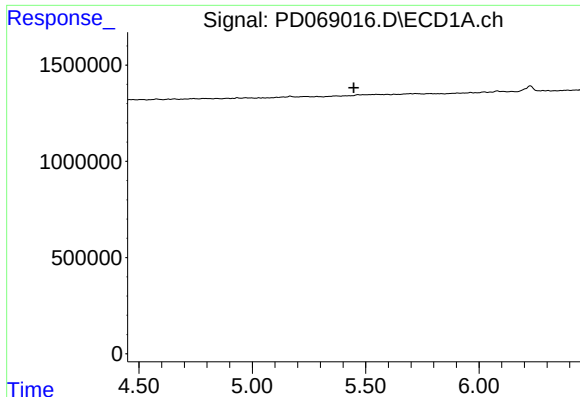

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

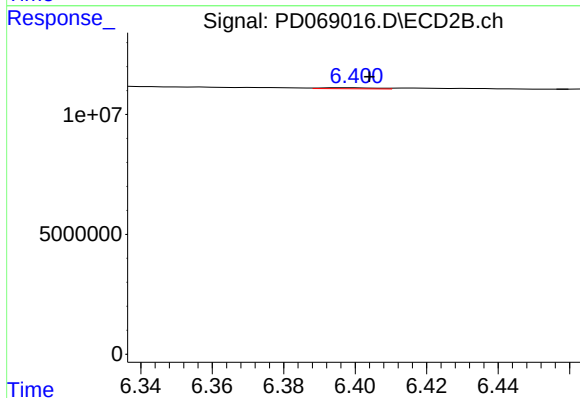


#26 Chlordane-4

R.T.: 6.398 min
Delta R.T.: -0.006 min
Response: 470369
Conc: 0.30 ng/ml

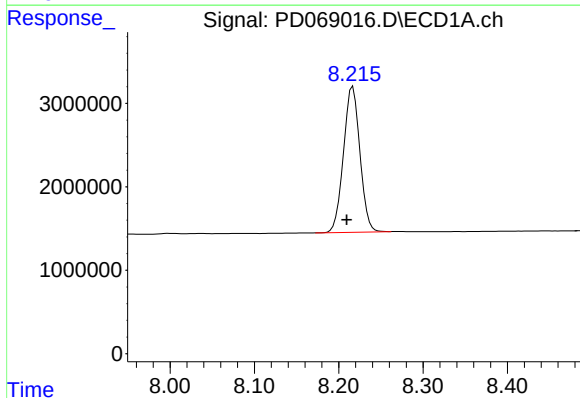

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: 0.007 min
Response: 23653297
Conc: 18.72 ng/ml

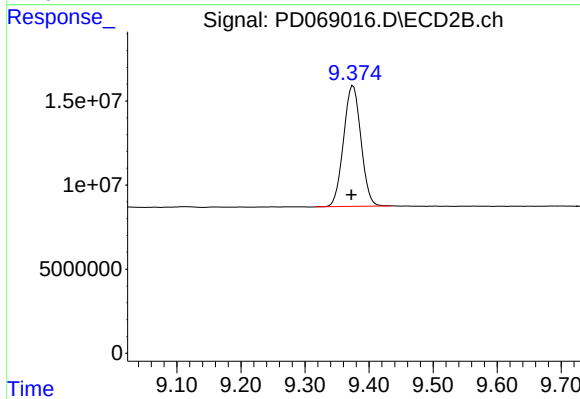

#28 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.003 min
Response: 135345664
Conc: 23.88 ng/ml