

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
 Data File : PD069038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 17:50
 Operator : AR\AJ
 Sample : N2317-23
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP2-B

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/09/2022
 Supervised By : mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 23:23:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.174	25970024	233.1E6	21.389	24.385
28) SA Decachlor...	8.206	9.370	21202637	105.4E6	16.782	18.606m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
Data File : PD069038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 17:50
Operator : AR\AJ
Sample : N2317-23
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP2-B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/09/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 23:23:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

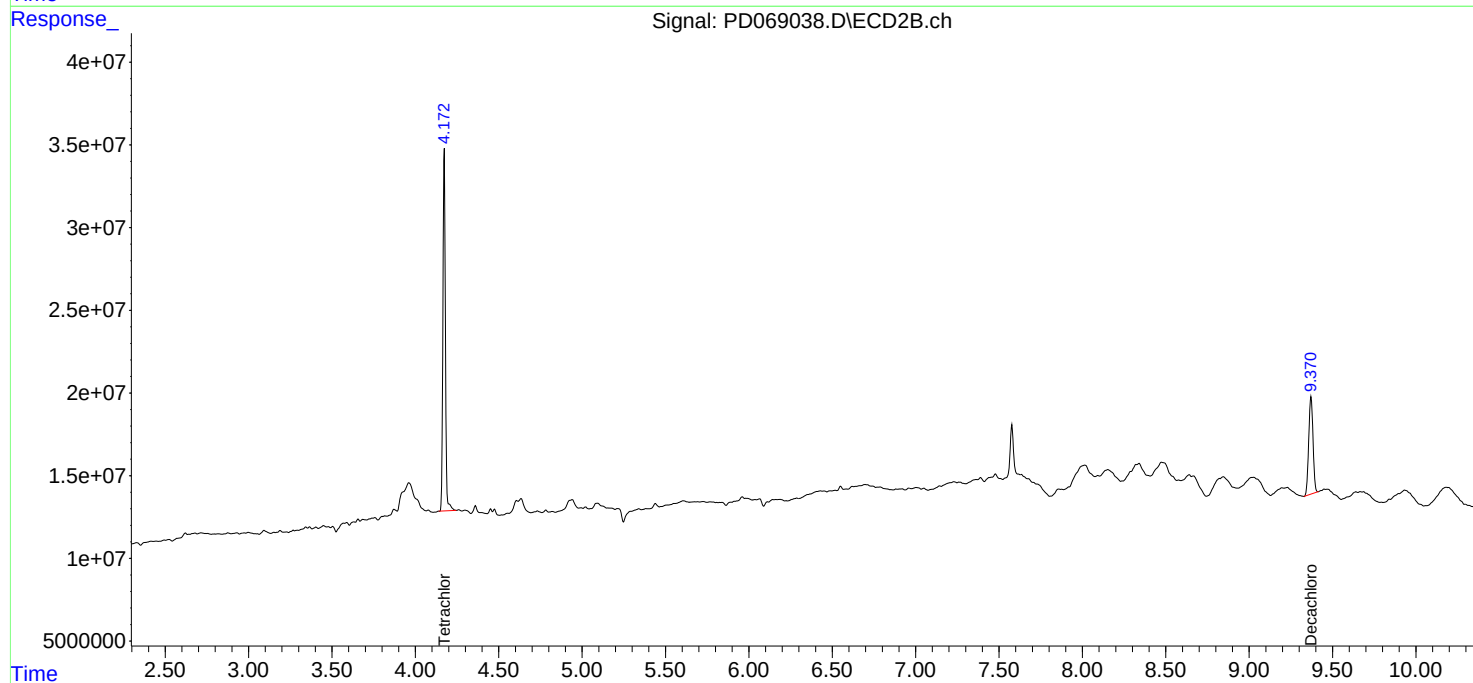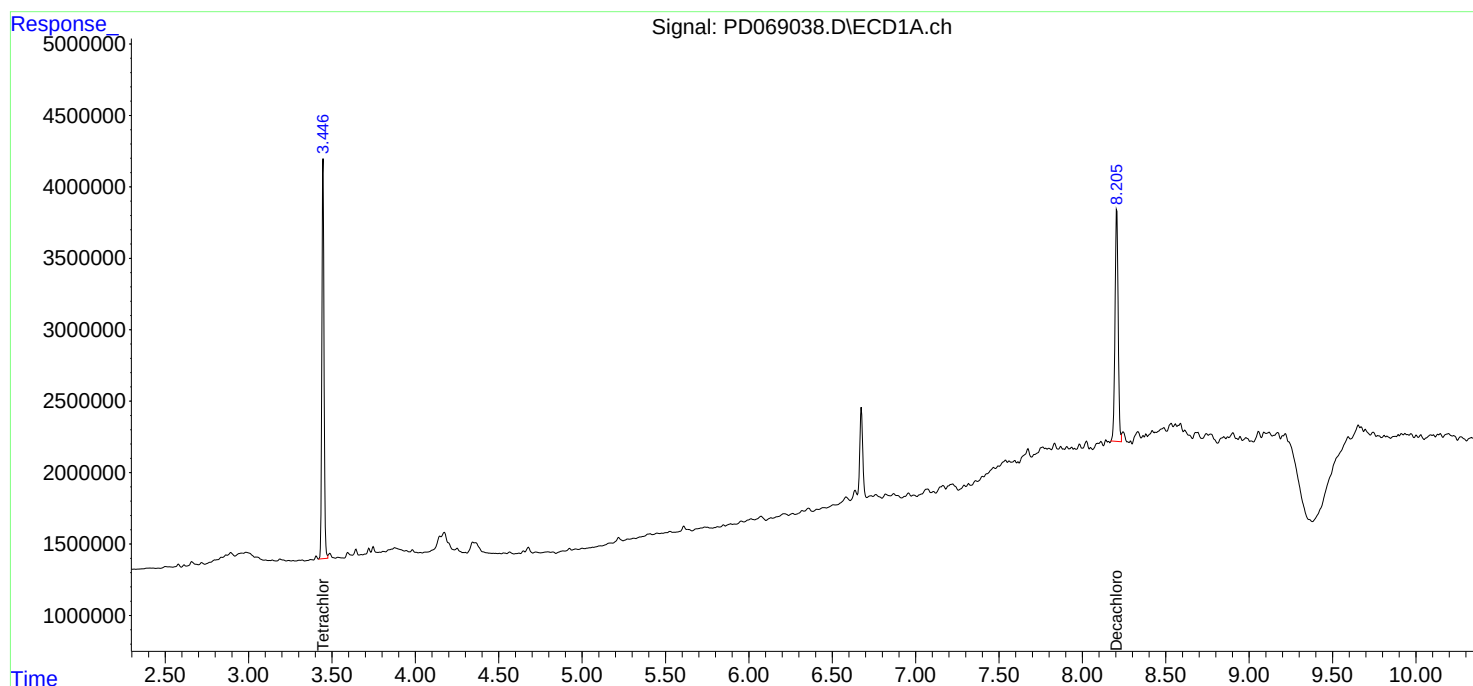

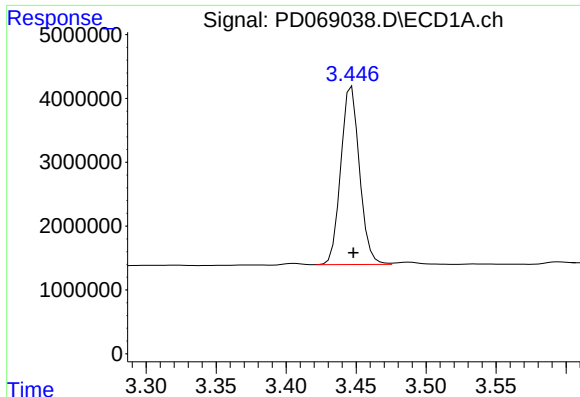


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.001 min
Response: 25970024
Conc: 21.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP2-B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/09/2022
Supervised By :mohammad ahmed 04/11/2022

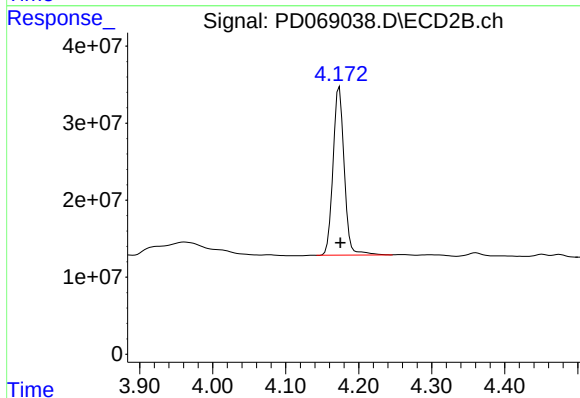


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.001 min
Response: 233142680
Conc: 24.39 ng/ml

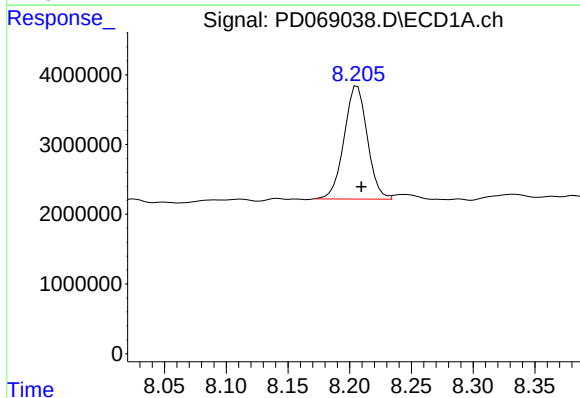

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.003 min
Response: 21202637
Conc: 16.78 ng/ml

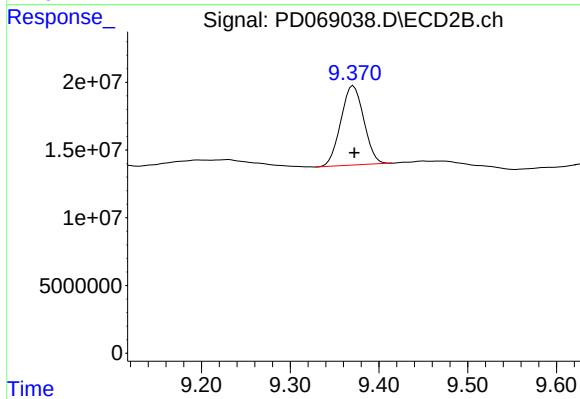

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: -0.003 min
Response: 105435789
Conc: 18.61 ng/ml m